

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
 Data File : BN021119.D
 Acq On : 10 Aug 2022 15:55
 Operator : CG/JU
 Sample : N4128-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBT4

Quant Time: Aug 10 16:40:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.788	152	2988	0.400	ng/ul	0.00
4) Naphthalene-d8	10.580	136	9988	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.438	164	5768	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.184	188	11148	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	8266	0.400	ng/ul	0.00
23) Perylene-d12	23.719	264	7925	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	14304	3.742	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	4147	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.226	212	9986	0.391	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	162	0.041	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
Data File : BN021119.D
Acq On : 10 Aug 2022 15:55
Operator : CG/JU
Sample : N4128-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBT4


Quant Time: Aug 10 16:40:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

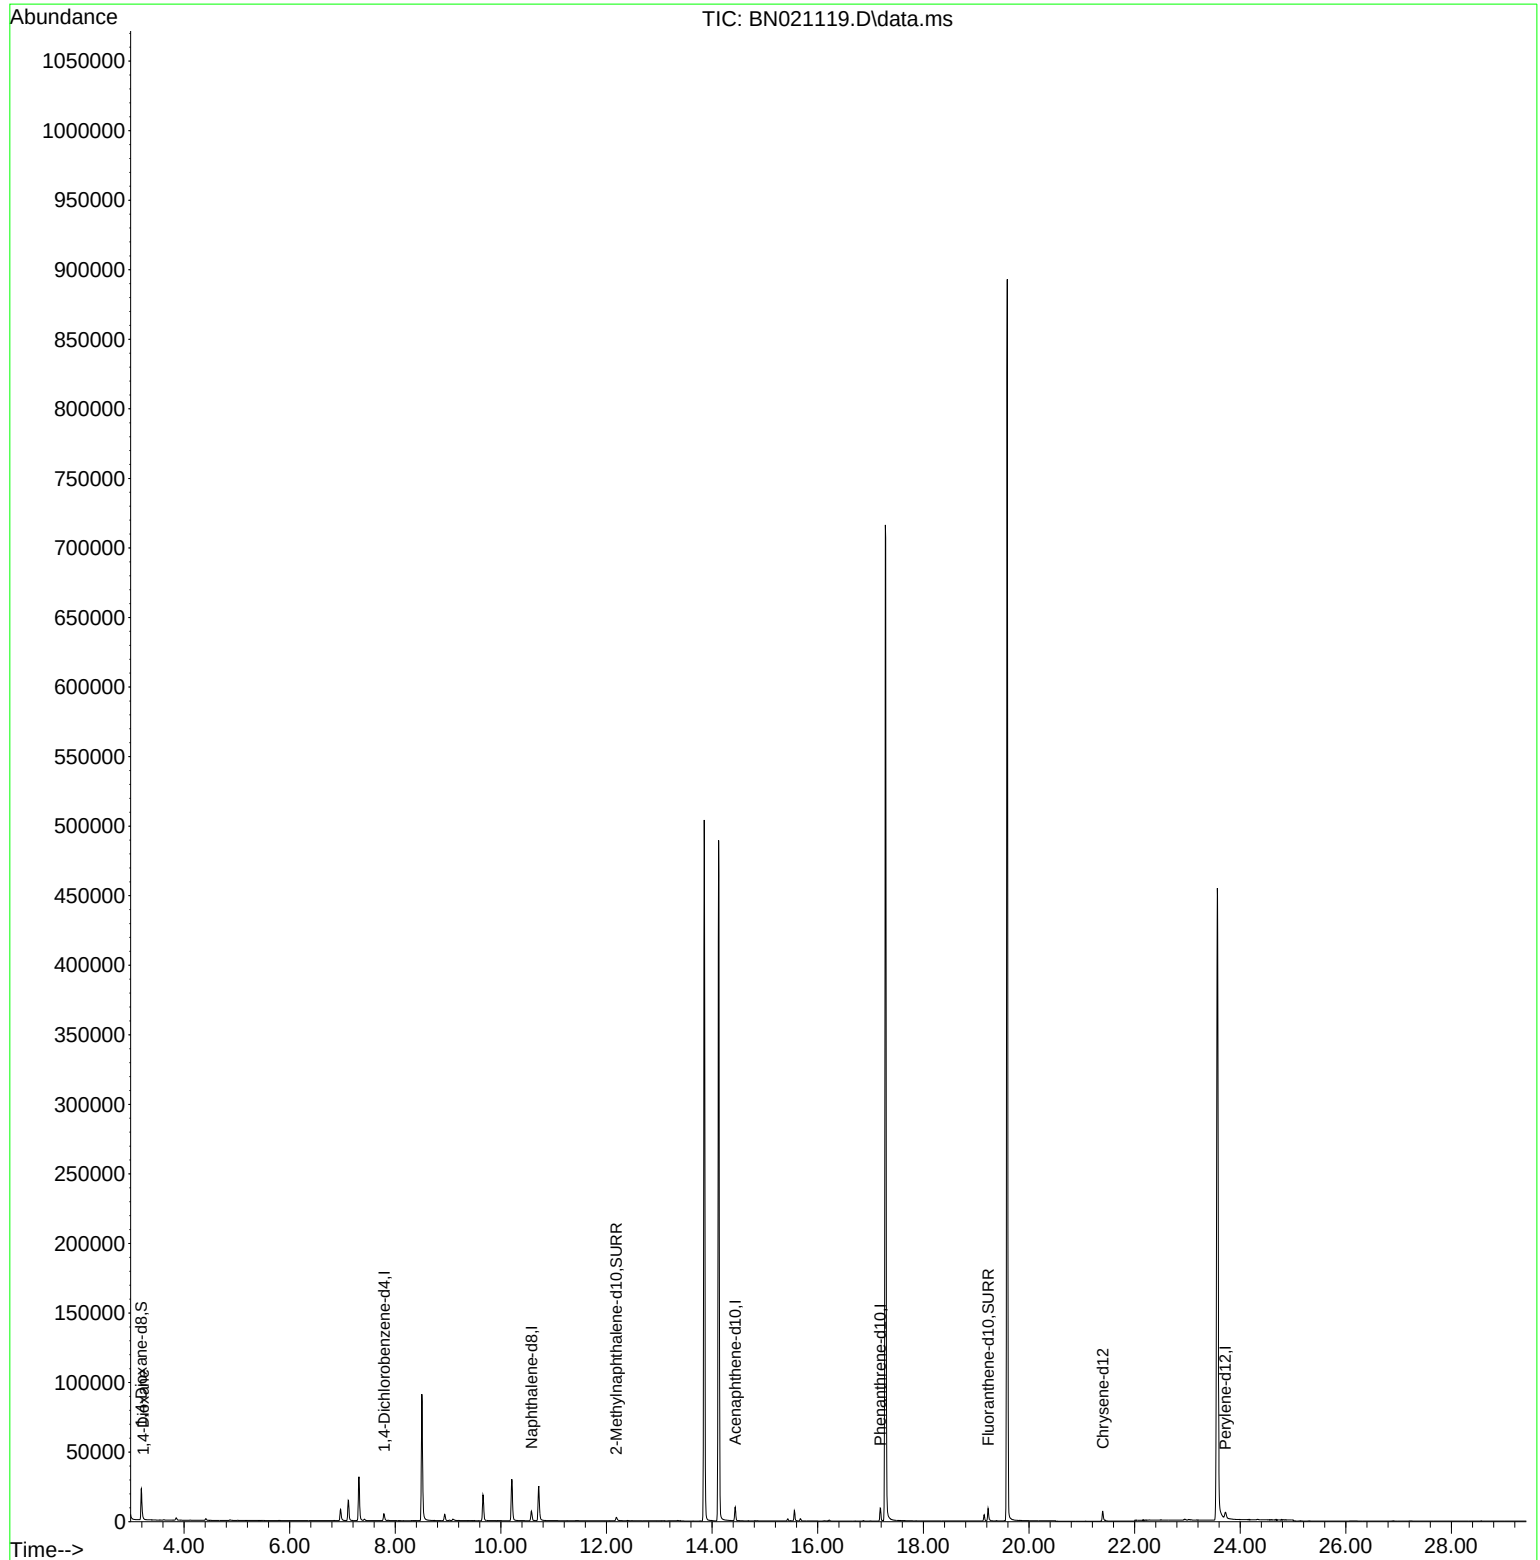

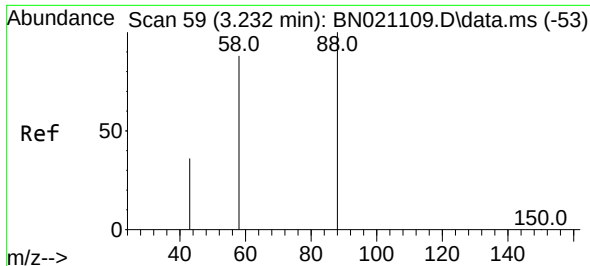

#2
 1,4-Dioxane
 Concen: 0.041 ng/ul
 RT: 3.228 min Scan# 58
 Delta R.T. -0.000 min
 Lab File: BN021119.D
 Acq: 10 Aug 2022 15:55

Instrument :
 BNA_N
 ClientSampleId :
 BGBT4

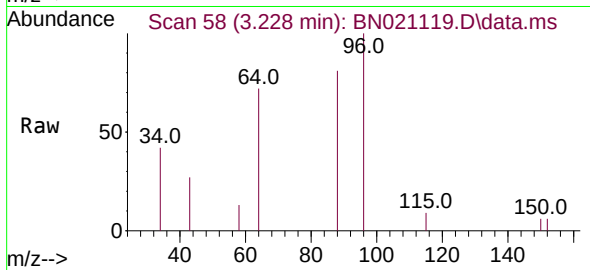

Tgt Ion: 88 Resp: 162

Ion	Ratio	Lower	Upper
88	100		
43	33.8	31.4	47.0
58	16.2	49.0	73.6

