

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
 Data File : BN021120.D
 Acq On : 10 Aug 2022 16:32
 Operator : CG/JU
 Sample : N4128-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBX3

Quant Time: Aug 10 17:42:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	2694	0.400	ng/ul	0.00
4) Naphthalene-d8	10.580	136	8993	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.438	164	5254	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.189	188	10179	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240	7281	0.400	ng/ul	0.00
23) Perylene-d12	23.722	264	7147	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	16009	4.645	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	4501	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.226	212	10644	0.473	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.232	88	411	0.116	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
Data File : BN021120.D
Acq On : 10 Aug 2022 16:32
Operator : CG/JU
Sample : N4128-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBX3

Quant Time: Aug 10 17:42:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

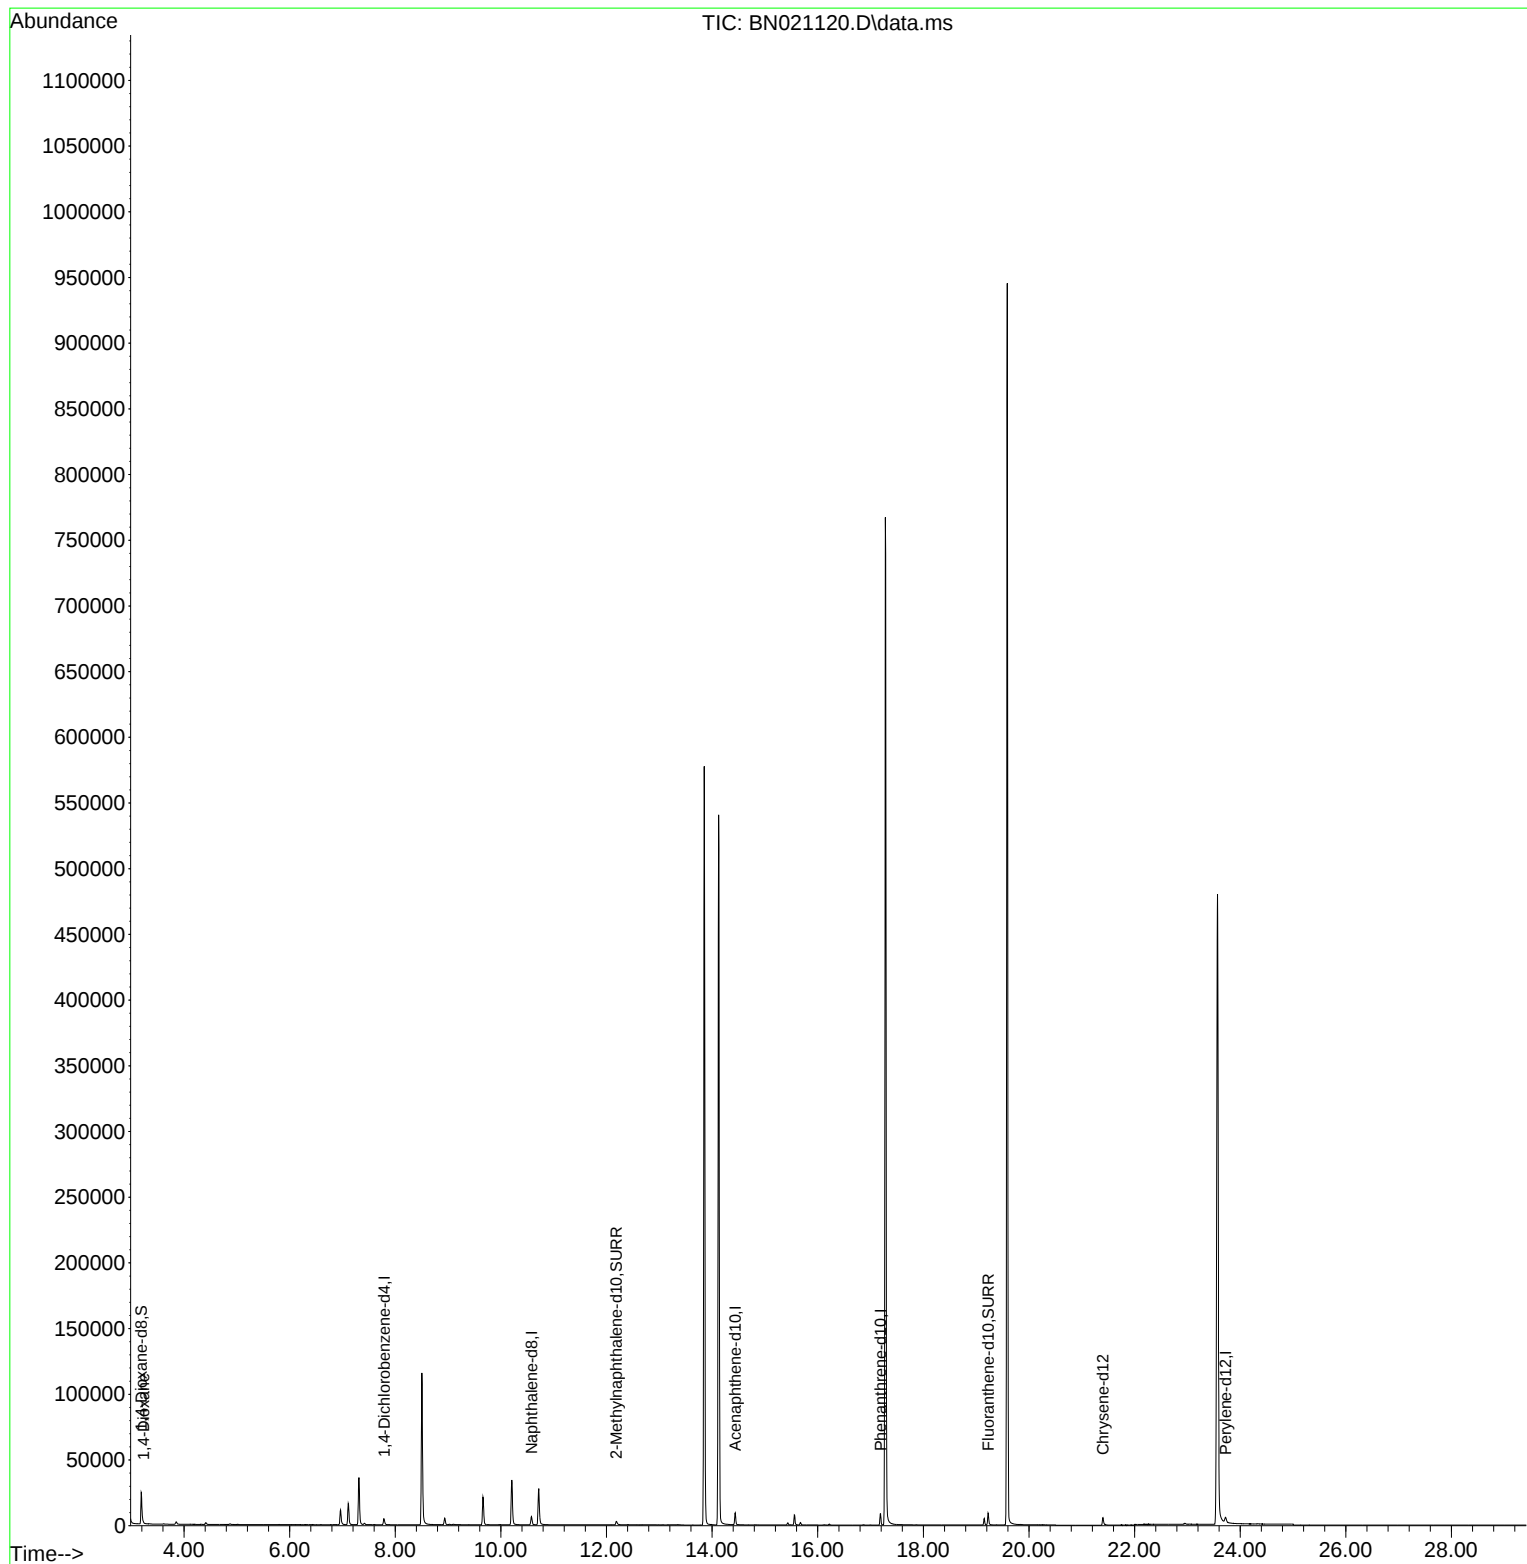

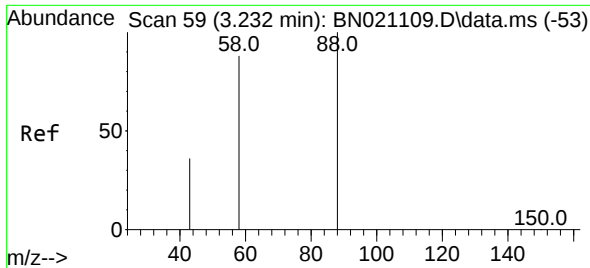

#2
 1,4-Dioxane
 Concen: 0.116 ng/ul
 RT: 3.232 min Scan# 59
 Delta R.T. 0.004 min
 Lab File: BN021120.D
 Acq: 10 Aug 2022 16:32

Instrument :
 BNA_N
 ClientSampleId :
 BGBX3

Tgt Ion:	88	Resp:	411
Ion	Ratio	Lower	Upper
88	100		
43	34.1	31.4	47.0
58	29.4	49.0	73.6

