

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
 Data File : BN021129.D
 Acq On : 10 Aug 2022 22:45
 Operator : CG/JU
 Sample : N4128-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBT8

Quant Time: Aug 11 02:20:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.788	152	2727	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	9076	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.438	164	5241	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	10226	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	7530	0.400	ng/ul	0.00
23) Perylene-d12	23.718	264	7725	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	15516	4.447	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.191	152	4322	0.325	ng/ul	0.01
18) Fluoranthene-d10	19.226	212	10678	0.459	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	370	0.103	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\  
Data File : BN021129.D  
Acq On    : 10 Aug 2022   22:45  
Operator  : CG/JU  
Sample    : N4128-11  
Misc      :  
ALS Vial  : 22    Sample Multiplier: 1
```

Quant Time: Aug 11 02:20:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

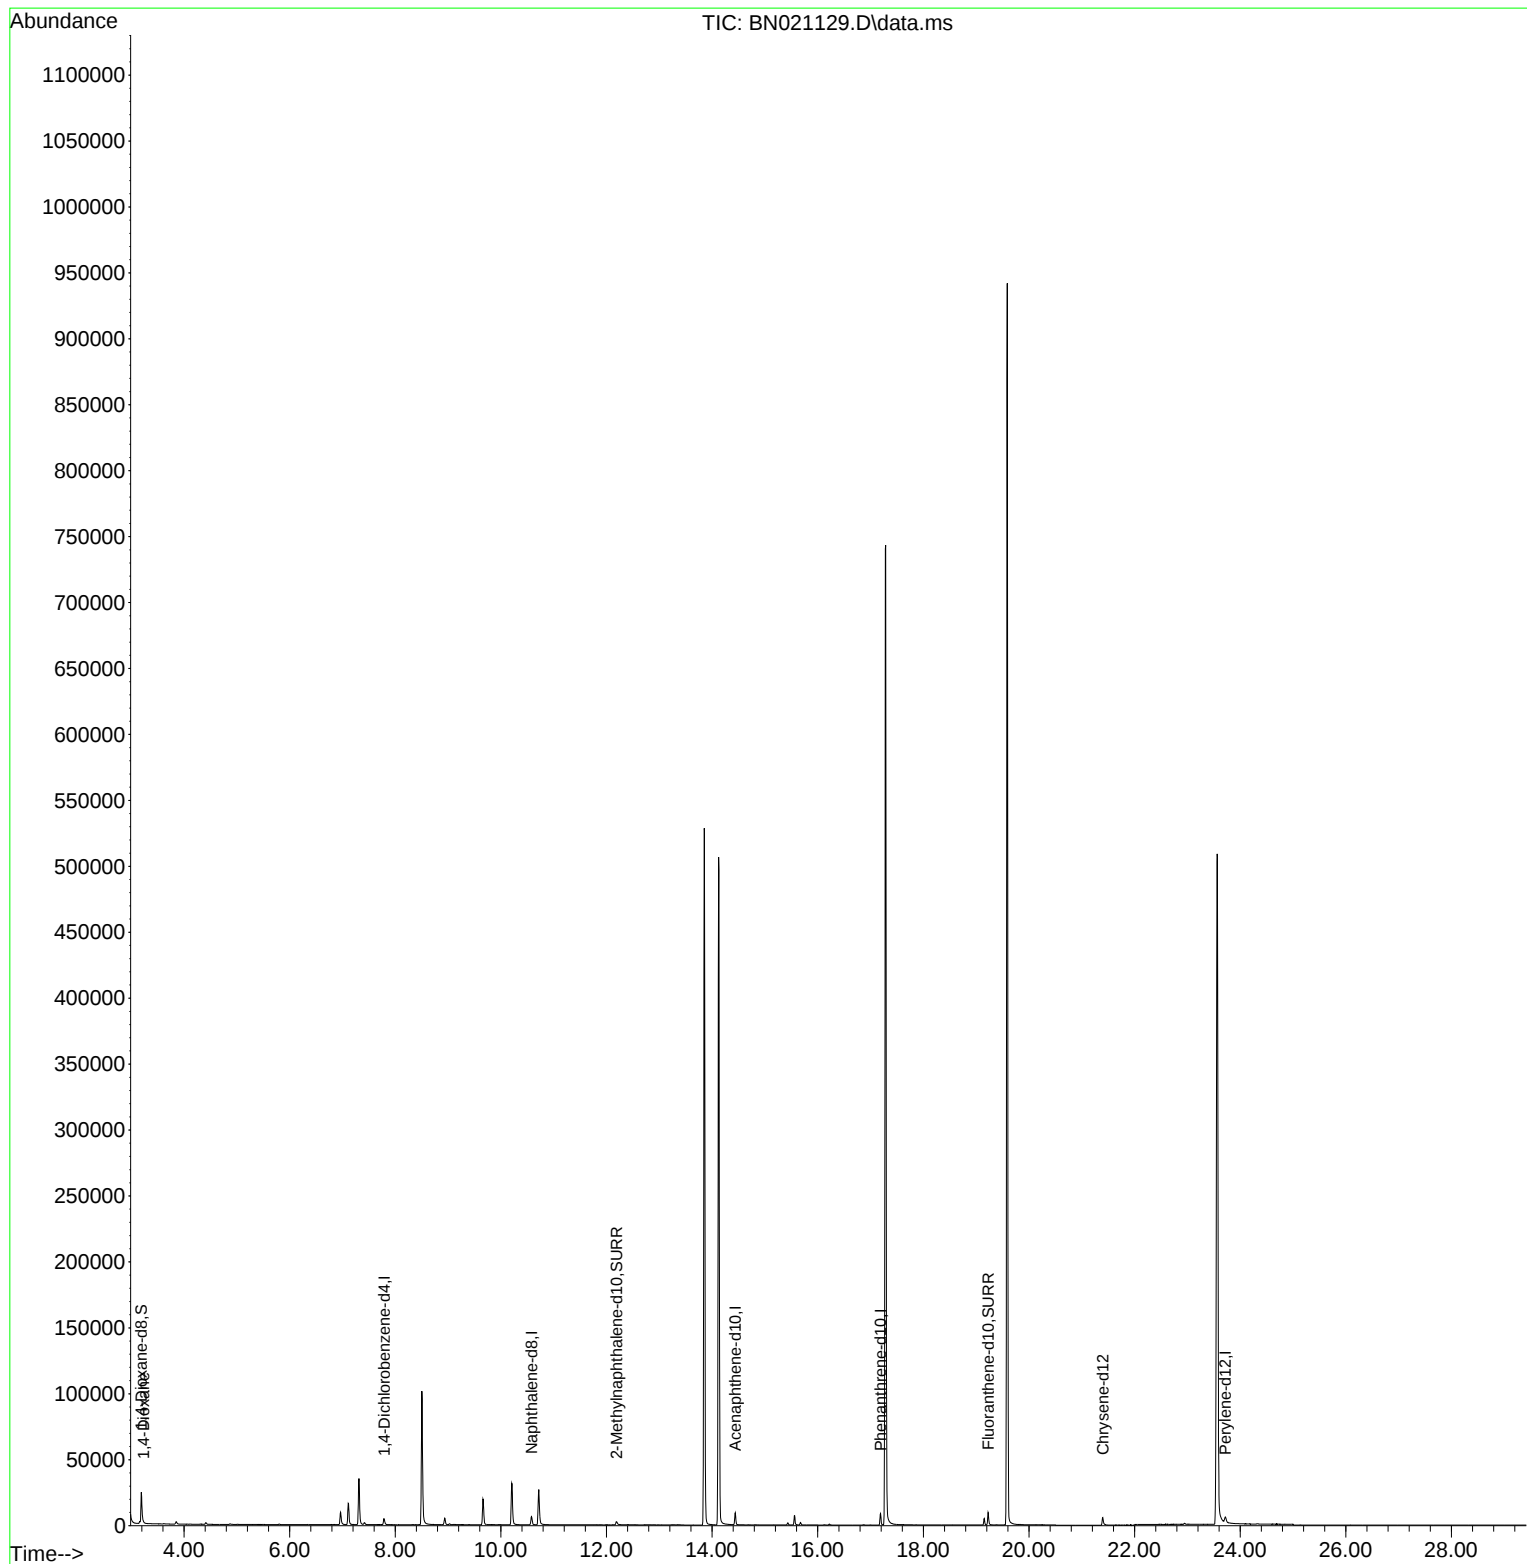

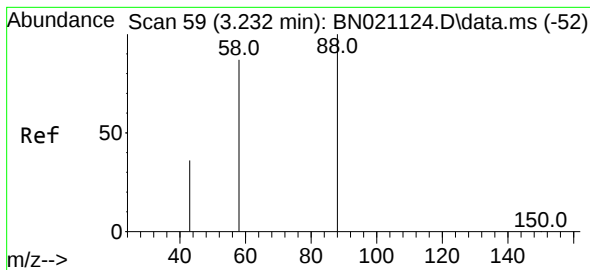

#2
 1,4-Dioxane
 Concen: 0.103 ng/ul
 RT: 3.231 min Scan# 59
 Delta R.T. 0.004 min
 Lab File: BN021129.D
 Acq: 10 Aug 2022 22:45

Instrument :
 BNA_N
 ClientSampleId :
 BGBT8

Tgt Ion:	88	Resp:	370
Ion	Ratio	Lower	Upper
88	100		
43	29.7	31.4	47.0#
58	21.8	49.0	73.6#

