

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
 Data File : BN021151.D
 Acq On : 11 Aug 2022 17:17
 Operator : CG/JU
 Sample : N4129-08
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBT1

Quant Time: Aug 11 18:19:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	2677	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	8984	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.437	164	5231	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.187	188	10196	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240	6869	0.400	ng/ul	0.00
23) Perylene-d12	23.725	264	6933	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	14333	4.185	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.190	152	3991	0.303	ng/ul	0.01
18) Fluoranthene-d10	19.229	212	9701	0.457	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.232	88	327	0.093	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
Data File : BN021151.D
Acq On : 11 Aug 2022 17:17
Operator : CG/JU
Sample : N4129-08
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBT1


Quant Time: Aug 11 18:19:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

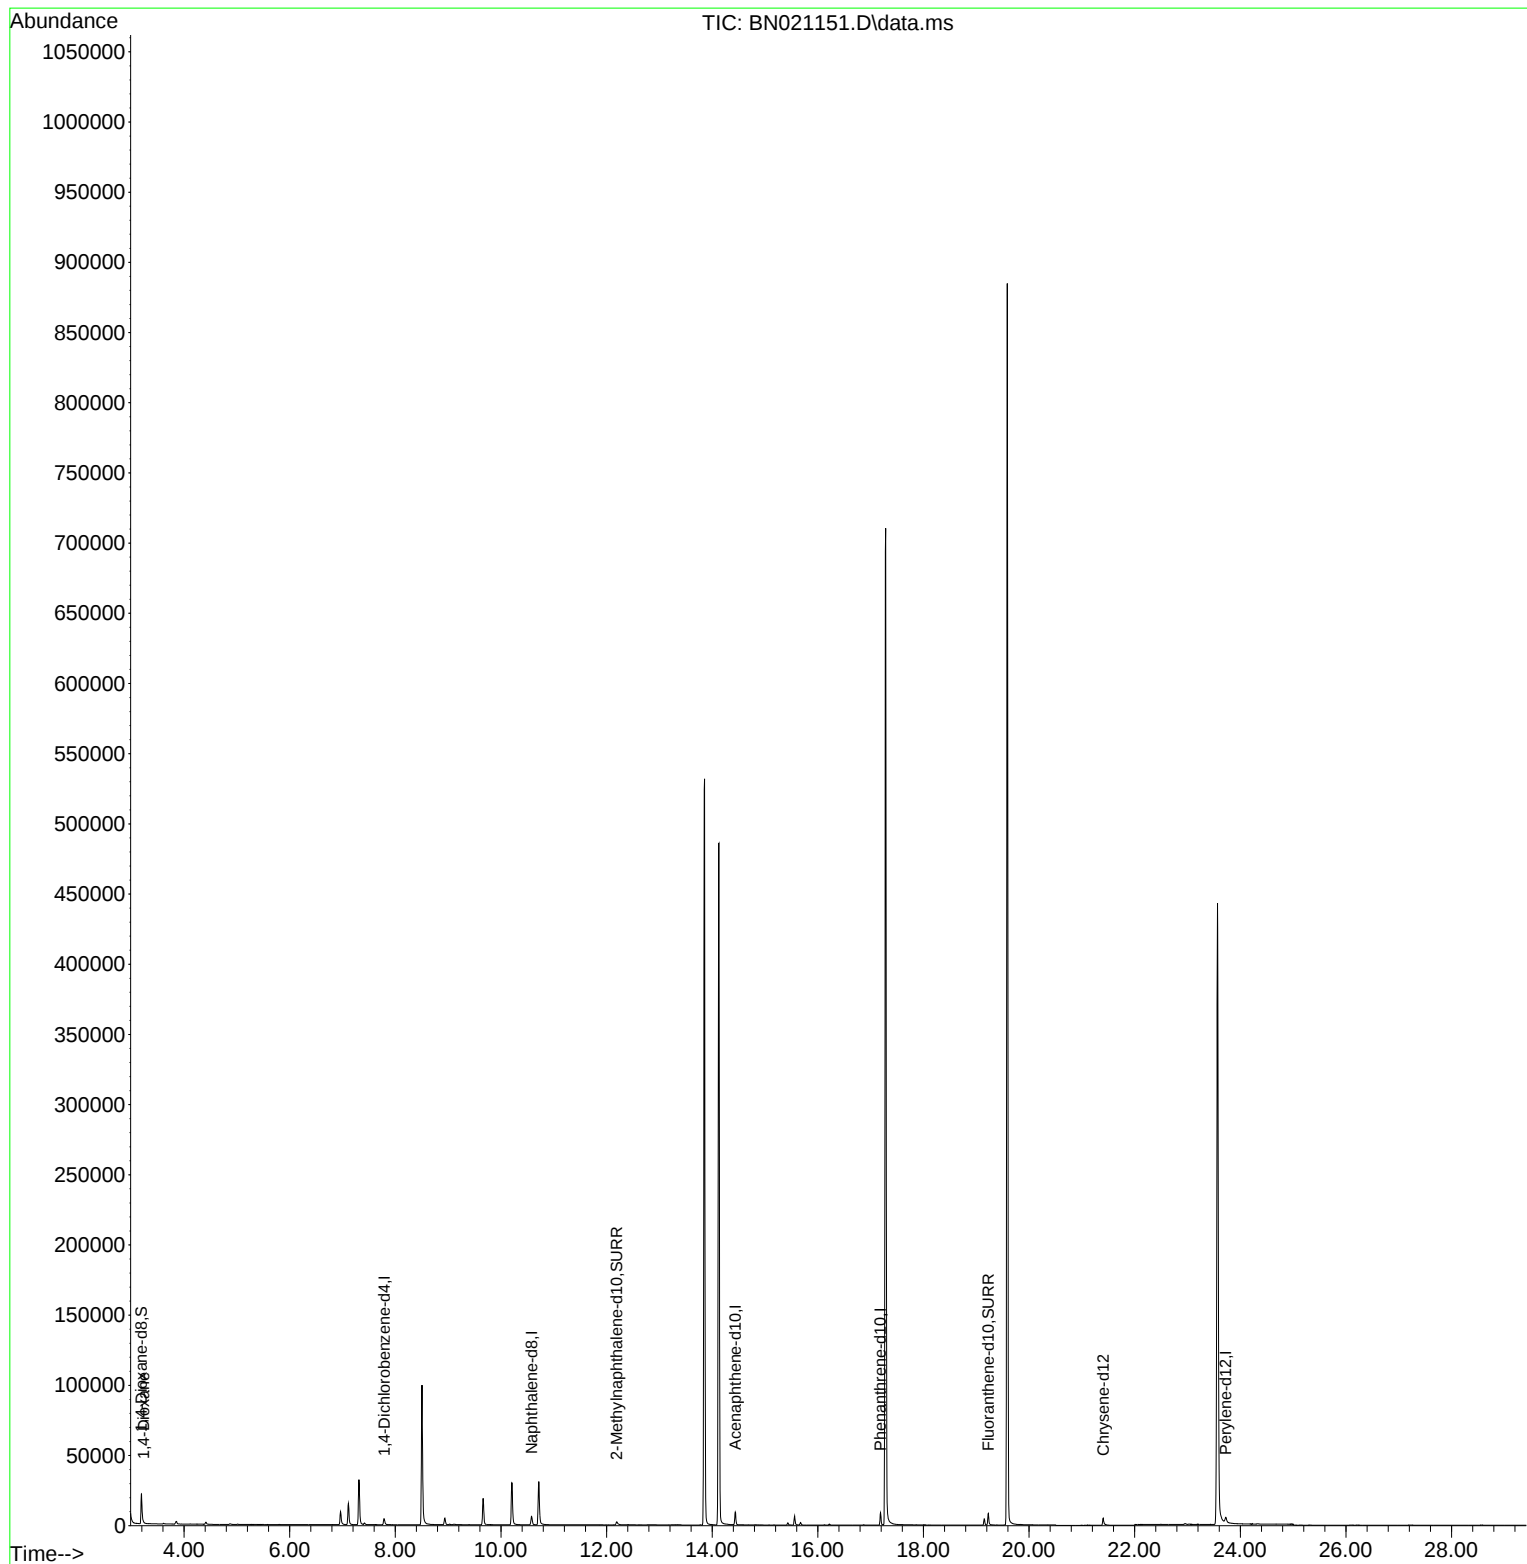

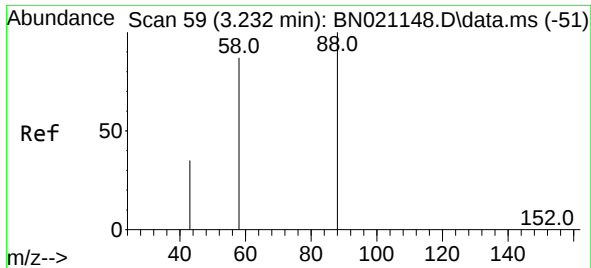

#2
 1,4-Dioxane
 Concen: 0.093 ng/ul
 RT: 3.232 min Scan# 51
 Delta R.T. 0.004 min
 Lab File: BN021151.D
 Acq: 11 Aug 2022 17:17

Instrument :
 BNA_N
 ClientSampleId :
 BGBT1

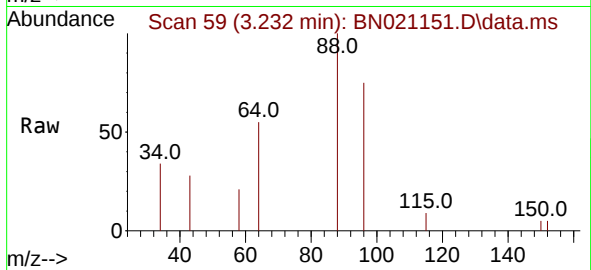

Tgt Ion: 88	Resp: 327
Ion Ratio	Lower Upper
88 100	
43 27.5	31.4 47.0#
58 20.6	49.0 73.6#

