

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
 Data File : BN021153.D
 Acq On : 11 Aug 2022 18:32
 Operator : CG/JU
 Sample : N4129-07
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBT0

Quant Time: Aug 11 19:01:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 09 23:10:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.788	152	2665	0.400	ng/ul	0.00
4) Naphthalene-d8	10.580	136	8956	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.438	164	5187	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	10208	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240	7322	0.400	ng/ul	0.00
23) Perylene-d12	23.721	264	7411	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	14766	4.331	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.191	152	4132	0.315	ng/ul	0.01
18) Fluoranthene-d10	19.226	212	10772	0.476	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	288	0.082	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
Data File : BN021153.D
Acq On : 11 Aug 2022 18:32
Operator : CG/JU
Sample : N4129-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBT0


Quant Time: Aug 11 19:01:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 09 23:10:06 2022
Response via : Initial Calibration

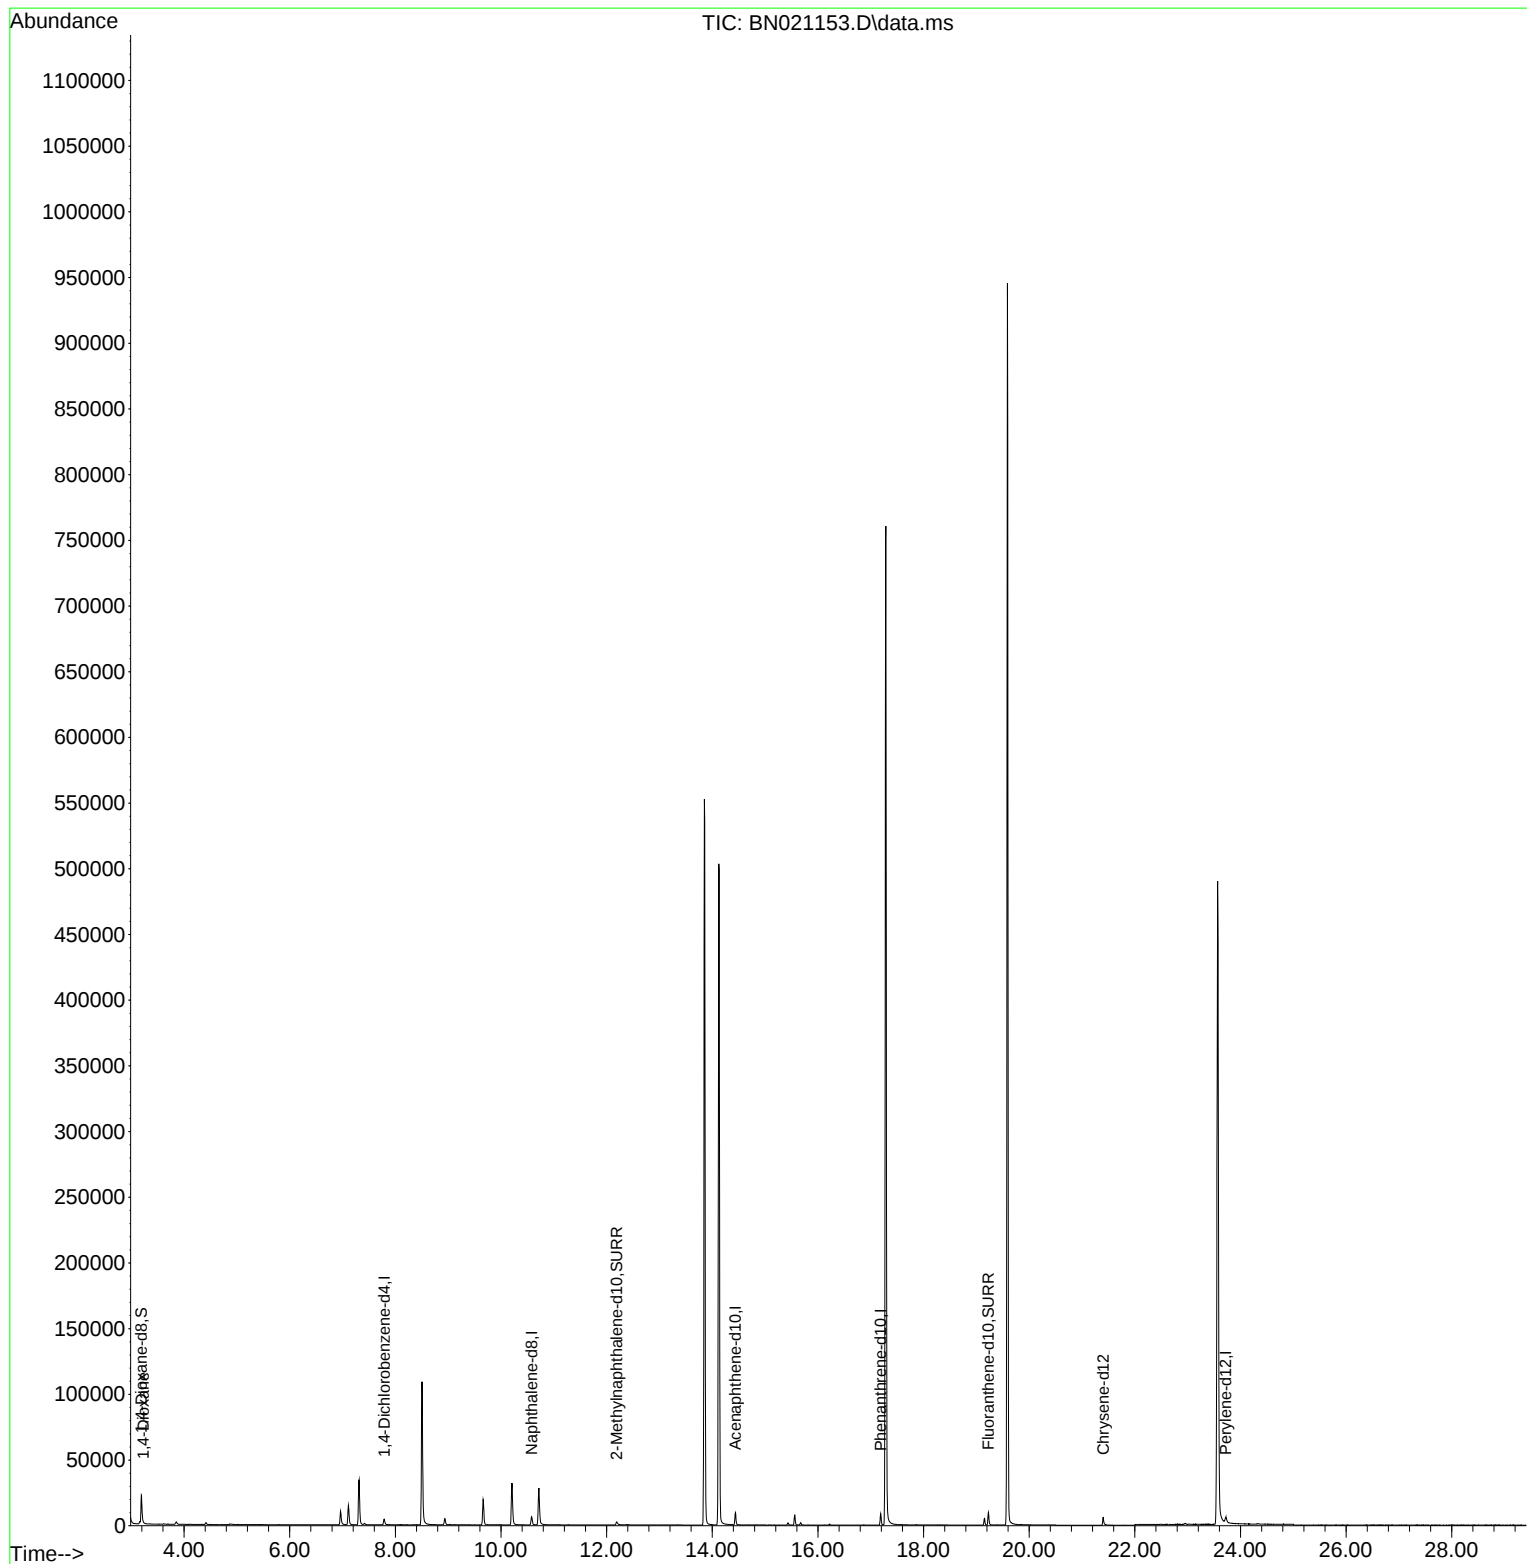

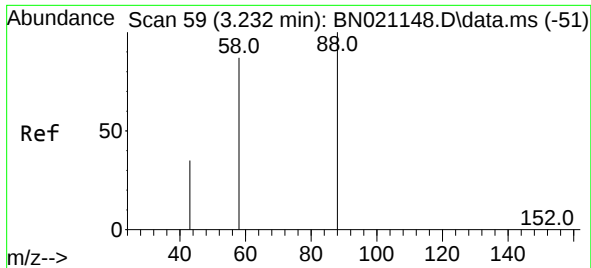

#2
 1,4-Dioxane
 Concen: 0.082 ng/ul
 RT: 3.228 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BN021153.D
 Acq: 11 Aug 2022 18:32

Instrument :
 BNA_N
 ClientSampleId :
 BGBT0

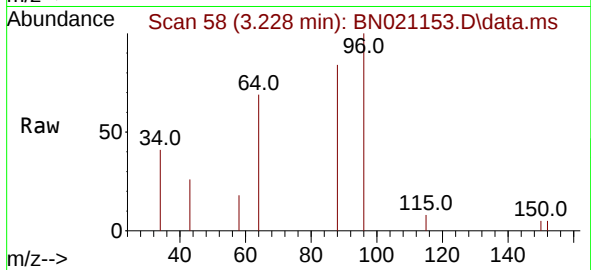

Tgt Ion:	88	Resp:	288
Ion	Ratio	Lower	Upper
88	100		
43	31.5	31.4	47.0
58	21.4	49.0	73.6

