

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
 Data File : BN021166.D
 Acq On : 12 Aug 2022 09:41
 Operator : CG/JU
 Sample : N4129-16
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBW8

Quant Time: Aug 12 11:49:53 2022
 Quant Title :
 QLast Update : Sat Aug 13 04:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	4499	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	14995	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.437	164	8716	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.187	188	17584	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	12207	0.400	ng/ul	0.00
23) Perylene-d12	23.719	264	12038	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.194	96	20537	3.568	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.184	152	6314	0.287	ng/ul	0.00
18) Fluoranthene-d10	19.225	212	15000	0.398	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.236	88	425	0.072	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081022\
Data File : BN021166.D
Acq On : 12 Aug 2022 09:41
Operator : CG/JU
Sample : N4129-16
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBW8

Quant Time: Aug 12 11:49:53 2022
Quant Title :
QLast Update : Sat Aug 13 04:02:44 2022
Response via : Initial Calibration

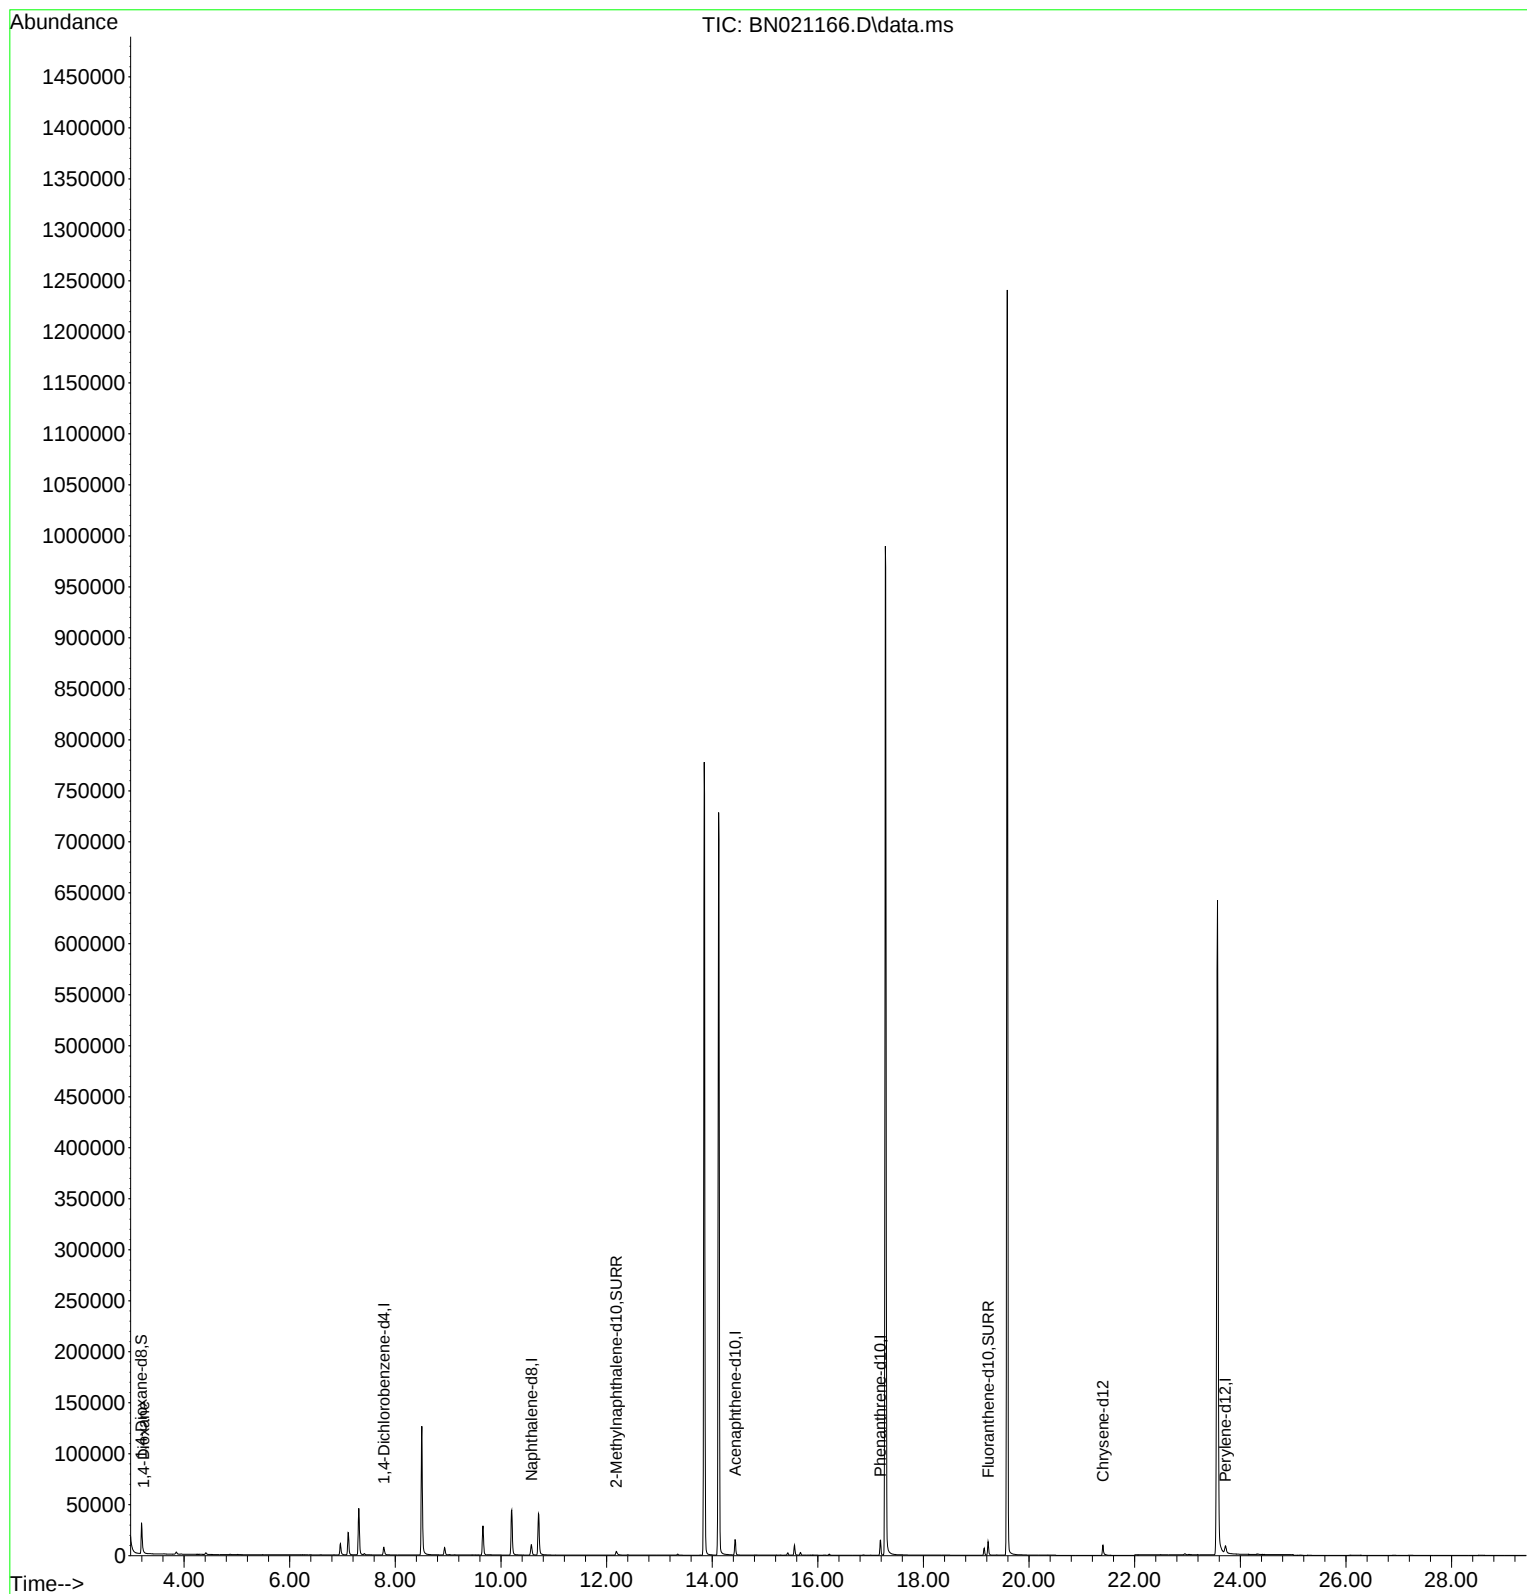

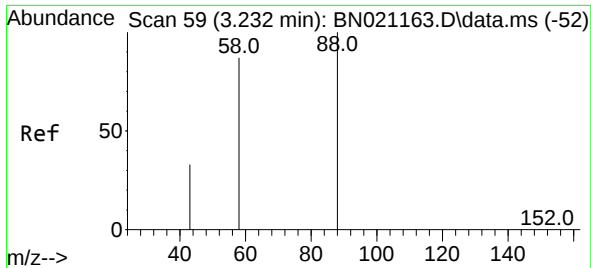

#2
 1,4-Dioxane
 Concen: 0.072 ng/ul
 RT: 3.236 min Scan# 60
 Delta R.T. 0.008 min
 Lab File: BN021166.D
 Acq: 12 Aug 2022 09:41

Instrument :
 BNA_N
 ClientSampleId :
 BGBW8

Tgt Ion: 88 Resp: 425
 Ion Ratio Lower Upper
 88 100
 43 23.4 31.4 47.0#
 58 12.1 49.0 73.6#

