

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081024\
 Data File : BN033336.D
 Acq On : 10 Aug 2024 14:53
 Operator : MA/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Aug 12 01:01:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 00:59:25 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.580	152	5313	0.400	ng	0.00
7) Naphthalene-d8	10.338	136	15448	0.400	ng	0.00
13) Acenaphthene-d10	14.212	164	9171	0.400	ng	0.00
19) Phenanthrene-d10	16.958	188	22066	0.400	ng	0.00
29) Chrysene-d12	21.166	240	19273	0.400	ng	0.00
35) Perylene-d12	23.349	264	19885	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.197	112	5977	0.427	ng	0.00
5) Phenol-d6	6.749	99	8038	0.420	ng	0.00
8) Nitrobenzene-d5	8.704	82	4546	0.482	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	9150	0.380	ng	0.00
14) 2,4,6-Tribromophenol	15.705	330	1755	0.473	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	14966	0.433	ng	0.00
27) Fluoranthene-d10	19.002	212	22394	0.369	ng	0.00
31) Terphenyl-d14	19.620	244	14573	0.438	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.196	88	2265	0.385	ng	100
3) n-Nitrosodimethylamine	3.485	42	2971	0.397	ng	100
6) bis(2-Chloroethyl)ether	7.017	93	6308	0.386	ng	100
9) Naphthalene	10.391	128	16562	0.382	ng	100
10) Hexachlorobutadiene	10.690	225	3219	0.404	ng	# 100
12) 2-Methylnaphthalene	12.015	142	11044	0.369	ng	100
16) Acenaphthylene	13.924	152	15945	0.356	ng	100
17) Acenaphthene	14.277	154	11171	0.393	ng	100
18) Fluorene	15.271	166	14815	0.390	ng	100
20) 4,6-Dinitro-2-methylph...	15.346	198	921	0.584	ng	100
21) 4-Bromophenyl-phenylether	16.164	248	5026	0.375	ng	100
22) Hexachlorobenzene	16.276	284	5784	0.411	ng	100
23) Atrazine	16.449	200	3811	0.344	ng	100
24) Pentachlorophenol	16.611	266	2039	0.414	ng	100
25) Phenanthrene	16.995	178	24483	0.383	ng	100
26) Anthracene	17.095	178	21138	0.340	ng	100
28) Fluoranthene	19.030	202	29596	0.368	ng	100
30) Pyrene	19.392	202	30305	0.400	ng	100
32) Benzo(a)anthracene	21.157	228	26737	0.357	ng	100
33) Chrysene	21.201	228	28851	0.398	ng	100
34) Bis(2-ethylhexyl)phtha...	21.130	149	11323	0.292	ng	100
36) Indeno(1,2,3-cd)pyrene	25.524	276	29809	0.343	ng	100
37) Benzo(b)fluoranthene	22.703	252	28235	0.382	ng	100
38) Benzo(k)fluoranthene	22.747	252	29564	0.412	ng	100
39) Benzo(a)pyrene	23.255	252	22964	0.350	ng	100
40) Dibenzo(a,h)anthracene	25.548	278	23448	0.341	ng	100
41) Benzo(g,h,i)perylene	26.176	276	26432	0.354	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081024\
Data File : BN033336.D
Acq On : 10 Aug 2024 14:53
Operator : MA/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Aug 12 01:01:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 00:59:25 2024
Response via : Initial Calibration




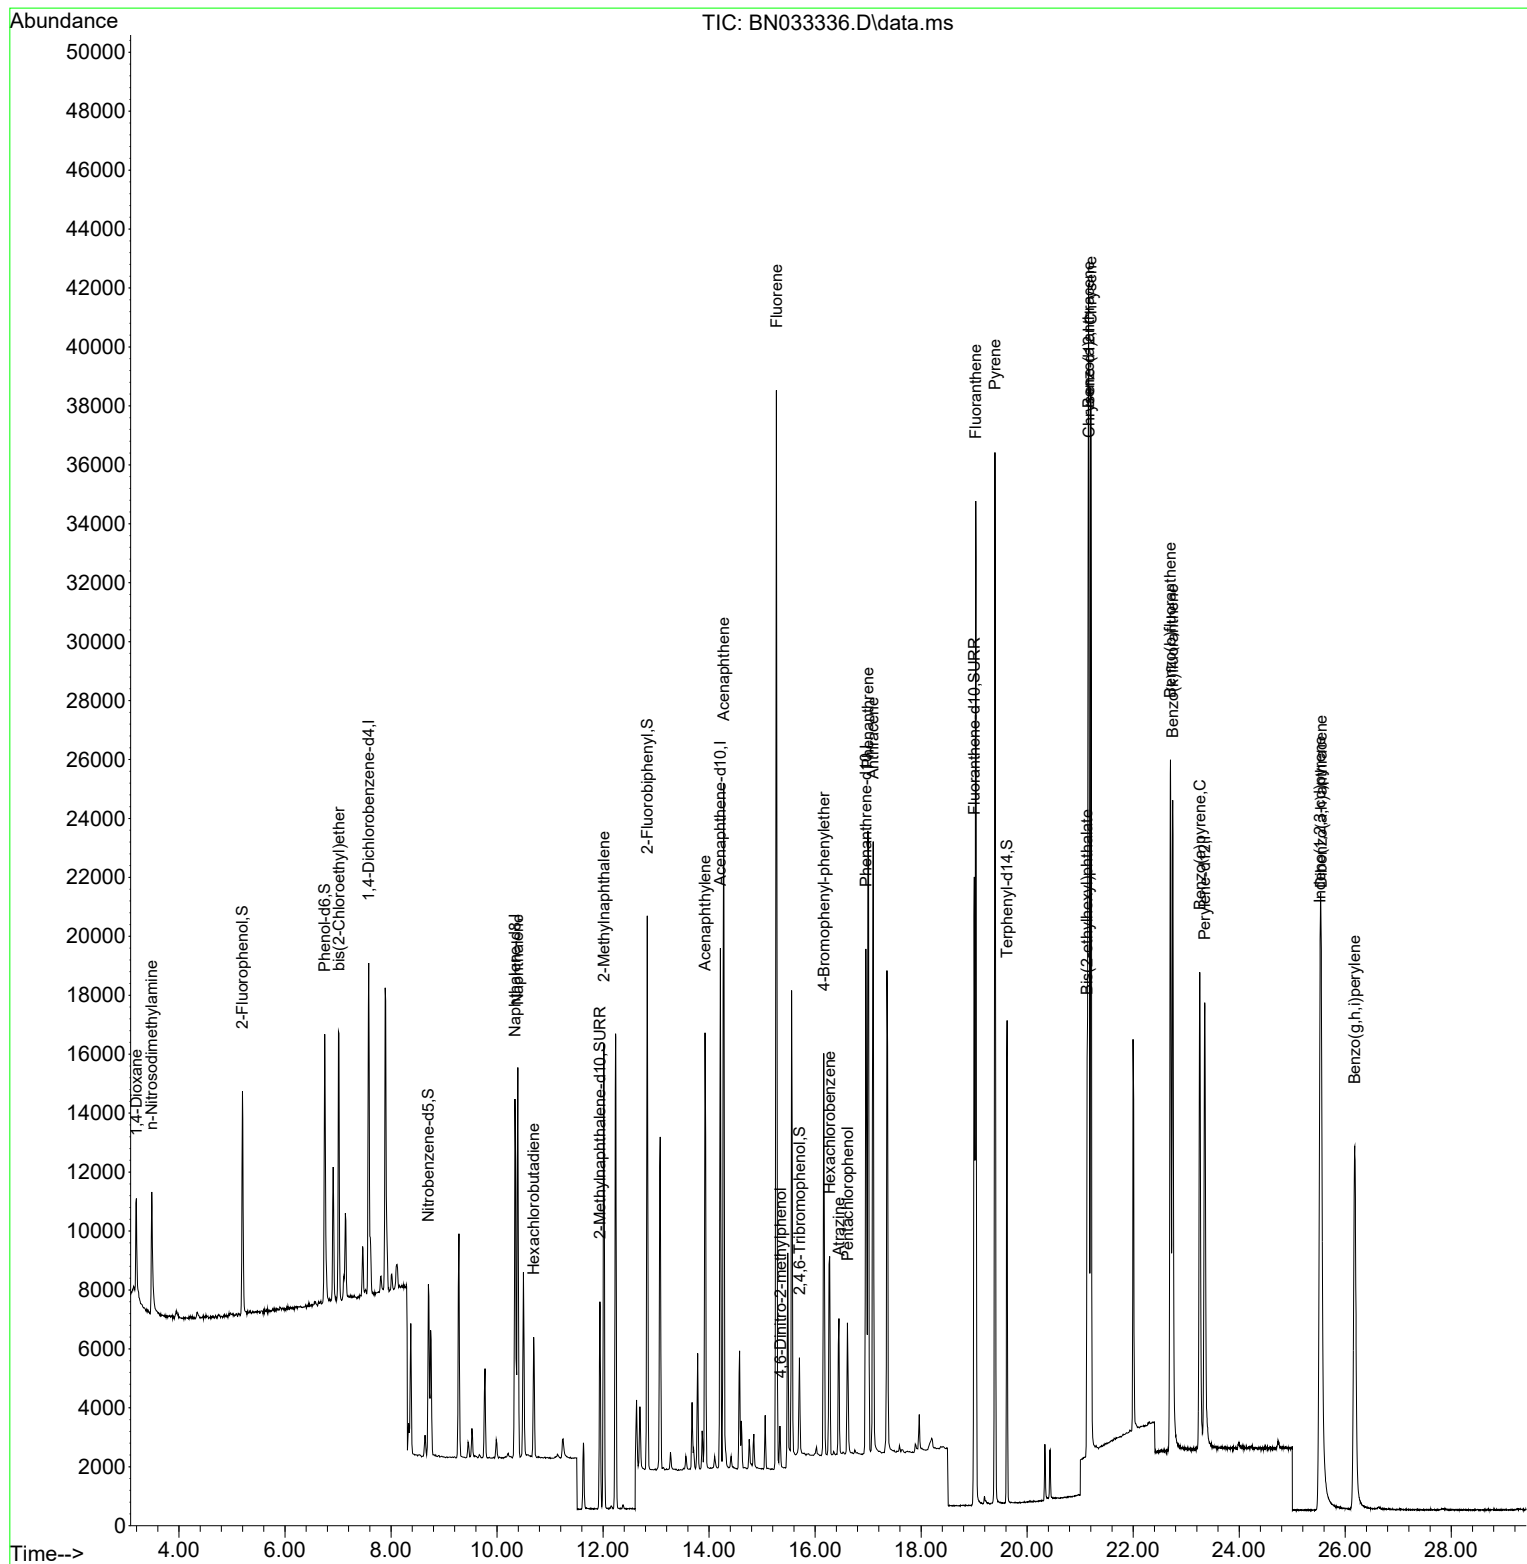




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.580 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:152 Resp: 5313
 Ion Ratio Lower Upper
 152 100
 150 152.9 122.3 183.5
 115 61.0 48.8 73.2

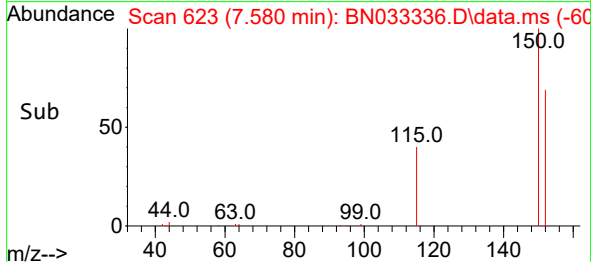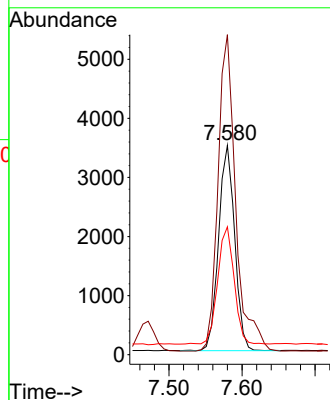

#2
 1,4-Dioxane
 Concen: 0.385 ng
 RT: 3.196 min Scan# 16
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53

Tgt Ion: 88 Resp: 2265
 Ion Ratio Lower Upper
 88 100
 43 38.3 30.6 46.0
 58 80.6 64.5 96.7


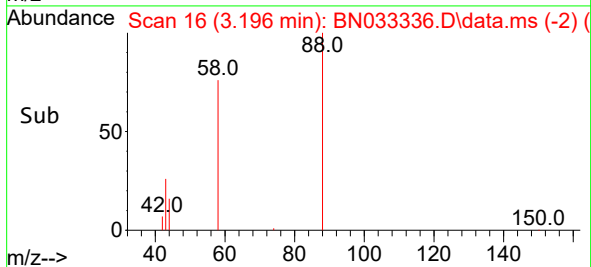
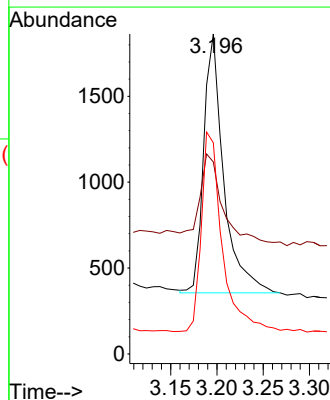
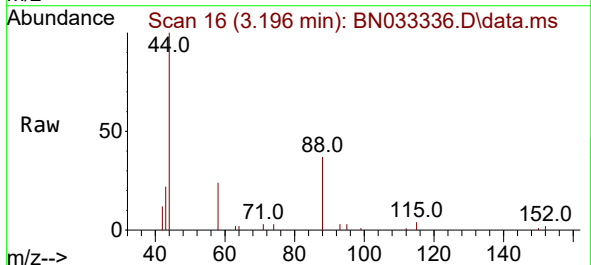




#3
n-Nitrosodimethylamine
Concen: 0.397 ng
RT: 3.485 min Scan# 56
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 42 Resp: 2971
Ion Ratio Lower Upper
42 100
74 111.0 89.0 133.6
44 13.8 11.0 16.4

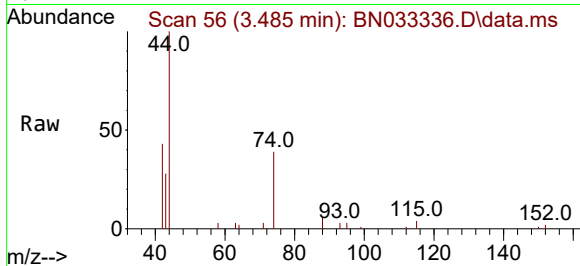

#4
2-Fluorophenol
Concen: 0.427 ng
RT: 5.197 min Scan# 293
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion: 112 Resp: 5977
Ion Ratio Lower Upper
112 100
64 60.2 48.1 72.1
63 31.8 25.4 38.2




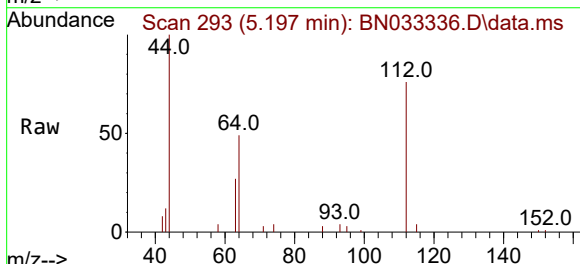




#5
Phenol-d6
Concen: 0.420 ng
RT: 6.749 min Scan# 508
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 8038
Ion Ratio Lower Upper
99 100
42 23.1 18.5 27.7
71 32.7 26.2 39.2

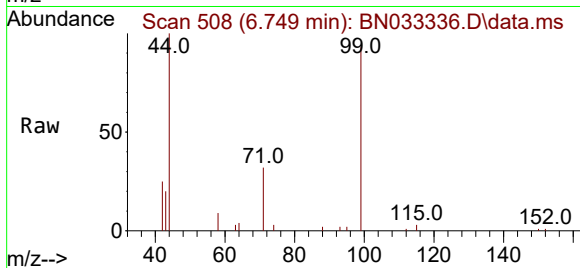

#6
bis(2-Chloroethyl)ether
Concen: 0.386 ng
RT: 7.017 min Scan# 545
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion: 93 Resp: 6308
Ion Ratio Lower Upper
93 100
63 81.5 65.2 97.8
95 32.8 26.2 39.4


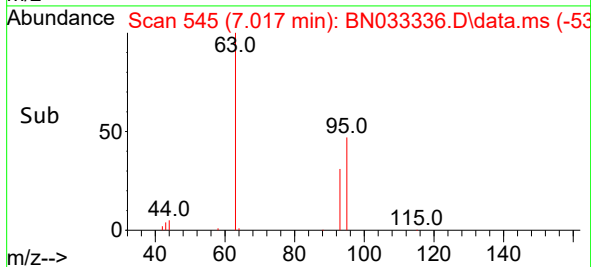

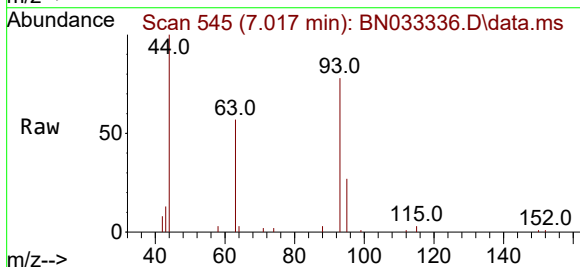




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.338 min Scan# 914
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	15448
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.1	13.7
54	11.7	9.4	14.0
68	8.7	7.0	10.4

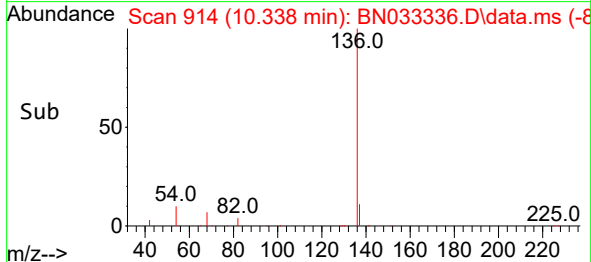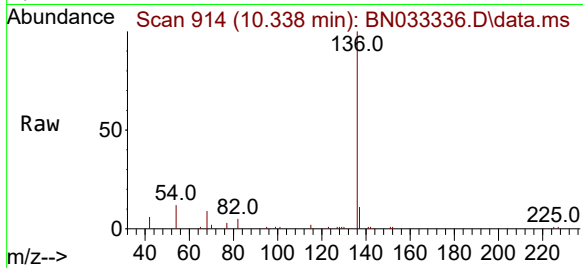

#8
Nitrobenzene-d5
Concen: 0.482 ng
RT: 8.704 min Scan# 761
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:	82	Resp:	4546
Ion	Ratio	Lower	Upper
82	100		
128	36.2	29.0	43.4
54	62.8	50.2	75.4


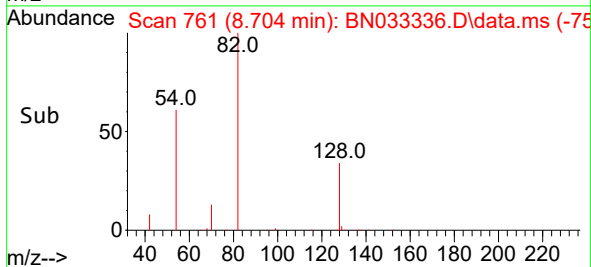

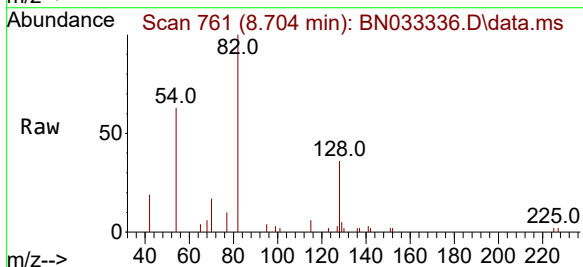




#9
Naphthalene
Concen: 0.382 ng
RT: 10.391 min Scan# 919
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:128 Resp: 16562
Ion Ratio Lower Upper
128 100
129 11.5 9.2 13.8
127 13.2 10.6 15.8

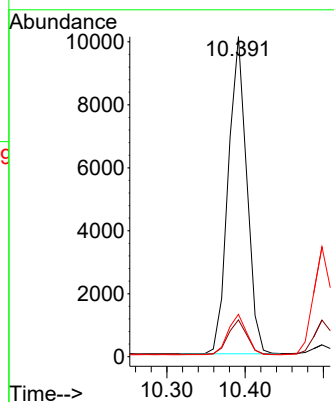

#10
Hexachlorobutadiene
Concen: 0.404 ng
RT: 10.690 min Scan# 947
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:225 Resp: 3219
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.5 50.8 76.2



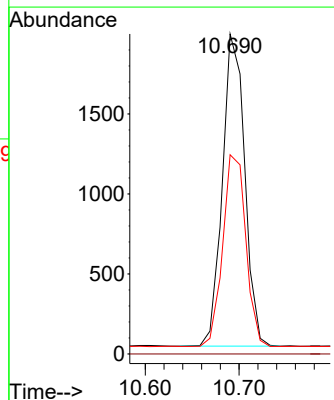





#11
2-Methylnaphthalene-d10
Concen: 0.380 ng
RT: 11.940 min Scan# 1137
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 9150
Ion Ratio Lower Upper
152 100
151 20.9 16.7 25.1

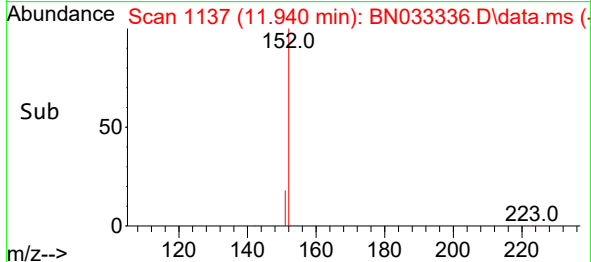

#12
2-Methylnaphthalene
Concen: 0.369 ng
RT: 12.015 min Scan# 1157
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:142 Resp: 11044
Ion Ratio Lower Upper
142 100
141 87.8 70.2 105.4
115 36.6 29.3 43.9

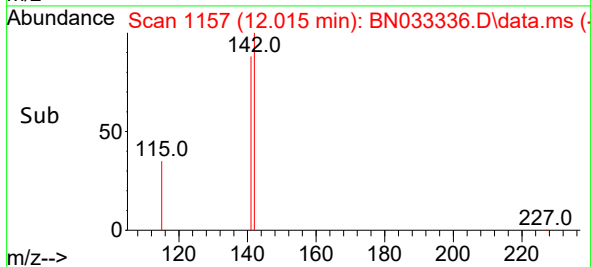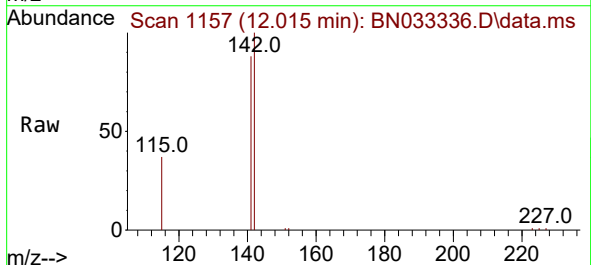



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.212 min Scan# 1464

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:164 Resp: 9171

Ion Ratio Lower Upper

164 100

162 103.9 83.1 124.7

160 51.4 41.1 61.7

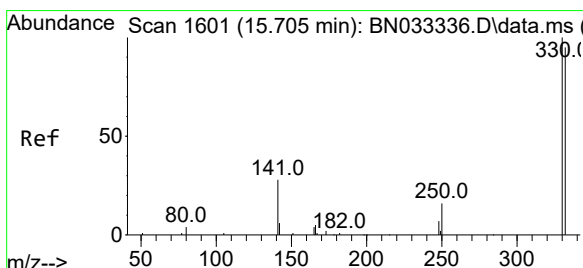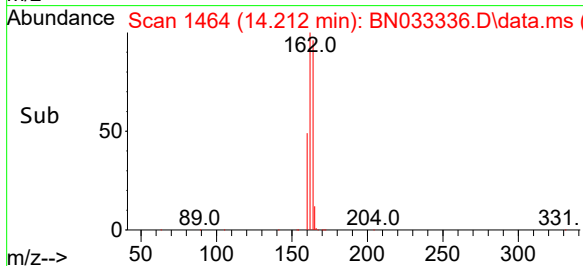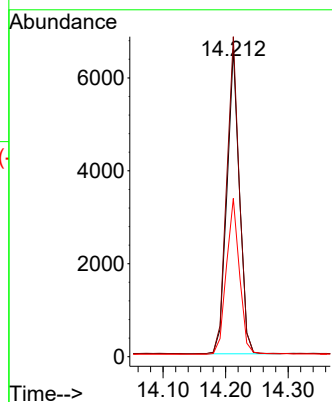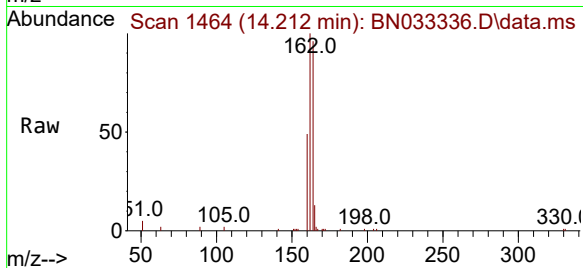

#14

2,4,6-Tribromophenol

Concen: 0.473 ng

RT: 15.705 min Scan# 1601

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53




Tgt Ion:330 Resp: 1755


Ion Ratio Lower Upper

330 100

332 96.4 77.1 115.7

141 41.7 33.4 50.0


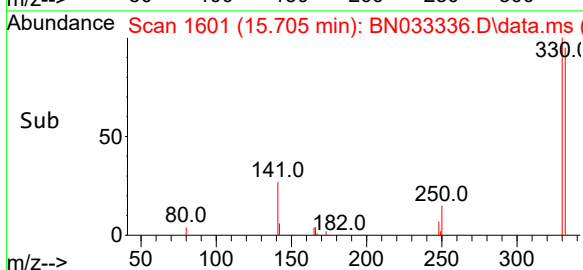

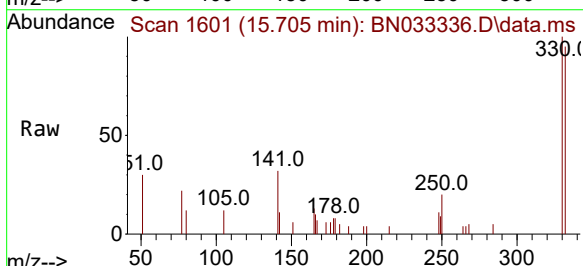




#15
2-Fluorobiphenyl
Concen: 0.433 ng
RT: 12.833 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:172 Resp: 14966
Ion Ratio Lower Upper
172 100
171 34.8 27.8 41.8
170 23.4 18.7 28.1



#16
Acenaphthylene
Concen: 0.356 ng
RT: 13.924 min Scan# 1437
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:152 Resp: 15945
Ion Ratio Lower Upper
152 100
151 19.6 15.7 23.5
153 13.0 10.4 15.6




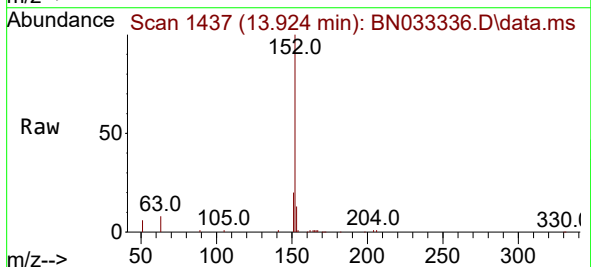




#17
Acenaphthene
Concen: 0.393 ng
RT: 14.277 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 11171
Ion Ratio Lower Upper
154 100
153 112.1 89.7 134.5
152 59.0 47.2 70.8



#18
Fluorene
Concen: 0.390 ng
RT: 15.271 min Scan# 1563
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:166 Resp: 14815
Ion Ratio Lower Upper
166 100
165 97.5 78.0 117.0
167 13.4 10.7 16.1

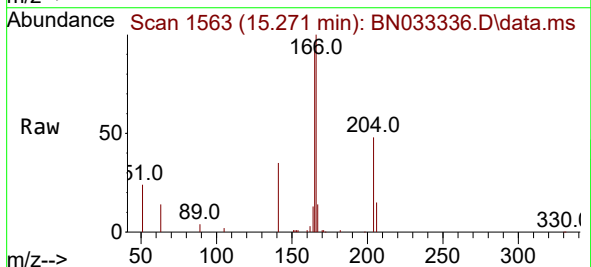



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.958 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:188 Resp: 22066

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 13.4 10.7 16.1

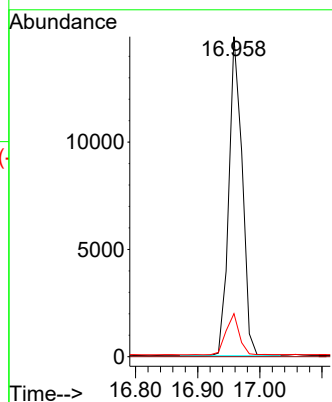

#20

4,6-Dinitro-2-methylphenol

Concen: 0.584 ng

RT: 15.346 min Scan# 1570

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53




Tgt Ion:198 Resp: 921


Ion Ratio Lower Upper

198 100

51 78.5 62.8 94.2

105 42.6 34.1 51.1


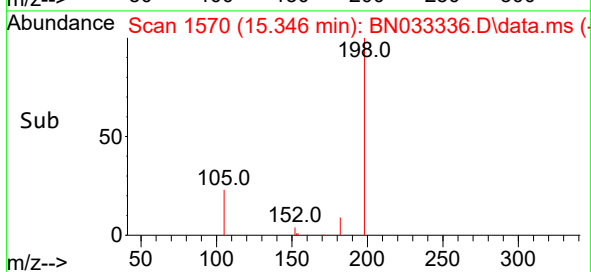
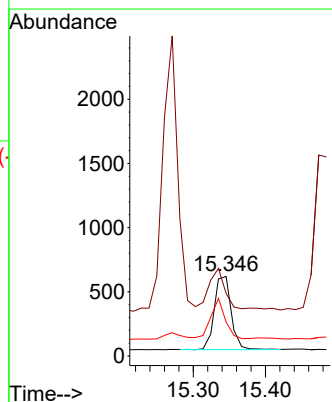





#21
4-Bromophenyl-phenylether
Concen: 0.375 ng
RT: 16.164 min Scan# 1638
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 5026
Ion Ratio Lower Upper
248 100
250 91.2 73.0 109.4
141 80.7 64.6 96.8

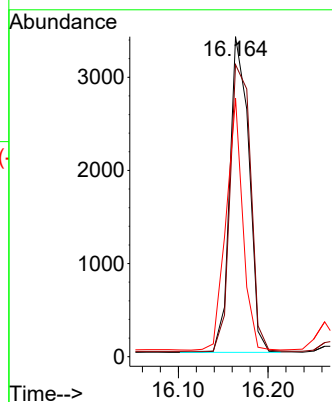

#22
Hexachlorobenzene
Concen: 0.411 ng
RT: 16.276 min Scan# 1647
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:284 Resp: 5784
Ion Ratio Lower Upper
284 100
142 40.3 32.2 48.4
249 31.6 25.3 37.9

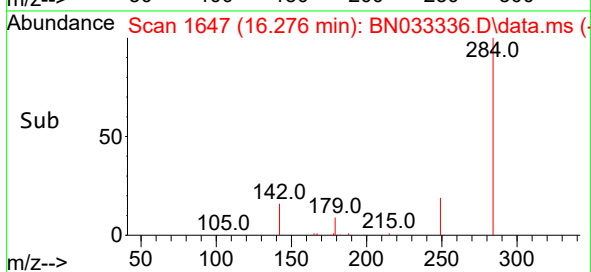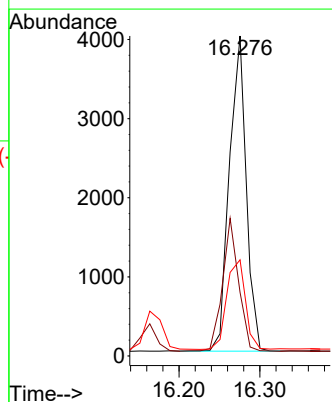

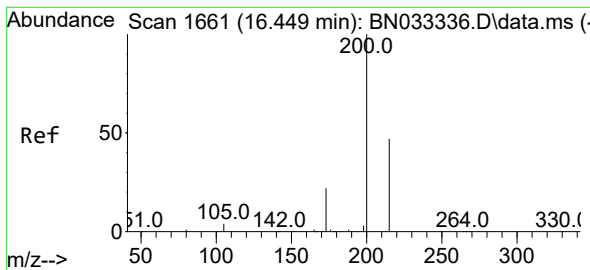

#23

Atrazine

Concen: 0.344 ng

RT: 16.449 min Scan# 1661

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:200 Resp: 3811

Ion Ratio Lower Upper

200 100

173 23.4 18.7 28.1

215 48.3 38.6 58.0

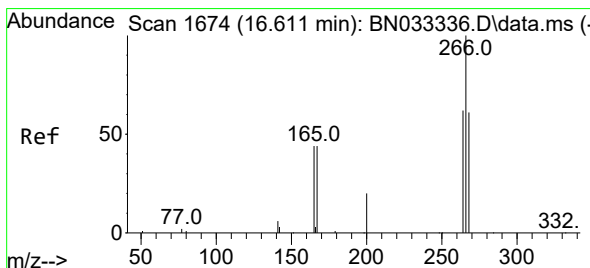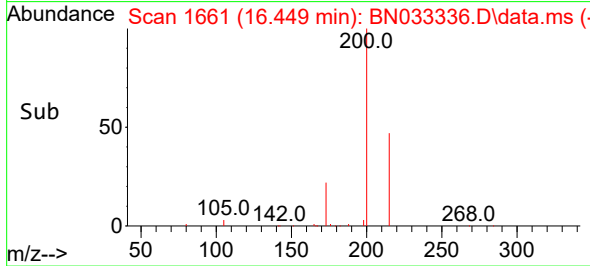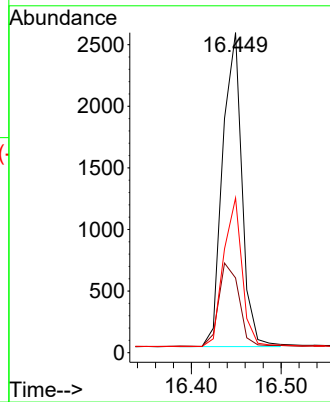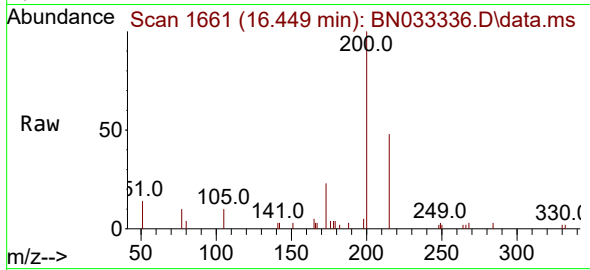

#24

Pentachlorophenol

Concen: 0.414 ng

RT: 16.611 min Scan# 1674

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53




Tgt Ion:266 Resp: 2039


Ion Ratio Lower Upper

266 100

264 61.5 49.2 73.8

268 64.0 51.2 76.8


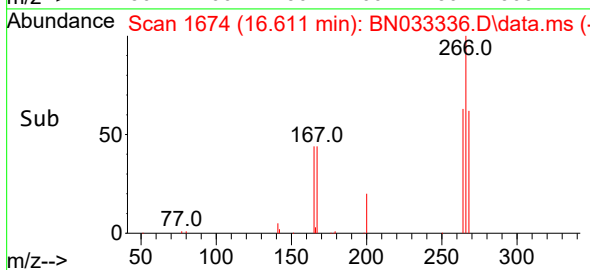
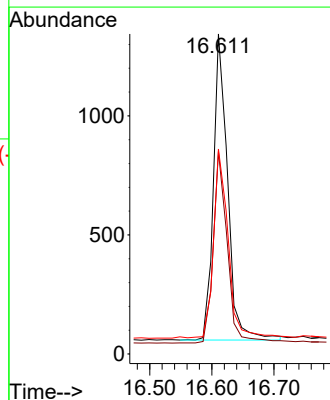
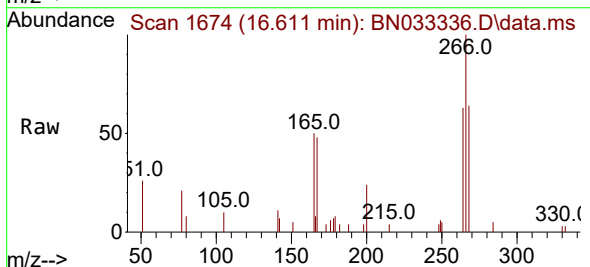




#25
Phenanthrene
Concen: 0.383 ng
RT: 16.995 min Scan# 1705
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 24483
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.0
179 15.2 12.2 18.2

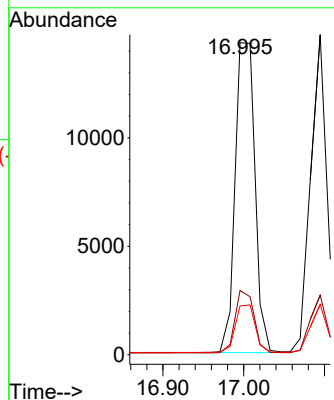

#26
Anthracene
Concen: 0.340 ng
RT: 17.095 min Scan# 1713
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:178 Resp: 21138
Ion Ratio Lower Upper
178 100
176 18.4 14.7 22.1
179 15.2 12.2 18.2



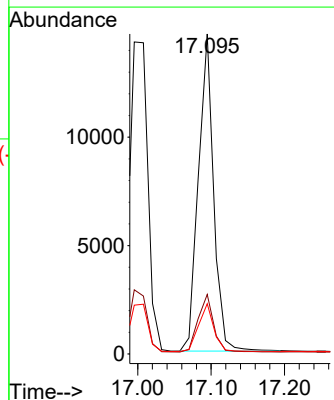
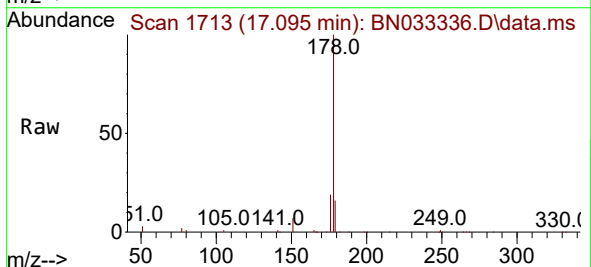


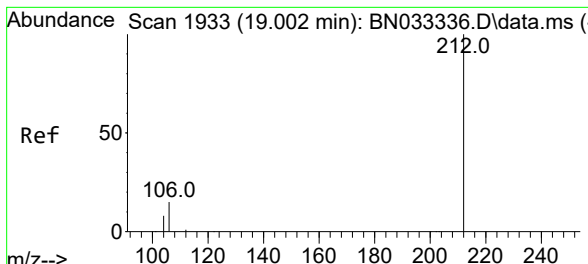

#27
Fluoranthene-d10
Concen: 0.369 ng
RT: 19.002 min Scan# 1933
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 22394
Ion Ratio Lower Upper
212 100
106 16.0 12.8 19.2
104 8.9 7.1 10.7

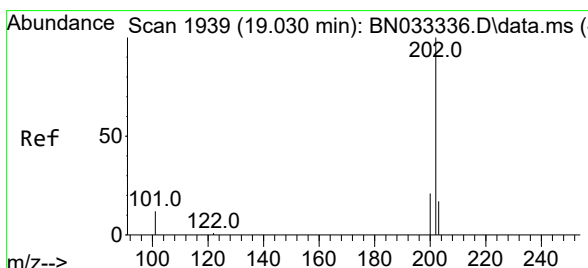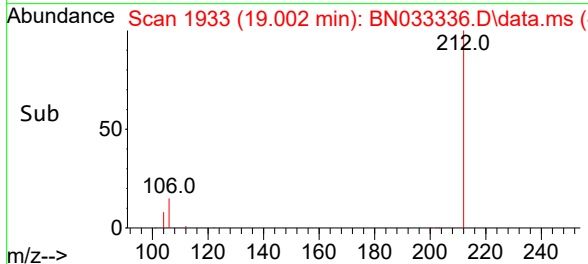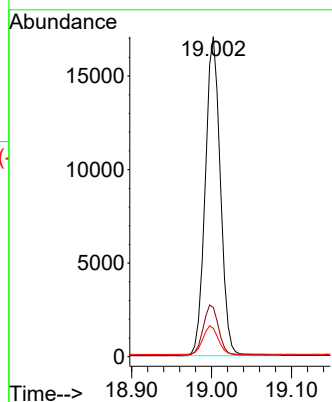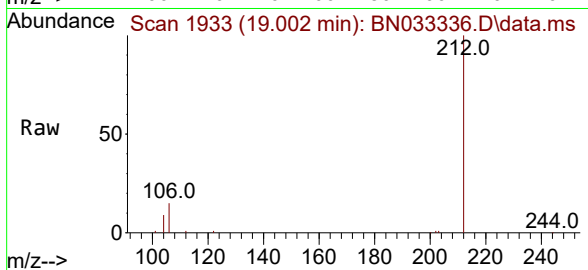

#28
Fluoranthene
Concen: 0.368 ng
RT: 19.030 min Scan# 1939
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:202 Resp: 29596
Ion Ratio Lower Upper
202 100
101 12.2 9.8 14.6
203 17.2 13.8 20.6


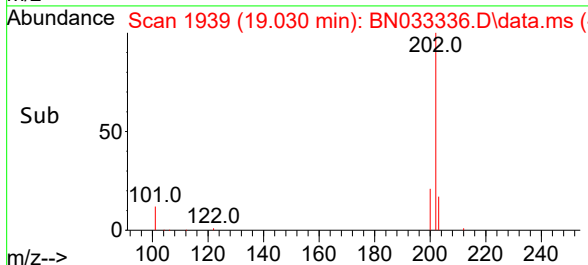

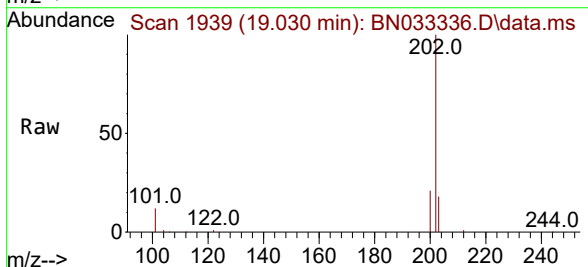




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.166 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:240 Resp: 19273
Ion Ratio Lower Upper
240 100
120 16.3 13.0 19.6
236 29.0 23.2 34.8



#30
Pyrene
Concen: 0.400 ng
RT: 19.392 min Scan# 2017
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Tgt Ion:202 Resp: 30305
Ion Ratio Lower Upper
202 100
200 20.9 16.7 25.1
203 17.8 14.2 21.4









#31
 Terphenyl-d14
 Concen: 0.438 ng
 RT: 19.620 min Scan# 2066
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:244 Resp: 14573
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.7 11.5
 122 17.5 14.0 21.0

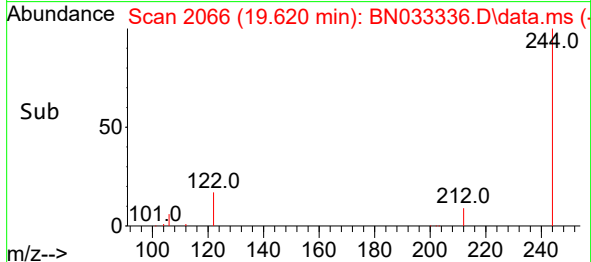

#32
 Benzo(a)anthracene
 Concen: 0.357 ng
 RT: 21.157 min Scan# 2381
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53

Tgt Ion:228 Resp: 26737
 Ion Ratio Lower Upper
 228 100
 226 27.0 21.6 32.4
 229 19.9 15.9 23.9







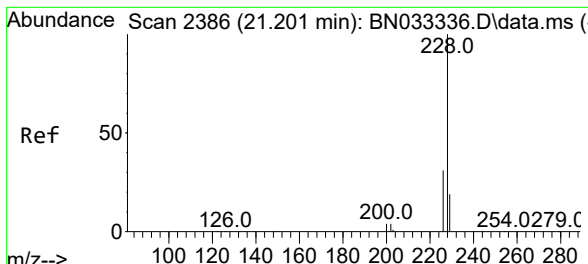

#33
 Chrysene
 Concen: 0.398 ng
 RT: 21.201 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:	228	Resp:	28851
Ion Ratio	Lower	Upper	
228	100		
226	30.9	24.7	37.1
229	19.3	15.4	23.2

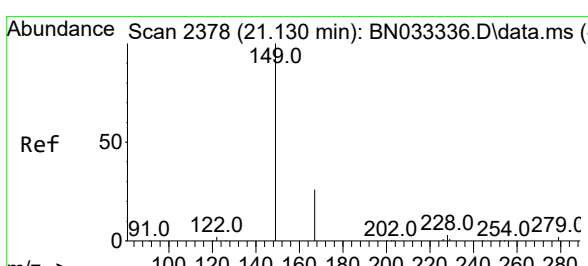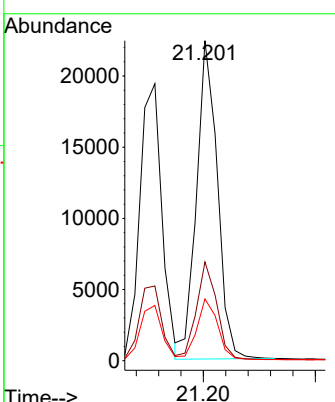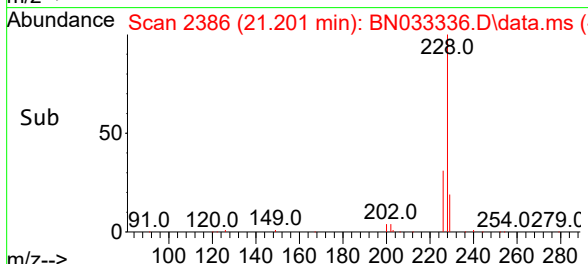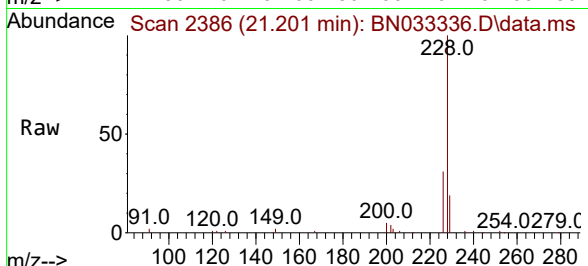

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.292 ng
 RT: 21.130 min Scan# 2378
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53

Tgt Ion:	149	Resp:	11323
Ion Ratio	Lower	Upper	
149	100		
167	26.0	20.9	31.3
279	2.8	2.2	3.4


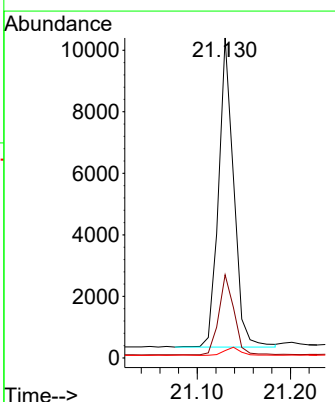
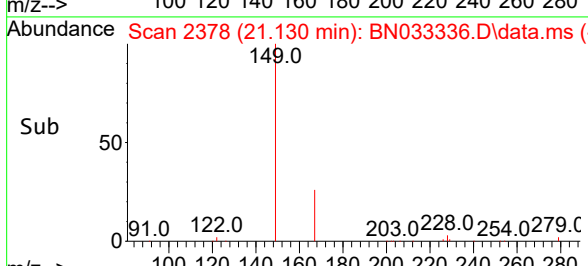
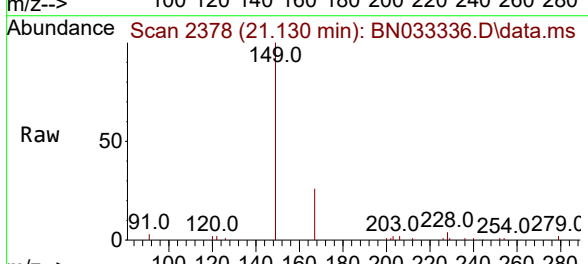


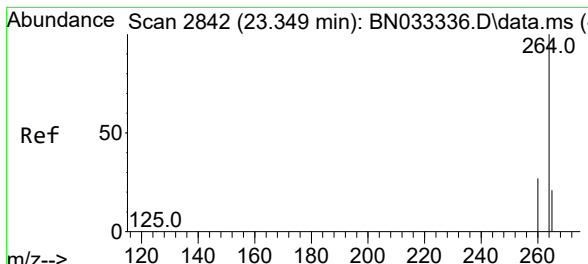

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.349 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:	264	Resp:	19885
Ion Ratio	Lower	Upper	
264	100		
260	27.0	21.6	32.4
265	36.6	29.3	43.9

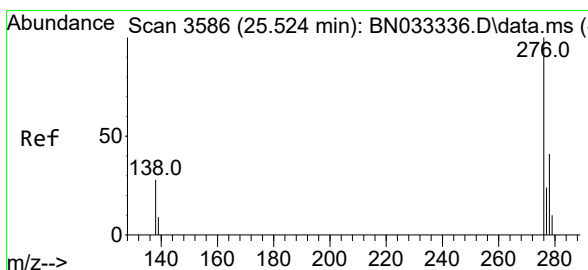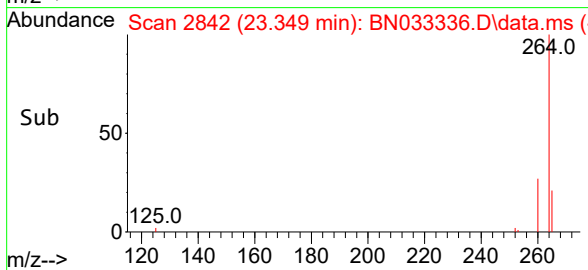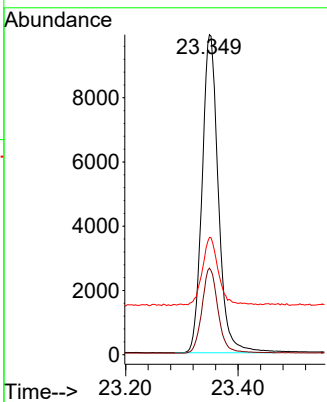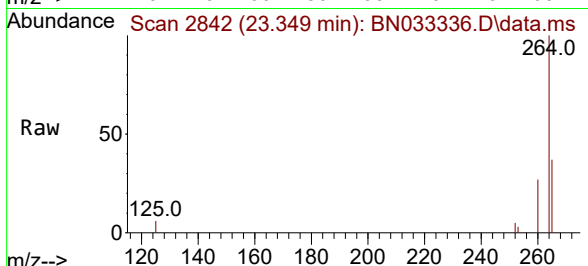

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.343 ng
 RT: 25.524 min Scan# 3586
 Delta R.T. 0.000 min
 Lab File: BN033336.D
 Acq: 10 Aug 2024 14:53

Tgt Ion:	276	Resp:	29809
Ion Ratio	Lower	Upper	
276	100		
138	31.1	24.9	37.3
277	24.7	19.8	29.6

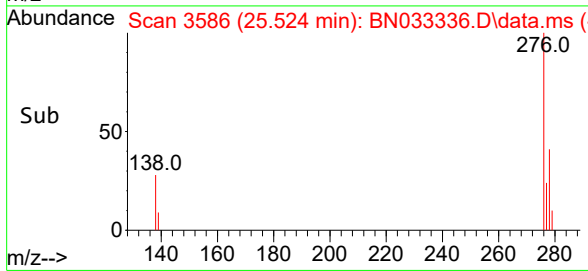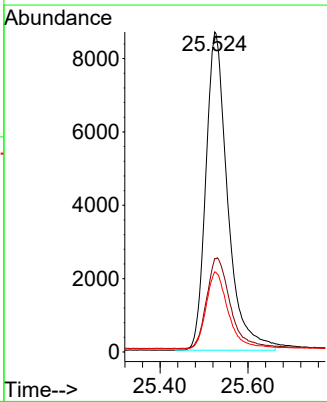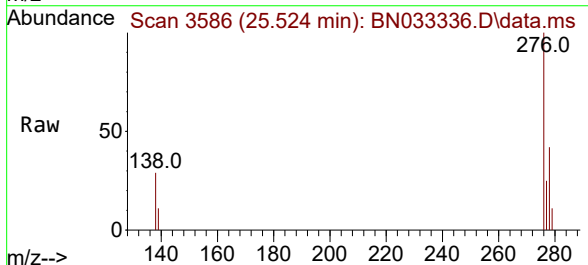



#37

Benzo(b)fluoranthene

Concen: 0.382 ng

RT: 22.703 min Scan# 2621

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:252 Resp: 28235

Ion Ratio Lower Upper

252 100

253 22.7 18.2 27.2

125 14.1 11.3 16.9



#38

Benzo(k)fluoranthene

Concen: 0.412 ng

RT: 22.747 min Scan# 2636

Delta R.T. 0.000 min

Lab File: BN033336.D

Acq: 10 Aug 2024 14:53




Tgt Ion:252 Resp: 29564


Ion Ratio Lower Upper

252 100

253 22.4 17.9 26.9


125 14.1 11.3 16.9

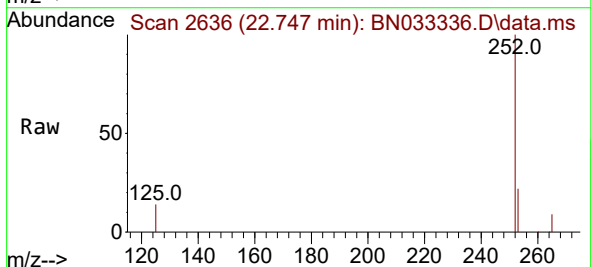






#39
Benzo(a)pyrene
Concen: 0.350 ng
RT: 23.255 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4







Tgt Ion:252 Resp: 22964
Ion Ratio Lower Upper
252 100
253 23.3 18.6 28.0
125 15.8 12.6 19.0



#40
Dibenzo(a,h)anthracene
Concen: 0.341 ng
RT: 25.548 min Scan# 3594
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53


Tgt Ion:278 Resp: 23448
Ion Ratio Lower Upper
278 100
139 21.3 17.0 25.6
279 25.0 20.0 30.0

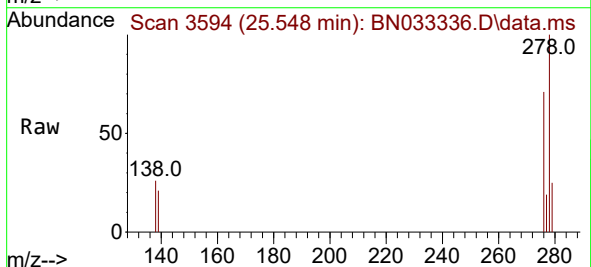

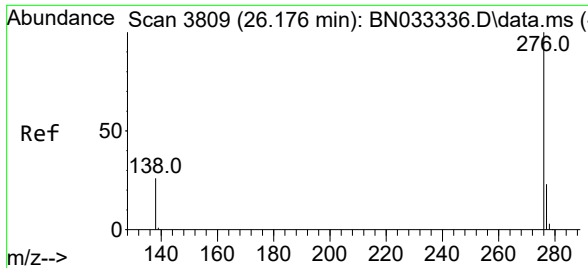

#41
Benzo(g,h,i)perylene
Concen: 0.354 ng
RT: 26.176 min Scan# 3809
Delta R.T. 0.000 min
Lab File: BN033336.D
Acq: 10 Aug 2024 14:53

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

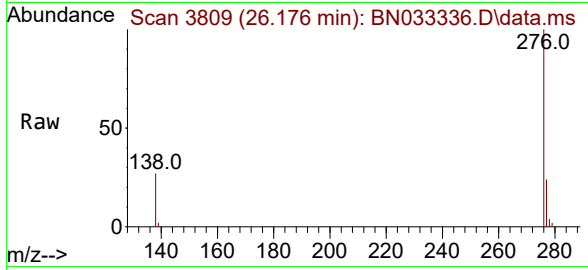

Tgt Ion:	276	Resp:	26432
Ion	Ratio	Lower	Upper
276	100		
277	24.3	19.4	29.2
138	27.0	21.6	32.4

