
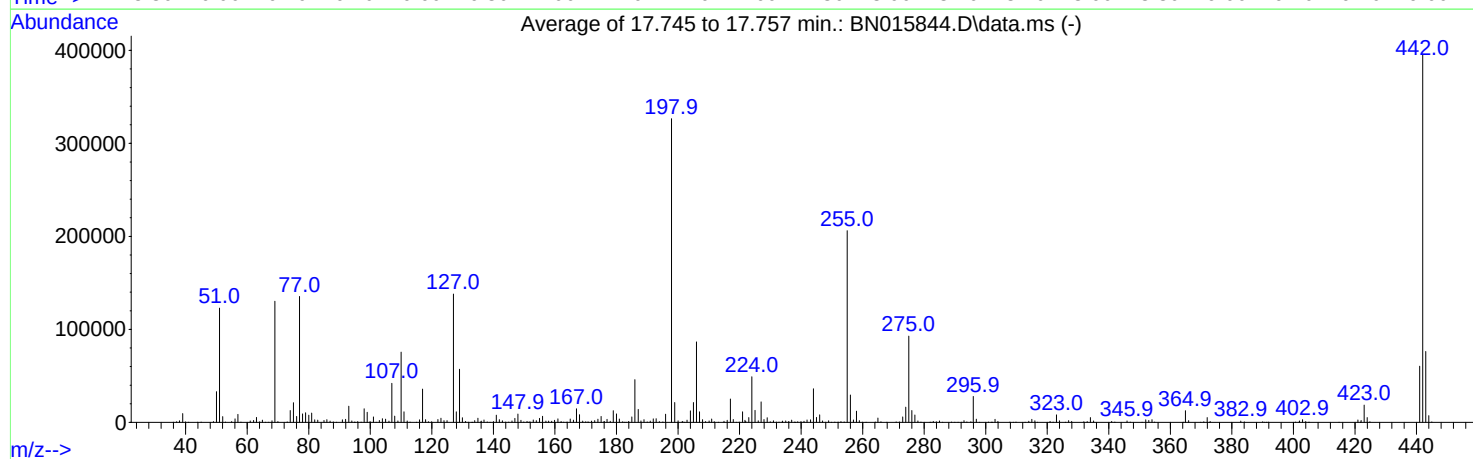


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081121\
 Data File : BN015844.D
 Acq On : 11 Aug 2021 08:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 09 19:13:08 2021

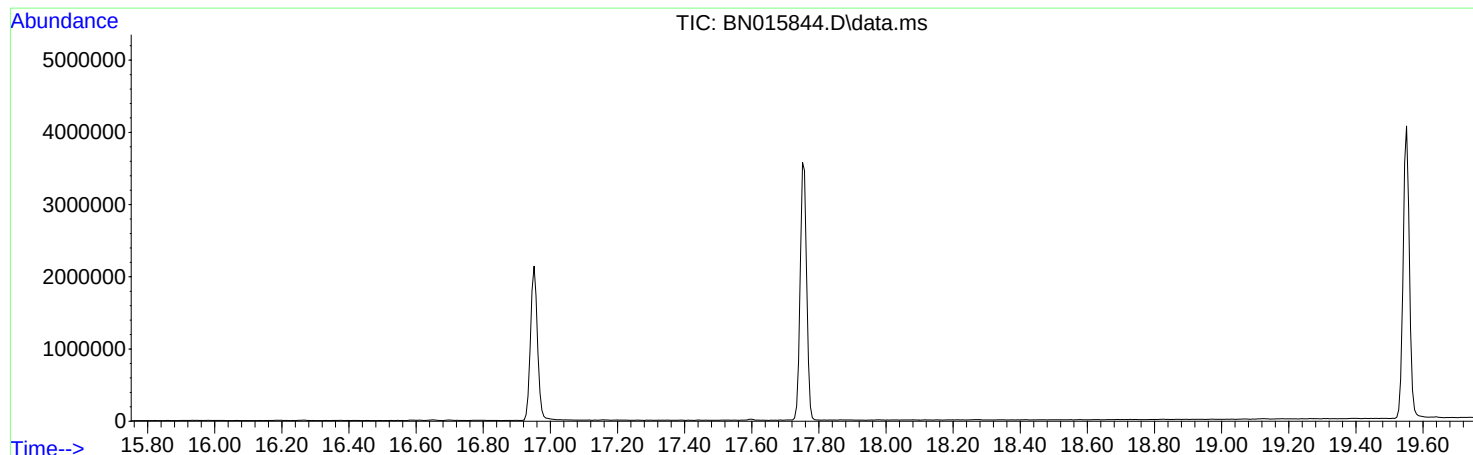




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	122931	PASS
68	69	0.00	2	1.3	1714	PASS
69	198	0.00	100	39.9	130232	PASS
70	69	0.00	2	0.6	792	PASS
127	198	10	80	42.3	138000	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	326507	PASS
199	198	5	9	6.6	21387	PASS
275	198	10	60	28.4	92712	PASS
365	198	1	100	3.9	12594	PASS
441	198	0.01	100	18.5	60448	PASS
442	442	50	100	100.0	395541	PASS
443	442	15	24	19.3	76285	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081121\
Data File : BN015844.D
Acq On : 11 Aug 2021 08:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 11 11:23:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 11 11:23:50 2021
Response via : Initial Calibration

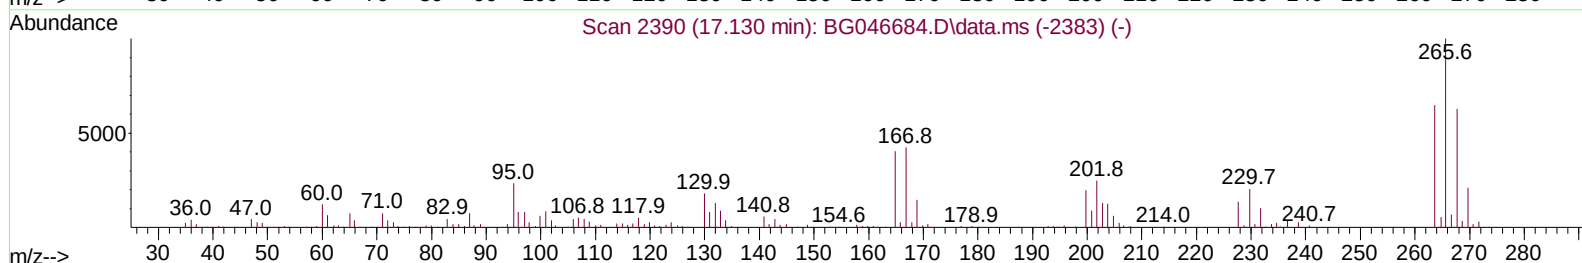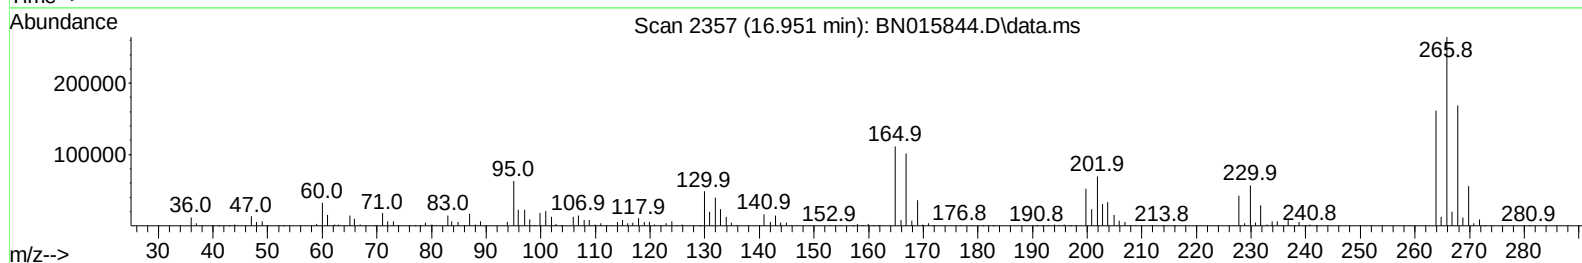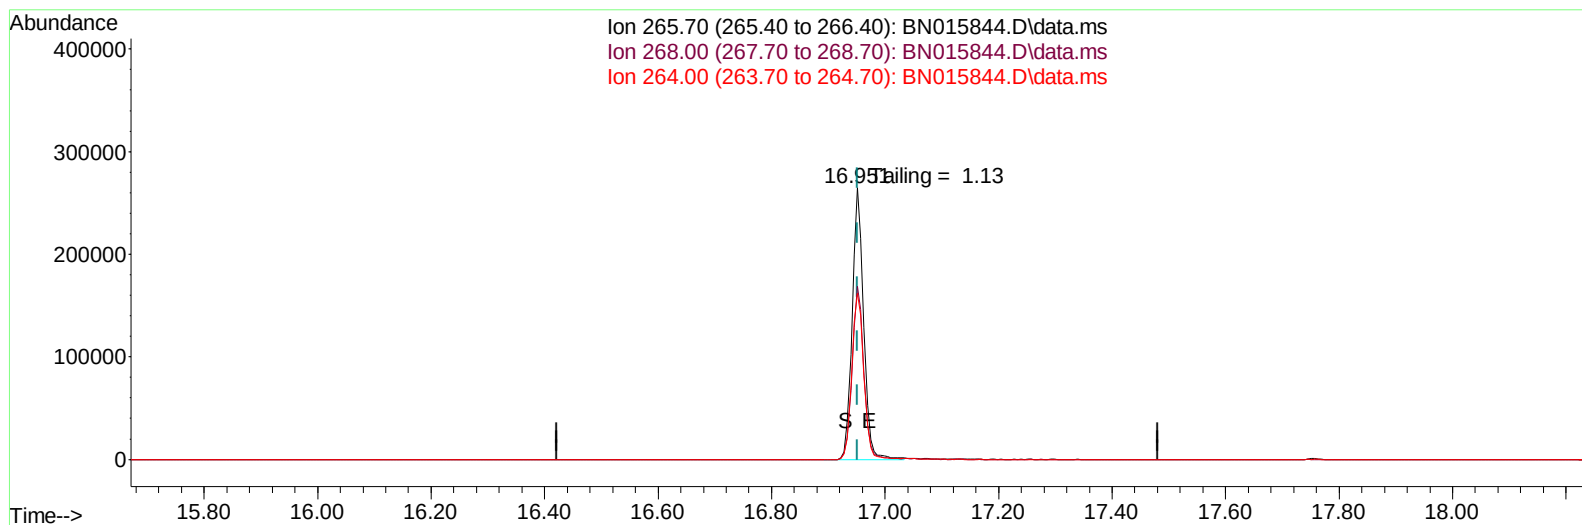

TIC: BN015844.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 22584.00 ng




response 374140

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.89
264.00	61.60	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081121\
Data File : BN015844.D
Acq On : 11 Aug 2021 08:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 11 11:23:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 11 11:23:50 2021
Response via : Initial Calibration

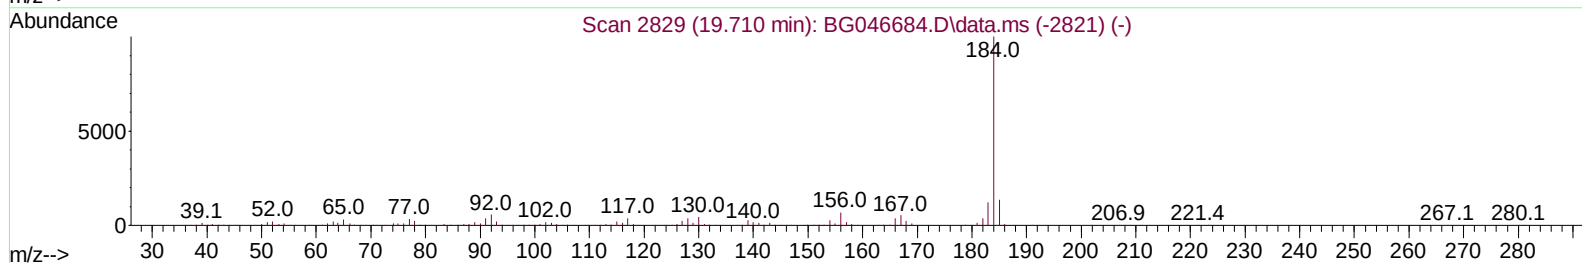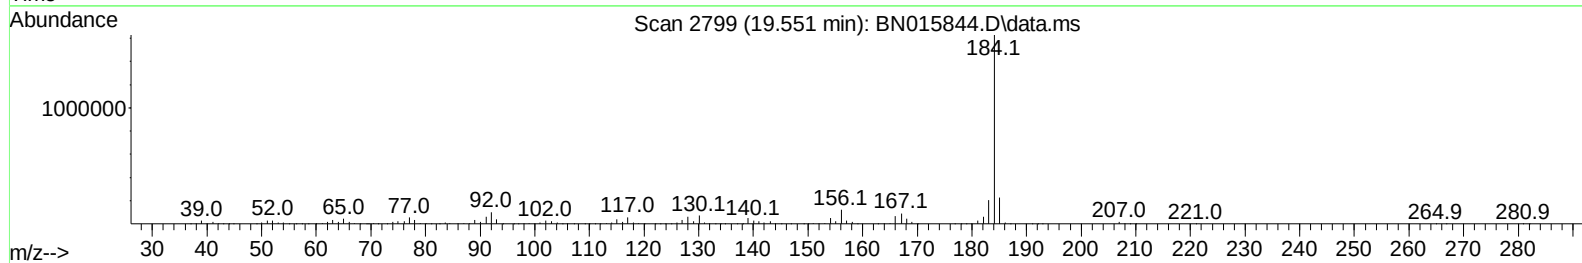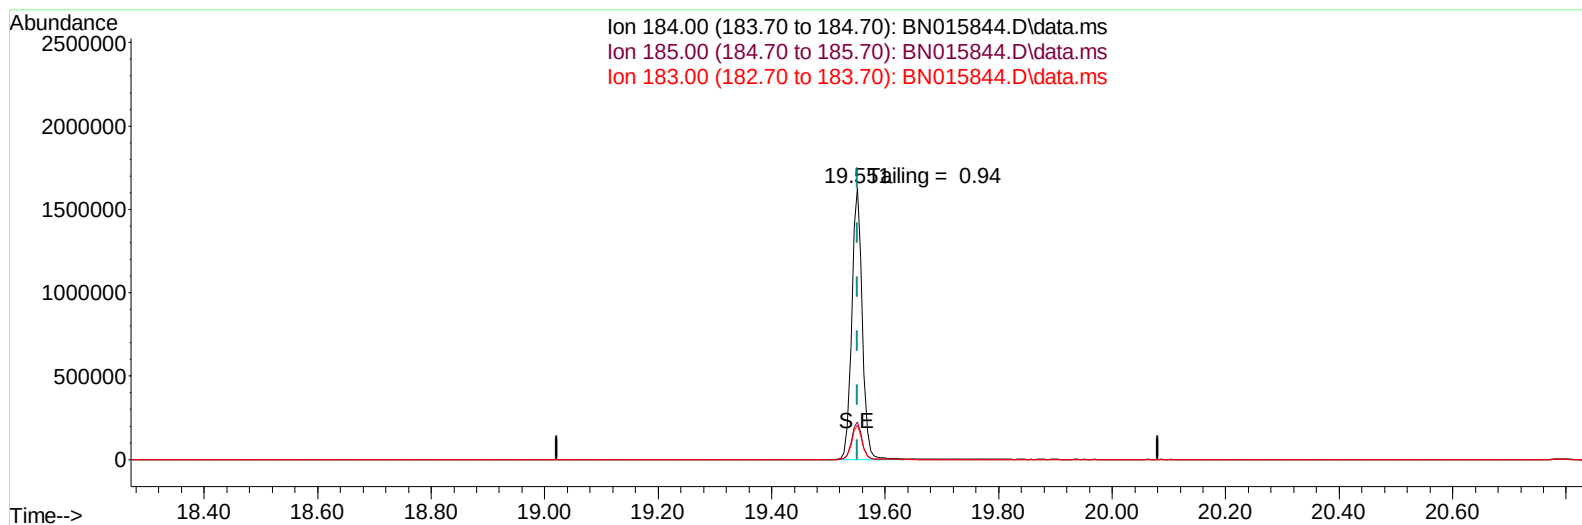

TIC: BN015844.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 2116347

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2021	BNA_N	<u>BN015844.D</u>
Compound Name	Response	Retention Time
DDT	1221467	20.79
DDD	10400	20.35
DDE	1899	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12299	1233766	1.00

Instrument :
BNA_N
ClientSampleId :
DFTPP