

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081219\
 Data File : BN007100.D
 Acq On : 12 Aug 2019 16:29
 Operator : HP/JU
 Sample : K4240-05MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:51:39 AM

Quant Time: Aug 13 05:07:53 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Aug 10 21:44:50 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	7426	0.40	ng	0.00
6) Naphthalene-d8	10.19	136	27353	0.40	ng	0.00
12) Acenaphthene-d10	14.08	164	15539	0.40	ng	0.00
18) Phenanthrene-d10	16.82	188	38116	0.40	ng	0.00
26) Chrysene-d12	21.05	240	40103	0.40	ng	-0.01
32) Perylene-d12	23.16	264	43622	0.40	ng	-0.01

System Monitoring Compounds

3) 2-Fluorophenol	5.06	112	6196	0.35	ng	0.00
4) Phenol-d6	6.61	99	8476	0.38	ng	0.00
7) Nitrobenzene-d5	8.56	82	6406	0.29	ng	0.00
10) 2-Methylnaphthalene-d10	11.79	152	17853m	0.35	ng	0.00
13) 2,4,6-Tribromophenol	15.57	330	1582	0.19	ng	0.00
14) 2-Fluorobiphenyl	12.71	172	4090	0.18	ng	0.00
24) Fluoranthene-d10	18.87	212	38543	0.29	ng	0.00
28) Terphenyl-d14	19.49	244	28240	0.26	ng	-0.01

Target Compounds

						Qvalue
2) n-Nitrosodimethylamine	3.34	42	1585	0.324	ng	# 96
5) bis(2-Chloroethyl)ether	6.87	93	6343	0.325	ng	98
8) Naphthalene	10.24	128	23752	0.310	ng	99
9) Hexachlorobutadiene	10.54	225	4802	0.294	ng	# 99
11) 2-Methylnaphthalene	11.86	142	16846	0.310	ng	98
15) Acenaphthylene	13.79	152	24738	0.305	ng	100
16) Acenaphthene	14.13	154	15621	0.300	ng	99
17) Fluorene	15.12	166	20452	0.263	ng	100
19) 4-Bromophenyl-phenylether	16.03	248	8473	0.359	ng	# 84
20) Hexachlorobenzene	16.14	284	7137	0.315	ng	99
21) Pentachlorophenol	16.48	266	1206	0.143	ng	97
22) Phenanthrene	16.87	178	42060	0.368	ng	100
23) Anthracene	16.95	178	32879	0.315	ng	99
25) Fluoranthene	18.90	202	56736	0.388	ng	100
27) Pyrene	19.26	202	57632	0.410	ng	99
29) Benzo(a)anthracene	21.02	228	53262	0.363	ng	99
30) Chrysene	21.08	228	53522	0.376	ng	99
31) Indeno(1,2,3-cd)pyrene	25.24	276	56018	0.357	ng	99
33) Benzo(b)fluoranthene	22.54	252	55270	0.369	ng	99
34) Benzo(k)fluoranthene	22.58	252	52902	0.358	ng	99
35) Benzo(a)pyrene	23.07	252	48690	0.359	ng	100
36) Dibenzo(a,h)anthracene	25.25	278	43857	0.324	ng	98
37) Benzo(g,h,i)perylene	25.86	276	48009	0.345	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081219\
Data File : BN007100.D
Acq On : 12 Aug 2019 16:29
Operator : HP/JU
Sample : K4240-05MS
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Manual Integrations
APPROVED

mohammad
8/14/2019 2:51:39 AM

Quant Time: Aug 13 05:07:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 10 21:44:50 2019
Response via : Initial Calibration





#1





1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 547
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
152	100		
150	147.1	121.7	182.5
115	54.8	46.2	69.4

Manual Integrations
APPROVED




mohammad
8/14/2019 2:51:39 AM






#2

n-Nitrosodimethylamine
Concen: 0.324 ng
RT: 3.34 min Scan# 39
Delta R.T. -0.02 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
42	100		
74	143.4	110.6	166.0
44	0.0	0.0	0.0



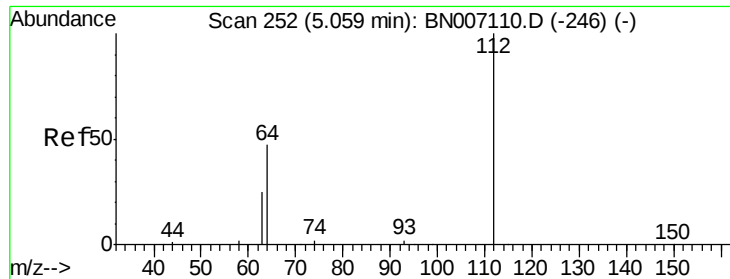

#3

2-Fluorophenol

Concen: 0.347 ng

RT: 5.06 min Scan# 252

Delta R.T. -0.00 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Tot Ion	Ratio	Resp	Lower	Upper
112	100	6196		
64	52.9		42.6	63.8
63	28.6		22.2	33.2

Instrument :





BNA_N

ClientSampleId :

PST-035-SW061-080619MS

Manual Integrations
APPROVED

mohammad
8/14/2019 2:51:39 AM



#4

Phenol-d6

Concen: 0.383 ng


RT: 6.61 min Scan# 445




Delta R.T. -0.00 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Resp	Lower	Upper
99	100	8476		
42	0.0		15.8	23.6#
71	35.4		27.0	40.4









#5
bis(2-Chloroethyl)ether
Concen: 0.325 ng
RT: 6.87 min Scan# 477
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tot Ion:	93	Resp:	6343
Ion	Ratio	Lower	Upper
93	100		
63	68.0	55.6	83.4
95	32.8	26.7	40.1

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS


Manual Integrations
APPROVED


mohammad
8/14/2019 2:51:39 AM



#6
Naphthalene-d8
Concen: 0.400 ng
RT: 10.19 min Scan# 813
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion:	136	Resp:	27353
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.4	14.0
54	5.9	6.6	9.8#
68	5.5	6.0	9.0#





#7

Nitrobenzene-d5

Concen: 0.290 ng

RT: 8.56 min Scan# 685

Delta R.T. -0.00 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Instrument :

BNA_N





ClientSampleId :

PST-035-SW061-080619MS

Tot Ion:	82	Resp:	6406
Ion	Ratio	Lower	Upper
82	100		
128	49.9	34.6	51.8
54	41.9	36.2	54.4

Manual Integrations
APPROVED

mohammad
8/14/2019 2:51:39 AM



#8

Naphthalene

Concen: 0.310 ng




RT: 10.24 min Scan# 817


Delta R.T. -0.00 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Tgt Ion:	128	Resp:	23752
Ion	Ratio	Lower	Upper
128	100		
129	11.6	9.4	14.2
127	13.2	11.0	16.6









#9
Hexachlorobutadiene
Concen: 0.294 ng
RT: 10.54 min Scan# 841
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	51.1	76.7




Manual Integrations
APPROVED


mohammad
8/14/2019 2:51:39 AM



#10
2-Methylnaphthalene-d10
Concen: 0.350 ng m
RT: 11.79 min Scan# 981
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
152	100		
151	17.1	15.5	23.3









#11
2-Methylnaphthalene
Concen: 0.310 ng
RT: 11.86 min Scan# 997
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
142	100		
141	88.3	69.0	103.6
115	34.6	27.1	40.7




Manual Integrations
APPROVED


mohammad
8/14/2019 2:51:39 AM



#12
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.08 min Scan# 1310
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.9	82.2	123.4
160	46.3	38.3	57.5









#13
 2,4,6-Tribromophenol
 Concen: 0.189 ng
 RT: 15.57 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	42.5	33.6	50.4




Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:51:39 AM



#14
 2-Fluorobiphenyl
 Concen: 0.181 ng
 RT: 12.71 min Scan# 1187
 Delta R.T. -0.00 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.5	26.3	39.5
170	21.1	17.0	25.4









#15
Acenaphthylene
Concen: 0.305 ng
RT: 13.79 min Scan# 1284
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
152	100		
151	19.7	15.8	23.6
153	13.4	10.4	15.6




Manual Integrations
APPROVED


mohammad
8/14/2019 2:51:39 AM



#16
Acenaphthene
Concen: 0.300 ng
RT: 14.13 min Scan# 1315
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
154	100		
153	110.6	89.5	134.3
152	54.8	44.8	67.2









#17
Fluorene
 Concen: 0.263 ng
 RT: 15.12 min Scan# 1404
 Delta R.T. -0.01 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
166	100		
165	97.7	77.9	116.9
167	13.3	10.9	16.3




Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:51:39 AM



#18
Phenanthrene-d10
 Concen: 0.400 ng
 RT: 16.82 min Scan# 1560
 Delta R.T. -0.00 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	7.1	7.8	11.6#









#19
4-Bromophenyl-phenylether
Concen: 0.359 ng
RT: 16.03 min Scan# 1485
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
248	100		
250	86.8	78.9	118.3
141	71.9	43.3	64.9




Manual Integrations
APPROVED




mohammad
8/14/2019 2:51:39 AM



#20
Hexachlorobenzene
Concen: 0.315 ng
RT: 16.14 min Scan# 1496
Delta R.T. -0.00 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
284	100		
142	39.1	30.5	45.7
249	33.5	26.7	40.1









#21
 Pentachlorophenol
 Concen: 0.143 ng
 RT: 16.48 min Scan# 1528
 Delta R.T. -0.00 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
266	100		
264	64.3	52.3	78.5
268	68.8	51.5	77.3


Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:51:39 AM



#22
 Phenanthrene
 Concen: 0.368 ng
 RT: 16.87 min Scan# 1564
 Delta R.T. -0.00 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.2	22.8
179	15.3	12.3	18.5









#23
 Anthracene
 Concen: 0.315 ng
 RT: 16.95 min Scan# 1572
 Delta R.T. -0.01 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
178	100		
176	18.6	14.6	21.8
179	15.2	12.5	18.7




Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:51:39 AM



#24
 Fluoranthene-d10
 Concen: 0.285 ng
 RT: 18.87 min Scan# 1844
 Delta R.T. -0.01 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
212	100		
106	10.2	8.2	12.2
104	5.6	4.5	6.7





#25

Fluoranthene

Concen: 0.388 ng

RT: 18.90 min Scan# 1850

Delta R.T. -0.01 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Instrument :

BNA_N





ClientSampleId :

PST-035-SW061-080619MS

Tot Ion:	202	Resp:	56736
Ion Ratio	Lower	Upper	
202	100		
101	8.8	7.0	10.4
203	17.3	13.8	20.8

Manual Integrations
APPROVED

mohammad
8/14/2019 2:51:39 AM



#26

Chrysene-d12

Concen: 0.400 ng




RT: 21.05 min Scan# 2171


Delta R.T. -0.01 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Tgt Ion:	240	Resp:	40103
Ion Ratio	Lower	Upper	
240	100		
120	6.4	4.0	6.0#
236	27.0	21.3	31.9









#27
Pvrene
Concen: 0.410 ng
RT: 19.26 min Scan# 1923
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
202	100		
200	20.8	16.6	24.8
203	18.4	14.0	21.0




Manual Integrations
APPROVED


mohammad
8/14/2019 2:51:39 AM



#28
Terphenyl-d14
Concen: 0.258 ng
RT: 19.49 min Scan# 1969
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.8	6.2	9.2
122	10.4	7.4	11.2





#29

Benzo(a)anthracene

Concen: 0.363 ng

RT: 21.02 min Scan# 2169

Delta R.T. -0.01 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Instrument :

BNA_N





ClientSampleId :

PST-035-SW061-080619MS

Tot Ion:	228	Resp:	53262
Ion Ratio	Lower	Upper	
228	100		
226	28.2	21.8	32.6
229	19.8	15.6	23.4

Manual Integrations
APPROVED

mohammad
8/14/2019 2:51:39 AM



#30

Chrysene

Concen: 0.376 ng




RT: 21.08 min Scan# 2174


Delta R.T. -0.01 min

Lab File: BN007100.D

Acq: 12 Aug 2019 16:29

Tgt Ion:	228	Resp:	53522
Ion Ratio	Lower	Upper	
228	100		
226	30.5	23.8	35.6
229	19.9	15.7	23.5









#31
 Indeno(1,2,3-cd)pyrene
 Concen: 0.357 ng
 RT: 25.24 min Scan# 3126
 Delta R.T. -0.02 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.9	16.0	24.0
277	24.3	19.9	29.9




Manual Integrations
 APPROVED


mohammad
 8/14/2019 2:51:39 AM



#32
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.16 min Scan# 2519
 Delta R.T. -0.01 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.8
265	30.7	26.2	39.4









#33
Benzo(b)fluoranthene
Concen: 0.369 ng
RT: 22.54 min Scan# 2338
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.1	18.2	27.2
125	9.2	7.4	11.0




Manual Integrations
APPROVED


mohammad
8/14/2019 2:51:39 AM



#34
Benzo(k)fluoranthene
Concen: 0.358 ng
RT: 22.58 min Scan# 2350
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	18.1	27.1
125	9.5	7.4	11.0









#35
Benzo(a)pyrene
Concen: 0.359 ng
RT: 23.07 min Scan# 2493
Delta R.T. -0.01 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Instrument :
BNA_N
ClientSampleId :
PST-035-SW061-080619MS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.1	18.5	27.7
125	10.1	8.2	12.4




Manual Integrations
APPROVED




mohammad
8/14/2019 2:51:39 AM



#36
Dibenzo(a,h)anthracene
Concen: 0.324 ng
RT: 25.25 min Scan# 3131
Delta R.T. -0.02 min
Lab File: BN007100.D
Acq: 12 Aug 2019 16:29

Tgt Ion	Ratio	Lower	Upper
278	100		
139	15.1	11.3	16.9
279	24.7	19.3	28.9





#37
 Benzo(a,h,i)perylene
 Concen: 0.345 ng
 RT: 25.86 min Scan# 3309
 Delta R.T. -0.02 min
 Lab File: BN007100.D
 Acq: 12 Aug 2019 16:29

Tot Ion	Ratio	Lower	Upper
276	100		
277	24.5	19.8	29.8
138	18.5	14.6	22.0

Instrument :
 BNA_N
 ClientSampleId :
 PST-035-SW061-080619MS

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:51:39 AM

