


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081219\
 Data File : BN007090.D
 Acq On : 12 Aug 2019 10:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 12:12:02 2019

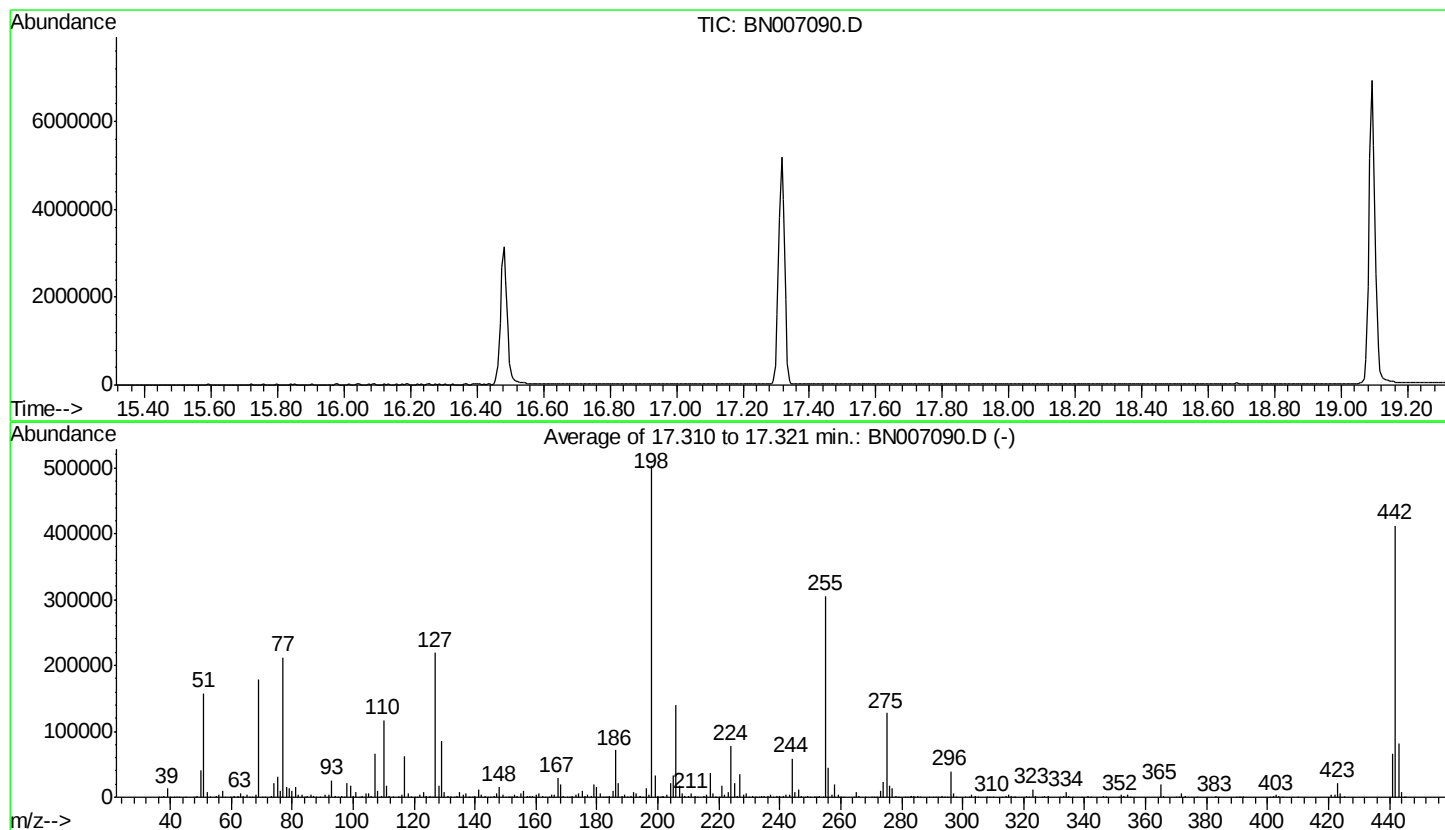

AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	158361	PASS
68	69	0.00	2	2.0	3632	PASS
69	198	0.00	100	35.4	178090	PASS
70	69	0.00	2	0.6	1032	PASS
127	198	10	80	43.6	219413	PASS
197	198	0.00	2	0.7	3732	PASS
198	198	100	100	100.0	503296	PASS
199	198	5	9	6.7	33754	PASS
275	198	10	60	25.3	127349	PASS
365	198	1	100	3.8	19127	PASS
441	198	0.01	100	13.1	65877	PASS
442	198	50	100	81.8	411904	PASS
443	442	15	24	19.7	81200	PASS