

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
 Data File : BN015855.D
 Acq On : 12 Aug 2021 08:38
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Aug 12 10:36:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 12 10:35:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	8659	0.400	ng	0.00
7) Naphthalene-d8	10.723	136	41848	0.400	ng	0.00
13) Acenaphthene-d10	14.548	164	23778	0.400	ng	0.00
19) Phenanthrene-d10	17.297	188	47871	0.400	ng	0.00
29) Chrysene-d12	21.493	240	53013	0.400	ng	0.00
35) Perylene-d12	23.916	264	49242	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.485	112	4169	0.185	ng	0.00
5) Phenol-d6	7.071	99	5583	0.183	ng	0.00
8) Nitrobenzene-d5	9.076	82	6792	0.207	ng	0.00
11) 2-Methylnaphthalene-d10	12.309	152	13402	0.199	ng	0.00
14) 2,4,6-Tribromophenol	16.044	330	1701	0.160	ng	0.00
15) 2-Fluorobiphenyl	13.178	172	20068	0.210	ng	0.00
27) Fluoranthene-d10	19.336	212	28108	0.193	ng	0.00
31) Terphenyl-d14	19.932	244	31070	0.200	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.410	88	653	0.180	ng	96
3) n-Nitrosodimethylamine	3.779	42	1566	0.177	ng	# 97
6) bis(2-Chloroethyl)ether	7.347	93	4689	0.197	ng	100
9) Naphthalene	10.774	128	21636	0.197	ng	99
10) Hexachlorobutadiene	11.066	225	5909	0.208	ng	# 99
12) 2-Methylnaphthalene	12.385	142	14595	0.191	ng	99
16) Acenaphthylene	14.269	152	17319	0.171	ng	99
17) Acenaphthene	14.611	154	12967	0.193	ng	99
18) Fluorene	15.601	166	16032	0.189	ng	99
20) 4,6-Dinitro-2-methylph...	15.677	198	562	0.120	ng	# 86
21) 4-Bromophenyl-phenylether	16.494	248	5031	0.196	ng	99
22) Hexachlorobenzene	16.616	284	6700	0.202	ng	99
23) Atrazine	16.762	200	3591	0.159	ng	98
24) Pentachlorophenol	16.957	266	1891	0.149	ng	99
25) Phenanthrene	17.346	178	25900	0.193	ng	99
26) Anthracene	17.431	178	21576	0.178	ng	100
28) Fluoranthene	19.366	202	30355	0.189	ng	99
30) Pyrene	19.728	202	30471	0.182	ng	100
32) Benzo(a)anthracene	21.472	228	32697	0.190	ng	100
33) Chrysene	21.525	228	33147	0.192	ng	100
34) Bis(2-ethylhexyl)phtha...	21.408	149	11550	0.147	ng	100
36) Indeno(1,2,3-cd)pyrene	26.431	276	30366	0.180	ng	98
37) Benzo(b)fluoranthene	23.176	252	32506	0.189	ng	98
38) Benzo(k)fluoranthene	23.224	252	31957	0.200	ng	99
39) Benzo(a)pyrene	23.810	252	27723	0.186	ng	97
40) Dibenzo(a,h)anthracene	26.455	278	24504	0.179	ng	# 95
41) Benzo(g,h,i)perylene	27.202	276	26709	0.179	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
Data File : BN015855.D
Acq On : 12 Aug 2021 08:38
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Aug 12 10:36:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 12 10:35:26 2021
Response via : Initial Calibration




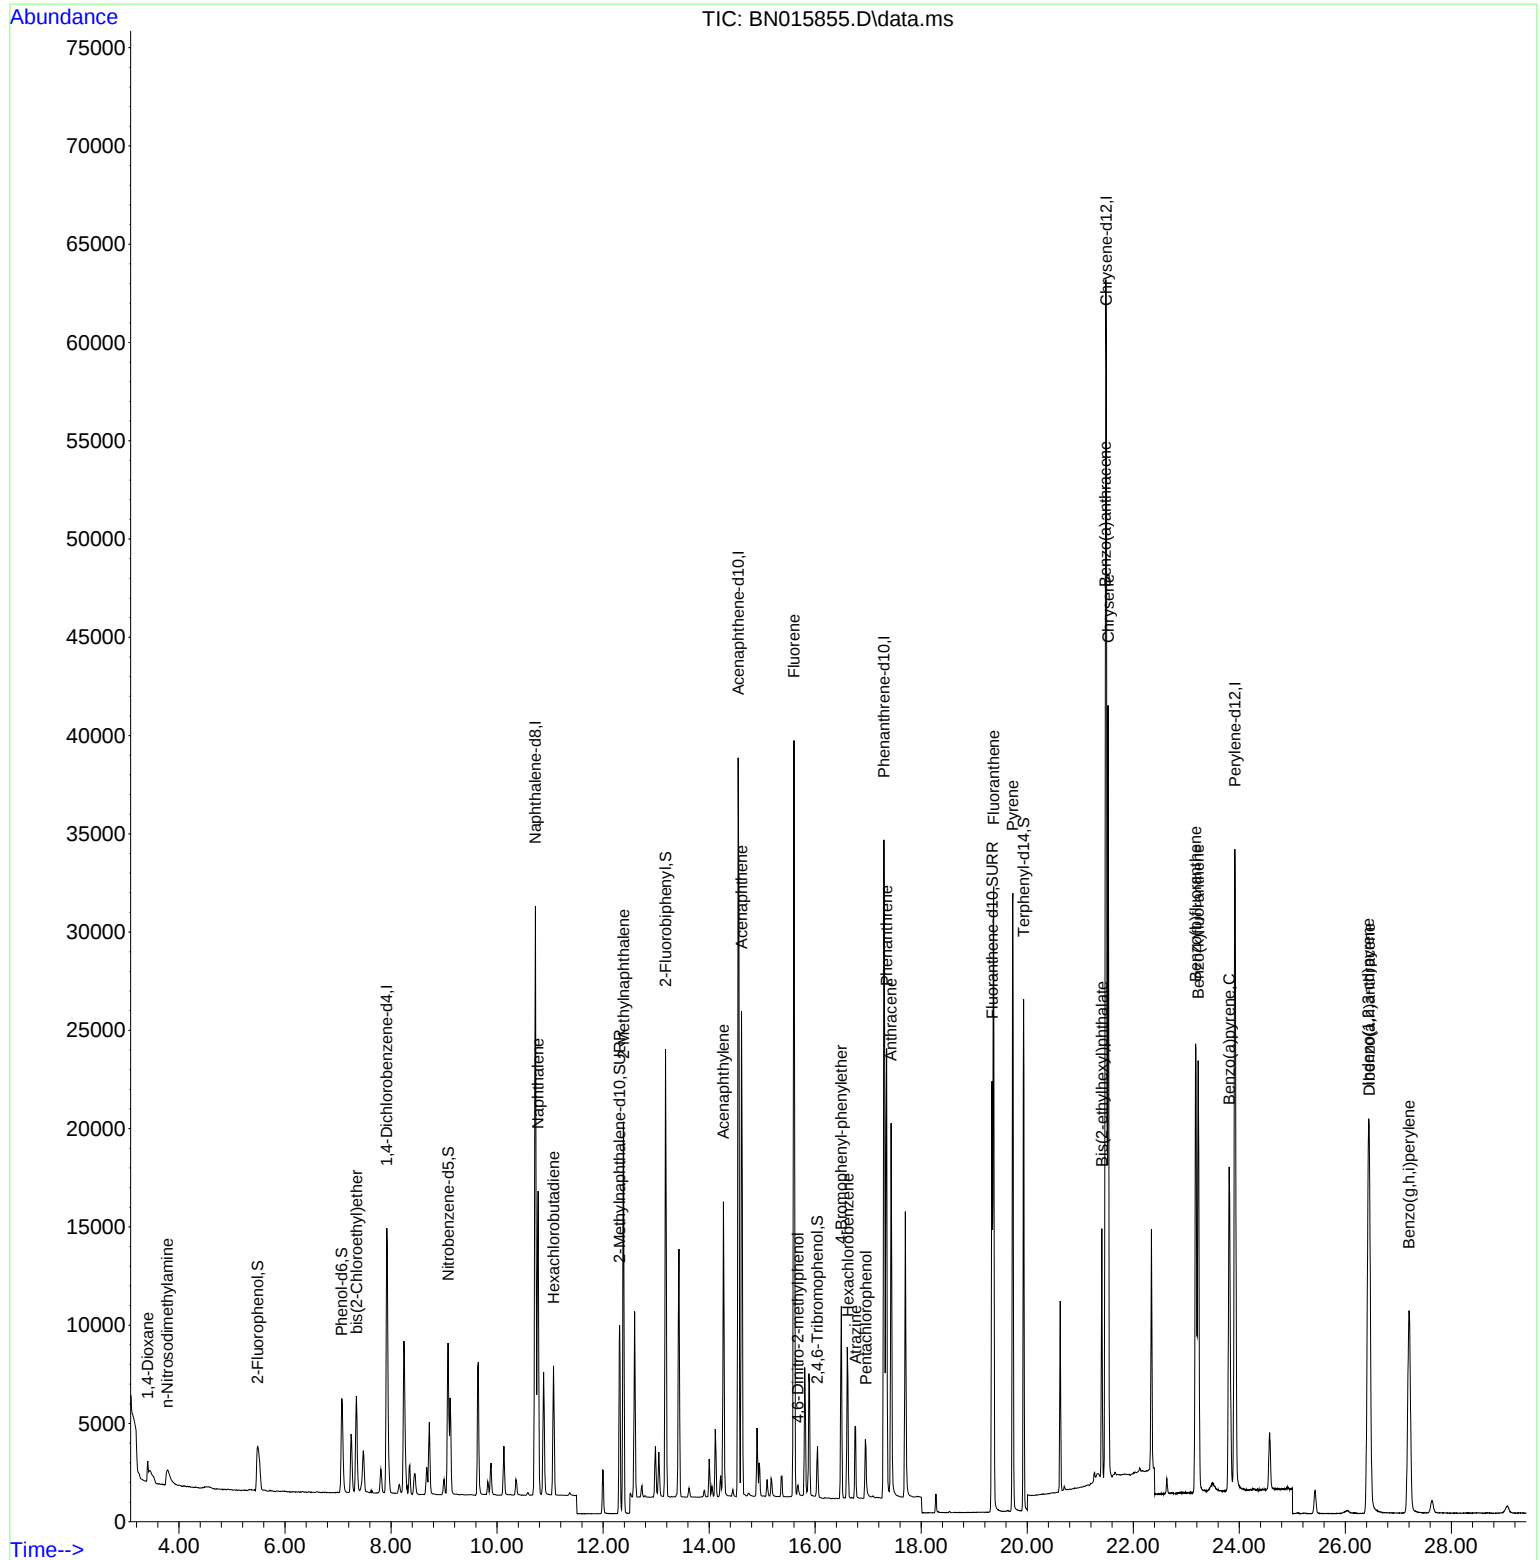


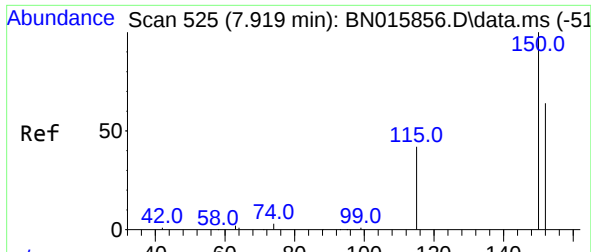

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.919 min Scan# 525
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:152 Resp: 8659
Ion Ratio Lower Upper
152 100
150 153.9 125.8 188.8
115 65.7 53.6 80.4

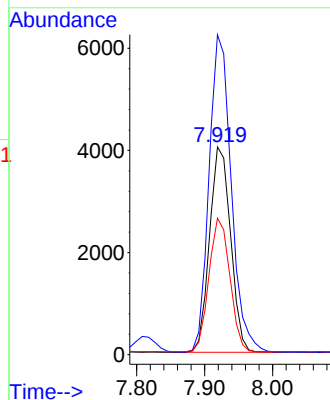

#2
1,4-Dioxane
Concen: 0.180 ng
RT: 3.410 min Scan# 36
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion: 88 Resp: 653
Ion Ratio Lower Upper
88 100
43 41.3 29.4 44.2
58 88.8 69.3 103.9


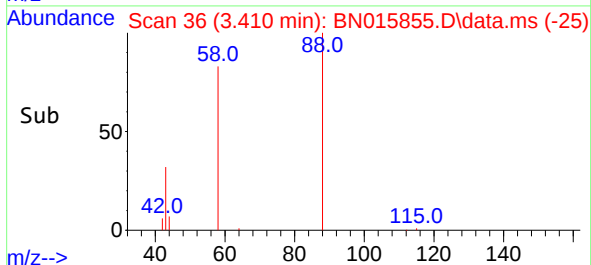
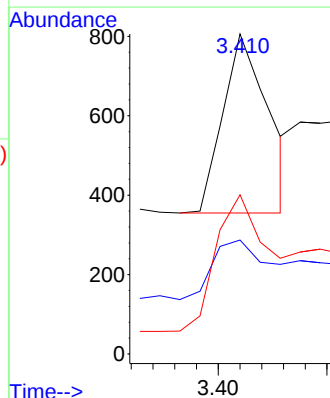
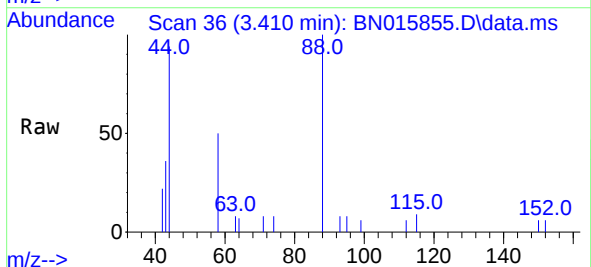




#3
n-Nitrosodimethylamine
Concen: 0.177 ng
RT: 3.779 min Scan# 76
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion: 42 Resp: 1566
Ion Ratio Lower Upper
42 100
74 104.0 86.1 129.1
44 3.8 3.8 5.8#



#4
2-Fluorophenol
Concen: 0.185 ng
RT: 5.485 min Scan# 261
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion: 112 Resp: 4169
Ion Ratio Lower Upper
112 100
64 66.7 53.3 79.9
63 36.7 28.6 42.8









#5
Phenol-d6
Concen: 0.183 ng
RT: 7.071 min Scan# 433
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion: 99 Resp: 5583




Ion	Ratio	Lower	Upper
99	100		
42	23.3	18.7	28.1
71	40.9	32.4	48.6




#6
bis(2-Chloroethyl)ether
Concen: 0.197 ng
RT: 7.347 min Scan# 463
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion: 93 Resp: 4689

Ion	Ratio	Lower	Upper
93	100		
63	79.9	63.8	95.6
95	32.8	26.0	39.0









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.723 min Scan# 758
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	136	Resp:	41848
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.0	13.4
54	6.8	5.4	8.2
68	4.7	3.8	5.8

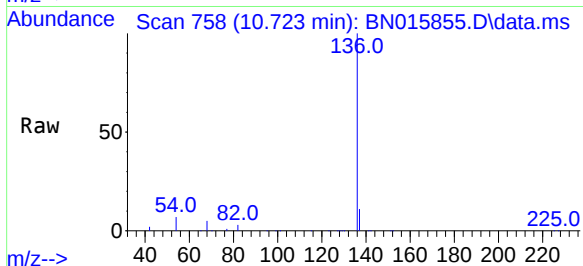

#8
Nitrobenzene-d5
Concen: 0.207 ng
RT: 9.076 min Scan# 628
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:	82	Resp:	6792
Ion	Ratio	Lower	Upper
82	100		
128	36.4	29.2	43.8
54	52.2	41.1	61.7



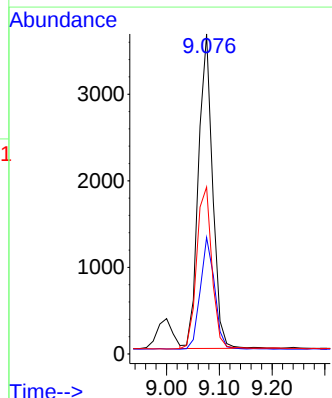
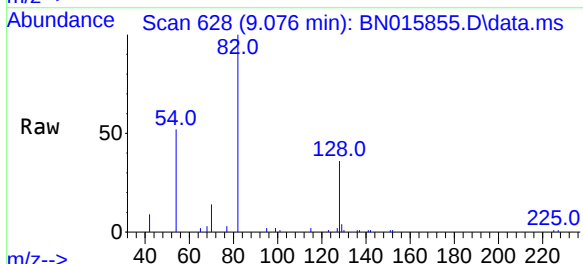




#9
Naphthalene
Concen: 0.197 ng
RT: 10.774 min Scan# 762
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	128	Resp:	21636
Ion	Ratio	Lower	Upper
128	100		
129	11.4	8.8	13.2
127	13.5	10.5	15.7



#10
Hexachlorobutadiene
Concen: 0.208 ng
RT: 11.066 min Scan# 785
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:	225	Resp:	5909
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.6	51.4	77.0









#11
2-Methylnaphthalene-d10
Concen: 0.199 ng
RT: 12.309 min Scan# 1000
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:152 Resp: 13402
Ion Ratio Lower Upper
152 100
151 20.4 16.5 24.7



#12
2-Methylnaphthalene
Concen: 0.191 ng
RT: 12.385 min Scan# 1017
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:142 Resp: 14595
Ion Ratio Lower Upper
142 100
141 87.4 70.5 105.7
115 37.1 29.8 44.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.548 min Scan# 1205
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:164 Resp: 23778
Ion Ratio Lower Upper
164 100
162 104.5 83.5 125.3
160 47.5 37.7 56.5



#14
2,4,6-Tribromophenol
Concen: 0.160 ng
RT: 16.044 min Scan# 1323
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:330 Resp: 1701
Ion Ratio Lower Upper
330 100
332 116.5 84.1 126.1
141 30.9 24.2 36.4









#15
2-Fluorobiphenyl
Concen: 0.210 ng
RT: 13.178 min Scan# 1097
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	172	Resp:	20068
Ion	Ratio	Lower	Upper
172	100		
171	35.6	28.7	43.1
170	23.7	19.0	28.4



#16
Acenaphthylene
Concen: 0.171 ng
RT: 14.269 min Scan# 1183
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:	152	Resp:	17319
Ion	Ratio	Lower	Upper
152	100		
151	19.8	15.4	23.2
153	13.2	10.5	15.7









#17
Acenaphthene
Concen: 0.193 ng
RT: 14.611 min Scan# 1210
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	154	Resp:	12967
Ion	Ratio	Lower	Upper
154	100		
153	111.7	90.1	135.1
152	53.5	43.5	65.3

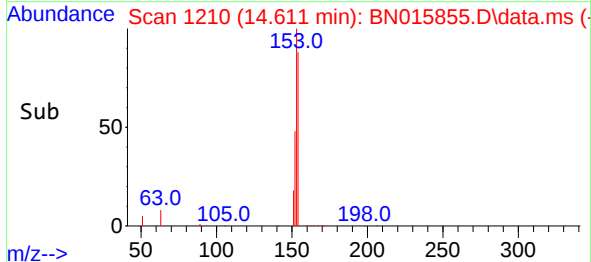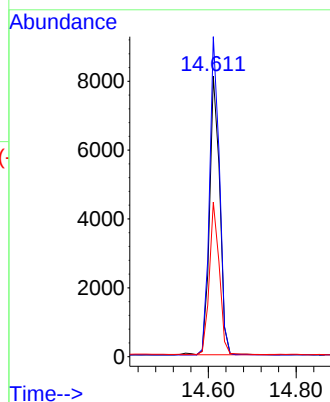

#18
Fluorene
Concen: 0.189 ng
RT: 15.601 min Scan# 1288
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:	166	Resp:	16032
Ion	Ratio	Lower	Upper
166	100		
165	98.3	77.8	116.6
167	13.6	11.0	16.4


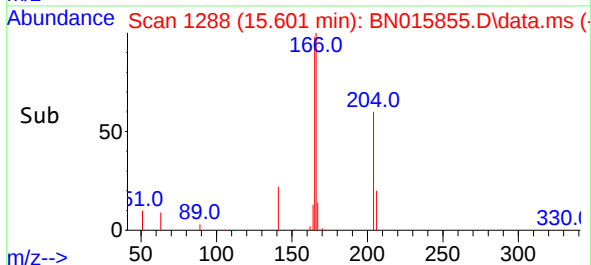
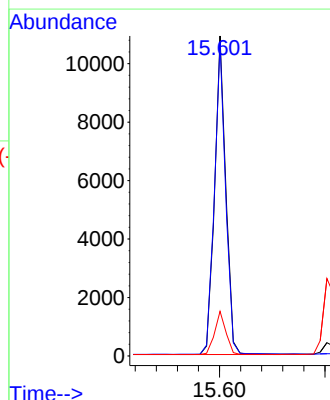
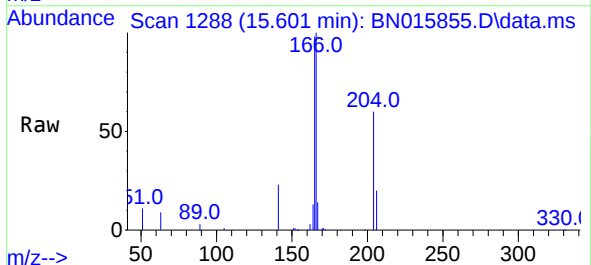




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.297 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:188	Resp:	47871
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	9.2	10.8



#20
4,6-Dinitro-2-methylphenol
Concen: 0.120 ng
RT: 15.677 min Scan# 1294
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:198	Resp:	562
Ion Ratio	Lower	Upper
198	100	
182	20.8	11.9
77	0.0	0.0






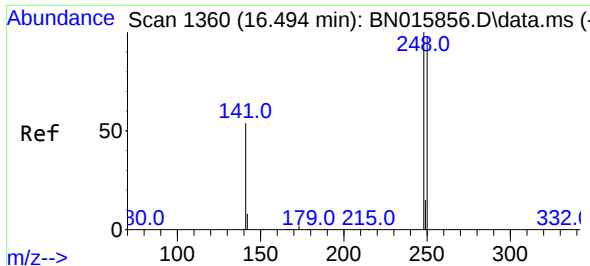


#21
4-Bromophenyl-phenylether
Concen: 0.196 ng
RT: 16.494 min Scan# 1360
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:248 Resp: 5031




Ion	Ratio	Lower	Upper
248	100		
250	96.9	78.6	118.0
141	54.5	43.4	65.2

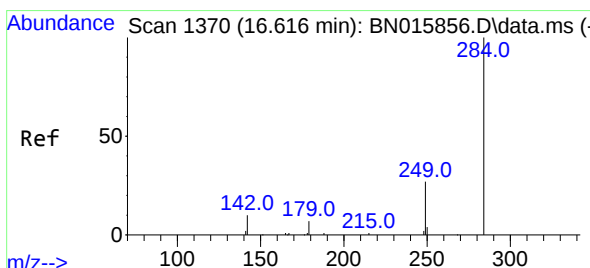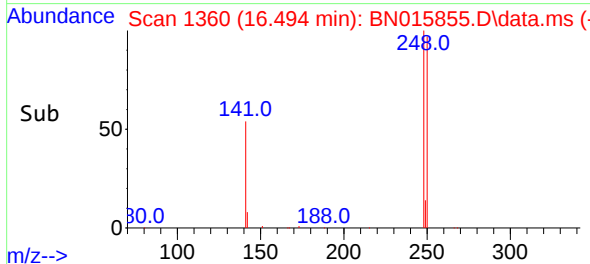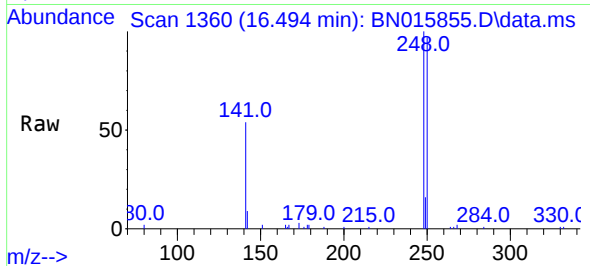


#22
Hexachlorobenzene
Concen: 0.202 ng
RT: 16.616 min Scan# 1370
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:284 Resp: 6700

Ion	Ratio	Lower	Upper
284	100		
142	28.4	22.6	34.0
249	32.3	25.2	37.8


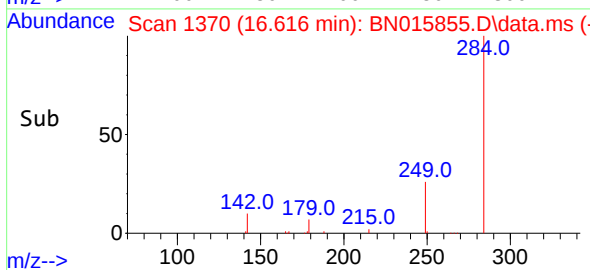

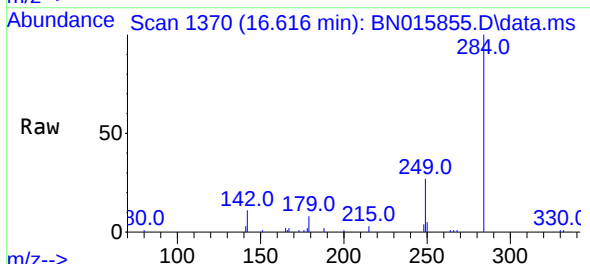




#23
Atrazine
Concen: 0.159 ng
RT: 16.762 min Scan# 1382
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	200	Resp:	3591
Ion	Ratio	Lower	Upper
200	100		
173	21.8	16.4	24.6
215	53.4	41.5	62.3



#24
Pentachlorophenol
Concen: 0.149 ng
RT: 16.957 min Scan# 1398
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:	266	Resp:	1891
Ion	Ratio	Lower	Upper
266	100		
264	61.1	50.1	75.1
268	63.7	51.0	76.6







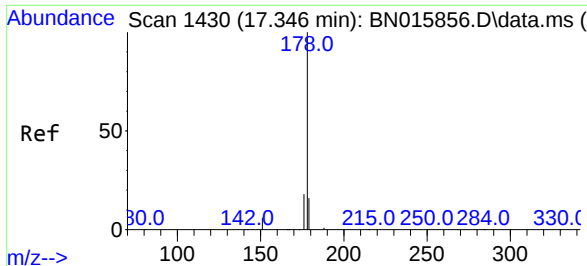

#25
Phenanthrene
Concen: 0.193 ng
RT: 17.346 min Scan# 1430
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:178 Resp: 25900
Ion Ratio Lower Upper
178 100
176 18.4 14.6 21.8
179 16.0 12.6 18.8

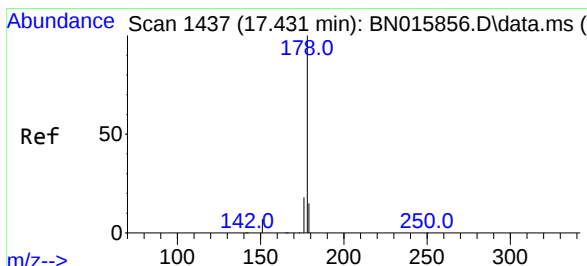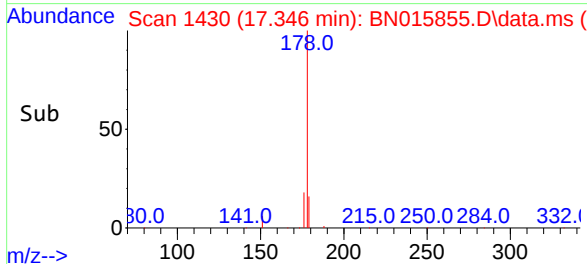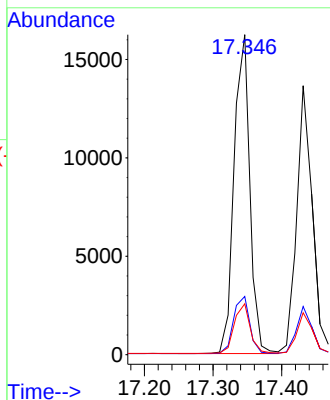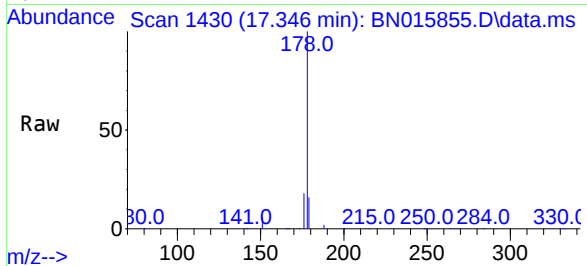

#26
Anthracene
Concen: 0.178 ng
RT: 17.431 min Scan# 1437
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:178 Resp: 21576
Ion Ratio Lower Upper
178 100
176 17.7 14.3 21.5
179 15.4 12.2 18.4

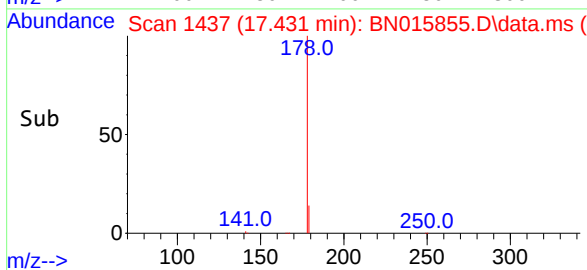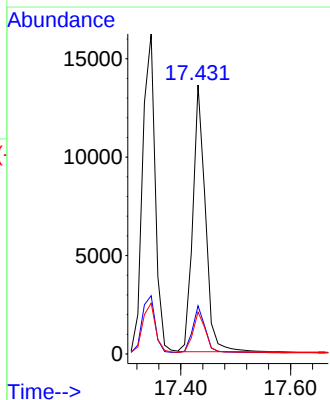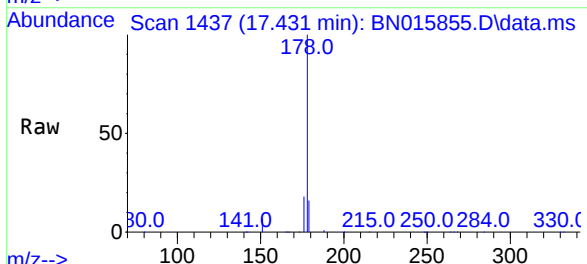







#27
Fluoranthene-d10
Concen: 0.193 ng
RT: 19.336 min Scan# 1751
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:212 Resp: 28108




Ion	Ratio	Lower	Upper
212	100		
106	9.2	7.4	11.2
104	5.4	4.3	6.5




#28
Fluoranthene
Concen: 0.189 ng
RT: 19.366 min Scan# 1757
Delta R.T. 0.005 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:202 Resp: 30355

Ion	Ratio	Lower	Upper
202	100		
101	8.8	6.8	10.2
203	17.5	13.8	20.8









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.493 min Scan# 2026
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:240 Resp: 53013
Ion Ratio Lower Upper
240 100
120 4.7 3.8 5.8
236 25.0 20.0 30.0

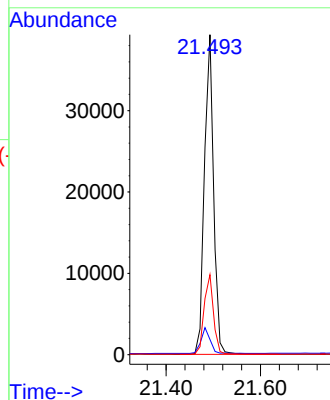

#30
Pyrene
Concen: 0.182 ng
RT: 19.728 min Scan# 1830
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:202 Resp: 30471
Ion Ratio Lower Upper
202 100
200 20.1 16.2 24.2
203 17.5 14.1 21.1



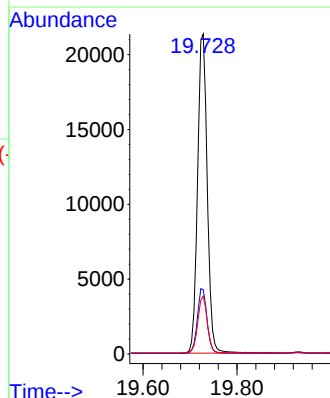



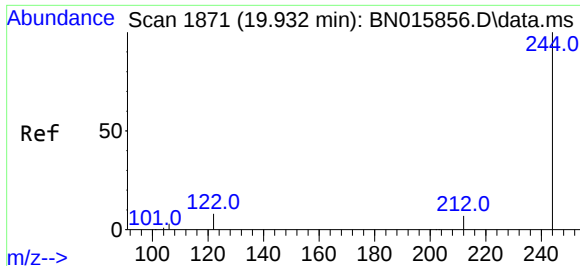

#31
Terphenyl-d14
Concen: 0.200 ng
RT: 19.932 min Scan# 1871
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:244 Resp: 31070
Ion Ratio Lower Upper
244 100
212 7.5 6.0 9.0
122 8.4 6.5 9.7

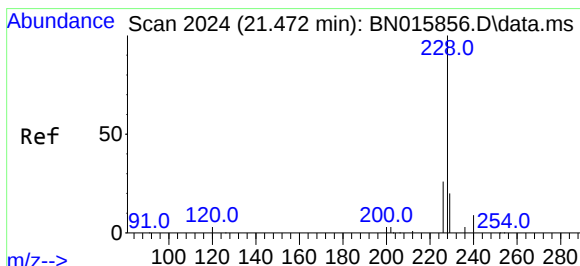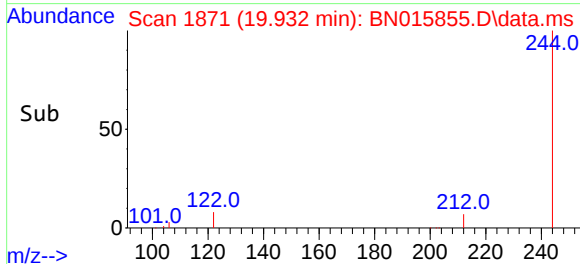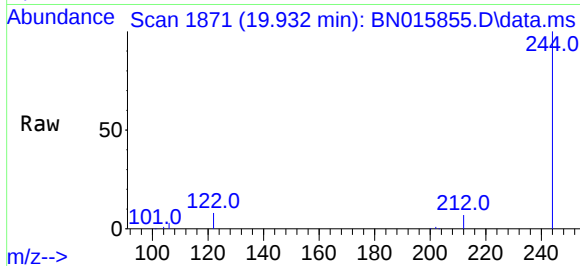

#32
Benzo(a)anthracene
Concen: 0.190 ng
RT: 21.472 min Scan# 2024
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:228 Resp: 32697
Ion Ratio Lower Upper
228 100
226 26.7 21.1 31.7
229 19.5 15.7 23.5


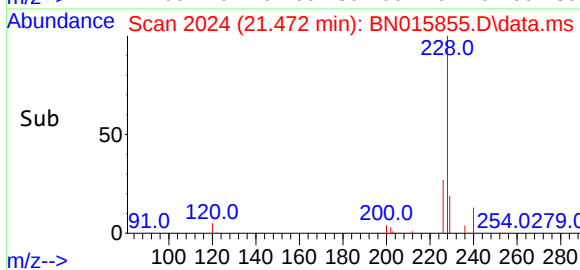

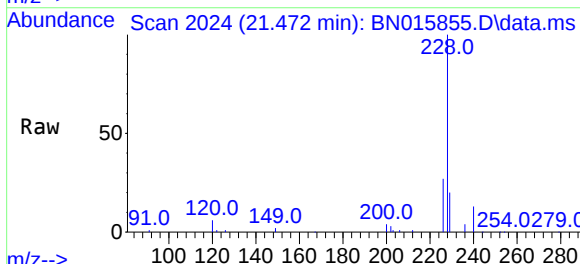


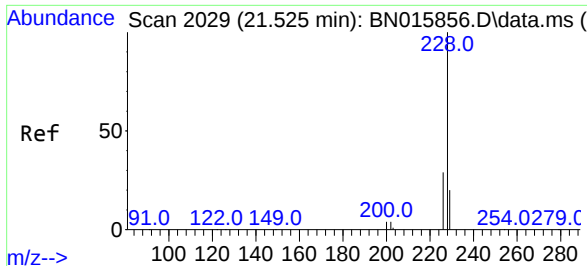

#33
Chrysene
Concen: 0.192 ng
RT: 21.525 min Scan# 2029
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	228	Resp:	33147
Ion Ratio	Lower	Upper	
228	100		
226	29.3	23.4	35.2
229	19.8	15.8	23.6

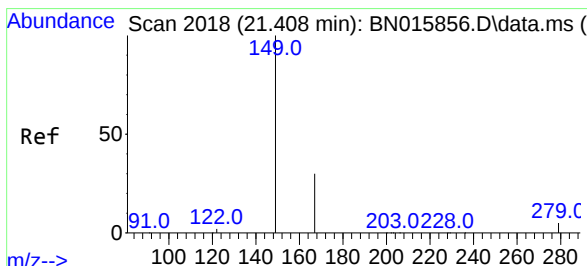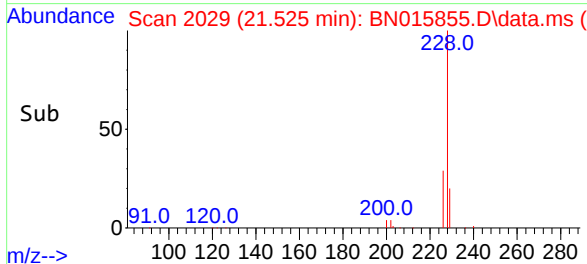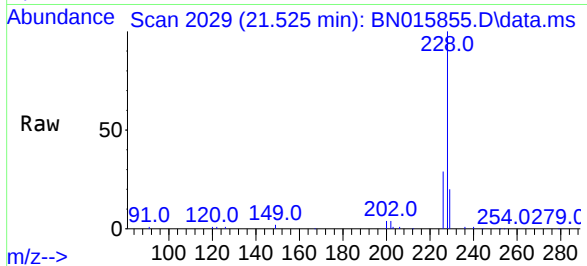

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.147 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38


Tgt Ion:	149	Resp:	11550
Ion Ratio	Lower	Upper	
149	100		
167	28.6	22.9	34.3
279	5.3	4.4	6.6

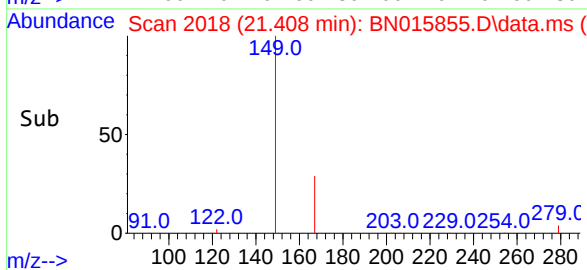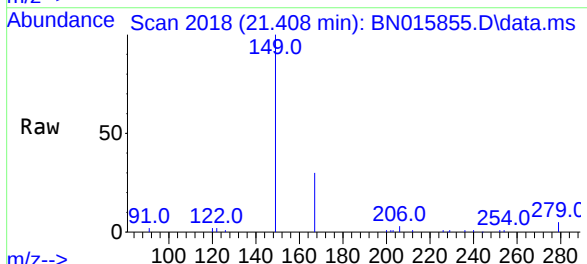





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.916 min Scan# 2553
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2





Tgt Ion:264 Resp: 49242
Ion Ratio Lower Upper
264 100
260 24.3 19.1 28.7
265 25.0 19.8 29.8

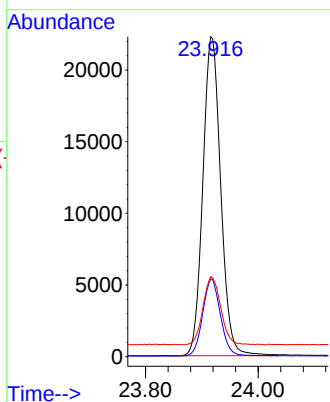


#36
Indeno(1,2,3-cd)pyrene
Concen: 0.180 ng
RT: 26.431 min Scan# 3288
Delta R.T. 0.003 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38



Tgt Ion:276 Resp: 30366
Ion Ratio Lower Upper
276 100
138 18.8 13.8 20.8
277 25.3 20.3 30.5

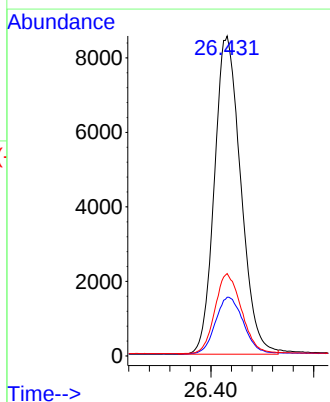



#37

Benzo(b)fluoranthene

Concen: 0.189 ng

RT: 23.176 min Scan# 2337





Delta R.T. -0.000 min

Lab File: BN015855.D

Acq: 12 Aug 2021 08:38

Tgt Ion:	252	Resp:	32506
Ion	Ratio	Lower	Upper
252	100		
253	23.4	18.2	27.2
125	8.8	6.2	9.4

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



#38

Benzo(k)fluoranthene

Concen: 0.200 ng




RT: 23.224 min Scan# 2351


Delta R.T. -0.000 min

Lab File: BN015855.D

Acq: 12 Aug 2021 08:38

Tgt Ion:	252	Resp:	31957
Ion	Ratio	Lower	Upper
252	100		
253	23.1	18.1	27.1
125	7.6	5.6	8.4




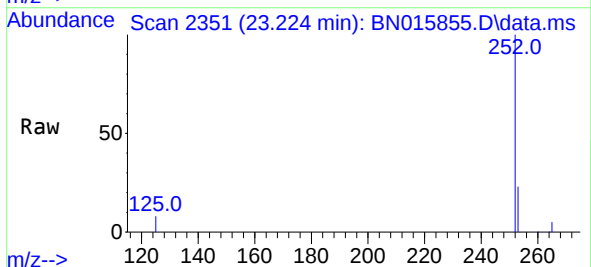




#39
Benzo(a)pyrene
Concen: 0.186 ng
RT: 23.810 min Scan# 2522
Delta R.T. -0.000 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:252	Resp:	27723
Ion Ratio	Lower	Upper
252	100	
253	24.3	18.6 27.8
125	10.5	7.3 10.9

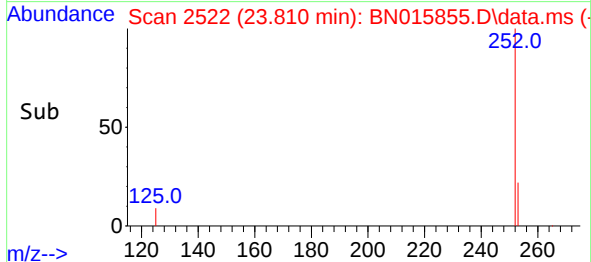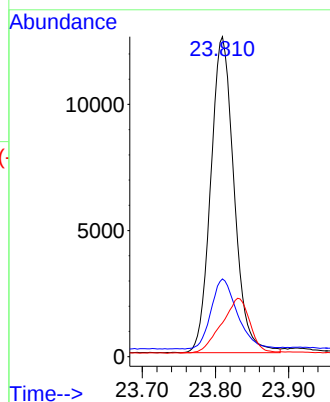

#40
Dibenzo(a,h)anthracene
Concen: 0.179 ng
RT: 26.455 min Scan# 3295
Delta R.T. 0.003 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Tgt Ion:278	Resp:	24504
Ion Ratio	Lower	Upper
278	100	
139	16.9	10.2 15.2#
279	25.5	19.5 29.3

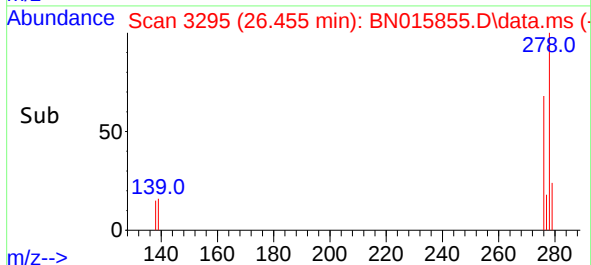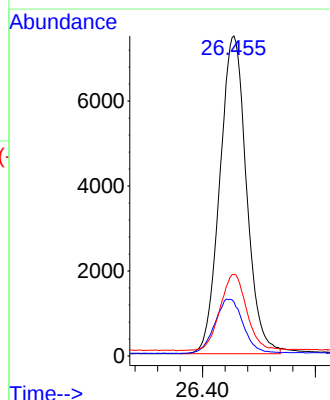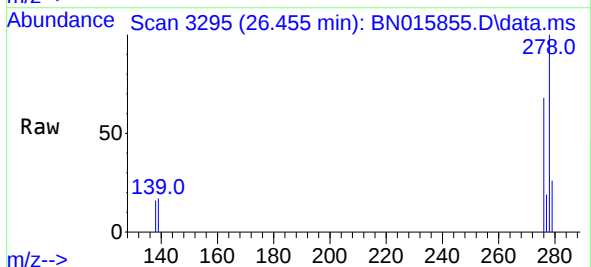

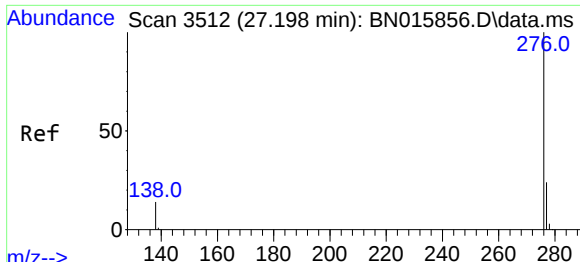

#41
Benzo(g,h,i)perylene
Concen: 0.179 ng
RT: 27.202 min Scan# 3513
Delta R.T. 0.003 min
Lab File: BN015855.D
Acq: 12 Aug 2021 08:38

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	276	Resp:	26709
Ion	Ratio	Lower	Upper
276	100		
277	24.7	19.5	29.3
138	15.2	11.8	17.8

