

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
 Data File : BN015861.D
 Acq On : 12 Aug 2021 13:30
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN081221

Quant Time: Aug 12 14:19:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 12 12:21:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	8578	0.400	ng	0.00
7) Naphthalene-d8	10.723	136	42306	0.400	ng	# 0.00
13) Acenaphthene-d10	14.560	164	24804	0.400	ng	0.01
19) Phenanthrene-d10	17.309	188	50336	0.400	ng	# 0.01
29) Chrysene-d12	21.503	240	57137	0.400	ng	# 0.01
35) Perylene-d12	23.936	264	52953	0.400	ng	0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.494	112	8404	0.396	ng	0.00
5) Phenol-d6	7.080	99	11437	0.397	ng	0.00
8) Nitrobenzene-d5	9.076	82	13101	0.370	ng	0.00
11) 2-Methylnaphthalene-d10	12.314	152	26798	0.393	ng	0.00
14) 2,4,6-Tribromophenol	16.044	330	3595	0.329	ng	0.00
15) 2-Fluorobiphenyl	13.190	172	36548	0.374	ng	0.01
27) Fluoranthene-d10	19.341	212	58641	0.378	ng	0.00
31) Terphenyl-d14	19.936	244	63238	0.390	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.410	88	1361	0.403	ng	97
3) n-Nitrosodimethylamine	3.779	42	3461	0.396	ng	# 99
6) bis(2-Chloroethyl)ether	7.347	93	9399	0.411	ng	100
9) Naphthalene	10.774	128	42905	0.393	ng	100
10) Hexachlorobutadiene	11.065	225	11723	0.393	ng	# 100
12) 2-Methylnaphthalene	12.389	142	31204	0.414	ng	100
16) Acenaphthylene	14.281	152	37746	0.377	ng	100
17) Acenaphthene	14.624	154	26288	0.380	ng	99
18) Fluorene	15.601	166	32624	0.378	ng	99
20) 4,6-Dinitro-2-methylph...	15.677	198	1343	0.420	ng	95
21) 4-Bromophenyl-phenylether	16.494	248	9996	0.366	ng	# 89
22) Hexachlorobenzene	16.616	284	13660	0.383	ng	100
23) Atrazine	16.762	200	7979	0.354	ng	98
24) Pentachlorophenol	16.956	266	4110	0.317	ng	100
25) Phenanthrene	17.346	178	52559	0.381	ng	99
26) Anthracene	17.431	178	45743	0.372	ng	100
28) Fluoranthene	19.370	202	64409	0.386	ng	100
30) Pyrene	19.733	202	64079	0.377	ng	100
32) Benzo(a)anthracene	21.482	228	68101	0.378	ng	99
33) Chrysene	21.535	228	69447	0.386	ng	100
34) Bis(2-ethylhexyl)phtha...	21.418	149	24951	0.334	ng	100
36) Indeno(1,2,3-cd)pyrene	26.448	276	65180	0.368	ng	100
37) Benzo(b)fluoranthene	23.193	252	69046	0.378	ng	100
38) Benzo(k)fluoranthene	23.241	252	67077	0.391	ng	100
39) Benzo(a)pyrene	23.826	252	58618	0.373	ng	100
40) Dibenzo(a,h)anthracene	26.469	278	53897	0.371	ng	99
41) Benzo(g,h,i)perylene	27.225	276	56042	0.366	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
Data File : BN015861.D
Acq On : 12 Aug 2021 13:30
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN081221

Quant Time: Aug 12 14:19:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 12 12:21:27 2021
Response via : Initial Calibration




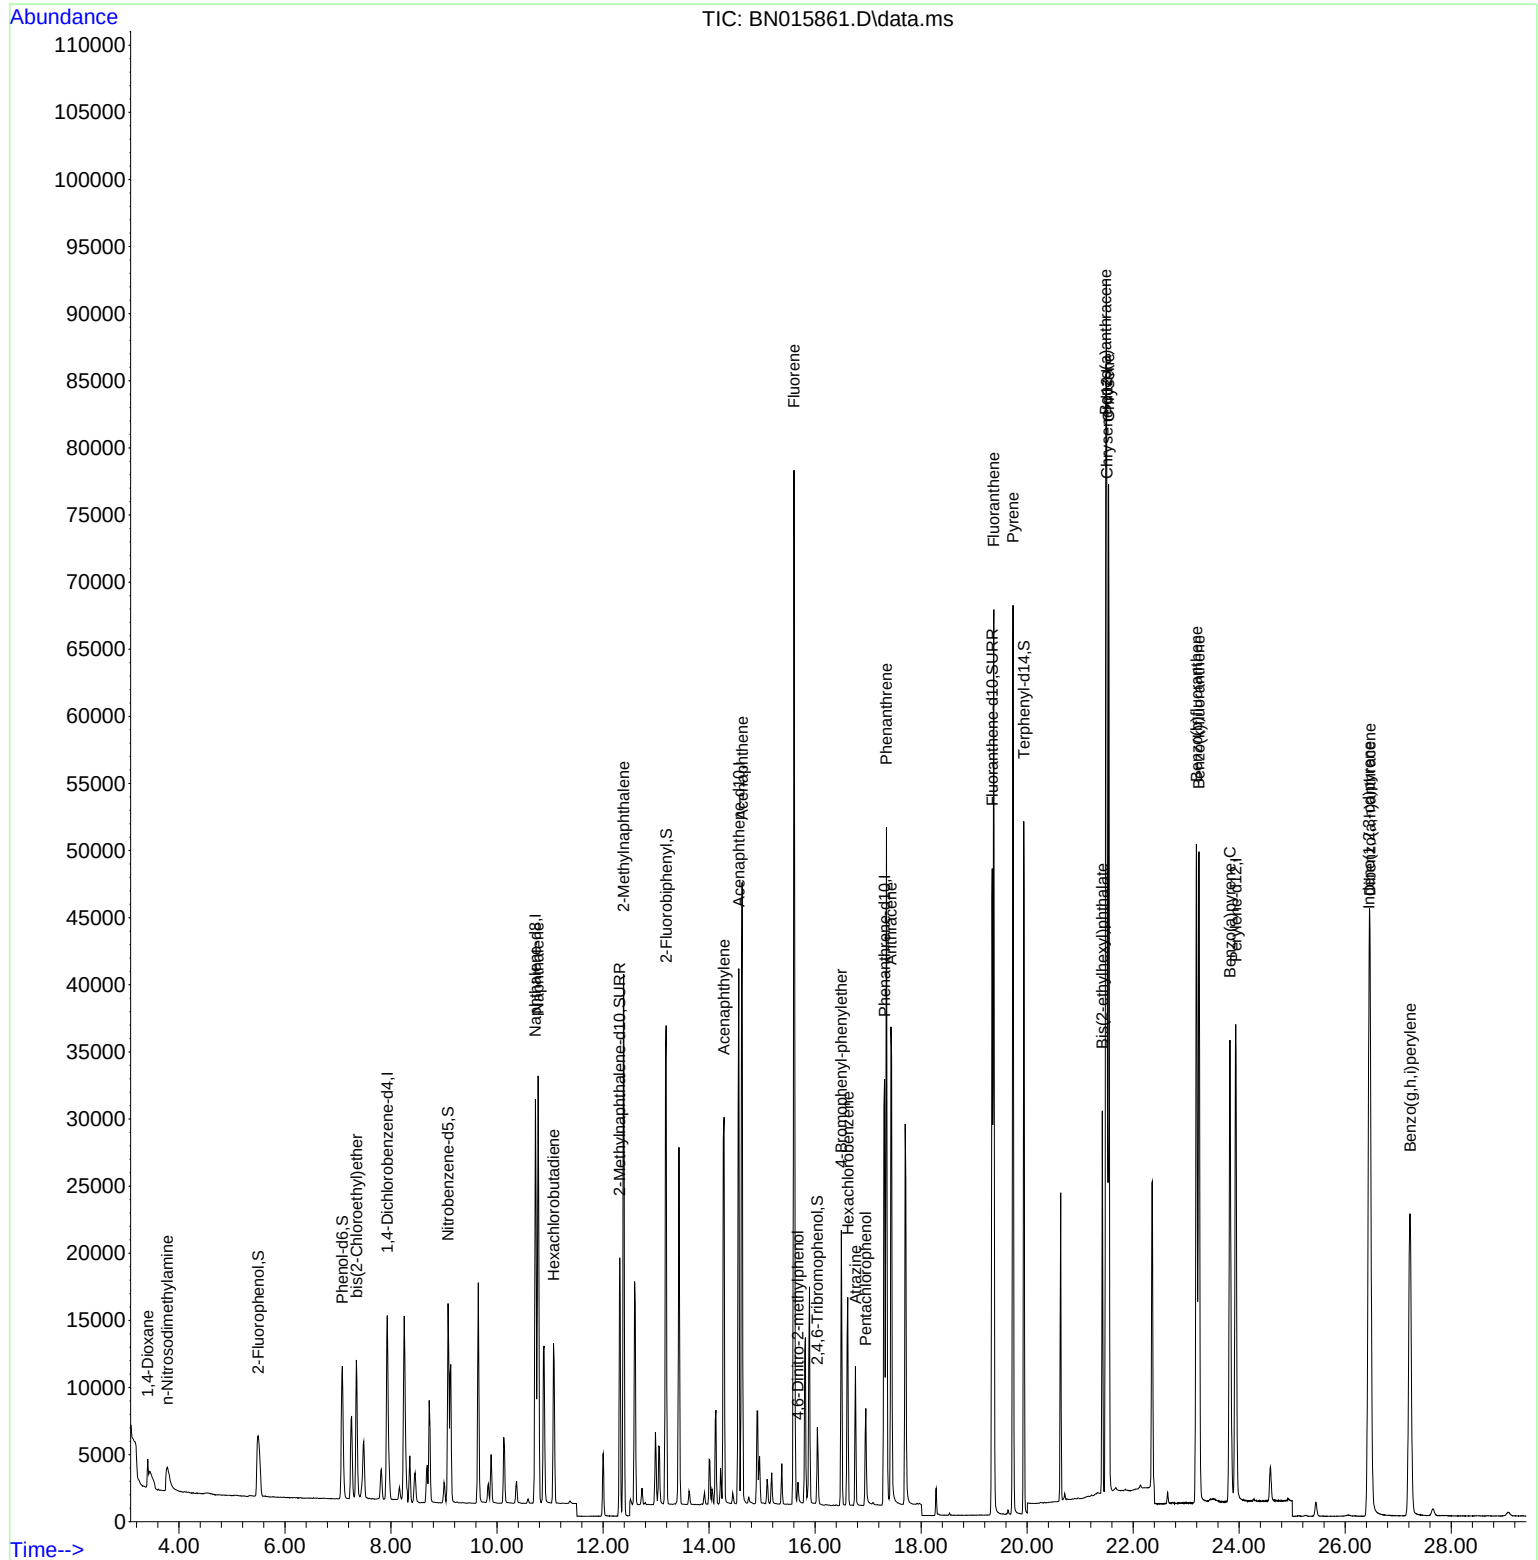




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.928 min Scan# 526
Delta R.T. 0.009 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:152 Resp: 8578
Ion Ratio Lower Upper
152 100
150 153.4 125.8 188.8
115 64.5 53.6 80.4

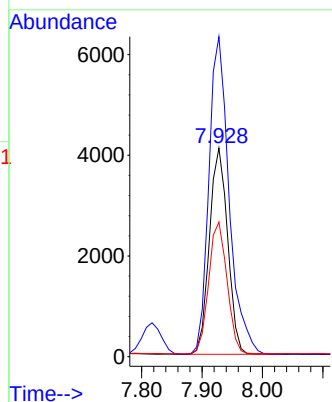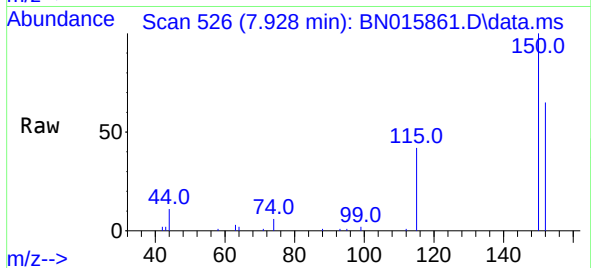

#2
1,4-Dioxane
Concen: 0.403 ng
RT: 3.410 min Scan# 36
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion: 88 Resp: 1361
Ion Ratio Lower Upper
88 100
43 35.6 29.4 44.2
58 83.3 69.3 103.9









#3
n-Nitrosodimethylamine
Concen: 0.396 ng
RT: 3.779 min Scan# 76
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion: 42 Resp: 3461
Ion Ratio Lower Upper
42 100
74 108.5 86.1 129.1
44 3.6 3.8 5.8#

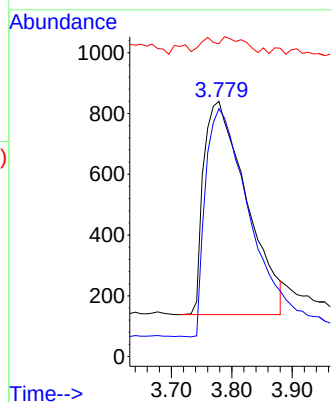

#4
2-Fluorophenol
Concen: 0.396 ng
RT: 5.494 min Scan# 262
Delta R.T. 0.009 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion: 112 Resp: 8404
Ion Ratio Lower Upper
112 100
64 67.3 53.3 79.9
63 35.6 28.6 42.8


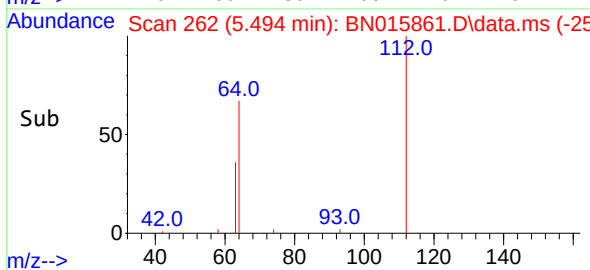
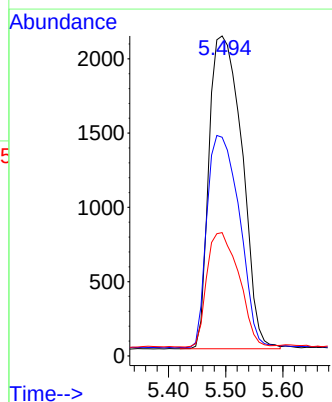



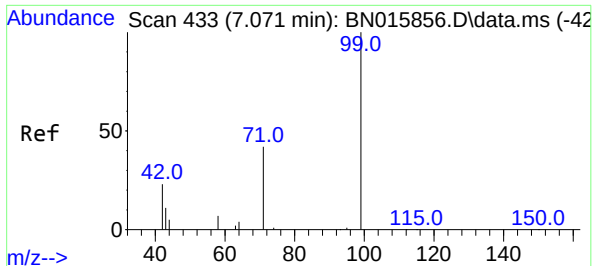

#5
Phenol-d6
Concen: 0.397 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.009 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion: 99 Resp: 11437
Ion Ratio Lower Upper
99 100
42 22.9 18.7 28.1
71 40.7 32.4 48.6

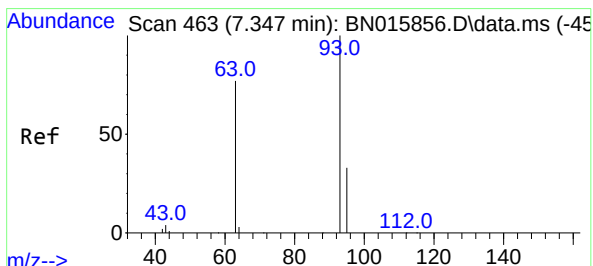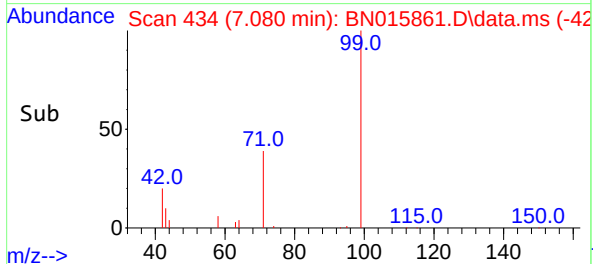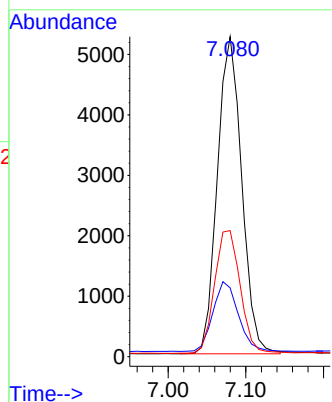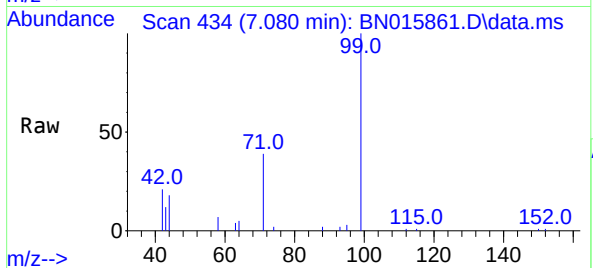

#6
bis(2-Chloroethyl)ether
Concen: 0.411 ng
RT: 7.347 min Scan# 463
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion: 93 Resp: 9399
Ion Ratio Lower Upper
93 100
63 79.8 63.8 95.6
95 33.0 26.0 39.0


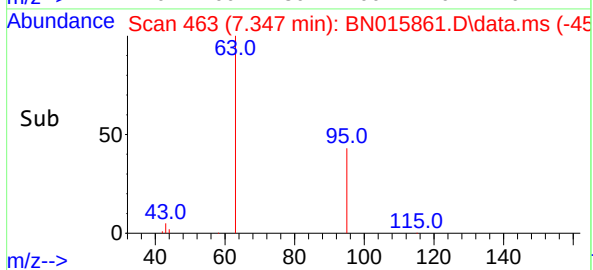

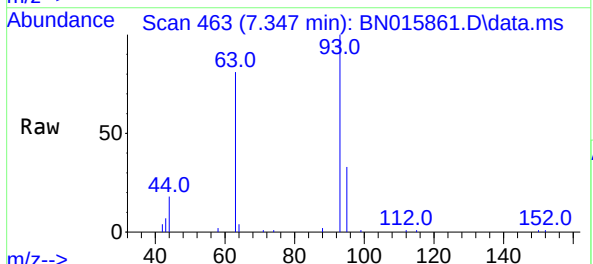




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.723 min Scan# 758
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:	136	Resp:	42306
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.0	13.4
54	8.9	5.4	8.2#
68	5.9	3.8	5.8#



#8
Nitrobenzene-d5
Concen: 0.370 ng
RT: 9.076 min Scan# 628
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:	82	Resp:	13101
Ion	Ratio	Lower	Upper
82	100		
128	32.8	29.2	43.8
54	56.4	41.1	61.7









#9
Naphthalene
Concen: 0.393 ng
RT: 10.774 min Scan# 762
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:	128	Resp:	42905
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.8	13.2
127	13.3	10.5	15.7

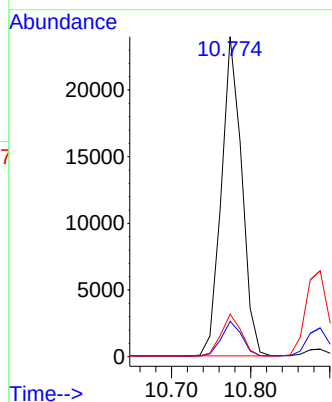

#10
Hexachlorobutadiene
Concen: 0.393 ng
RT: 11.065 min Scan# 785
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:	225	Resp:	11723
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.0	51.4	77.0


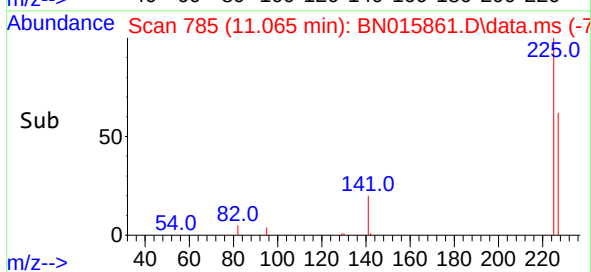






#11
2-Methylnaphthalene-d10
Concen: 0.393 ng
RT: 12.314 min Scan# 1001
Delta R.T. 0.004 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:152 Resp: 26798
Ion Ratio Lower Upper
152 100
151 20.5 16.5 24.7

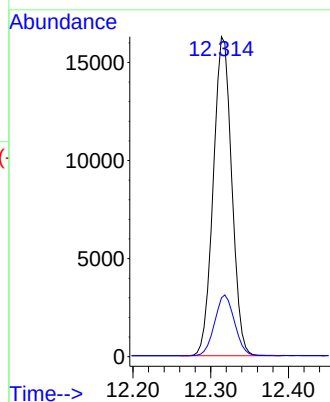

#12
2-Methylnaphthalene
Concen: 0.414 ng
RT: 12.389 min Scan# 1018
Delta R.T. 0.004 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:142 Resp: 31204
Ion Ratio Lower Upper
142 100
141 87.6 70.5 105.7
115 37.2 29.8 44.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.560 min Scan# 1206
Delta R.T. 0.012 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:164 Resp: 24804
Ion Ratio Lower Upper
164 100
162 100.7 83.5 125.3
160 43.9 37.7 56.5



#14
2,4,6-Tribromophenol
Concen: 0.329 ng
RT: 16.044 min Scan# 1323
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:330 Resp: 3595
Ion Ratio Lower Upper
330 100
332 108.5 84.1 126.1
141 29.7 24.2 36.4









#15
2-Fluorobiphenyl
Concen: 0.374 ng
RT: 13.190 min Scan# 1098
Delta R.T. 0.012 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:172 Resp: 36548
Ion Ratio Lower Upper
172 100
171 34.0 28.7 43.1
170 21.4 19.0 28.4



#16
Acenaphthylene
Concen: 0.377 ng
RT: 14.281 min Scan# 1184
Delta R.T. 0.012 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:152 Resp: 37746
Ion Ratio Lower Upper
152 100
151 19.5 15.4 23.2
153 13.0 10.5 15.7


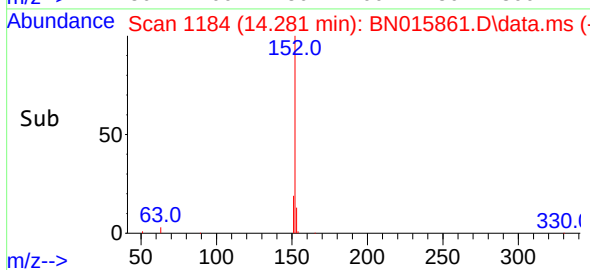




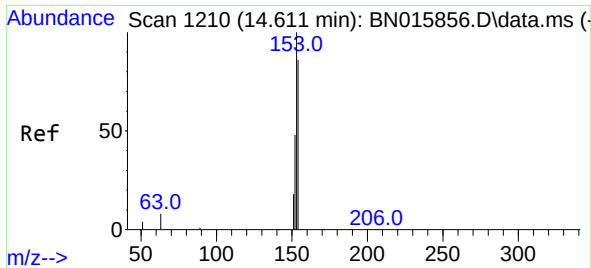

#17
Acenaphthene
Concen: 0.380 ng
RT: 14.624 min Scan# 1211
Delta R.T. 0.012 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:154 Resp: 26288
Ion Ratio Lower Upper
154 100
153 112.1 90.1 135.1
152 53.4 43.5 65.3

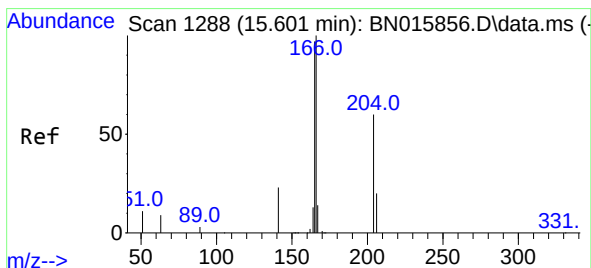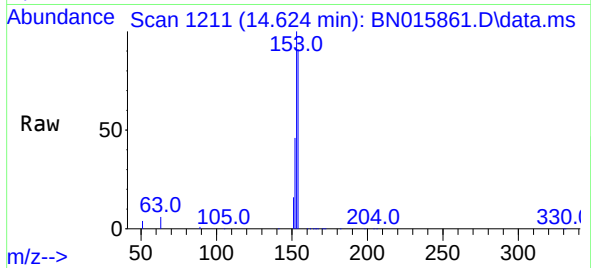

#18
Fluorene
Concen: 0.378 ng
RT: 15.601 min Scan# 1288
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:166 Resp: 32624
Ion Ratio Lower Upper
166 100
165 98.4 77.8 116.6
167 13.6 11.0 16.4




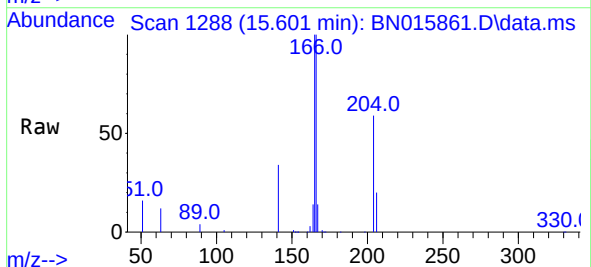




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.309 min Scan# 1427
Delta R.T. 0.012 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:188 Resp: 50336
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 5.8 7.2 10.8#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.420 ng
RT: 15.677 min Scan# 1294
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:198 Resp: 1343
Ion Ratio Lower Upper
198 100
182 12.9 11.9 17.9
77 0.0 0.0 0.0


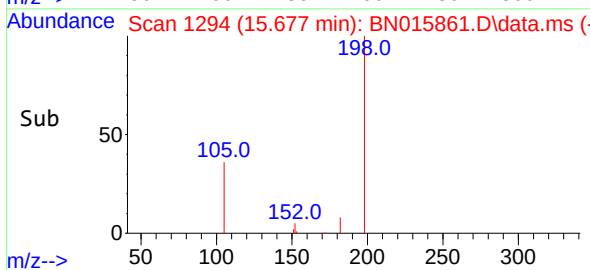






#21
4-Bromophenyl-phenylether
Concen: 0.366 ng
RT: 16.494 min Scan# 1360
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:248 Resp: 9996
Ion Ratio Lower Upper
248 100
250 96.0 78.6 118.0
141 73.0 43.4 65.2#



#22
Hexachlorobenzene
Concen: 0.383 ng
RT: 16.616 min Scan# 1370
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:284 Resp: 13660
Ion Ratio Lower Upper
284 100
142 28.2 22.6 34.0
249 31.9 25.2 37.8


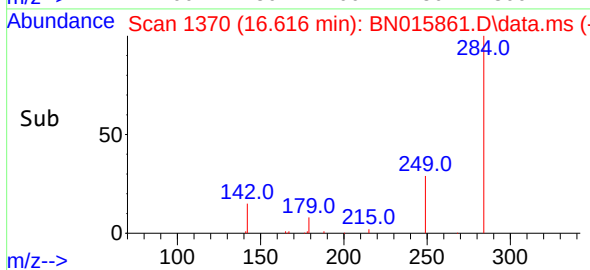






#23
Atrazine
Concen: 0.354 ng
RT: 16.762 min Scan# 1382
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:	200	Resp:	7979
Ion	Ratio	Lower	Upper
200	100		
173	22.7	16.4	24.6
215	51.4	41.5	62.3



#24
Pentachlorophenol
Concen: 0.317 ng
RT: 16.956 min Scan# 1398
Delta R.T. -0.001 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:	266	Resp:	4110
Ion	Ratio	Lower	Upper
266	100		
264	62.9	50.1	75.1
268	64.2	51.0	76.6









#25
Phenanthrene
Concen: 0.381 ng
RT: 17.346 min Scan# 1430
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:178 Resp: 52559
Ion Ratio Lower Upper
178 100
176 18.5 14.6 21.8
179 15.9 12.6 18.8



#26
Anthracene
Concen: 0.372 ng
RT: 17.431 min Scan# 1437
Delta R.T. -0.000 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:178 Resp: 45743
Ion Ratio Lower Upper
178 100
176 17.8 14.3 21.5
179 15.4 12.2 18.4


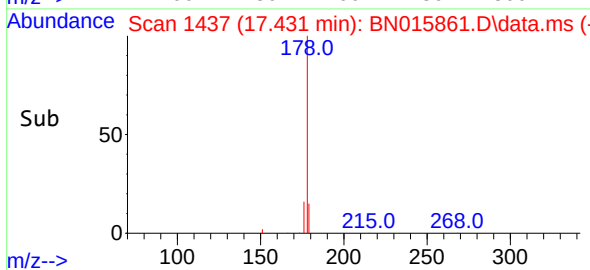






#27
Fluoranthene-d10
Concen: 0.378 ng
RT: 19.341 min Scan# 1752
Delta R.T. 0.005 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:212 Resp: 58641
Ion Ratio Lower Upper
212 100
106 9.4 7.4 11.2
104 5.4 4.3 6.5

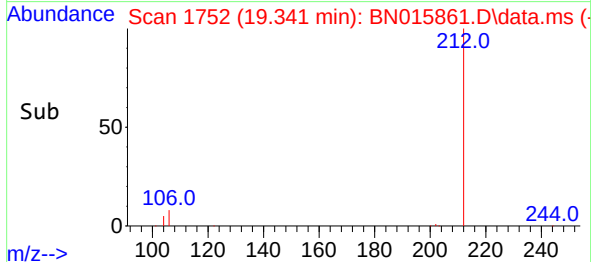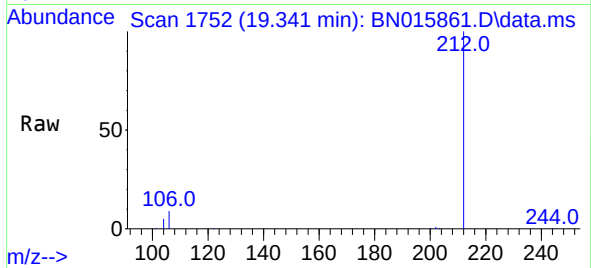

#28
Fluoranthene
Concen: 0.386 ng
RT: 19.370 min Scan# 1758
Delta R.T. 0.010 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:202 Resp: 64409
Ion Ratio Lower Upper
202 100
101 8.7 6.8 10.2
203 17.3 13.8 20.8









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.503 min Scan# 2027
Delta R.T. 0.010 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:240 Resp: 57137
Ion Ratio Lower Upper
240 100
120 6.0 3.8 5.8#
236 25.8 20.0 30.0



#30
Pyrene
Concen: 0.377 ng
RT: 19.733 min Scan# 1831
Delta R.T. 0.005 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:202 Resp: 64079
Ion Ratio Lower Upper
202 100
200 20.3 16.2 24.2
203 17.6 14.1 21.1







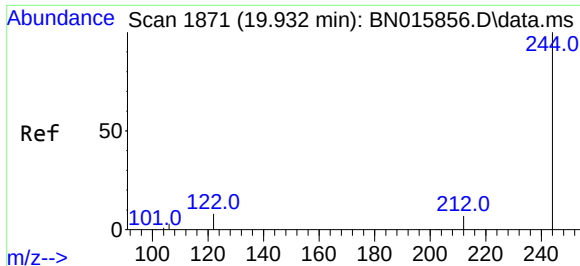

#31
Terphenyl-d14
Concen: 0.390 ng
RT: 19.936 min Scan# 1872
Delta R.T. 0.005 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:244 Resp: 63238
Ion Ratio Lower Upper
244 100
212 7.5 6.0 9.0
122 8.5 6.5 9.7

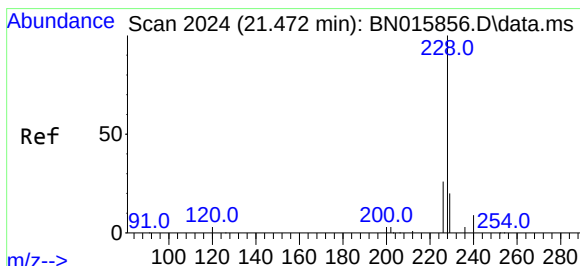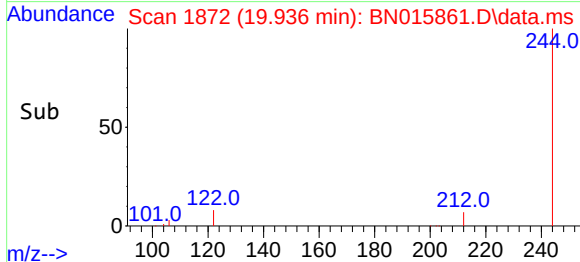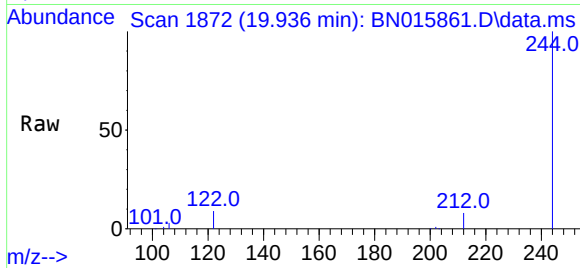

#32
Benzo(a)anthracene
Concen: 0.378 ng
RT: 21.482 min Scan# 2025
Delta R.T. 0.010 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:228 Resp: 68101
Ion Ratio Lower Upper
228 100
226 26.8 21.1 31.7
229 19.4 15.7 23.5


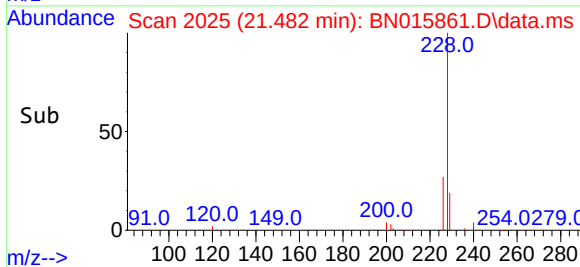

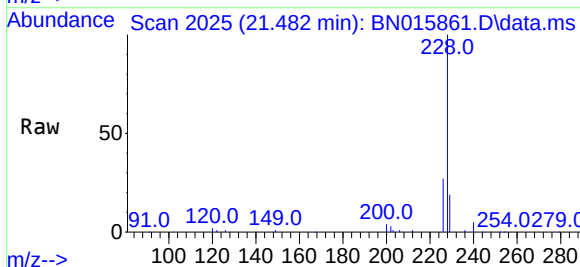


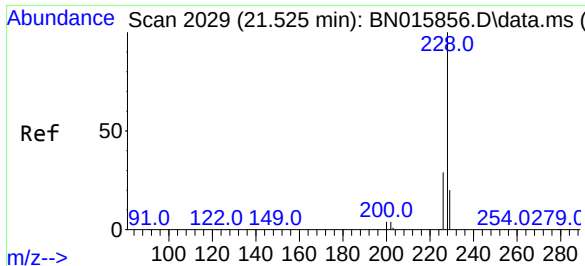

#33
Chrysene
Concen: 0.386 ng
RT: 21.535 min Scan# 2030
Delta R.T. 0.010 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:228	Resp: 69447
Ion Ratio	Lower Upper
228	100
226	29.6 23.4 35.2
229	19.6 15.8 23.6

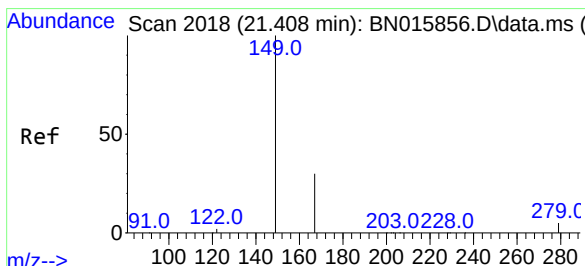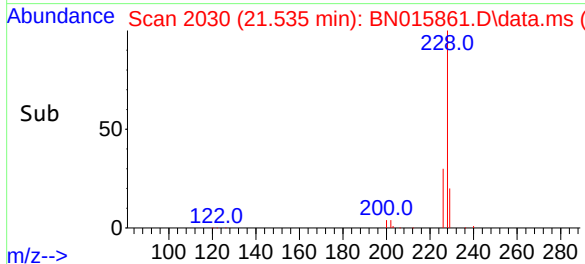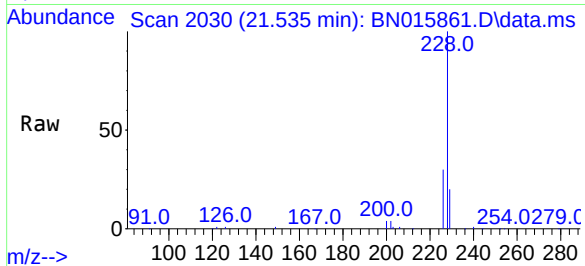

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.334 ng
RT: 21.418 min Scan# 2019
Delta R.T. 0.010 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30


Tgt Ion:149	Resp: 24951
Ion Ratio	Lower Upper
149	100
167	28.8 22.9 34.3
279	5.7 4.4 6.6

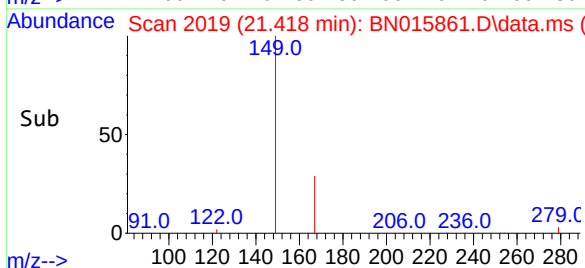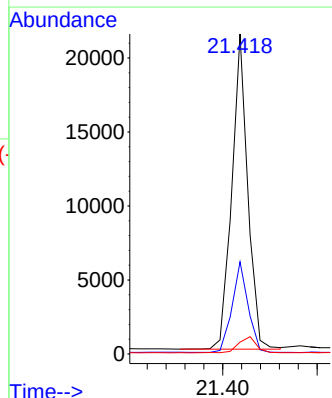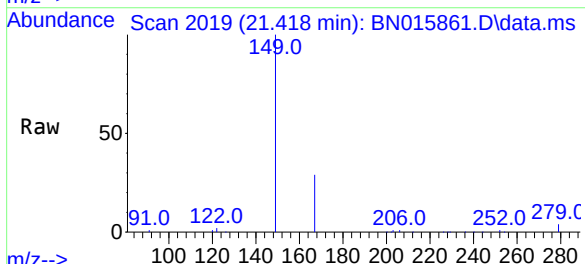






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.936 min Scan# 2559
Delta R.T. 0.020 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Instrument :
BNA_N
ClientSampleId :
ICVBN081221



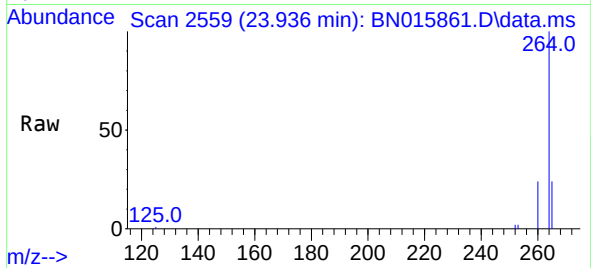



Tgt Ion:264 Resp: 52953
Ion Ratio Lower Upper
264 100
260 23.7 19.1 28.7
265 24.3 19.8 29.8

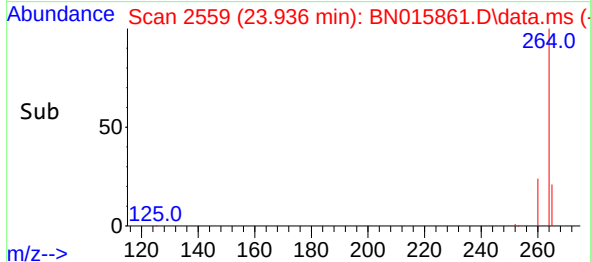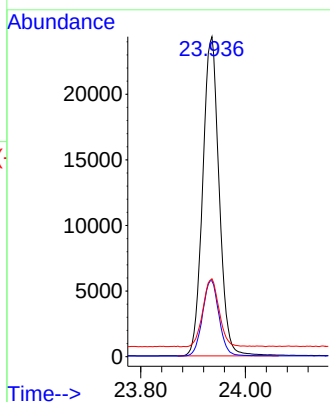

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.368 ng
RT: 26.448 min Scan# 3293
Delta R.T. 0.020 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:276 Resp: 65180
Ion Ratio Lower Upper
276 100
138 17.6 13.8 20.8
277 25.4 20.3 30.5




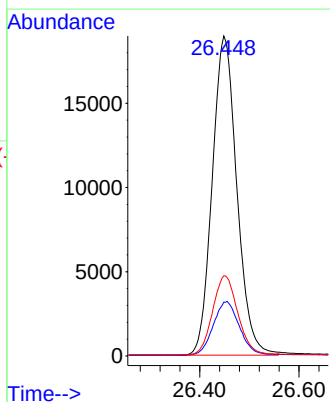




#37
Benzo(b)fluoranthene
Concen: 0.378 ng
RT: 23.193 min Scan# 2342
Delta R.T. 0.017 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:252 Resp: 69046
Ion Ratio Lower Upper
252 100
253 22.6 18.2 27.2
125 7.8 6.2 9.4

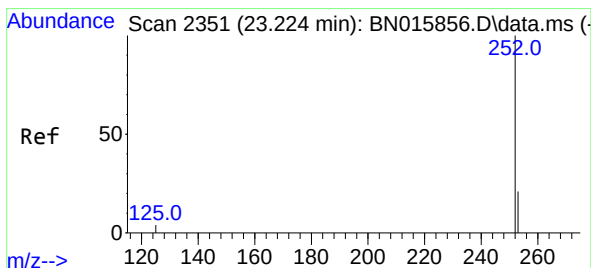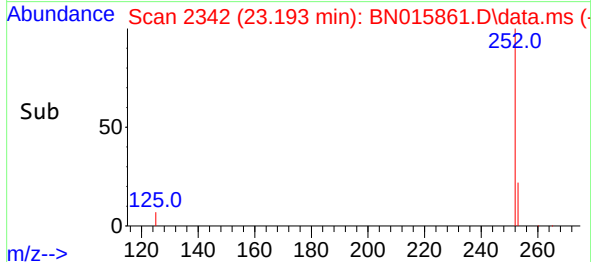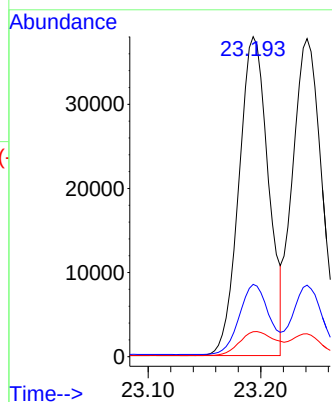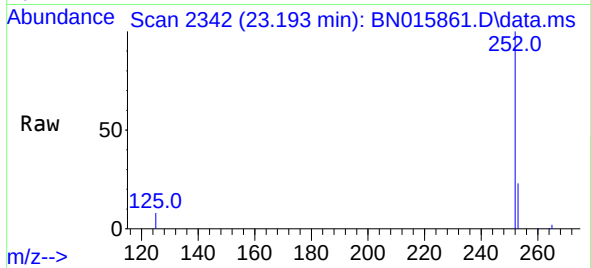

#38
Benzo(k)fluoranthene
Concen: 0.391 ng
RT: 23.241 min Scan# 2356
Delta R.T. 0.017 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:252 Resp: 67077
Ion Ratio Lower Upper
252 100
253 22.5 18.1 27.1
125 7.2 5.6 8.4


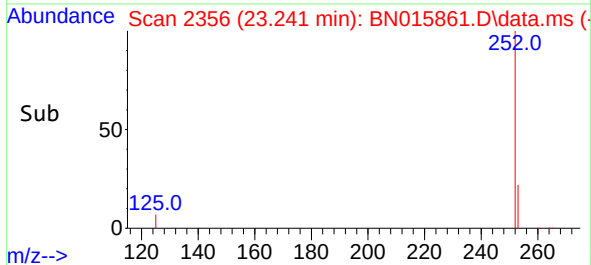
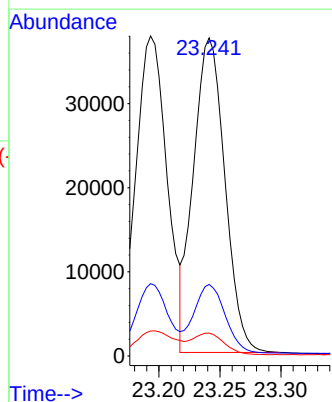
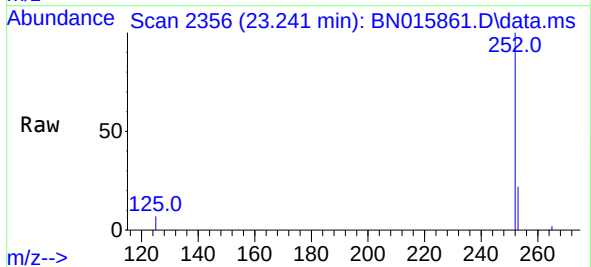




#39
Benzo(a)pyrene
Concen: 0.373 ng
RT: 23.826 min Scan# 2527
Delta R.T. 0.017 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30




Instrument :
BNA_N
ClientSampleId :
ICVBN081221


Tgt Ion:252	Resp:	58618
Ion Ratio	Lower	Upper
252	100	
253	23.1	18.6 27.8
125	9.1	7.3 10.9



#40
Dibenzo(a,h)anthracene
Concen: 0.371 ng
RT: 26.469 min Scan# 3299
Delta R.T. 0.017 min
Lab File: BN015861.D
Acq: 12 Aug 2021 13:30

Tgt Ion:278	Resp:	53897
Ion Ratio	Lower	Upper
278	100	
139	13.4	10.2 15.2
279	24.0	19.5 29.3



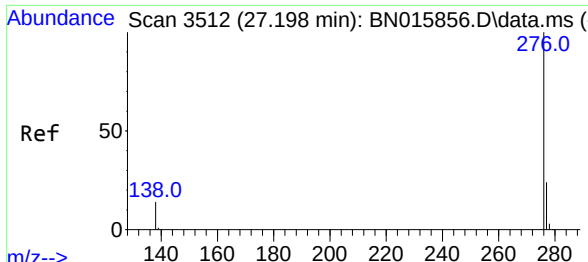

#41
 Benzo(g,h,i)perylene
 Concen: 0.366 ng
 RT: 27.225 min Scan# 3520
 Delta R.T. 0.027 min
 Lab File: BN015861.D
 Acq: 12 Aug 2021 13:30

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN081221

Tgt Ion:	276	Resp:	56042
Ion	Ratio	Lower	Upper
276	100		
277	23.8	19.5	29.3
138	14.5	11.8	17.8

