
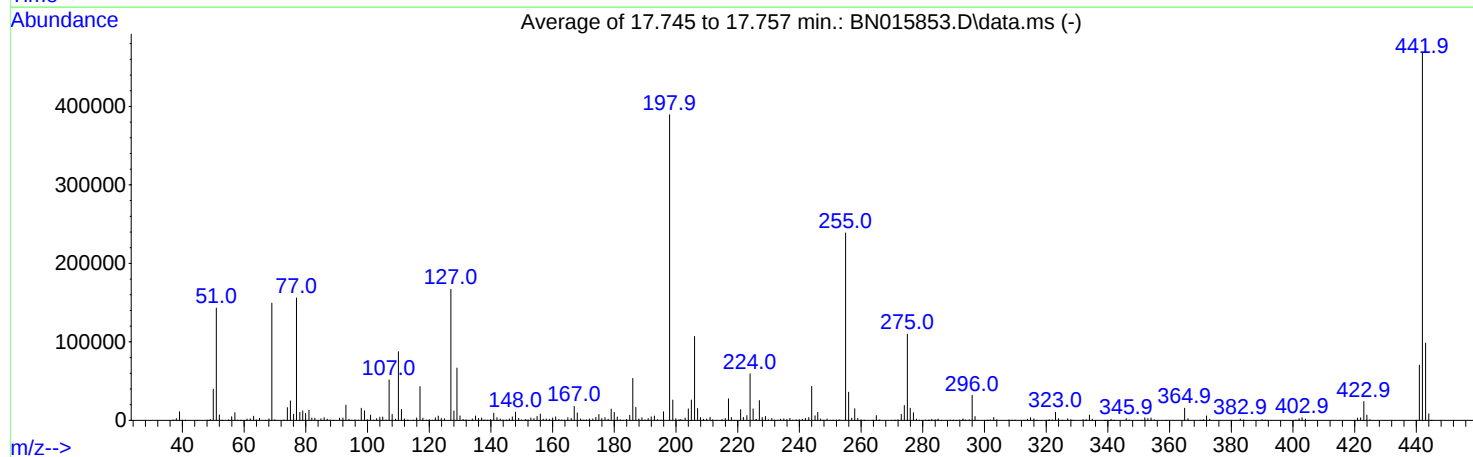


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
 Data File : BN015853.D
 Acq On : 12 Aug 2021 06:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 13 10:53:03 2021

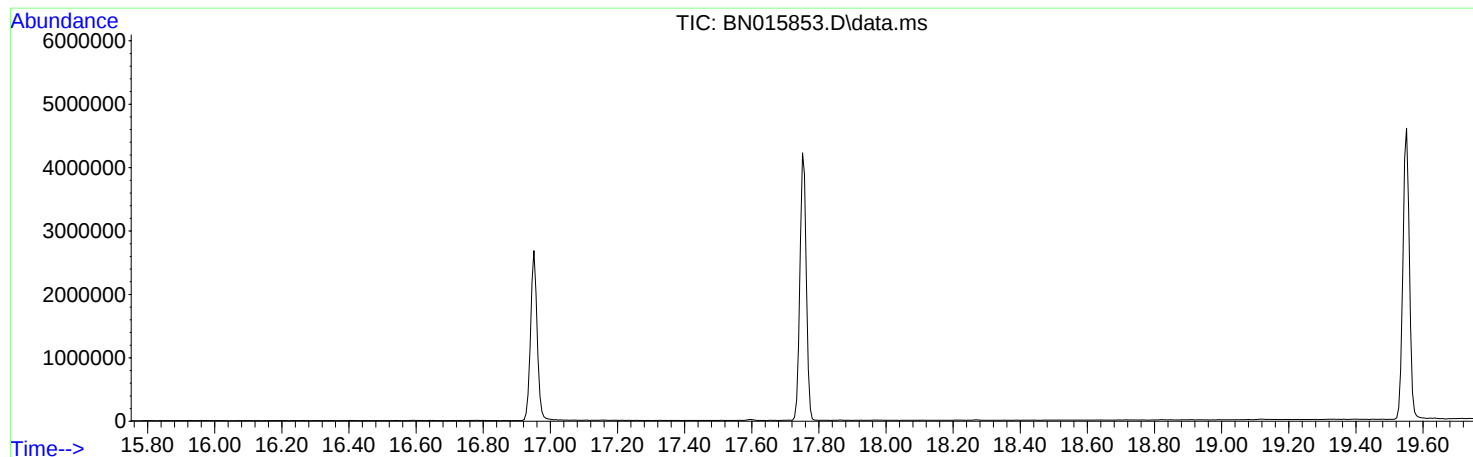




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	143019	PASS
68	69	0.00	2	1.4	2078	PASS
69	198	0.00	100	38.4	149483	PASS
70	69	0.00	2	0.6	870	PASS
127	198	10	80	42.9	167040	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	389333	PASS
199	198	5	9	6.7	25979	PASS
275	198	10	60	28.2	109699	PASS
365	198	1	100	4.0	15534	PASS
441	198	0.01	100	18.1	70352	PASS
442	442	50	100	100.0	468672	PASS
443	442	15	24	21.0	98437	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
 Data File : BN015853.D
 Acq On : 12 Aug 2021 06:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 12 10:13:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 11 11:23:50 2021
 Response via : Initial Calibration

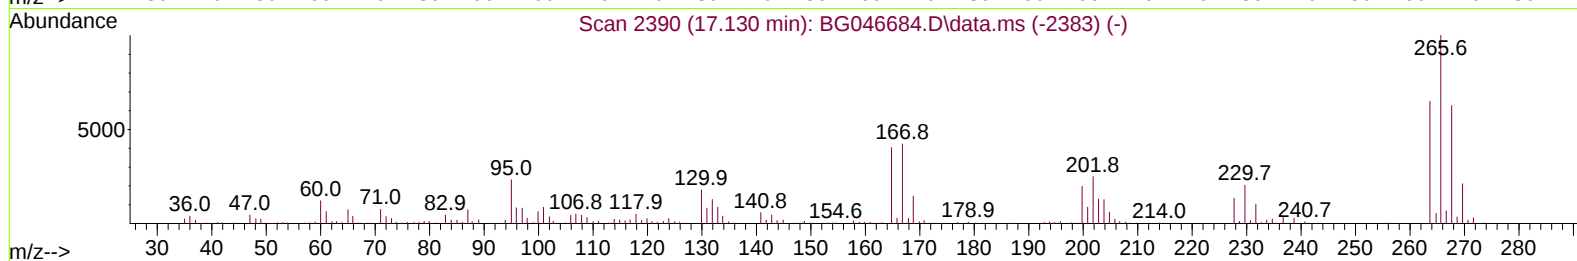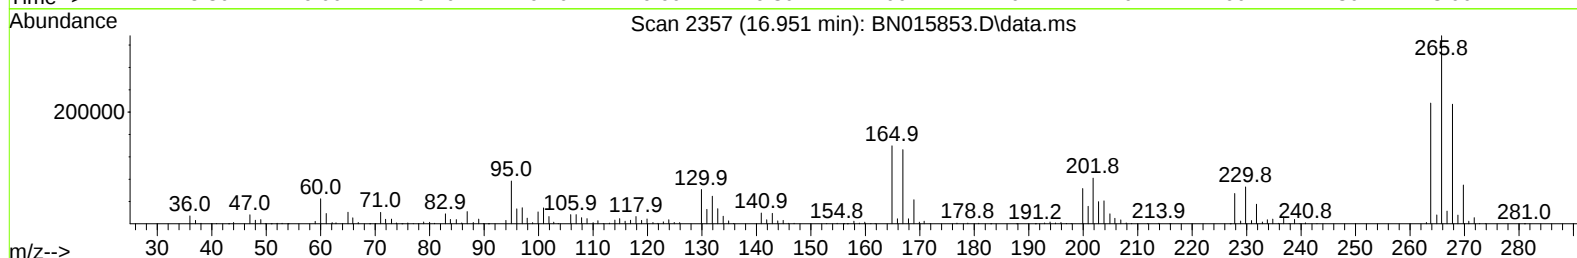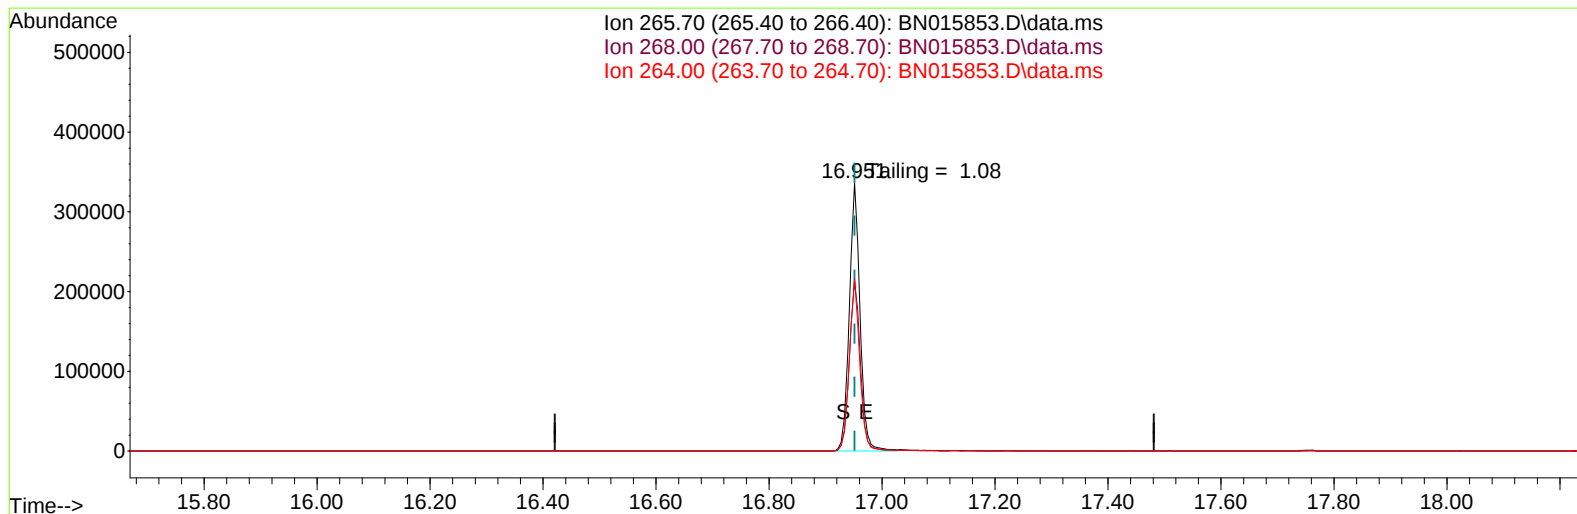

TIC: BN015853.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 21283.45 ng




response 443457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.57
264.00	61.60	64.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081221\
Data File : BN015853.D
Acq On : 12 Aug 2021 06:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 12 10:13:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 11 11:23:50 2021
Response via : Initial Calibration

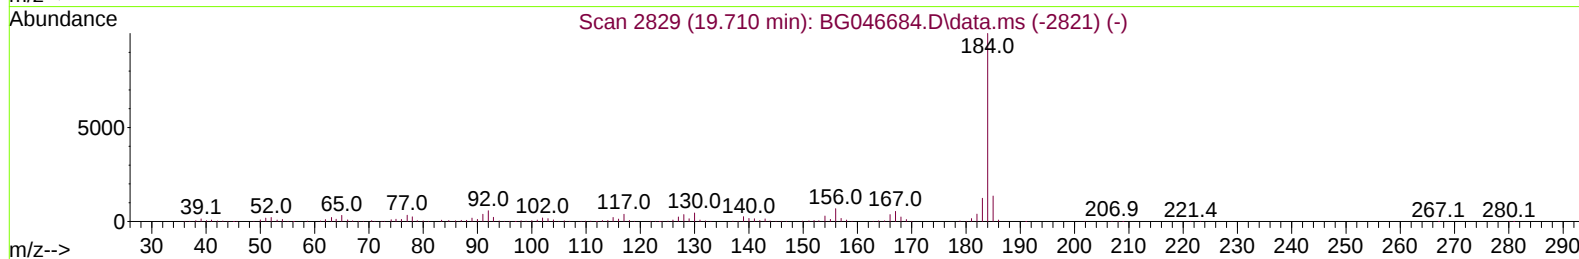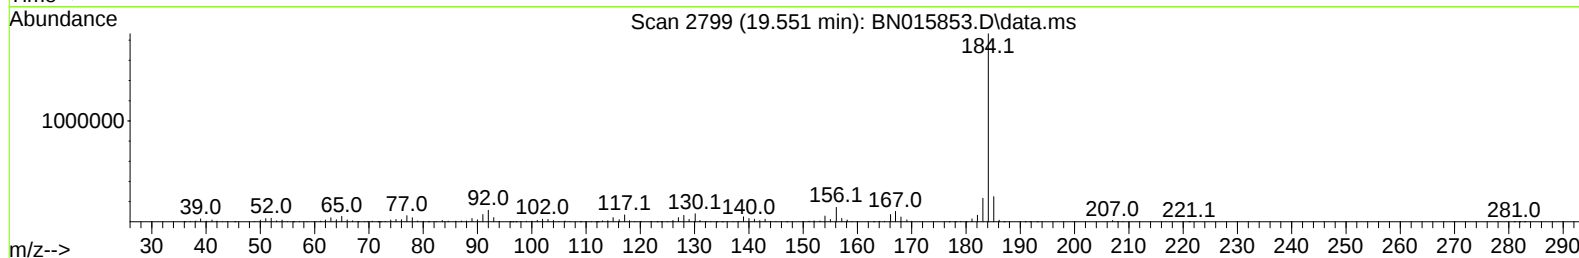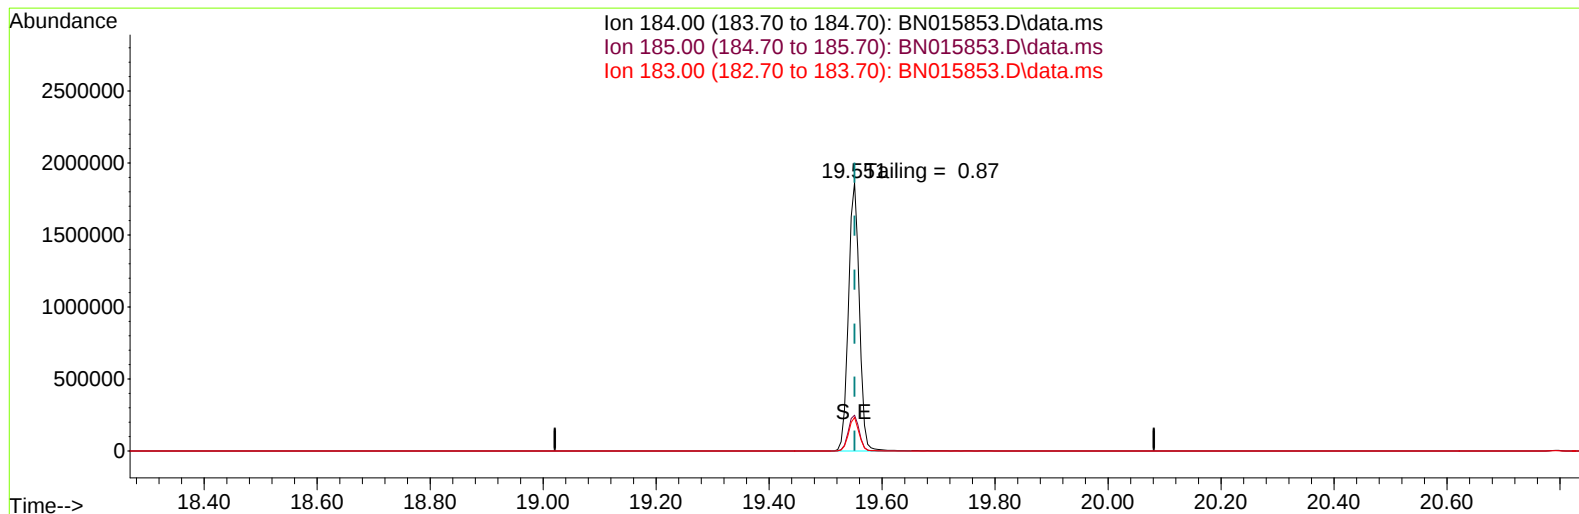

TIC: BN015853.D\data.ms

(77) Benzidine

19.551min (-0.000) 0.00 ng

response 2499021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.39
183.00	13.20	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/12/2021	BNA_N	<u>BN015853.D</u>
Compound Name	Response	Retention Time
DDT	1404546	20.792
DDD	15305	20.351
DDE	2096	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17401	1421947	1.22

Instrument :
BNA_N
ClientSampleId :
DFTPP