
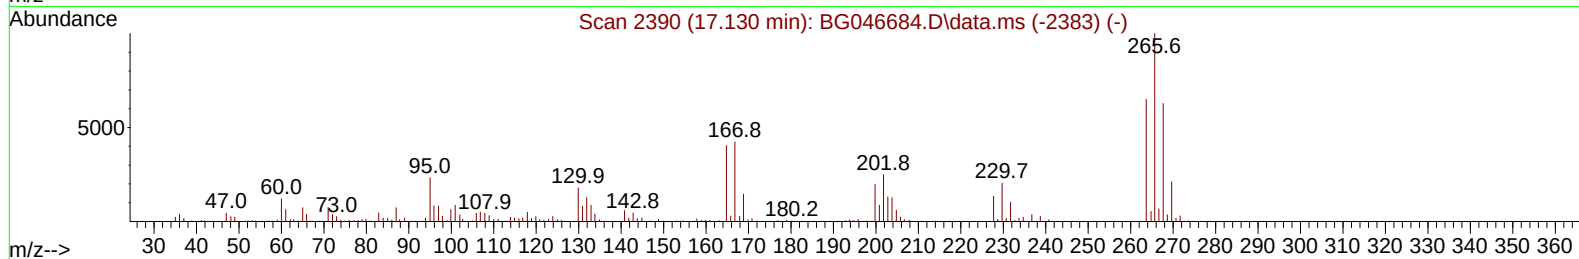
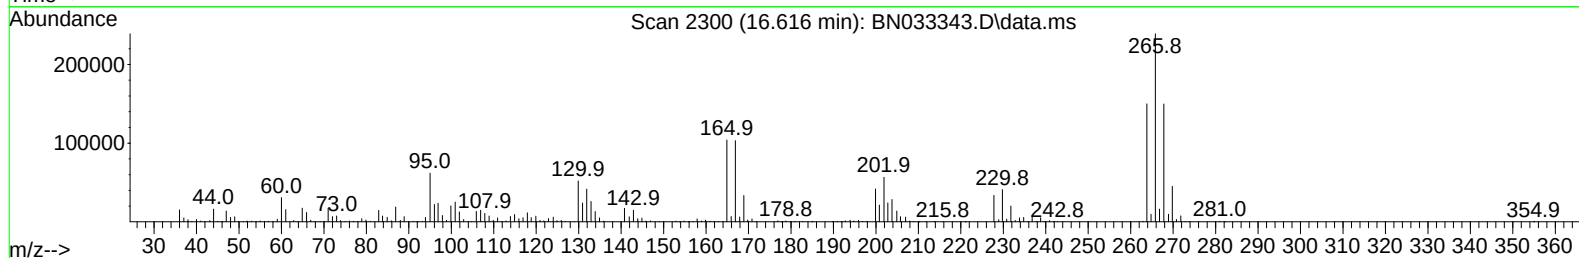


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081224\
Data File : BN033343.D
Acq On : 12 Aug 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 18:23:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

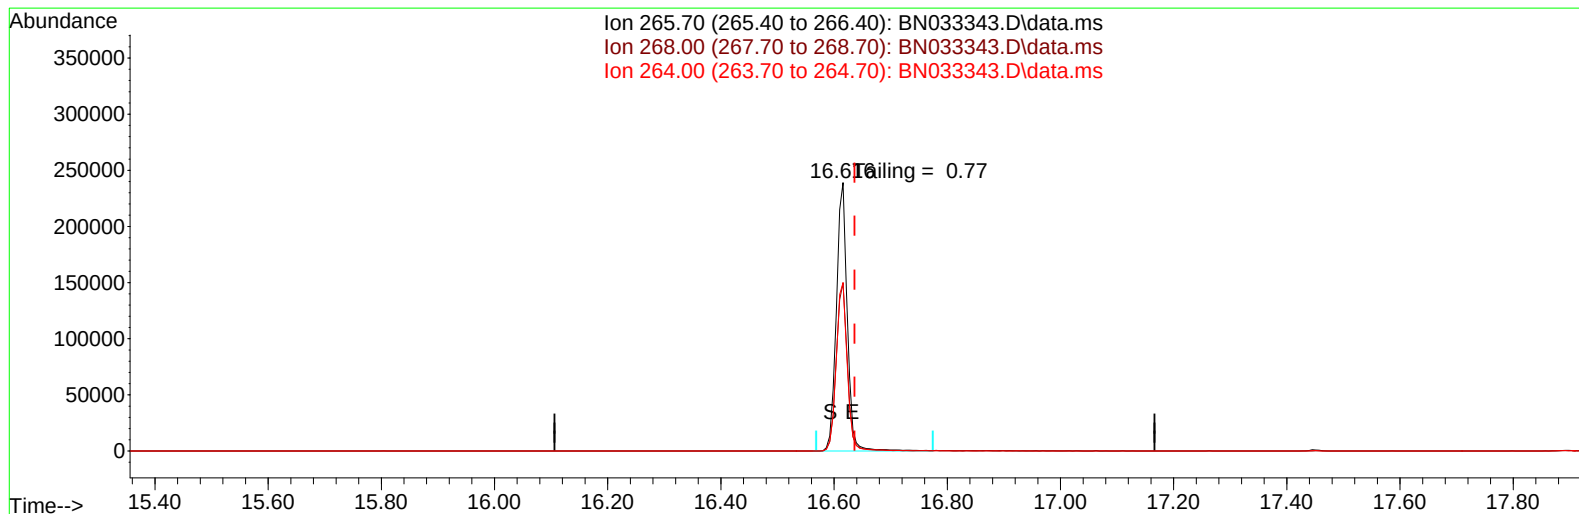

TIC: BN033343.D\data.ms

(70) Pentachlorophenol (C)




16.616min (-0.020) 19636.73 ng

response 321307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.68
264.00	61.60	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081224\
Data File : BN033343.D
Acq On : 12 Aug 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 18:23:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

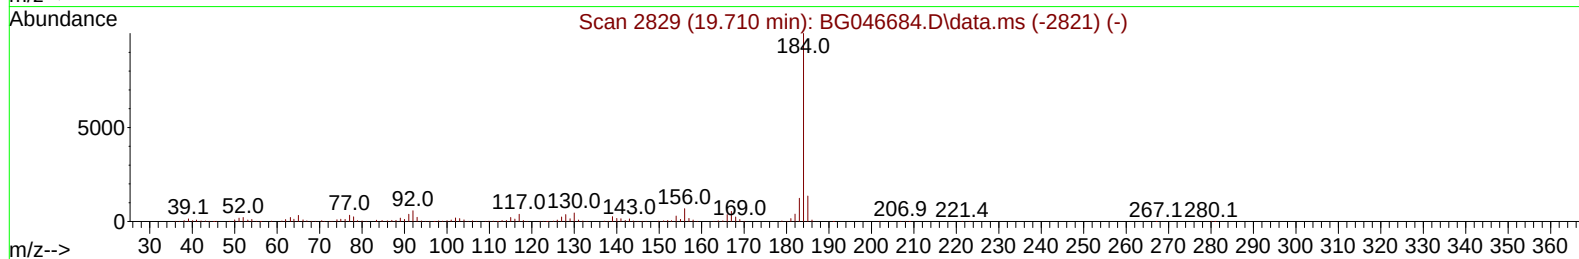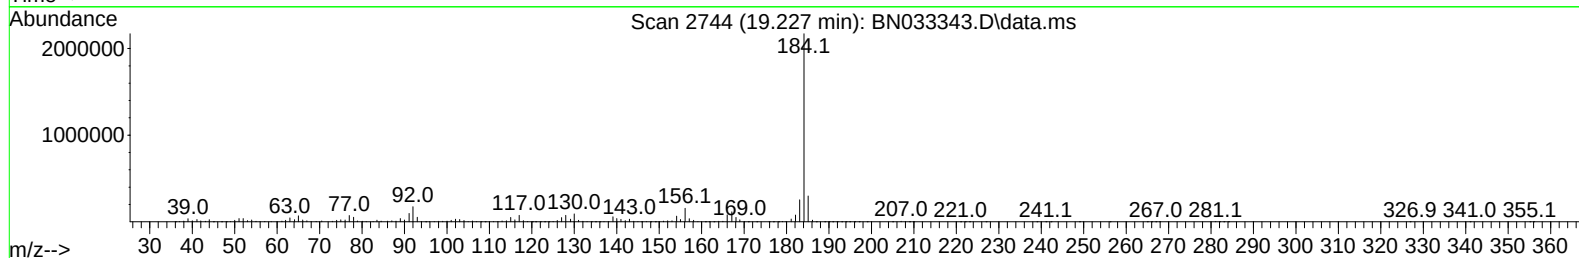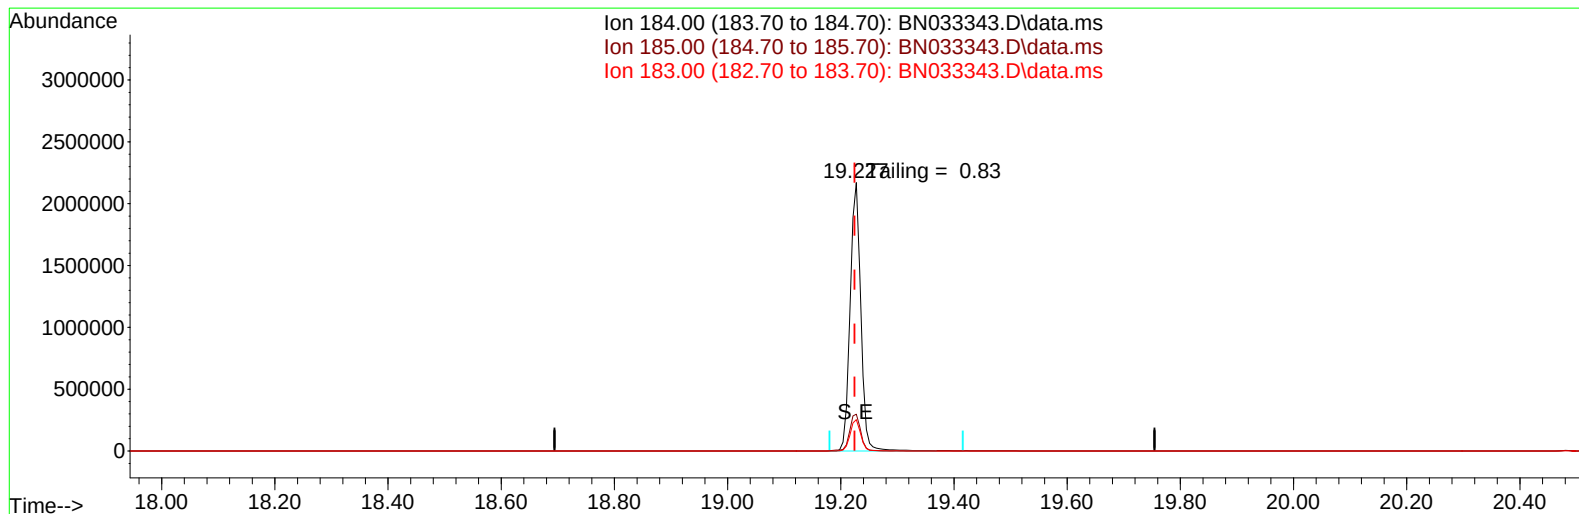

TIC: BN033343.D\data.ms

(77) Benzidine

19.227min (+ 0.003) 0.00 ng

response 2842000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	11.67
0.00	0.00	0.00