
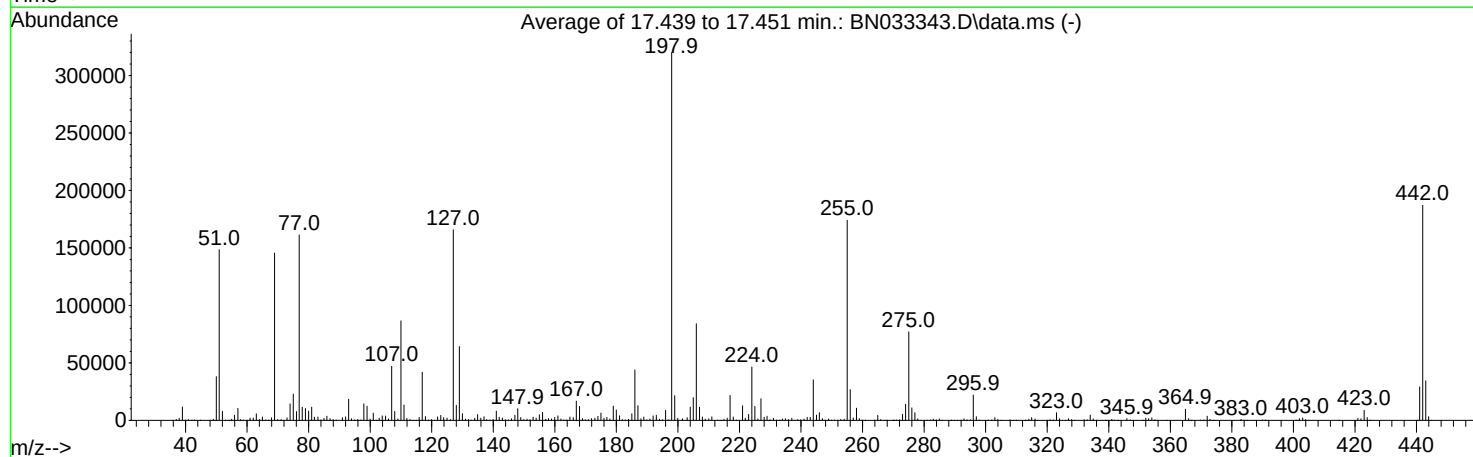


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081224\
Data File : BN033343.D
Acq On : 12 Aug 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 12 01:09:50 2024

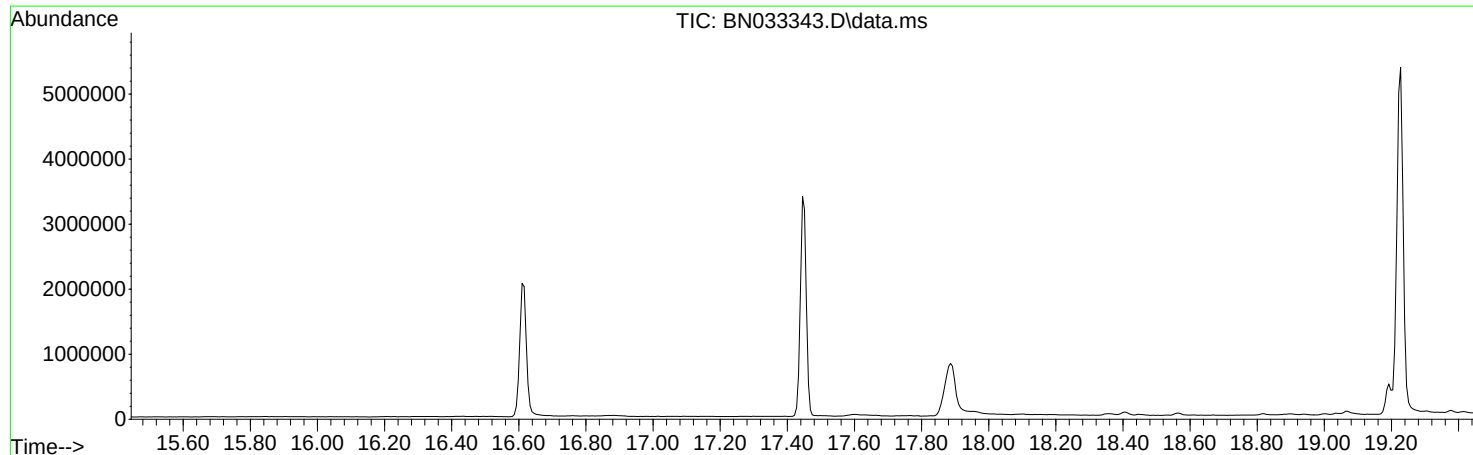

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	148602	PASS
68	69	0.00	2	1.6	2285	PASS
69	198	0.00	100	45.5	145661	PASS
70	69	0.00	2	0.5	742	PASS
127	198	10	80	51.8	165867	PASS
197	198	0.00	2	0.2	486	PASS
198	198	100	100	100.0	320043	PASS
199	198	5	9	6.7	21477	PASS
275	198	10	60	24.0	76968	PASS
365	198	1	100	3.0	9690	PASS
441	198	0.01	100	9.1	29096	PASS
442	442	50	100	100.0	187096	PASS
443	442	15	24	18.3	34331	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/12/2024	BNA_N	<u>BN033343.D</u>
Compound Name	Response	Retention Time
DDT	1207737	20.48
DDD	20186	20.039
DDE	510	19.533
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20696	1228433	1.68

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081224\
Data File : BN033343.D
Acq On : 12 Aug 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 12 18:23:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

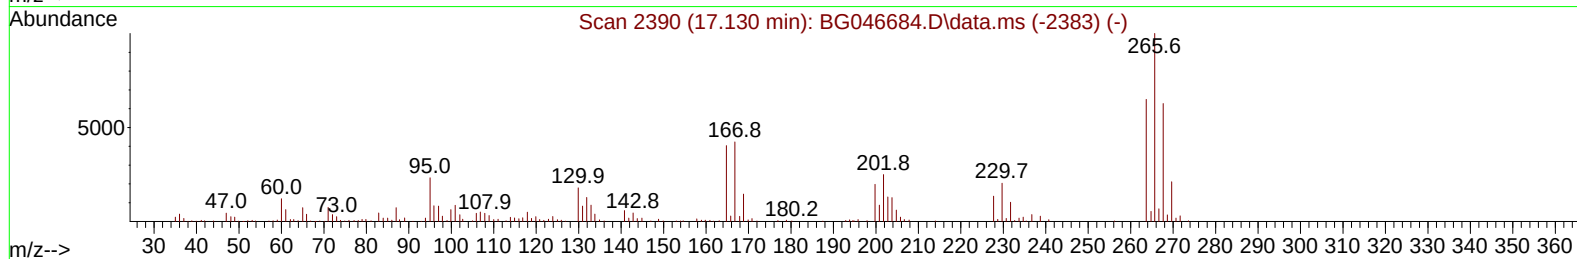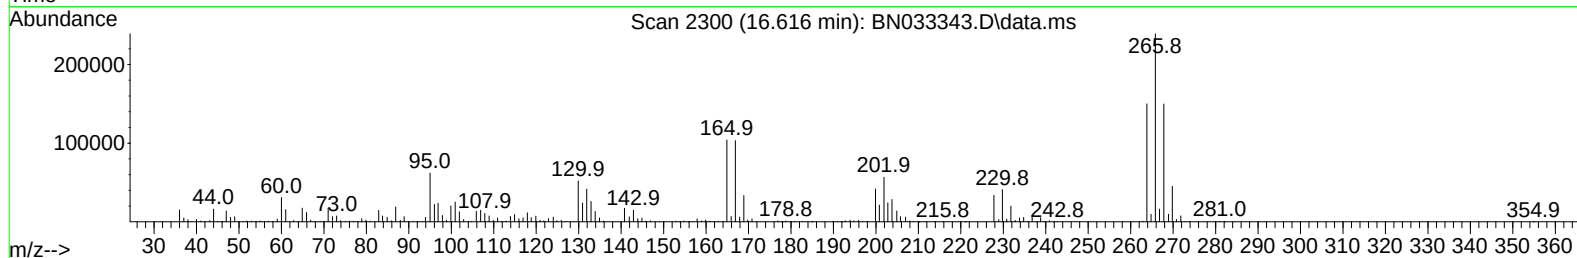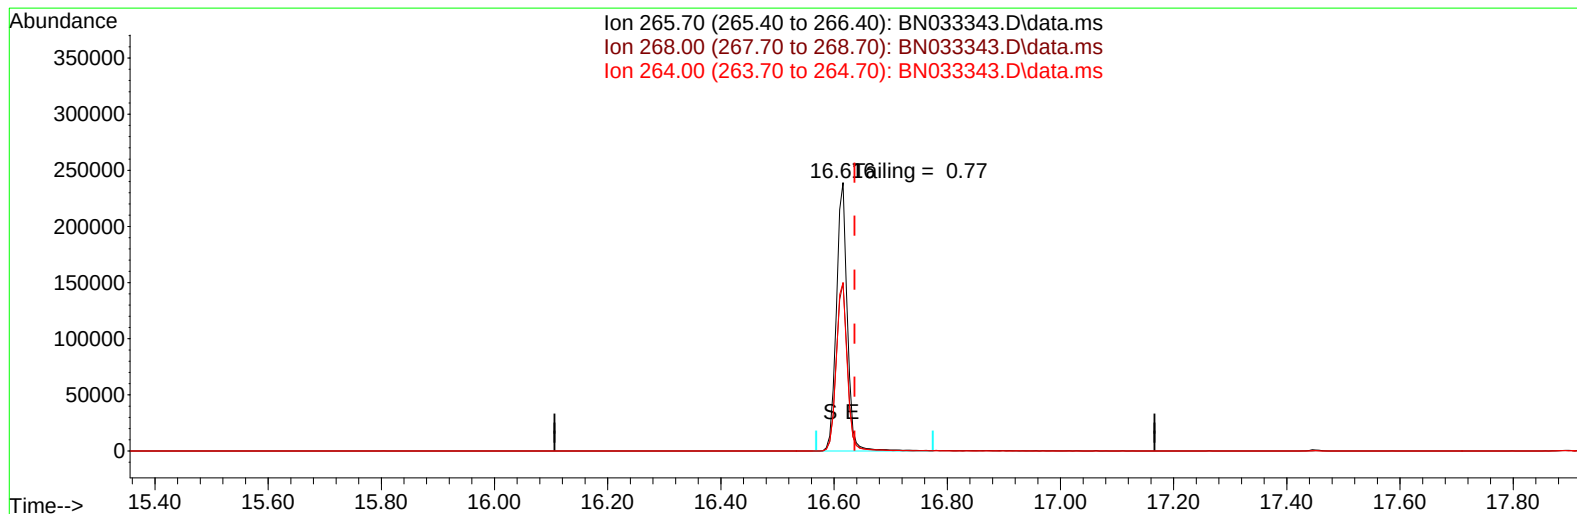

TIC: BN033343.D\data.ms

(70) Pentachlorophenol (C)

16.616min (-0.020) 19636.73 ng




response 321307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.68
264.00	61.60	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081224\
Data File : BN033343.D
Acq On : 12 Aug 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 12 18:23:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

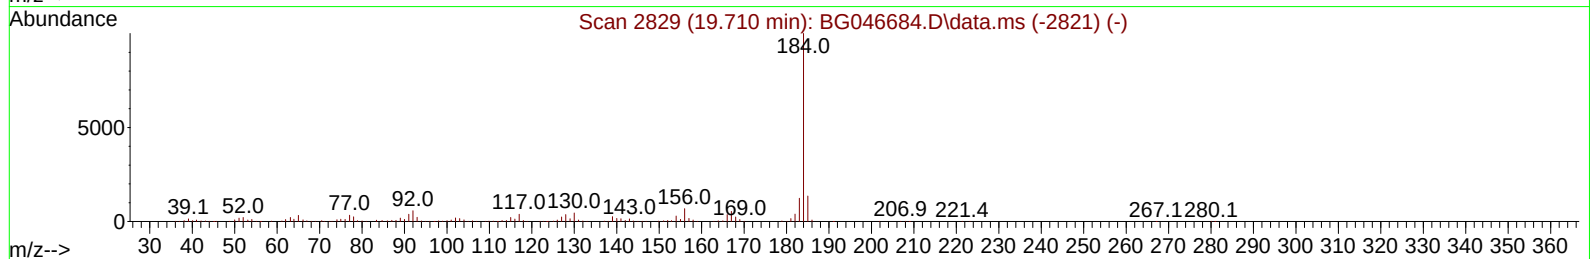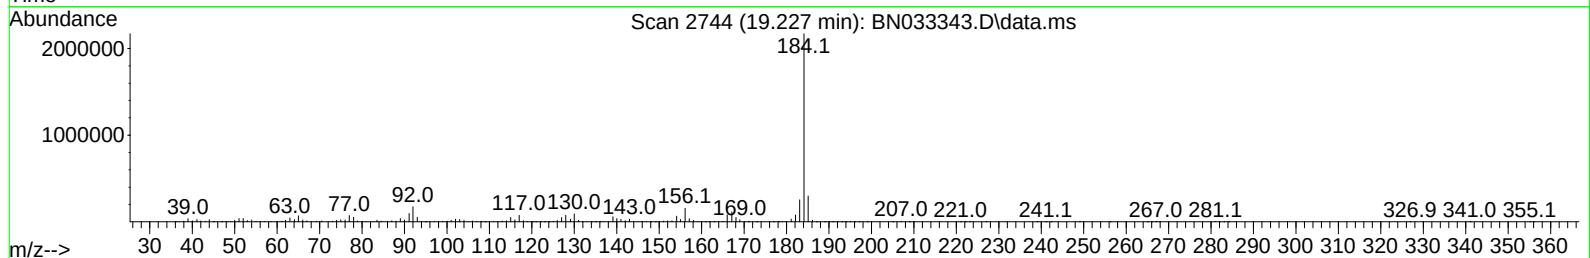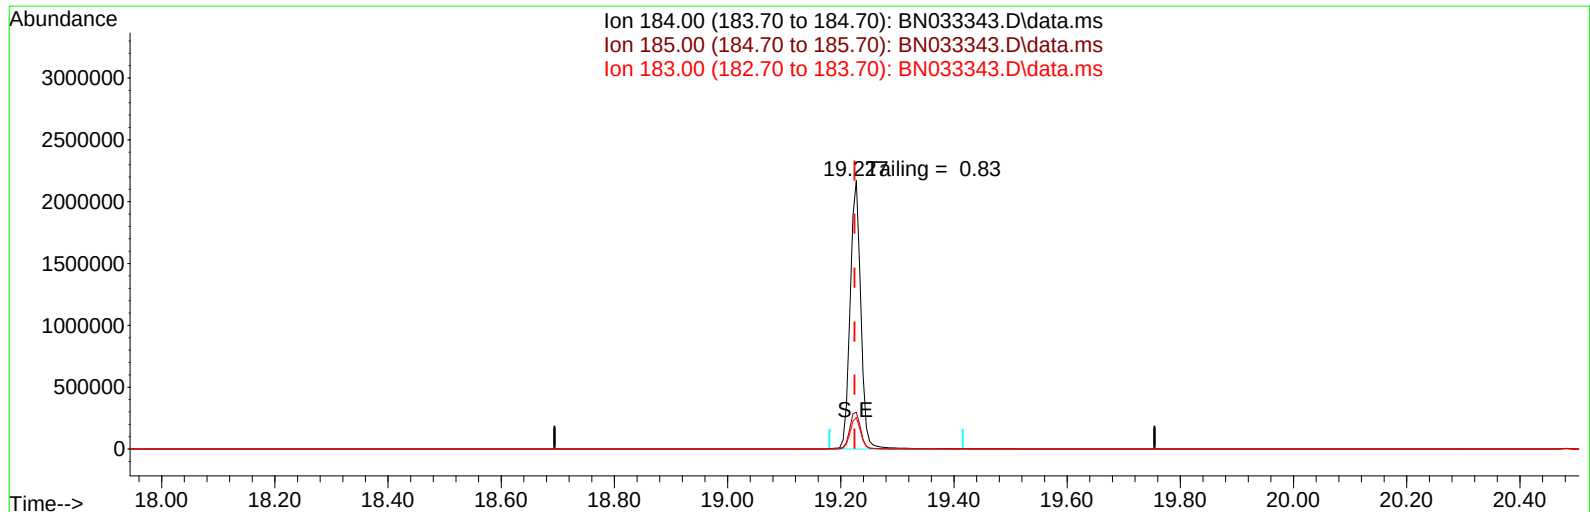

TIC: BN033343.D\data.ms

(77) Benzidine

19.227min (+ 0.003) 0.00 ng

response 2842000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	11.67
0.00	0.00	0.00