
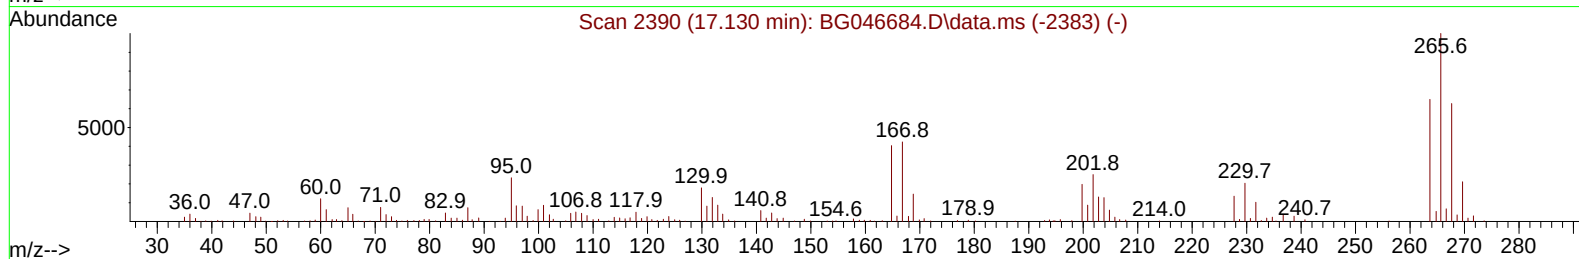
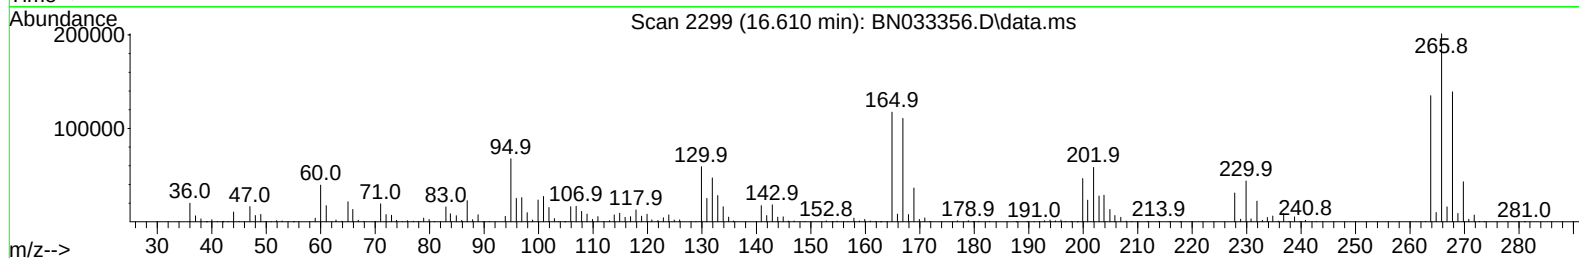


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081324\
Data File : BN033356.D
Acq On : 13 Aug 2024 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 13:50:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

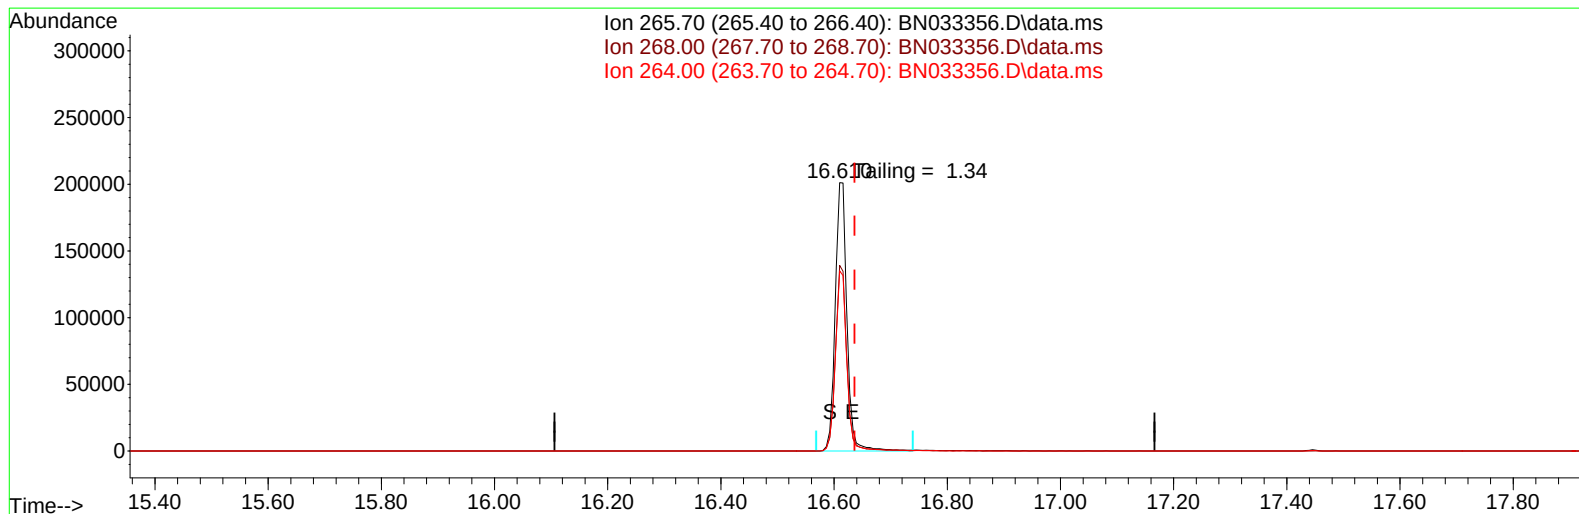

TIC: BN033356.D\data.ms

(70) Pentachlorophenol (C)




16.610min (-0.026) 16013.18 ng

response 288658

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.15
264.00	61.60	67.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081324\
Data File : BN033356.D
Acq On : 13 Aug 2024 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 13:50:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

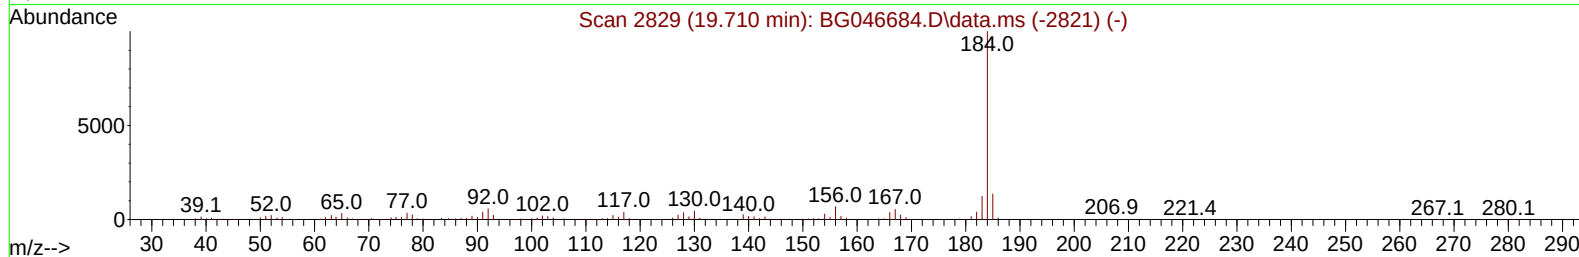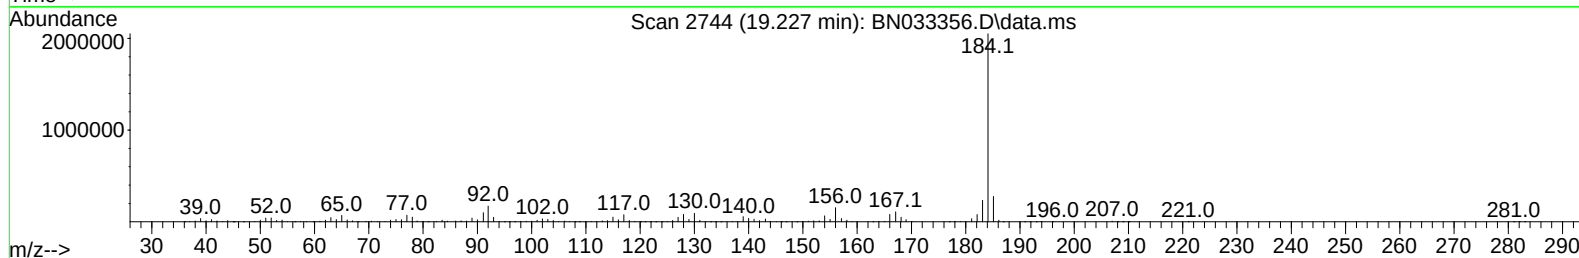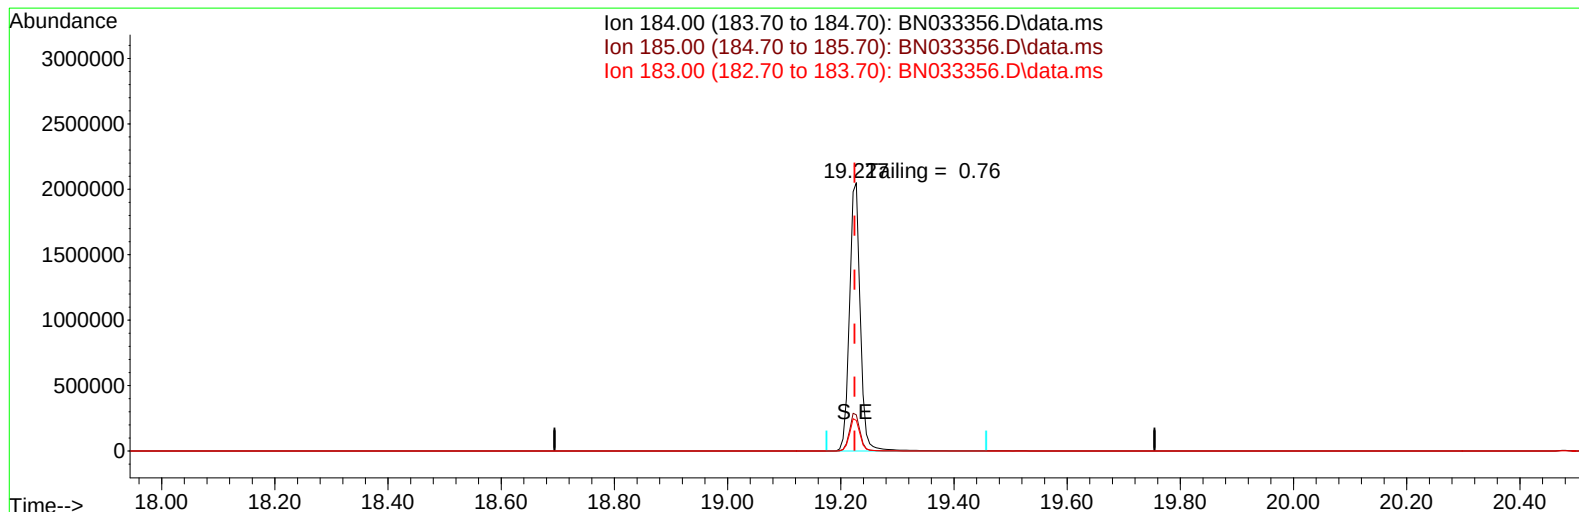

TIC: BN033356.D\data.ms

(77) Benzidine**19.227min (+ 0.003) 0.00 ng****response 2726985**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.50
183.00	13.20	11.40
0.00	0.00	0.00