


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081324\
Data File : BN033356.D
Acq On : 13 Aug 2024 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 12 01:09:50 2024

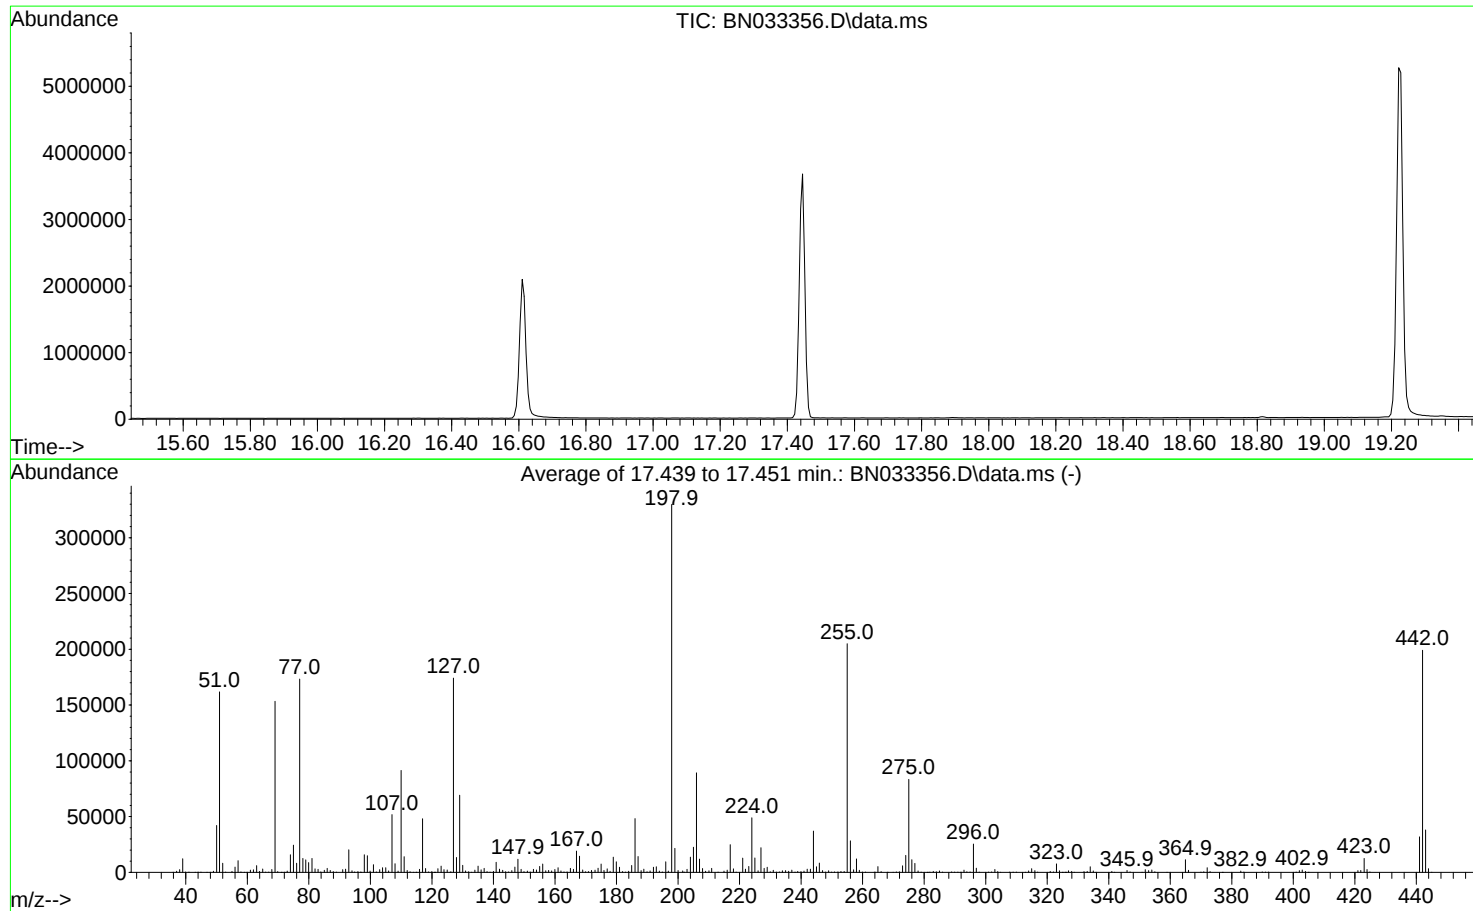




AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	161769	PASS
68	69	0.00	2	1.6	2528	PASS
69	198	0.00	100	46.5	153331	PASS
70	69	0.00	2	0.5	752	PASS
127	198	10	80	52.8	174083	PASS
197	198	0.00	2	0.3	1131	PASS
198	198	100	100	100.0	329792	PASS
199	198	5	9	6.5	21573	PASS
275	198	10	60	25.3	83387	PASS
365	198	1	100	3.5	11422	PASS
441	198	0.01	100	9.6	31792	PASS
442	442	50	100	100.0	199104	PASS
443	442	15	24	19.1	38019	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081324\
Data File : BN033356.D
Acq On : 13 Aug 2024 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 13:50:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

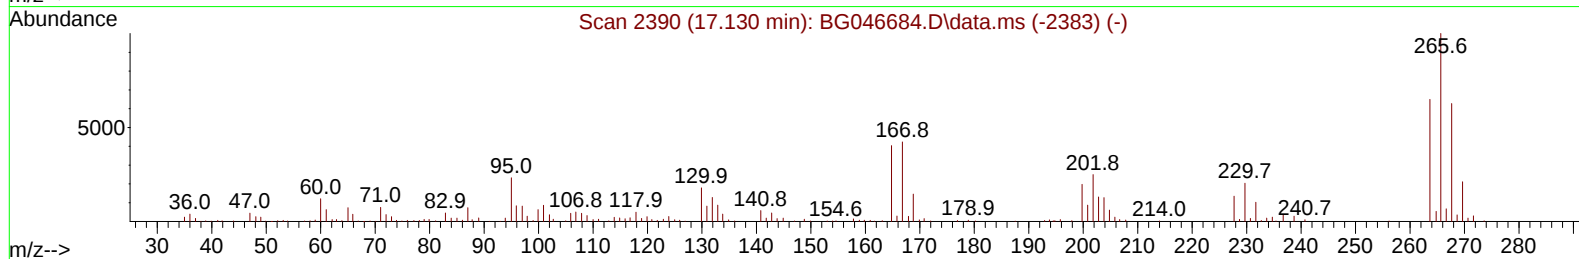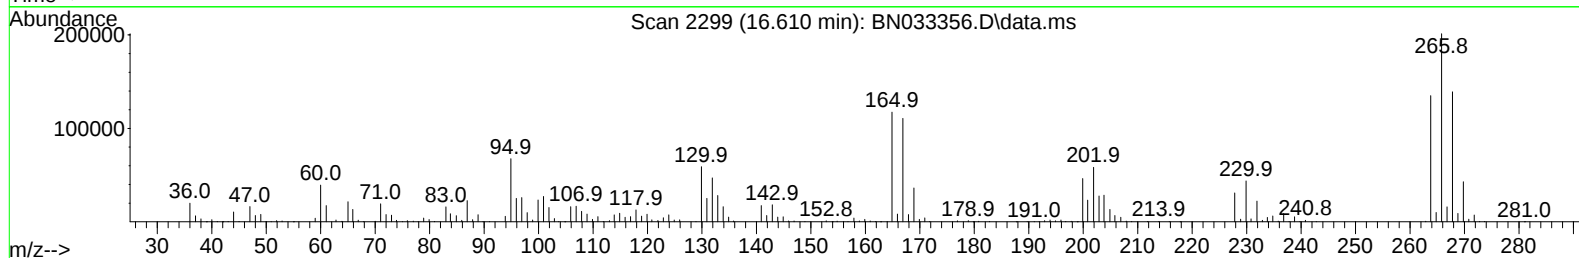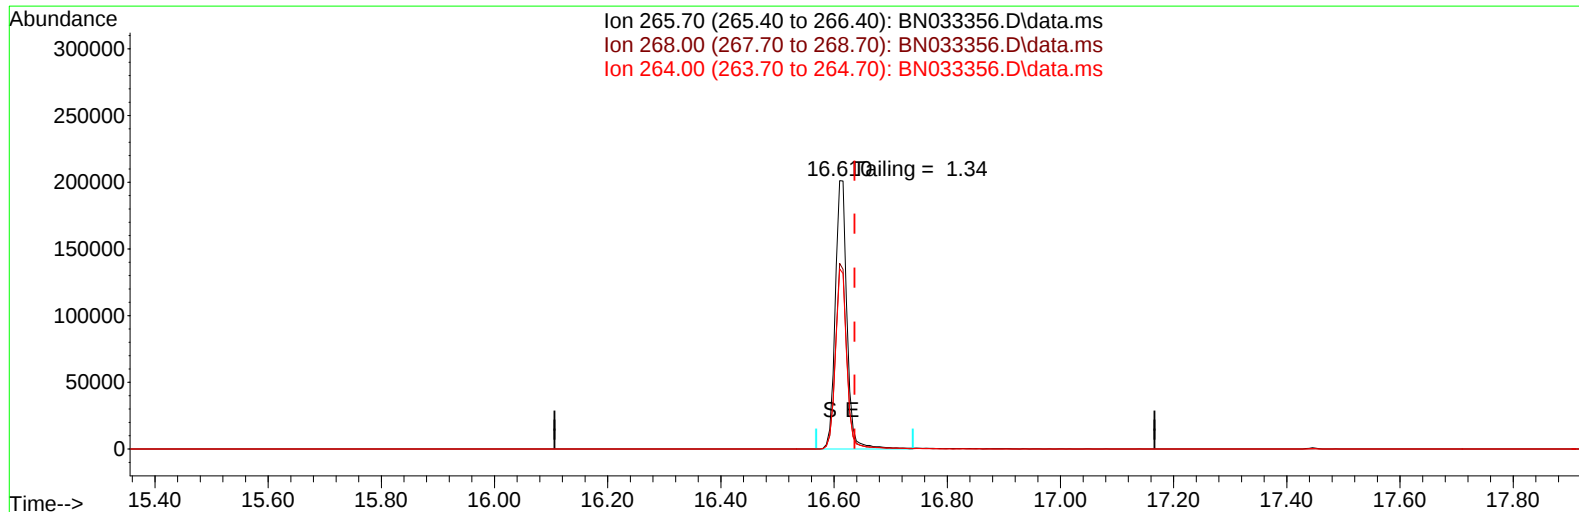

TIC: BN033356.D\data.ms

(70) Pentachlorophenol (C)

16.610min (-0.026) 16013.18 ng




response 288658

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.15
264.00	61.60	67.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081324\
Data File : BN033356.D
Acq On : 13 Aug 2024 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 13:50:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 01:45:39 2024
Response via : Initial Calibration

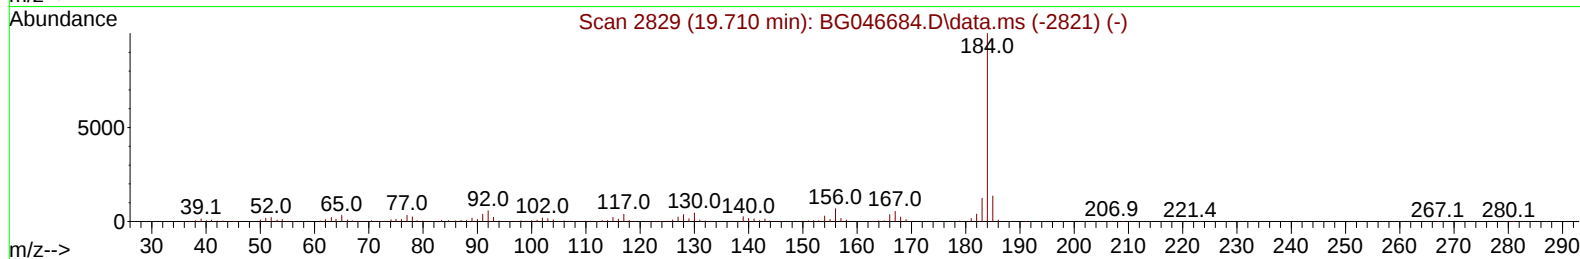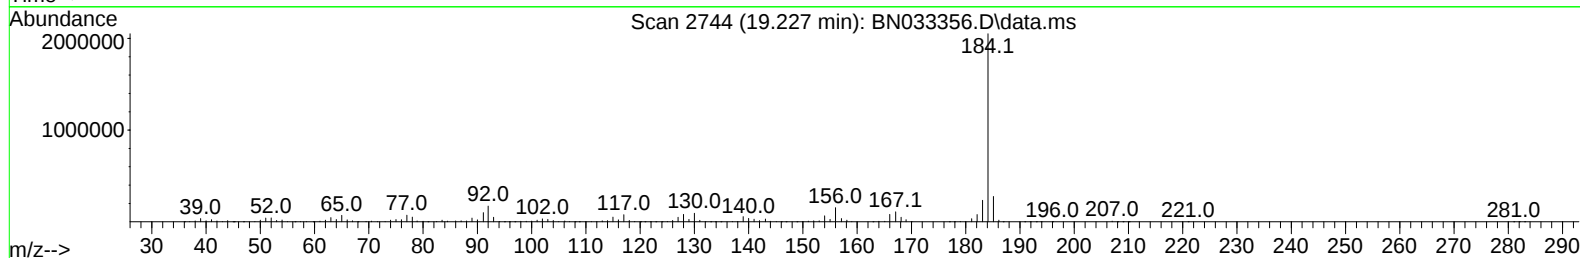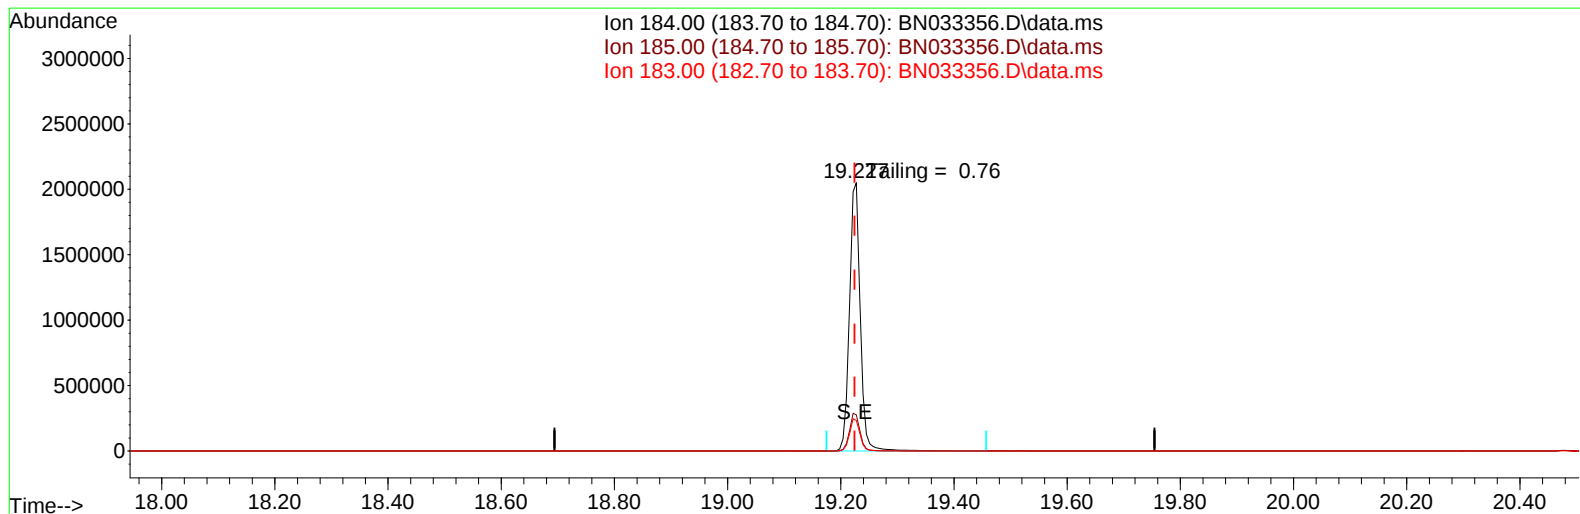

TIC: BN033356.D\data.ms

(77) Benzidine

19.227min (+ 0.003) 0.00 ng

response 2726985

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.50
183.00	13.20	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/13/2024	BNA_N	<u>BN033356.D</u>
Compound Name	Response	Retention Time
DDT	1206879	20.48
DDD	16046	20.033
DDE	527	19.527
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16573	1223452	1.35

Instrument :
BNA_N
ClientSampleId :
DFTPP