
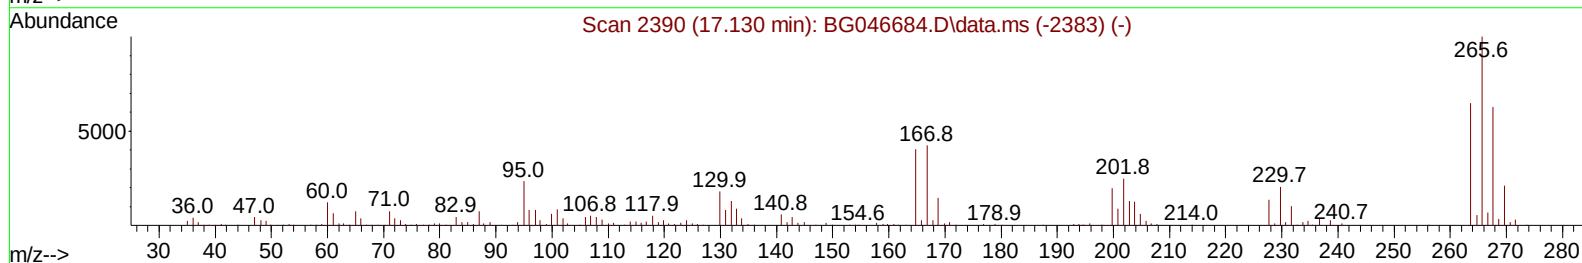
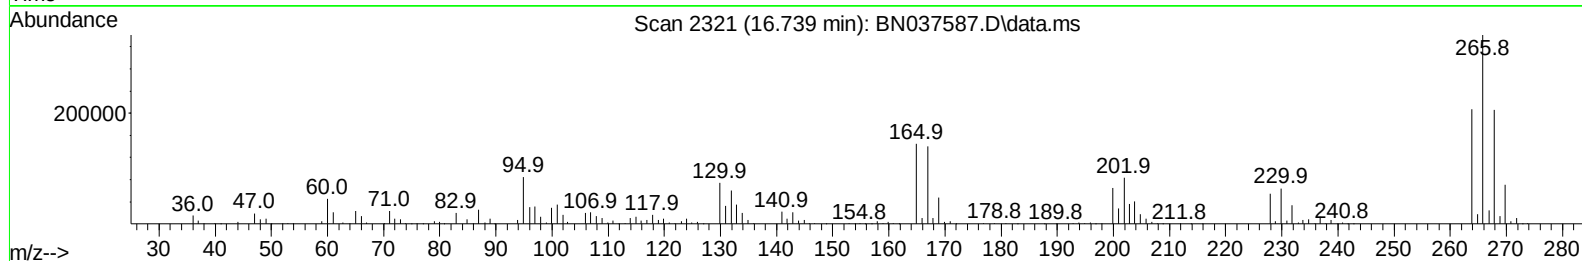


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081325\
Data File : BN037587.D
Acq On : 13 Aug 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 12:38:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

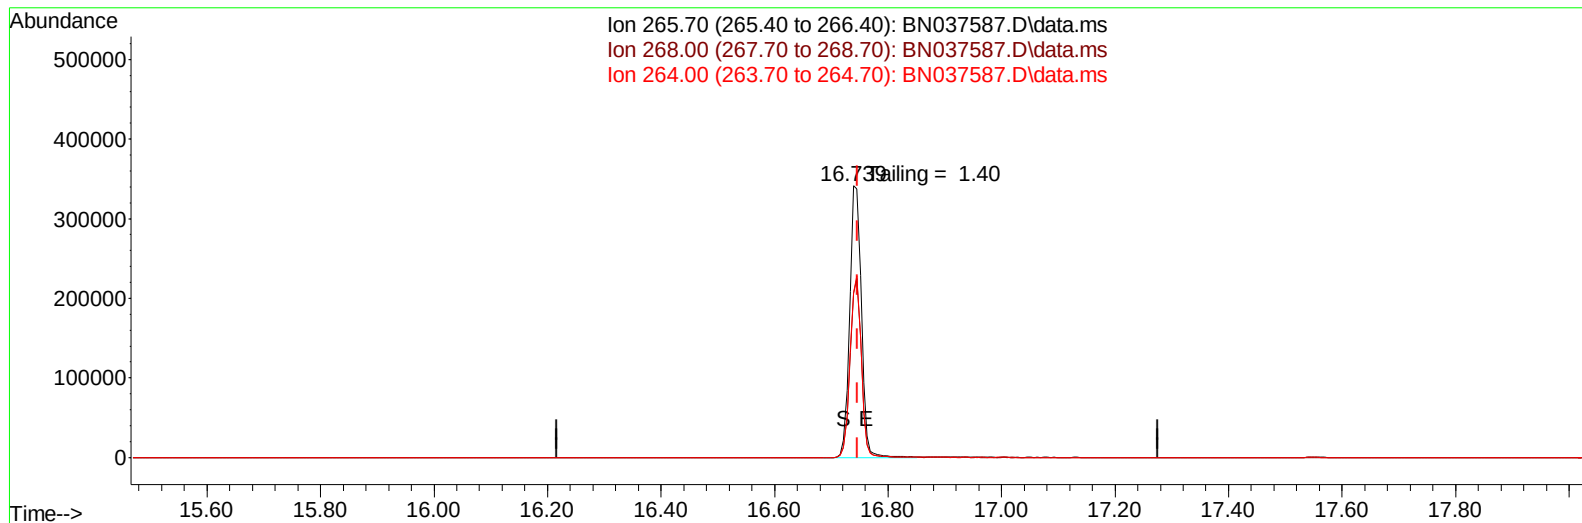

TIC: BN037587.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.007) 26359.62 ng

response 484061

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.50
264.00	61.60	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081325\
Data File : BN037587.D
Acq On : 13 Aug 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 12:38:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

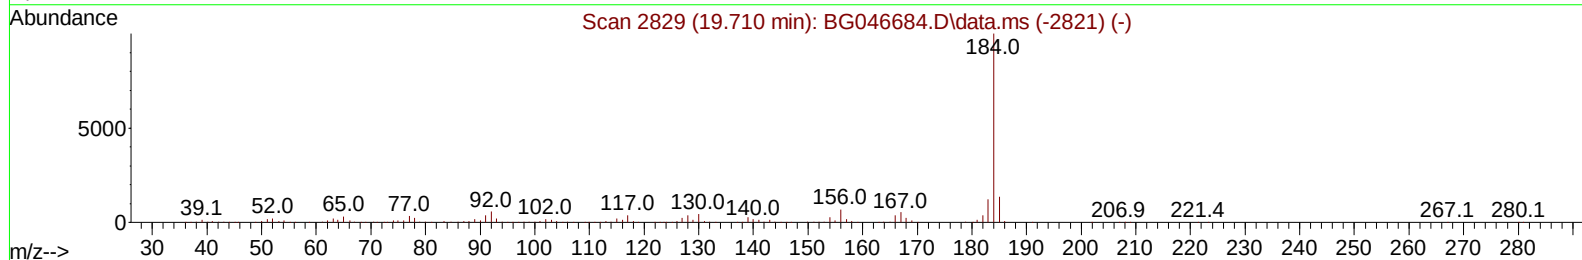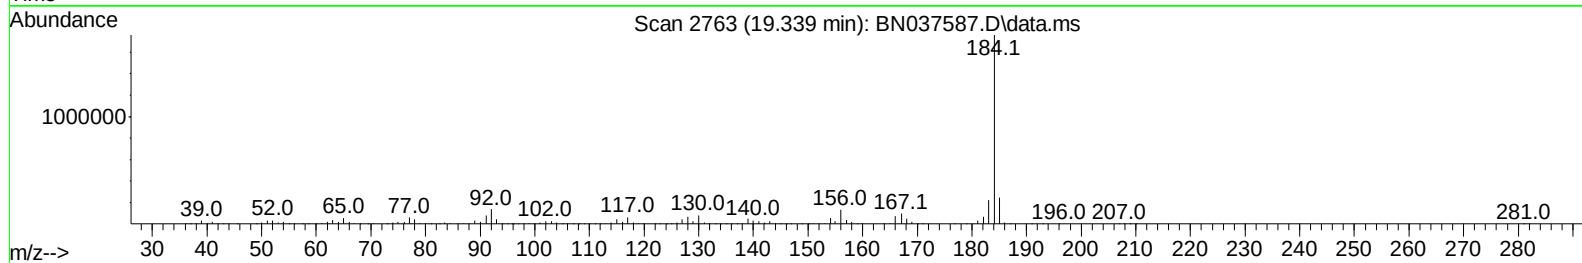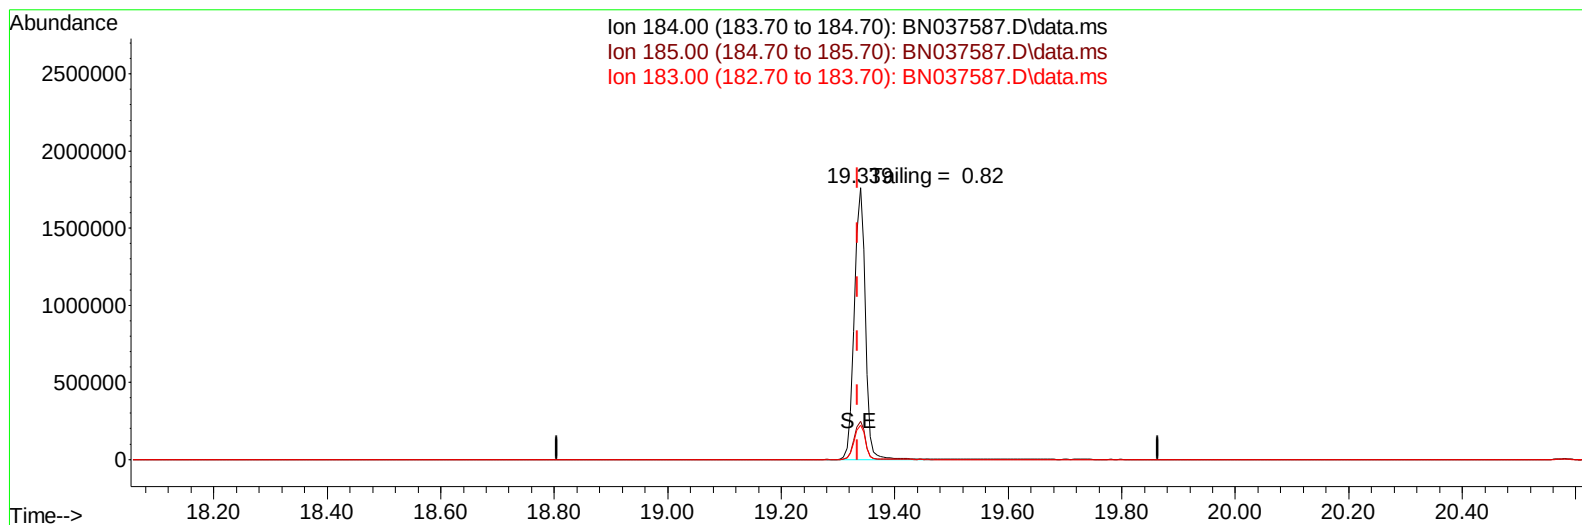

TIC: BN037587.D\data.ms

(77) Benzidine**19.339min (+ 0.005) 0.00 ng****response 2377211**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	12.54
0.00	0.00	0.00