

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081422\
 Data File : BN021220.D
 Acq On : 14 Aug 2022 16:49
 Operator : CG/JU
 Sample : N4166-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGC02

Quant Time: Aug 15 00:42:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 13 04:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	3069	0.400	ng/ul	0.00
4) Naphthalene-d8	10.573	136	10256	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.432	164	5858	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.183	188	11553	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	7230	0.400	ng/ul	0.00
23) Perylene-d12	23.713	264	7240	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.190	96	16095	4.099	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.190	152	4516	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.225	212	10661	0.477	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.232	88	112	0.028	ng/ul#	55
20) Pyrene	19.583	202	1401	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.558	252	2209	0.072	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081422\
Data File : BN021220.D
Acq On : 14 Aug 2022 16:49
Operator : CG/JU
Sample : N4166-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGC02

Quant Time: Aug 15 00:42:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 04:02:44 2022
Response via : Initial Calibration




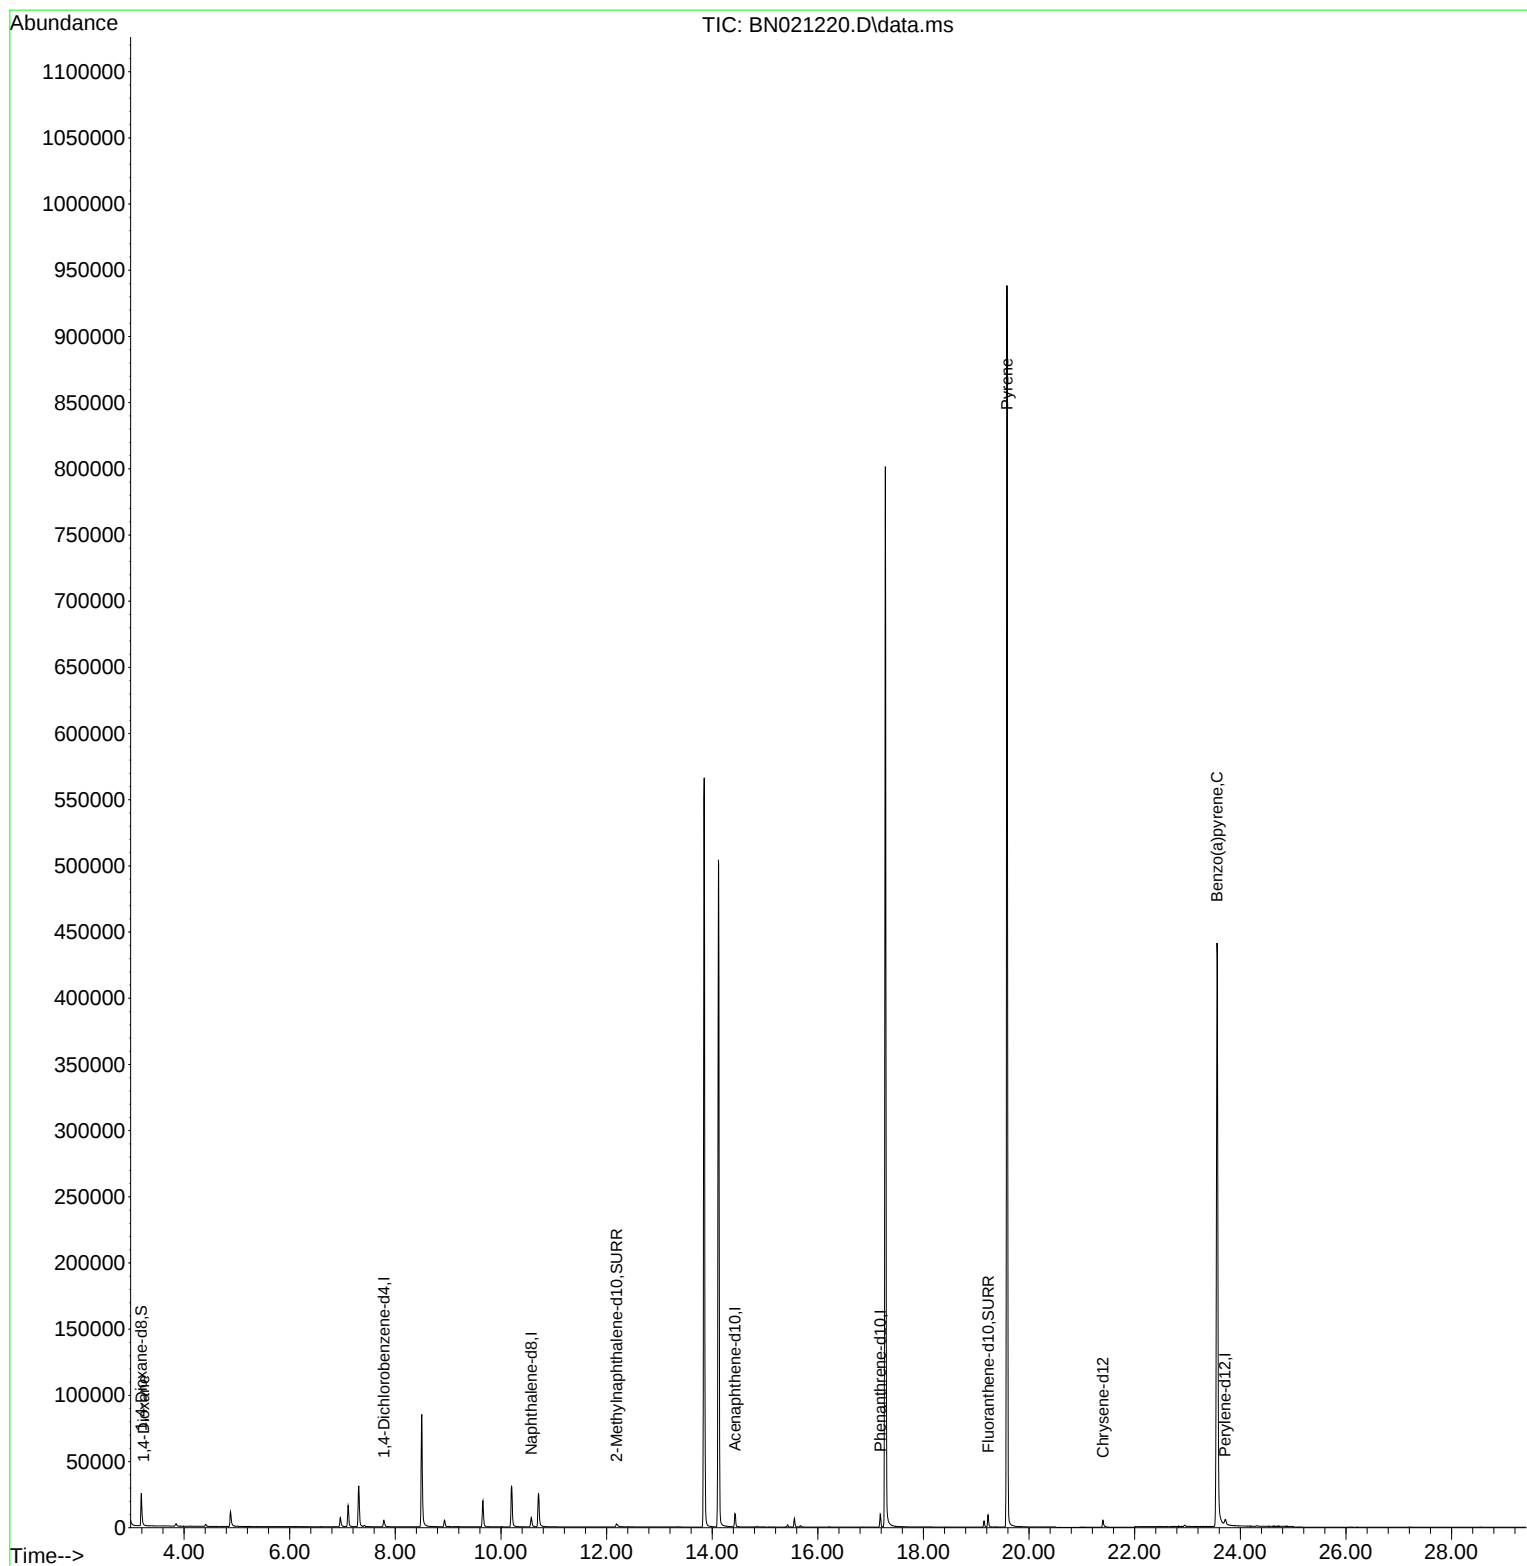


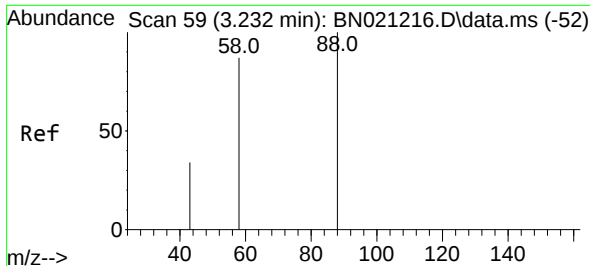

#2
1,4-Dioxane
Concen: 0.028 ng/ul
RT: 3.232 min Scan# 59
Delta R.T. 0.000 min
Lab File: BN021220.D
Acq: 14 Aug 2022 16:49




Instrument :
BNA_N
ClientSampleId :
BGC02


Tgt Ion: 88 Resp: 112
Ion Ratio Lower Upper
88 100
43 31.2 31.4 47.0#
58 11.3 49.0 73.6#

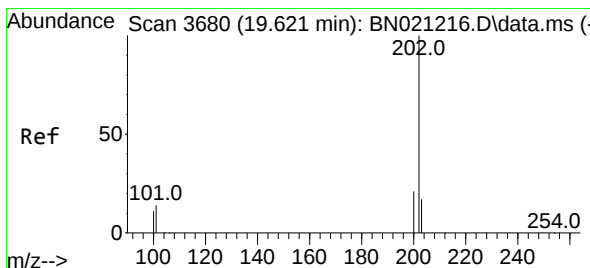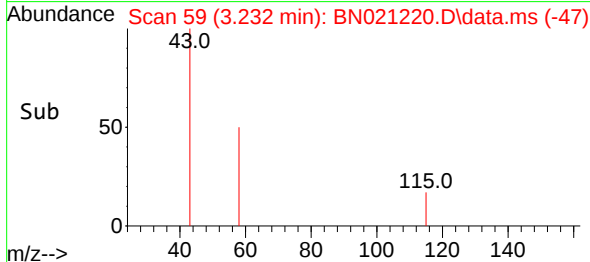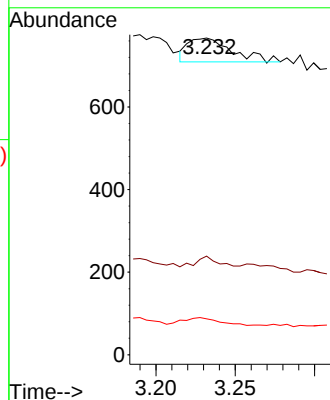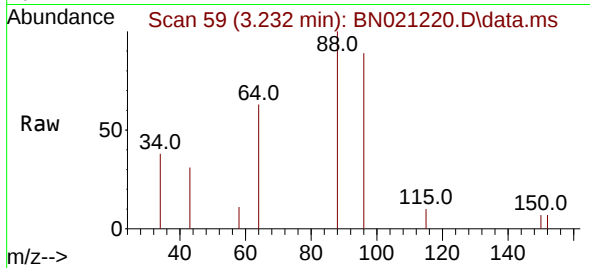

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.583 min Scan# 3672
Delta R.T. -0.038 min
Lab File: BN021220.D
Acq: 14 Aug 2022 16:49


Tgt Ion: 202 Resp: 1401
Ion Ratio Lower Upper
202 100
101 181.4 11.3 16.9#
100 1321.8 9.0 13.4#

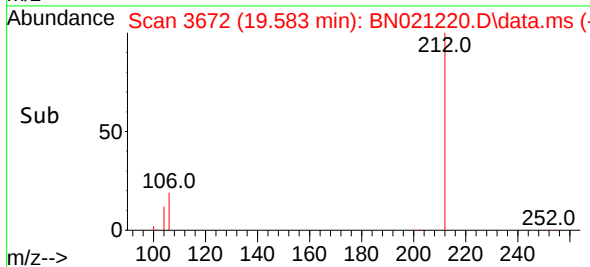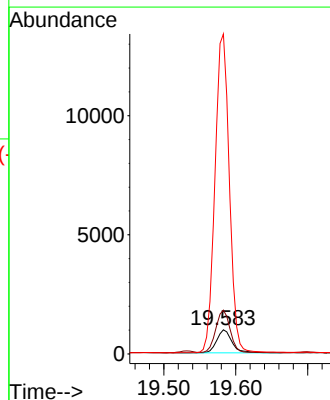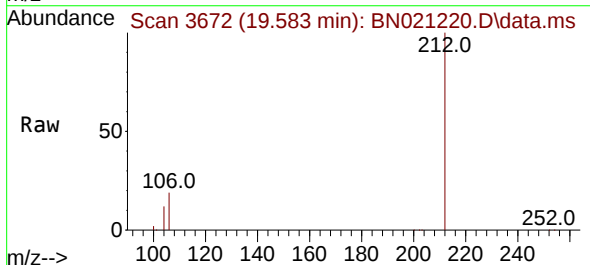

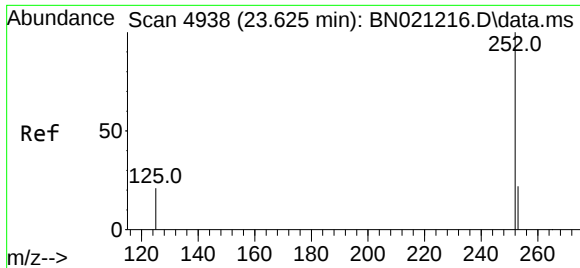

#26
 Benzo(a)pyrene
 Concen: 0.072 ng/ul
 RT: 23.558 min Scan# 4915
 Delta R.T. -0.064 min
 Lab File: BN021220.D
 Acq: 14 Aug 2022 16:49

Instrument :
 BNA_N
 ClientSampleId :
 BGC02

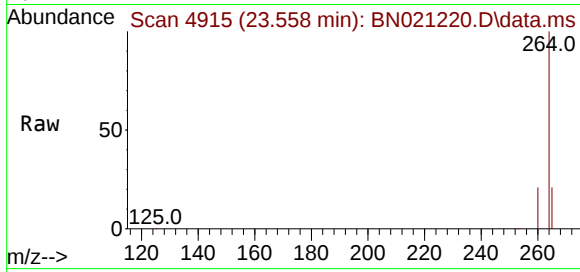

Tgt Ion:252 Resp: 2209

Ion	Ratio	Lower	Upper
252	100		
253	46.0	22.1	33.1#
125	34.3	14.7	22.1#

