
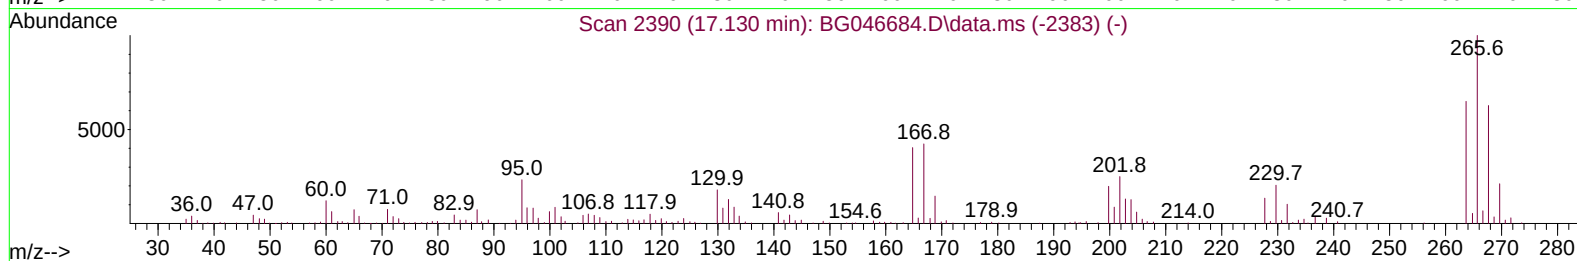
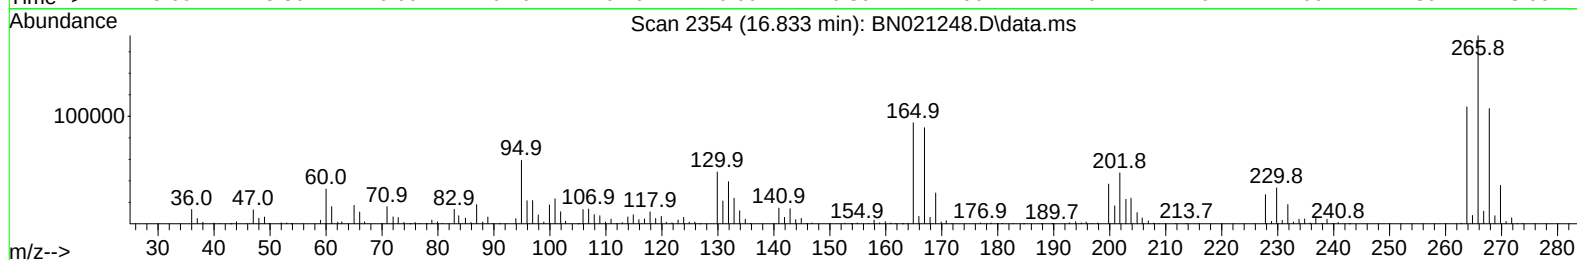


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021248.D
Acq On : 16 Aug 2022 08:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 12:56:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 04:36:00 2022
Response via : Initial Calibration

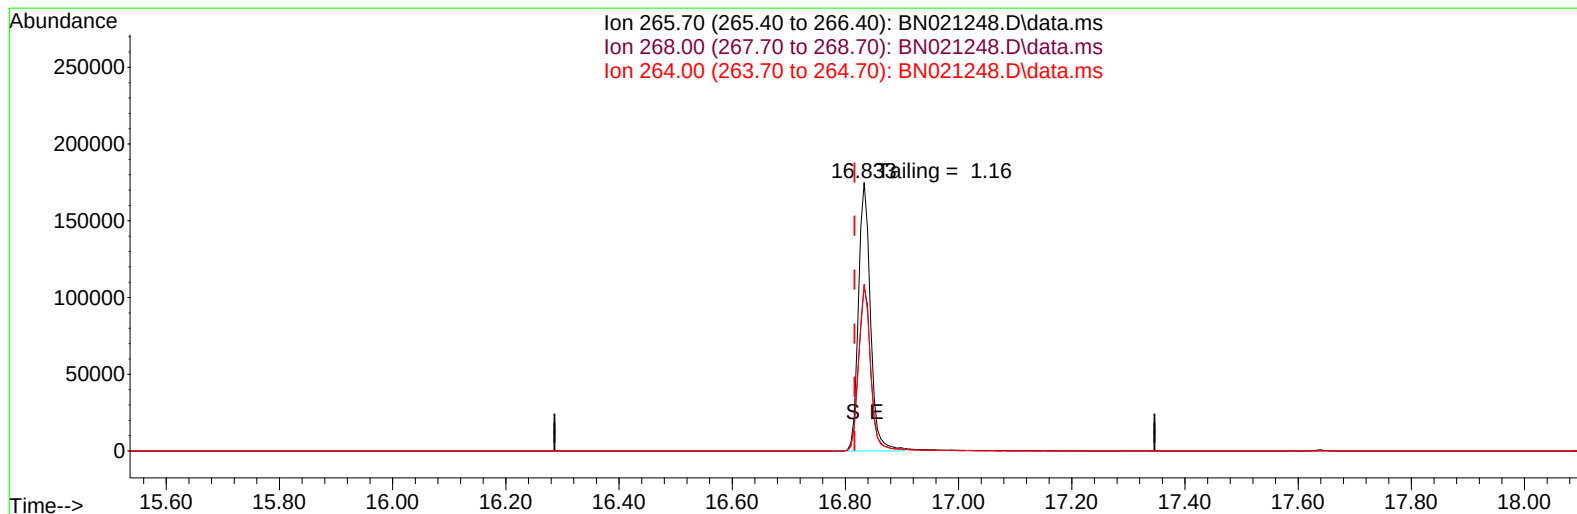

TIC: BN021248.D\data.ms

(70) Pentachlorophenol (C)




16.833min (+ 0.017) 17747.84 ng

response 260594

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.29
264.00	61.60	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021248.D
Acq On : 16 Aug 2022 08:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 12:56:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 04:36:00 2022
Response via : Initial Calibration

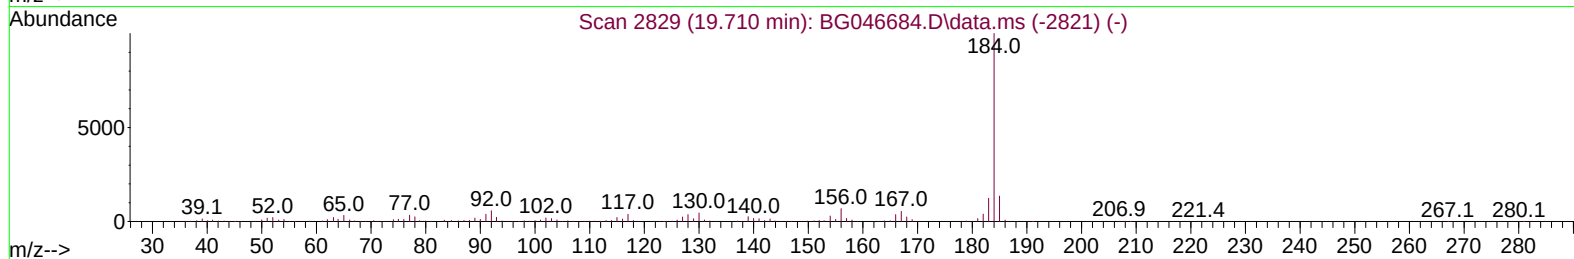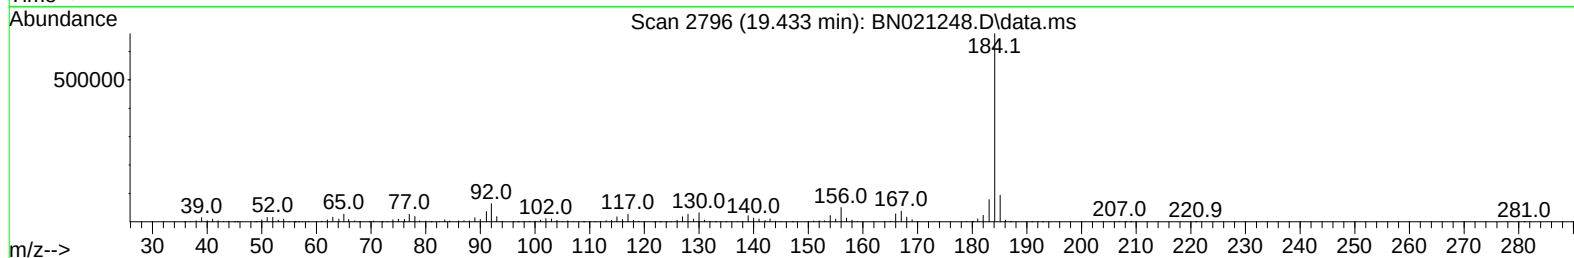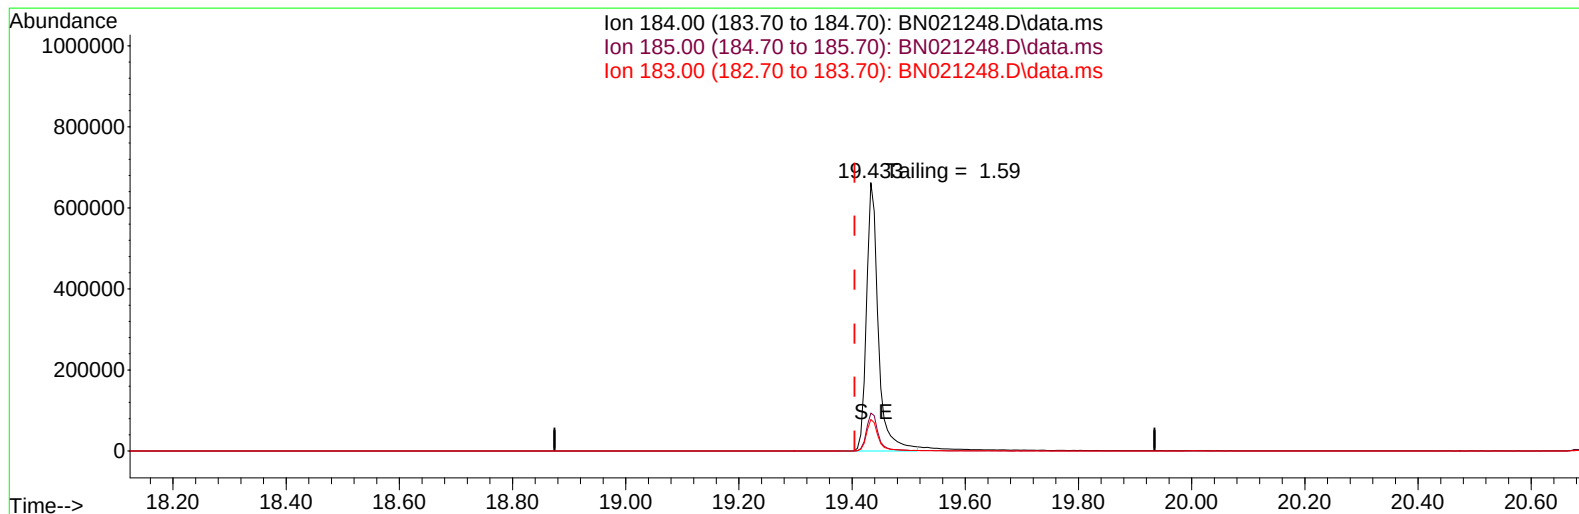

TIC: BN021248.D\data.ms

(77) Benzidine**19.433min (+ 0.029) 0.00 ng****response 996876**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.16
183.00	13.20	11.76
0.00	0.00	0.00