


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
 Data File : BN021237.D
 Acq On : 15 Aug 2022 16:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 16 09:19:59 2022

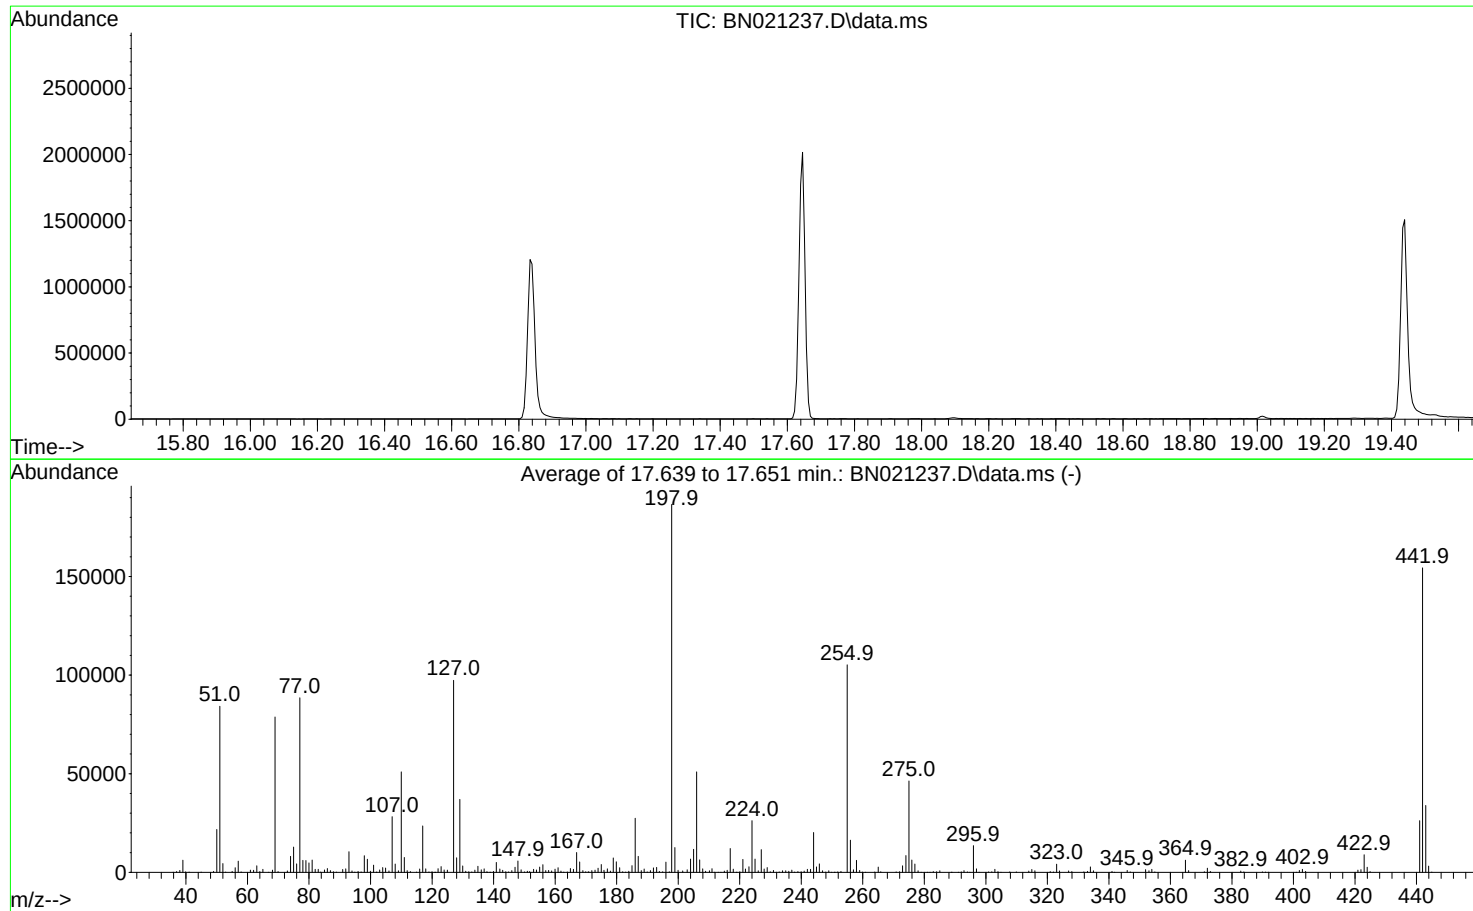

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	84213	PASS
68	69	0.00	2	1.5	1161	PASS
69	198	0.00	100	42.2	78749	PASS
70	69	0.00	2	0.5	381	PASS
127	198	10	80	52.2	97347	PASS
197	198	0.00	2	0.2	324	PASS
198	198	100	100	100.0	186496	PASS
199	198	5	9	6.7	12564	PASS
275	198	10	60	24.8	46323	PASS
365	198	1	100	3.3	6150	PASS
441	198	0.01	100	14.0	26181	PASS
442	442	50	100	100.0	154349	PASS
443	442	15	24	22.0	33941	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/16/2022	BNA_N	<u>BN021237.D</u>
Compound Name	Response	Retention Time
DDT	597695	20.68
DDD	27245	20.239
DDE	0	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27245	624940	4.36

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021237.D
Acq On : 15 Aug 2022 16:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 16 04:36:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 04:36:00 2022
Response via : Initial Calibration

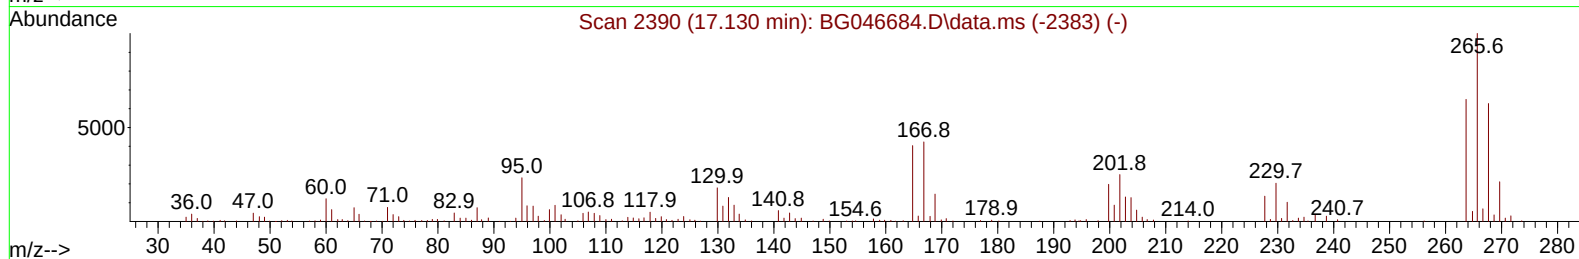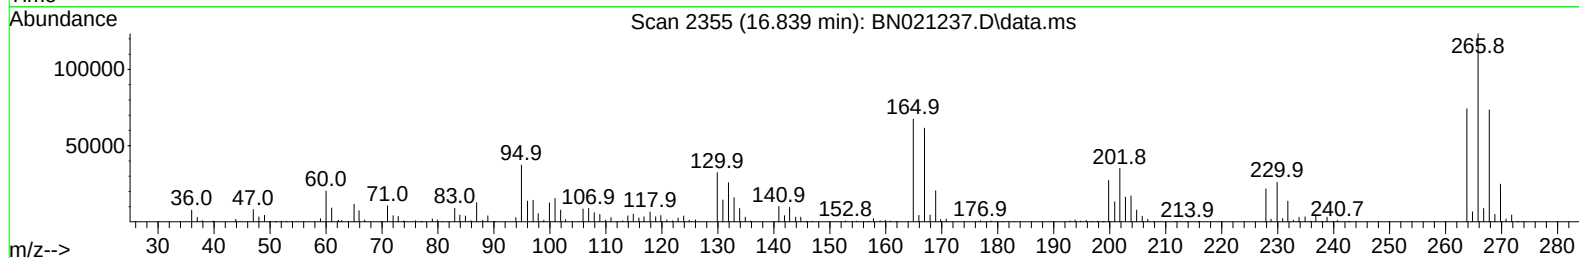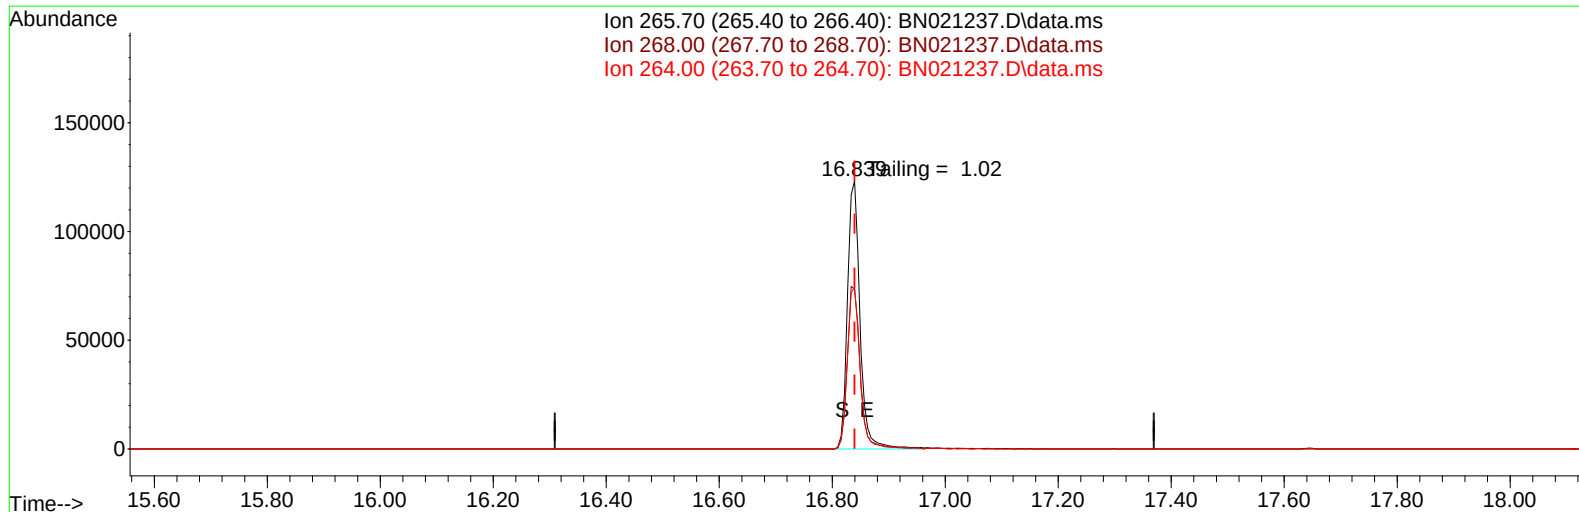

TIC: BN021237.D\data.ms

(70) Pentachlorophenol (C)

16.839min (0.000) 17986.37 ng




response 189709

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.58
264.00	61.60	60.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021237.D
Acq On : 15 Aug 2022 16:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 16 04:36:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 04:36:00 2022
Response via : Initial Calibration

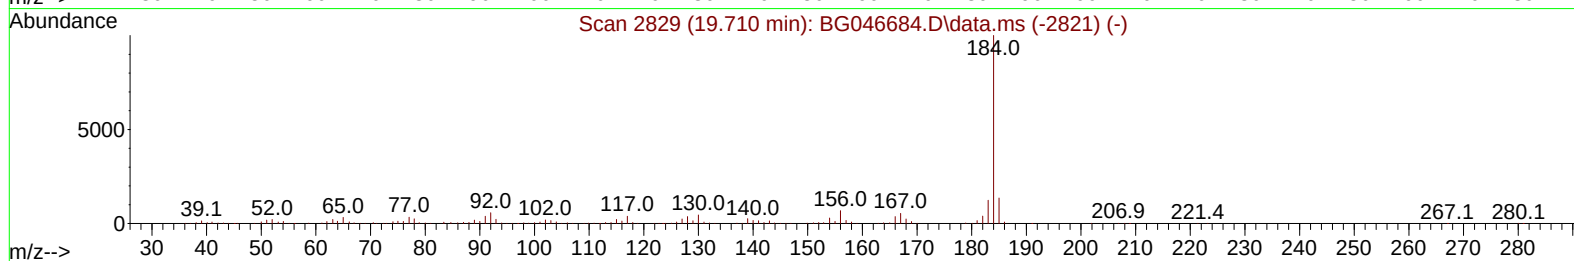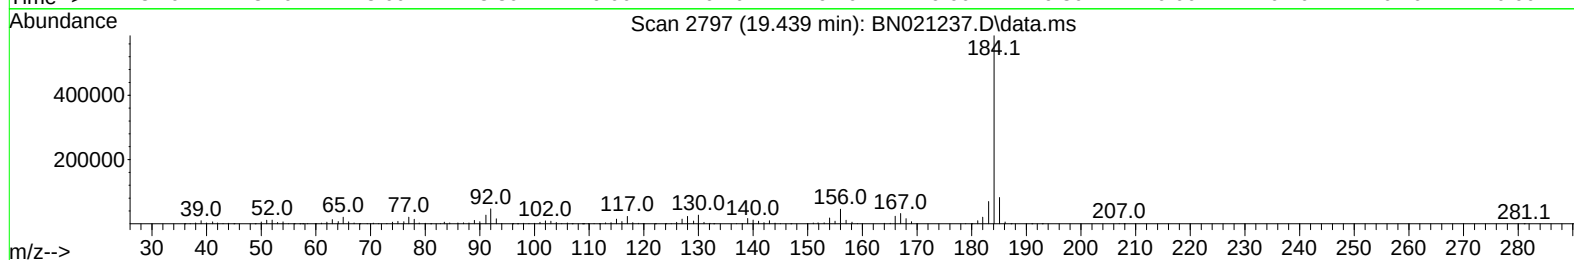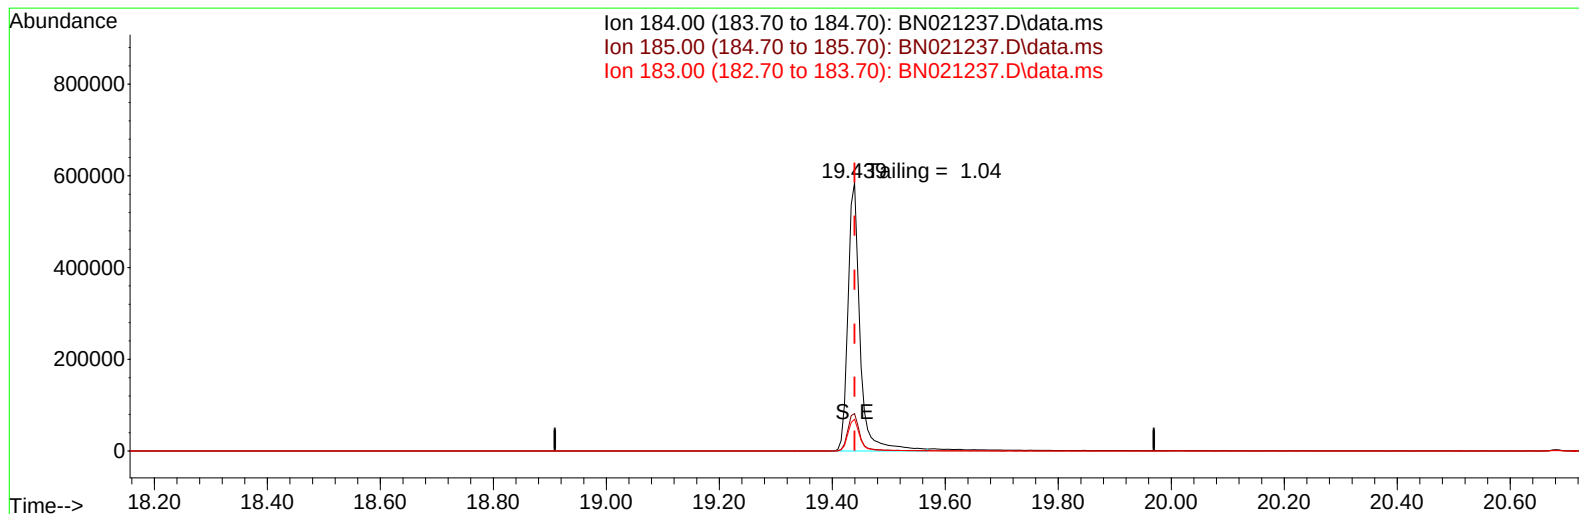

TIC: BN021237.D\data.ms

(77) Benzidine

19.439min (0.000) 0.00 ng

response 870789

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.95
183.00	13.20	11.88
0.00	0.00	0.00