
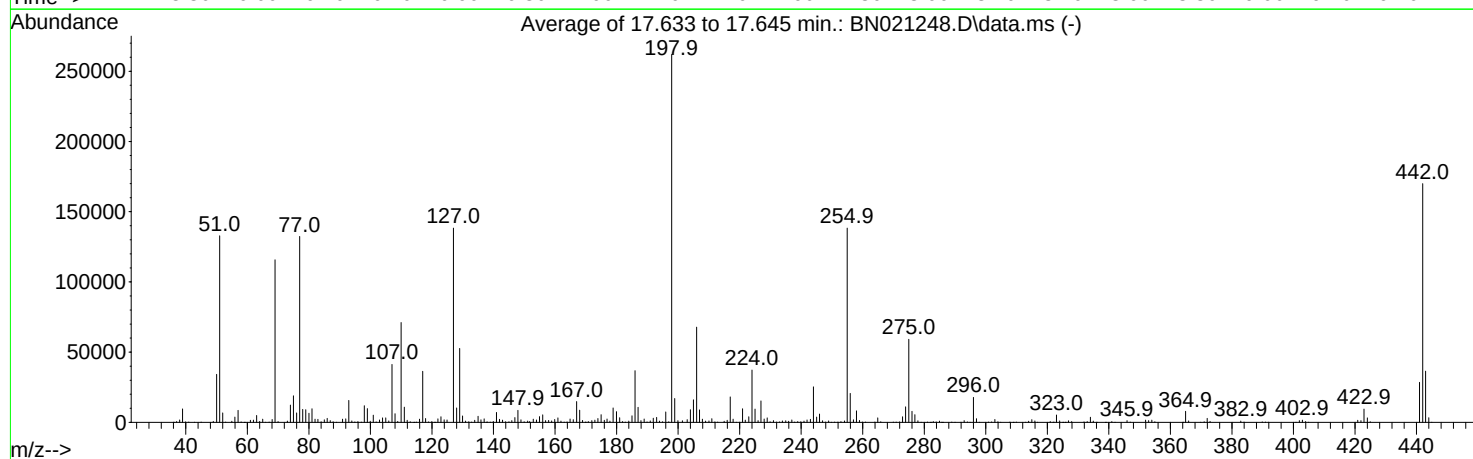


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
 Data File : BN021248.D
 Acq On : 16 Aug 2022 08:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 16 09:19:59 2022

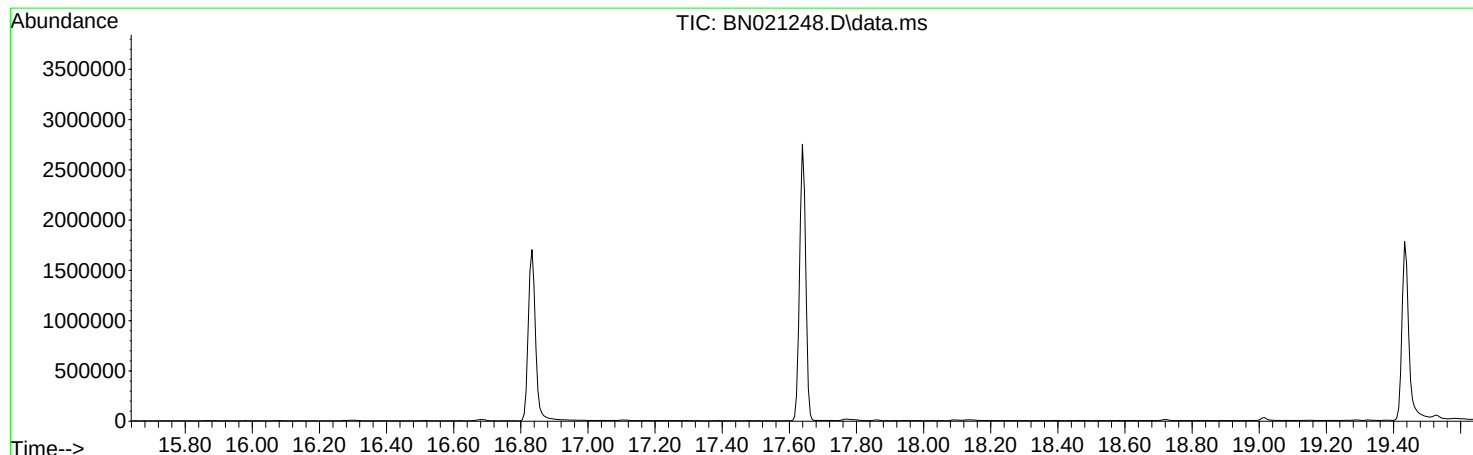

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	132891	PASS
68	69	0.00	2	1.7	2022	PASS
69	198	0.00	100	44.2	115744	PASS
70	69	0.00	2	0.5	560	PASS
127	198	10	80	52.8	138341	PASS
197	198	0.00	2	0.2	446	PASS
198	198	100	100	100.0	261931	PASS
199	198	5	9	6.5	17033	PASS
275	198	10	60	22.6	59139	PASS
365	198	1	100	3.0	7851	PASS
441	198	0.01	100	10.9	28504	PASS
442	442	50	100	100.0	169995	PASS
443	442	15	24	21.5	36464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/16/2022	BNA_N	<u>BN021248.D</u>
Compound Name	Response	Retention Time
DDT	788271	20.68
DDD	40180	20.23
DDE	5351	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45531	833802	5.46

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021248.D
Acq On : 16 Aug 2022 08:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 16 12:56:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 04:36:00 2022
Response via : Initial Calibration

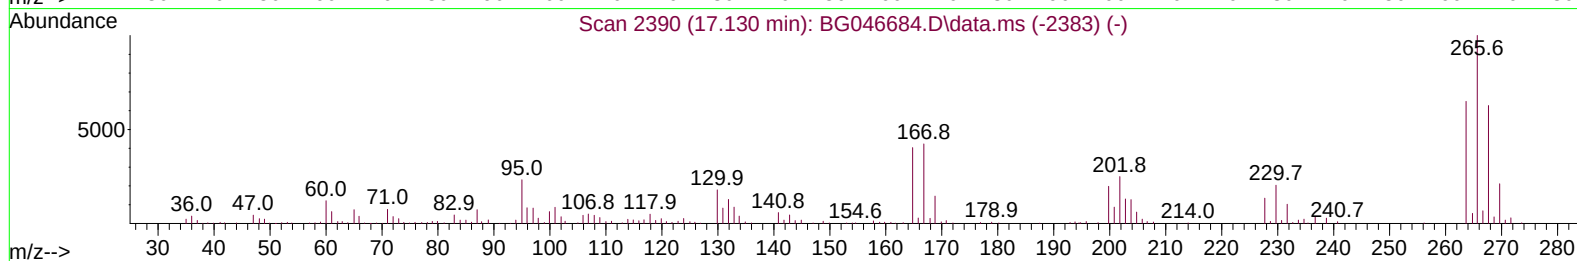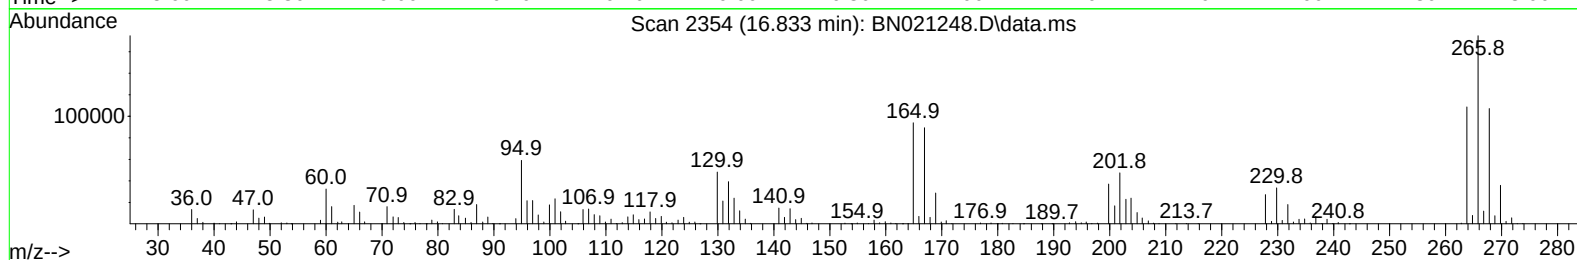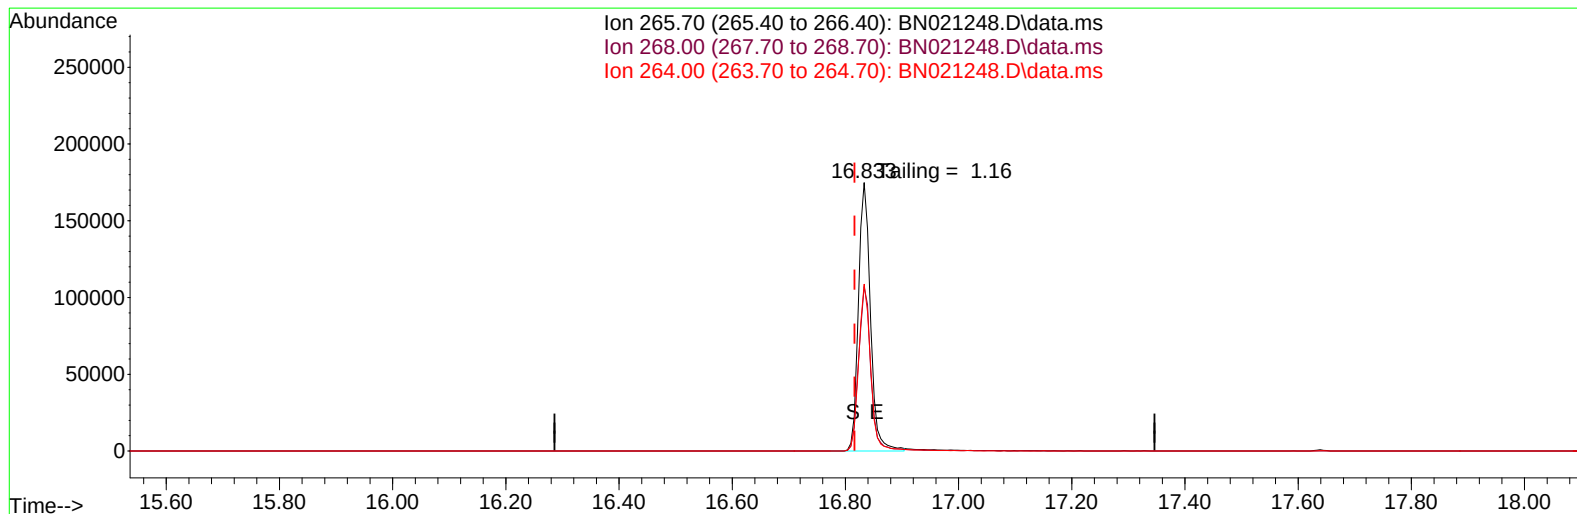

TIC: BN021248.D\data.ms

(70) Pentachlorophenol (C)

16.833min (+ 0.017) 17747.84 ng




response 260594

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.29
264.00	61.60	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021248.D
Acq On : 16 Aug 2022 08:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 16 12:56:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 04:36:00 2022
Response via : Initial Calibration

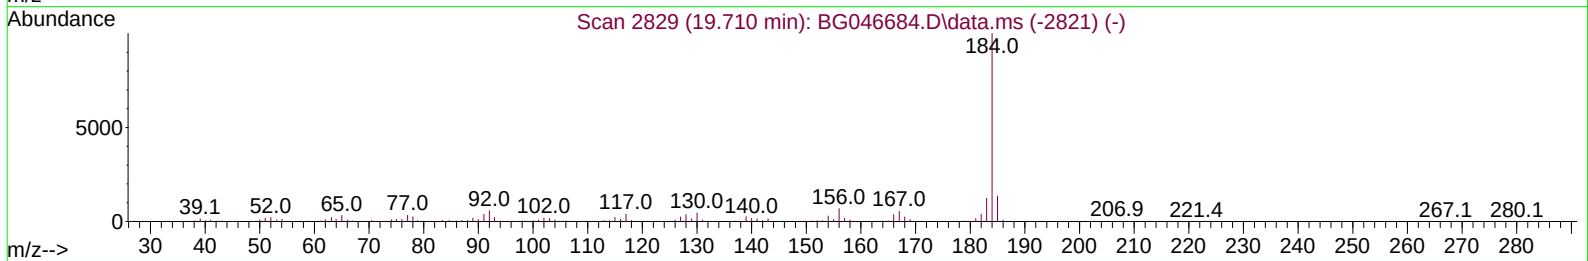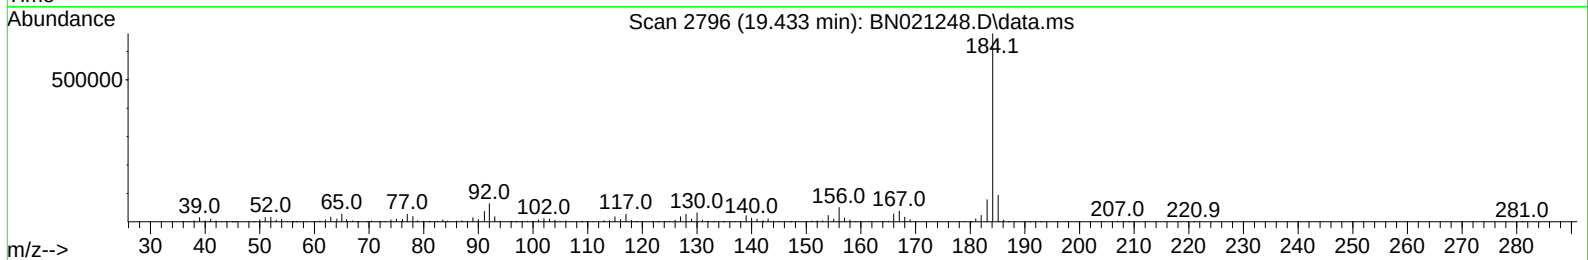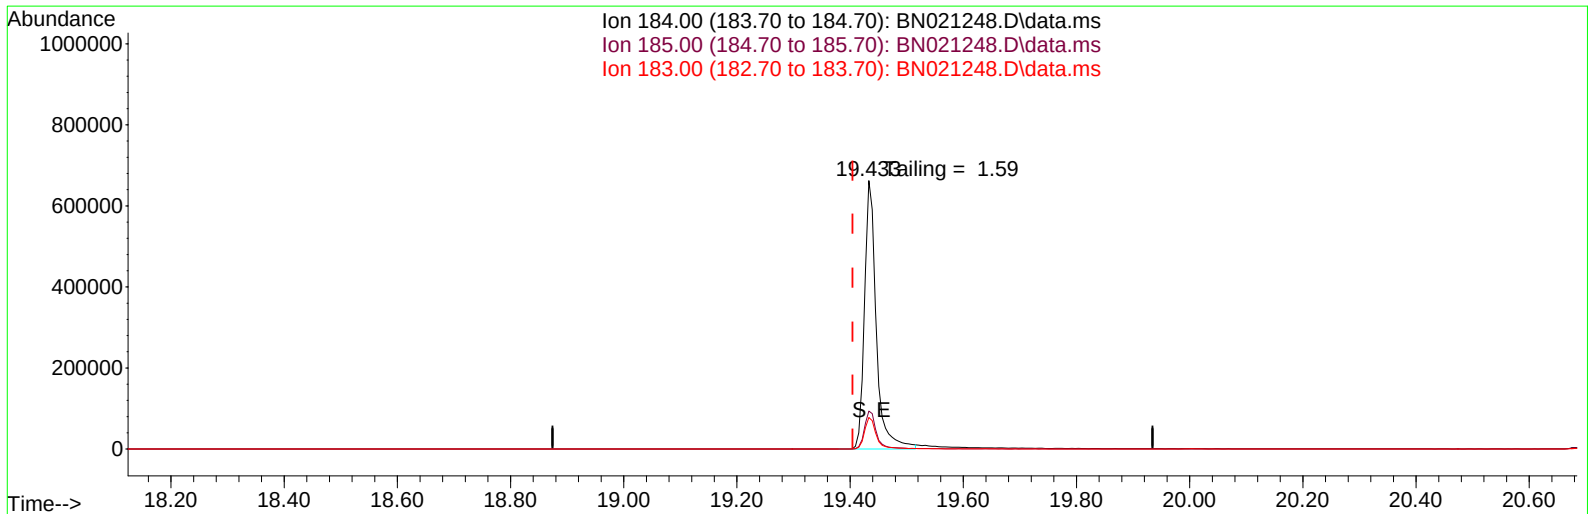

TIC: BN021248.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 0.00 ng

response 996876

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.16
183.00	13.20	11.76
0.00	0.00	0.00