
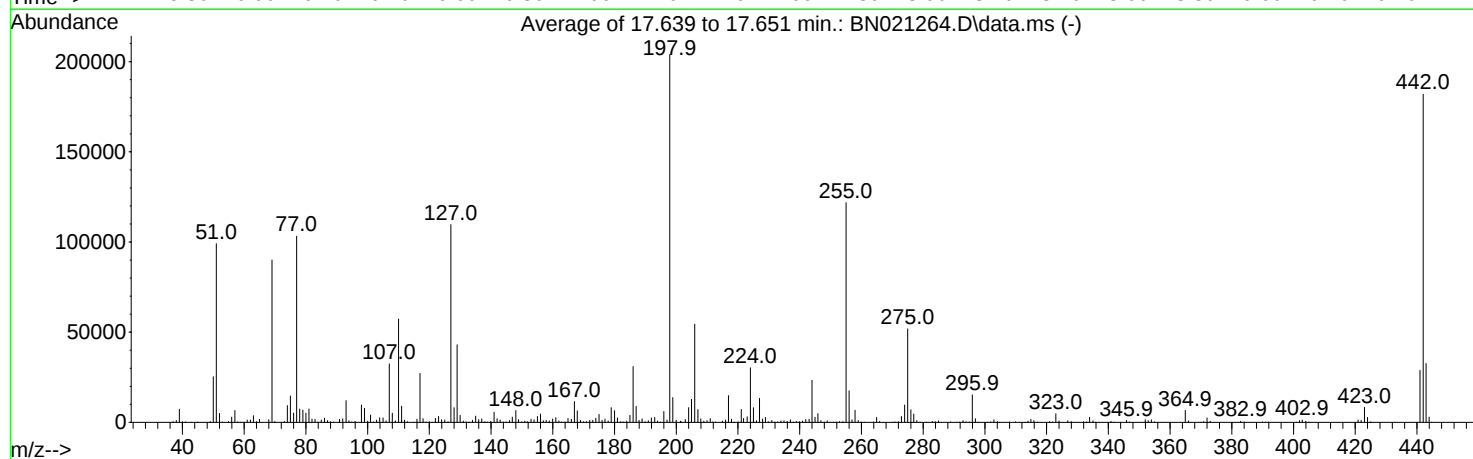


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
 Data File : BN021264.D
 Acq On : 16 Aug 2022 21:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 16 09:19:59 2022

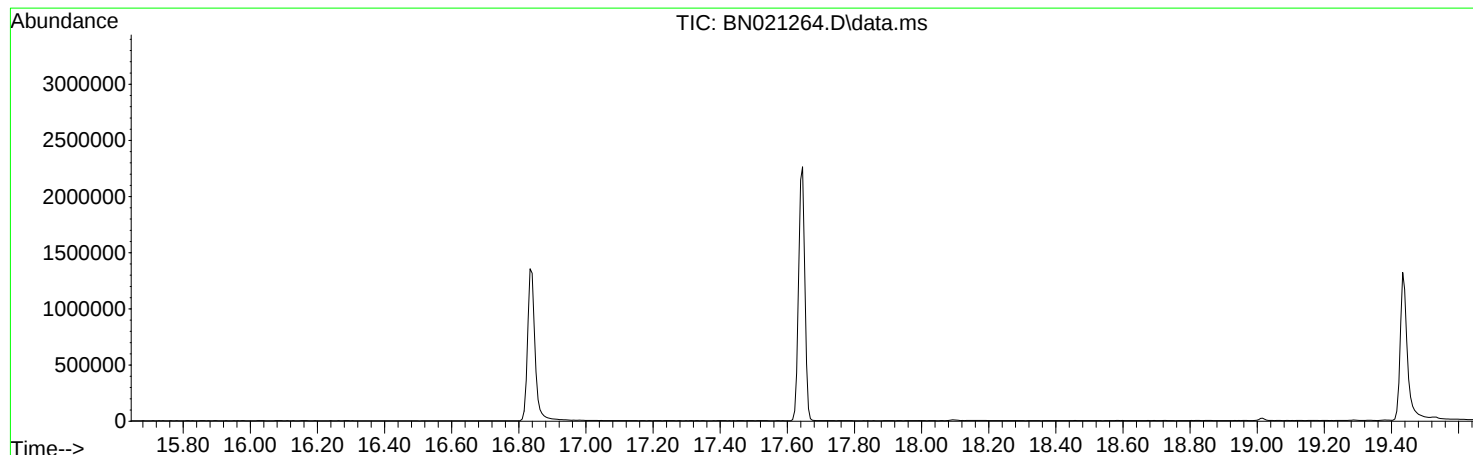

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	99107	PASS
68	69	0.00	2	1.7	1538	PASS
69	198	0.00	100	44.1	90029	PASS
70	69	0.00	2	0.5	411	PASS
127	198	10	80	53.8	109672	PASS
197	198	0.00	2	0.7	1367	PASS
198	198	100	100	100.0	203968	PASS
199	198	5	9	6.7	13713	PASS
275	198	10	60	25.4	51827	PASS
365	198	1	100	3.2	6620	PASS
441	198	0.01	100	14.1	28827	PASS
442	442	50	100	100.0	181952	PASS
443	442	15	24	17.9	32629	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/16/2022	BNA_N	<u>BN021264.D</u>
Compound Name	Response	Retention Time
DDT	704674	20.68
DDD	38046	20.239
DDE	2572	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40618	745292	5.45

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021264.D
Acq On : 16 Aug 2022 21:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 06:35:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 17 06:35:06 2022
Response via : Initial Calibration

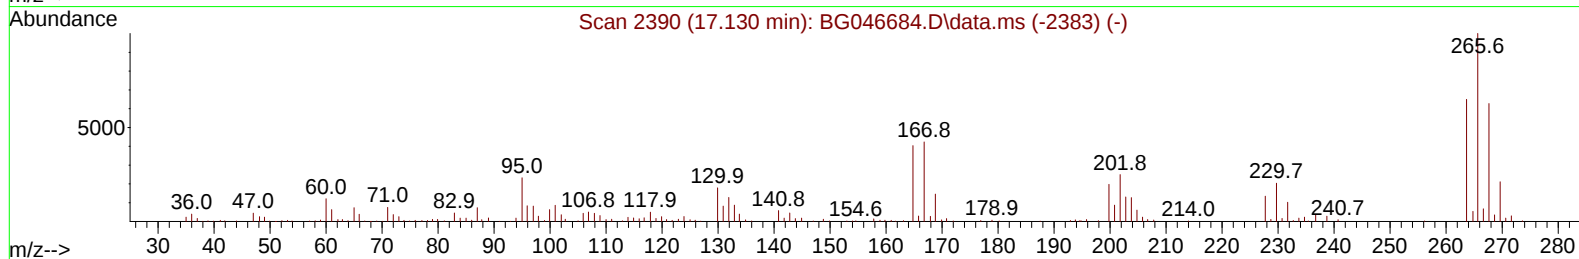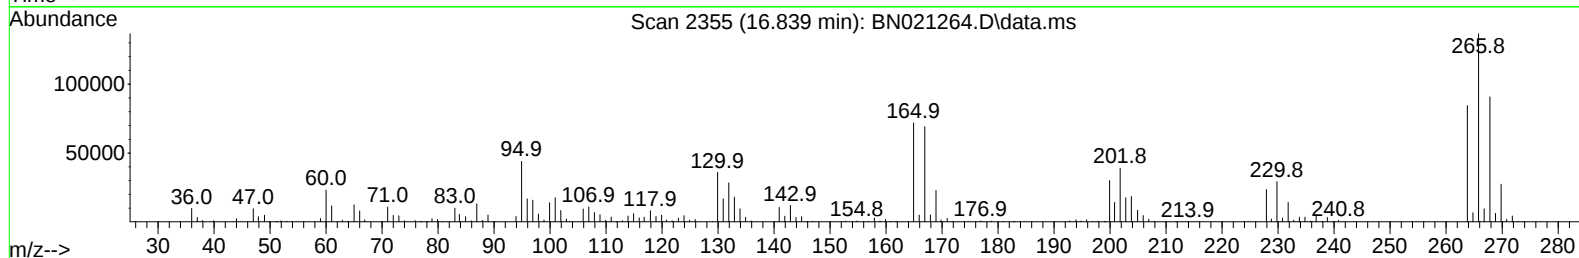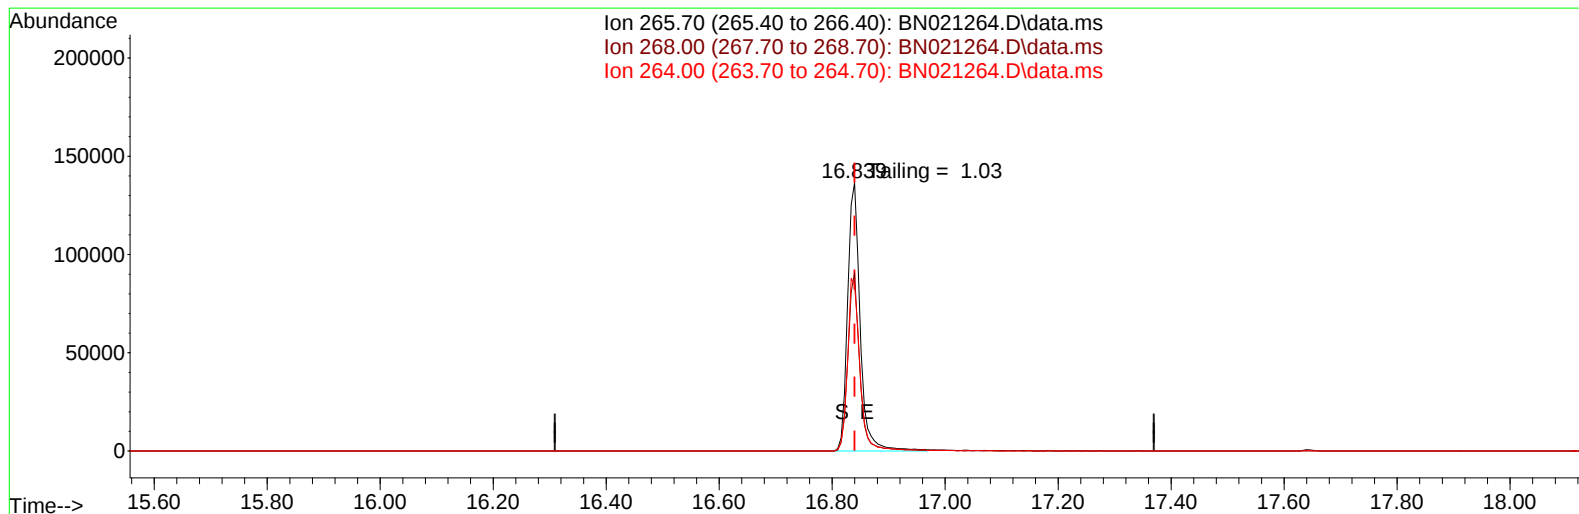

TIC: BN021264.D\data.ms

(70) Pentachlorophenol (C)

16.839min (0.000) 15569.65 ng




response 212727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.41
264.00	61.60	61.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081622\
Data File : BN021264.D
Acq On : 16 Aug 2022 21:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 06:35:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 17 06:35:06 2022
Response via : Initial Calibration

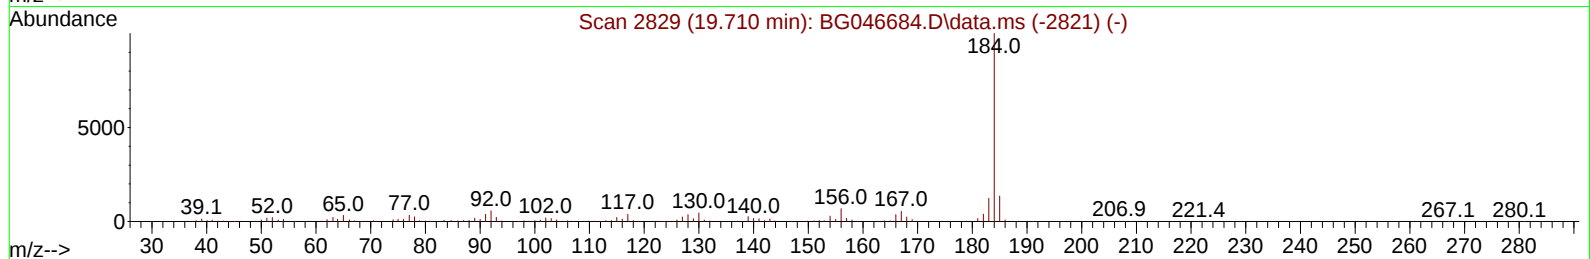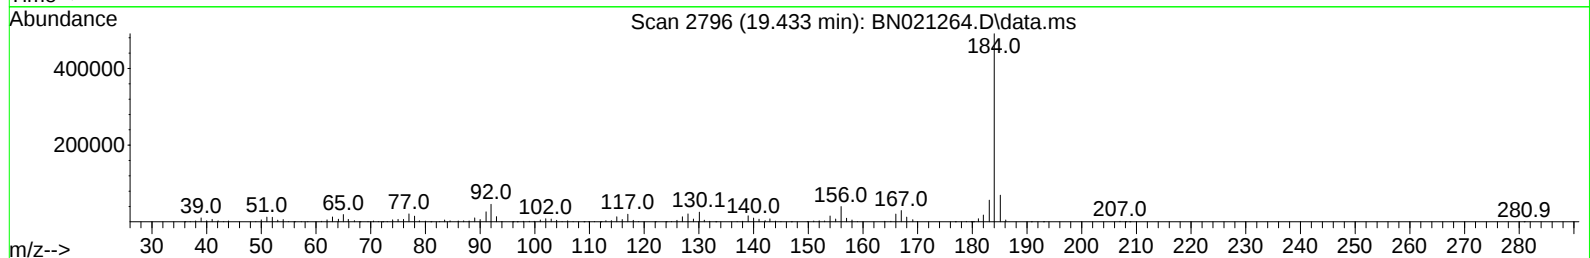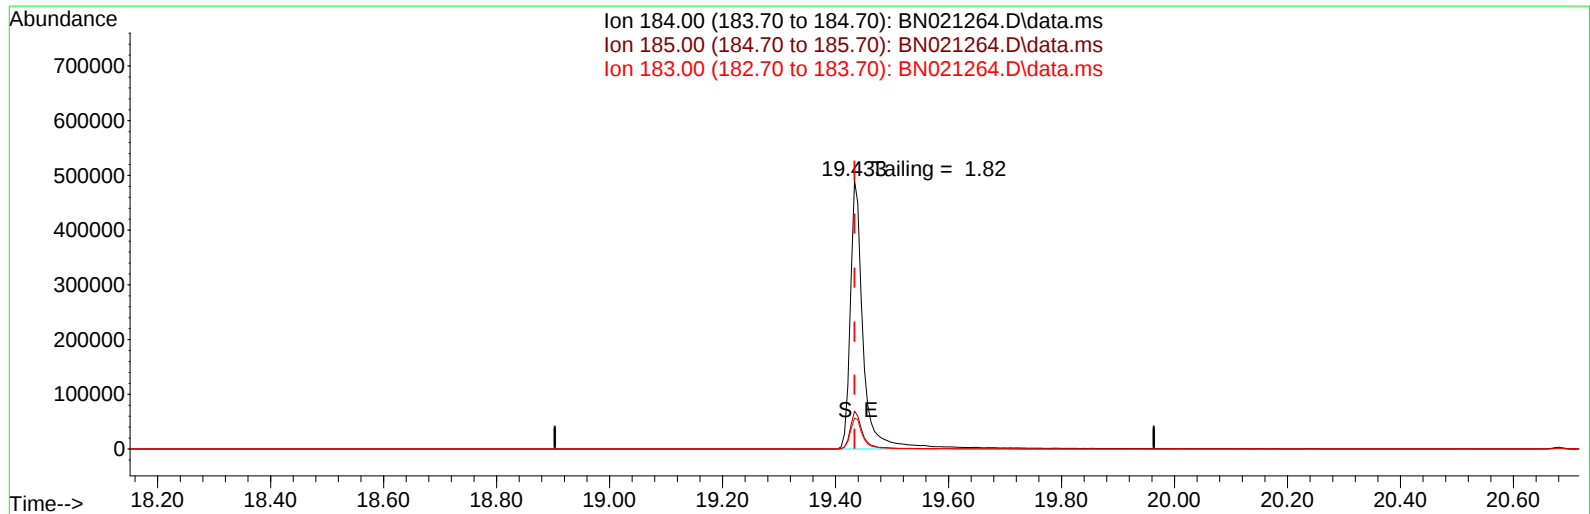

TIC: BN021264.D\data.ms

(77) Benzidine

19.433min (0.000) 0.00 ng

response 780702

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.13
183.00	13.20	11.53
0.00	0.00	0.00