

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081718\
 Data File : BN002390.D
 Acq On : 17 Aug 2018 22:00
 Operator : JU/SJ
 Sample : J4421-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 18 03:24:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 18 03:20:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	174778	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	849193	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	537262	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1259133	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1404920	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1478013	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.24	96	10105	2.73	ng/uL	0.00
5) Phenol-d5	6.86	99	221419	13.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	161348	16.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	187611	15.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	196423	15.33	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	104489	15.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	112547	15.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	191480	14.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	263561	18.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	739132	16.60	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	903408	16.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	83980	9.98	ng/ul	0.00
57) Fluorene-d10	15.30	176	640006	16.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	86689	10.81	ng/ul	0.00
70) Anthracene-d10	17.16	188	1019182	16.94	ng/ul	0.00
78) Pyrene-d10	19.45	212	1181793	17.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1280930	16.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	111444	2.551	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081718\
Data File : BN002390.D
Acq On : 17 Aug 2018 22:00
Operator : JU/SJ
Sample : J4421-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 18 03:24:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 18 03:20:23 2018
Response via : Initial Calibration

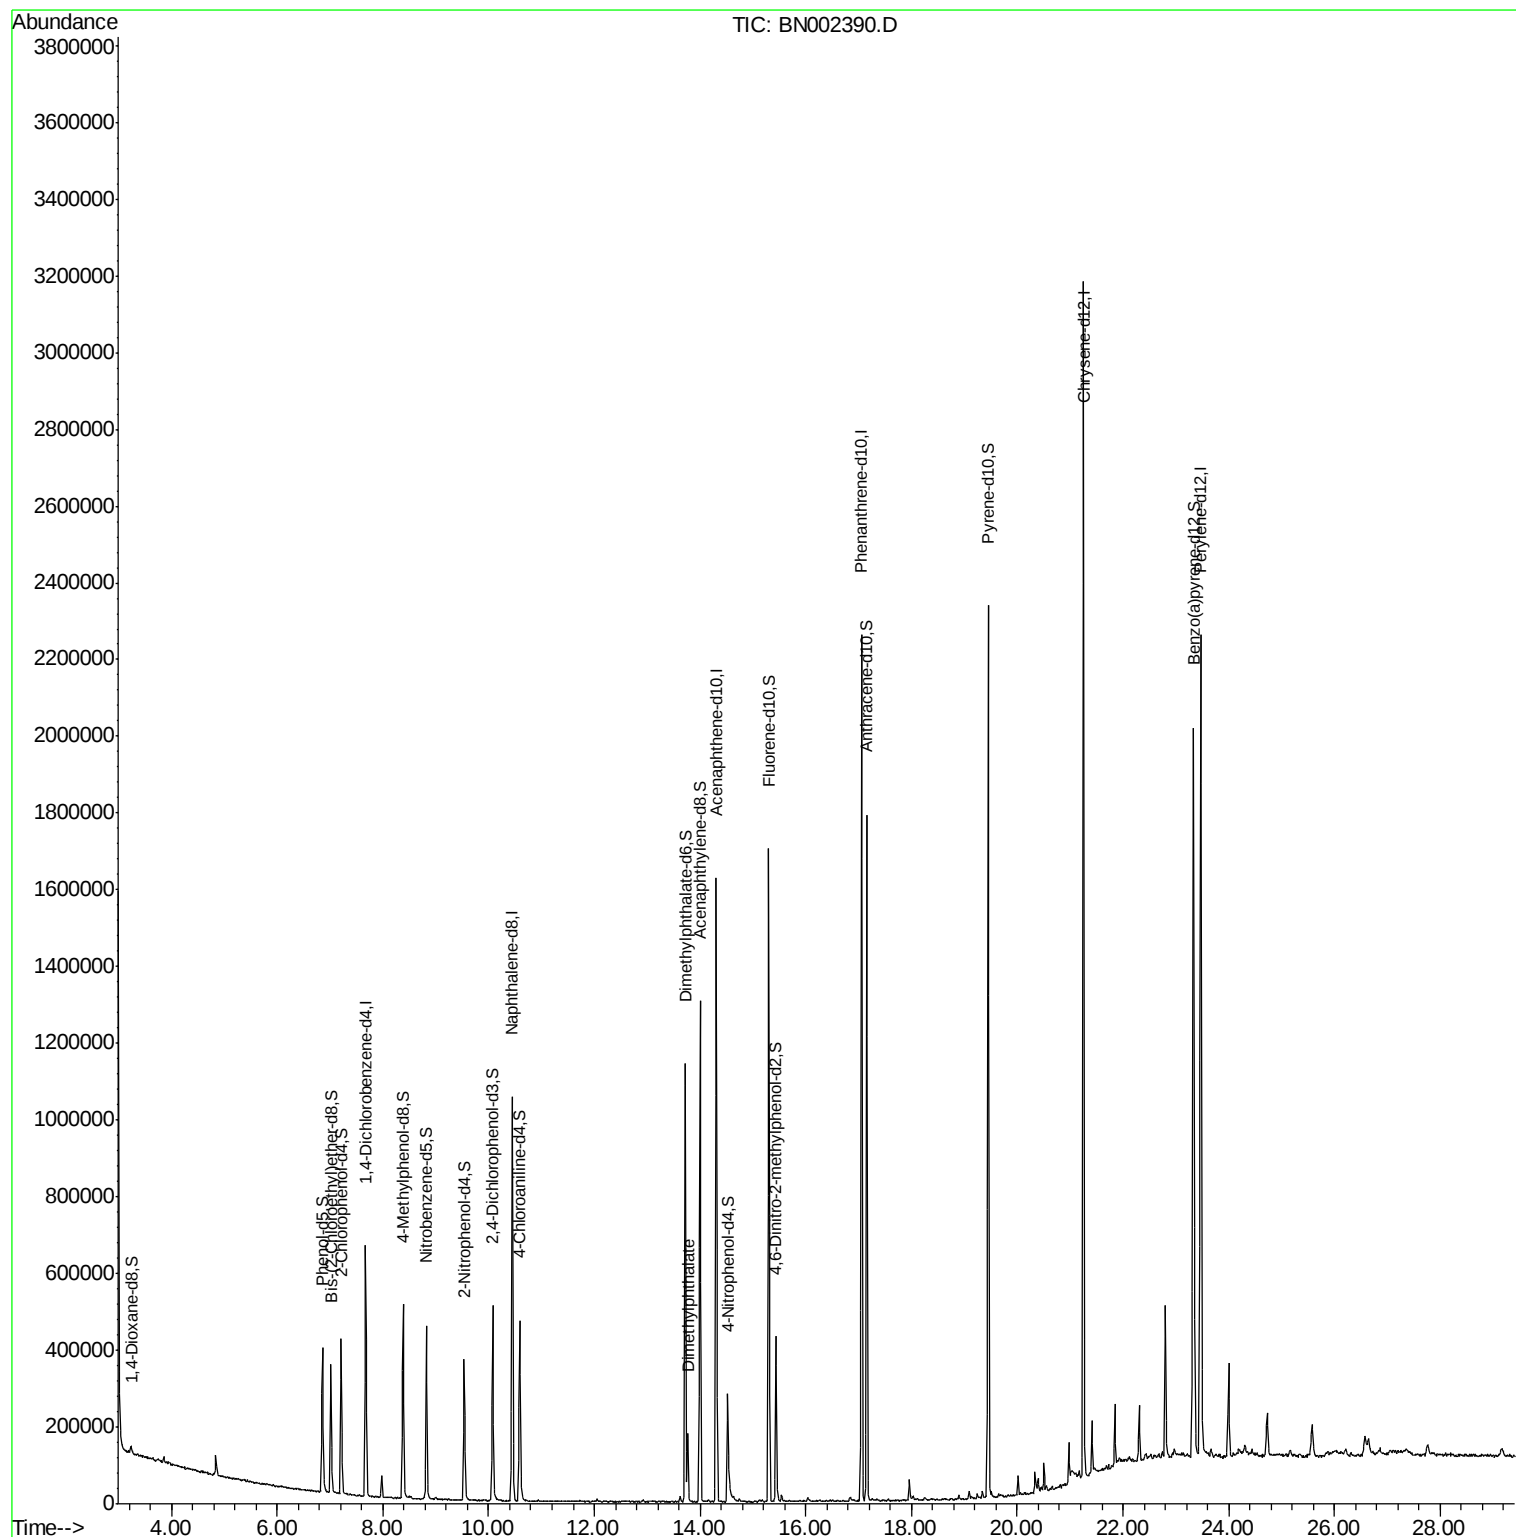

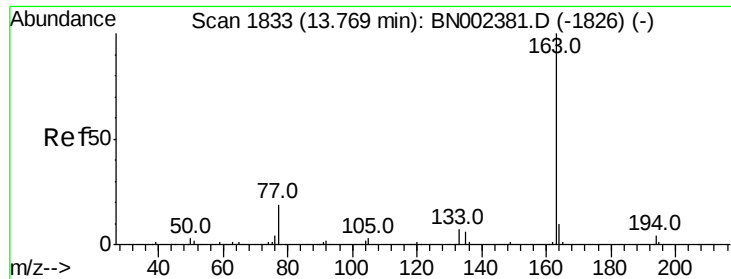

#44

Dimethylphthalate

Concen: 2.551 ng/ul

RT: 13.77 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BN002390.D

Acq: 17 Aug 2018 22:00

Instrument :

BNA_N

ClientSampleId :

Tot Ion:163 Resp: 111444

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.1 7.8 11.8

