

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081718\
 Data File : BN002383.D
 Acq On : 17 Aug 2018 17:50
 Operator : JU/SJ
 Sample : J4424-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YR7

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:14:06 PM

Quant Time: Aug 18 03:58:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 18 03:20:23 2018
 Response via : Initial Calibration

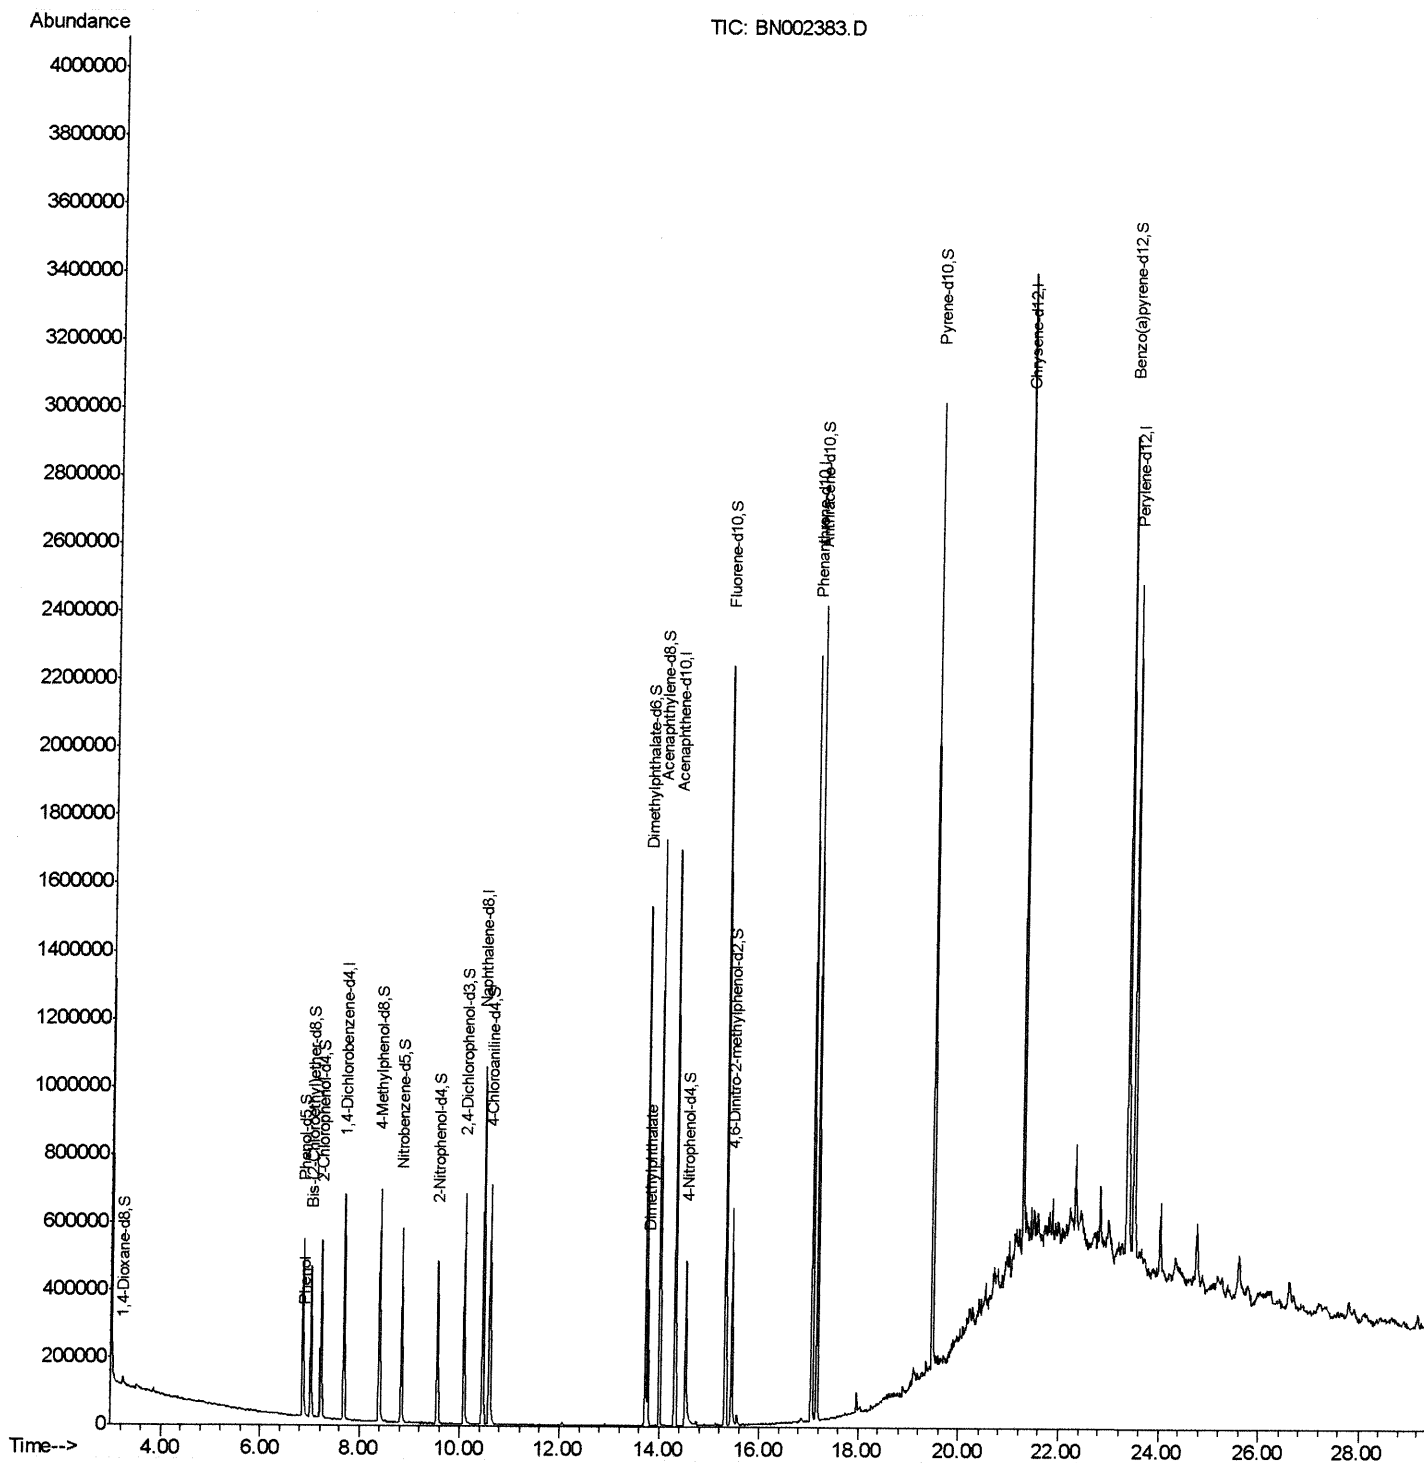

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081718\
 Data File : BN002383.D
 Acq On : 17 Aug 2018 17:50
 Operator : JU/SJ
 Sample : J4424-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YR7

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:14:06 PM

Quant Time: Aug 18 03:23:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 18 03:20:23 2018
 Response via : Initial Calibration

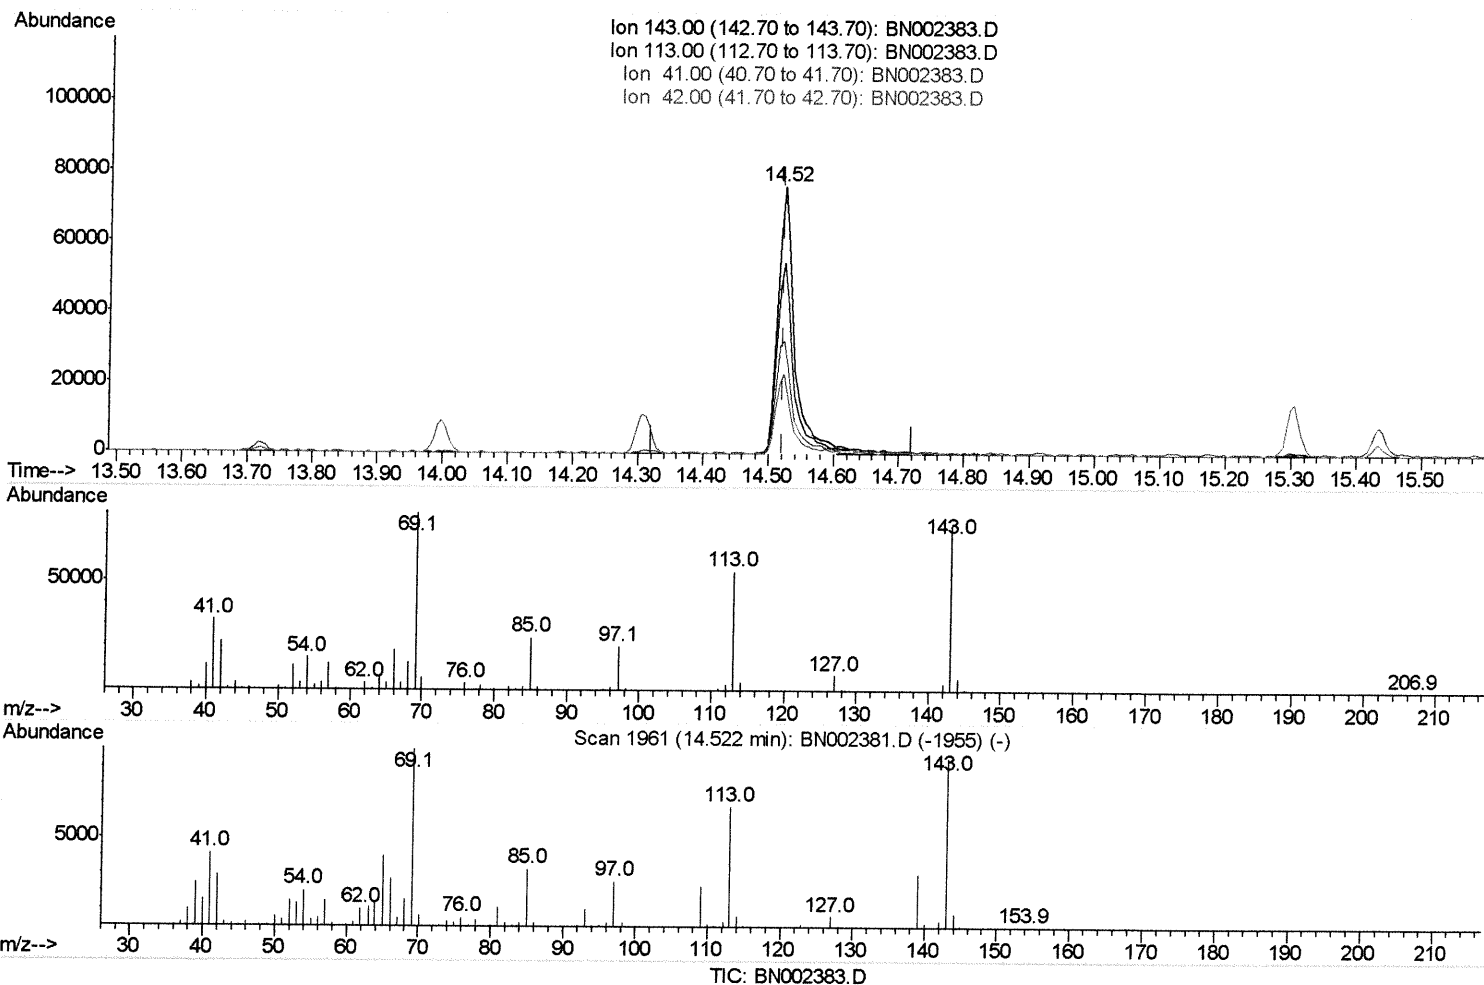

(51) 4-Nitrophenol-d4 (S)

14.522min (+0.000) 15.54ng/ui

response 133947

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	71.49
41.00	28.80	42.42#
42.00	19.10	29.79#

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081718\
 Data File : BN002383.D
 Acq On : 17 Aug 2018 17:50
 Operator : JU/SJ
 Sample : J4424-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YR7

Manual Integrations
 APPROVED

Sohil
 8/20/2018 4:14:06 PM

Quant Time: Aug 18 03:23:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 18 03:20:23 2018
 Response via : Initial Calibration

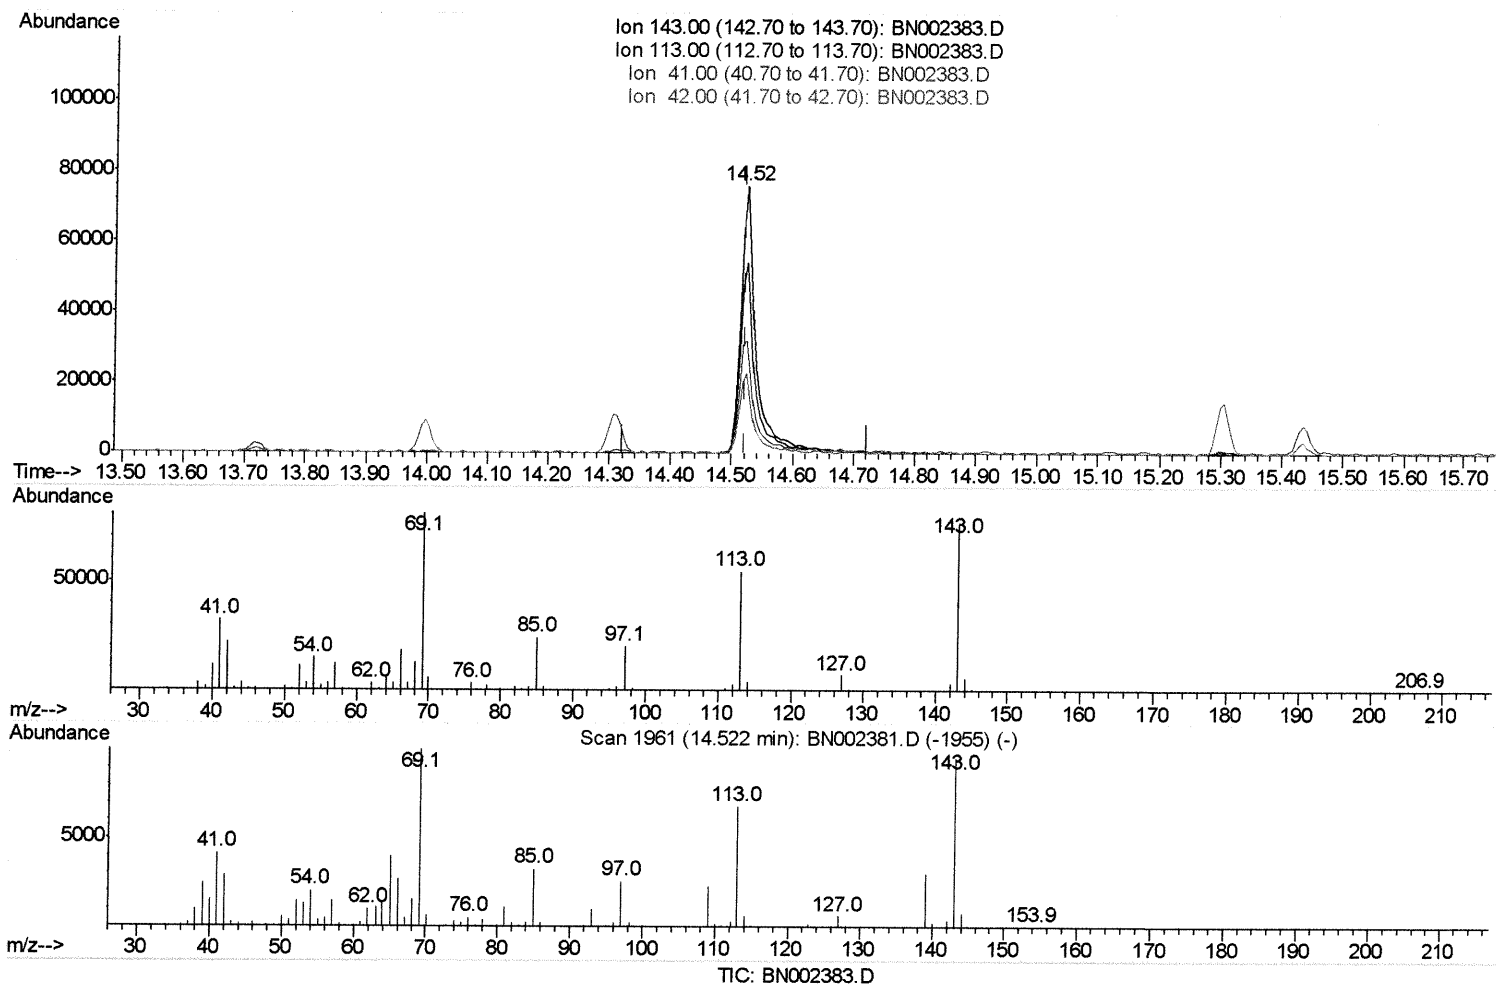

(51) 4-Nitrophenol-d4 (S)

14.522min (+0.000) 16.56ng/ul m

5/8/20/18

response 142746

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	71.49
41.00	28.80	42.42#
42.00	19.10	29.79#

Quantitation Report (QT Reviewed)

Instrument :
BNA_N
ClientSampleId :
A3YR7

Manual Integrations
APPROVED

Sohil
8/20/2018 4:14:06 PM

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081718\
Data File : BN002383.D
Acq On : 17 Aug 2018 17:50
Operator : JU/SJ
Sample : J4424-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 18 03:58:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 18 03:20:23 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	176509	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	857337	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	550197	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1269553	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1298815	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1389716	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	14144	3.78	ng/uL	0.00
5) Phenol-d5	6.86	99	307586	19.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	212027	20.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	253232	20.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	267829	20.70	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	138900	20.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	151415	21.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	259856	19.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	390172	27.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	983518	21.56	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1194281	21.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	142746m	16.56	ng/ul	0.00
57) Fluorene-d10	15.30	176	838223	21.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	125622	15.54	ng/ul	0.00
70) Anthracene-d10	17.16	188	1353185	22.31	ng/ul	0.00
78) Pyrene-d10	19.45	212	1476913	23.76	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1583933	21.80	ng/ul	0.00

5/18/20/18

Target Compounds

				Ovalue	
6) Phenol	6.88	94	31112	1.888	ng/ul# 92
44) Dimethylphthalate	13.77	163	267125	5.972	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed