

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011449.D
 Acq On : 17 Aug 2020 12:30
 Operator : CG/JU
 Sample : L3611-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFL5

Quant Time: Aug 17 13:15:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 14 15:37:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	136935	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	475194	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	281611	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	670891	20.00	ng/ul	0.00
78) Chrysene-d12	21.05	240	611452	20.00	ng/ul	0.00
86) Perylene-d12	23.15	264	681196	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	8393	2.94	ng/uL	0.00
5) Phenol-d5	6.64	99	137303	14.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	83183	16.85	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	131065	15.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	81282	10.34	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	74788	20.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	80278	19.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	125947	16.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	136877	14.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	417219	19.03	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	456519	17.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	33752	9.09	ng/ul	0.00
58) Fluorene-d10	15.07	176	356804	18.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.21	200	47967	10.78	ng/ul	0.00
71) Anthracene-d10	16.92	188	553953	17.29	ng/ul	0.00
79) Pyrene-d10	19.23	212	527760	16.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	629210	16.63	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.54	163	95217	4.230	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011449.D
Acq On : 17 Aug 2020 12:30
Operator : CG/JU
Sample : L3611-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFL5

Quant Time: Aug 17 13:15:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 14 15:37:33 2020
Response via : Initial Calibration

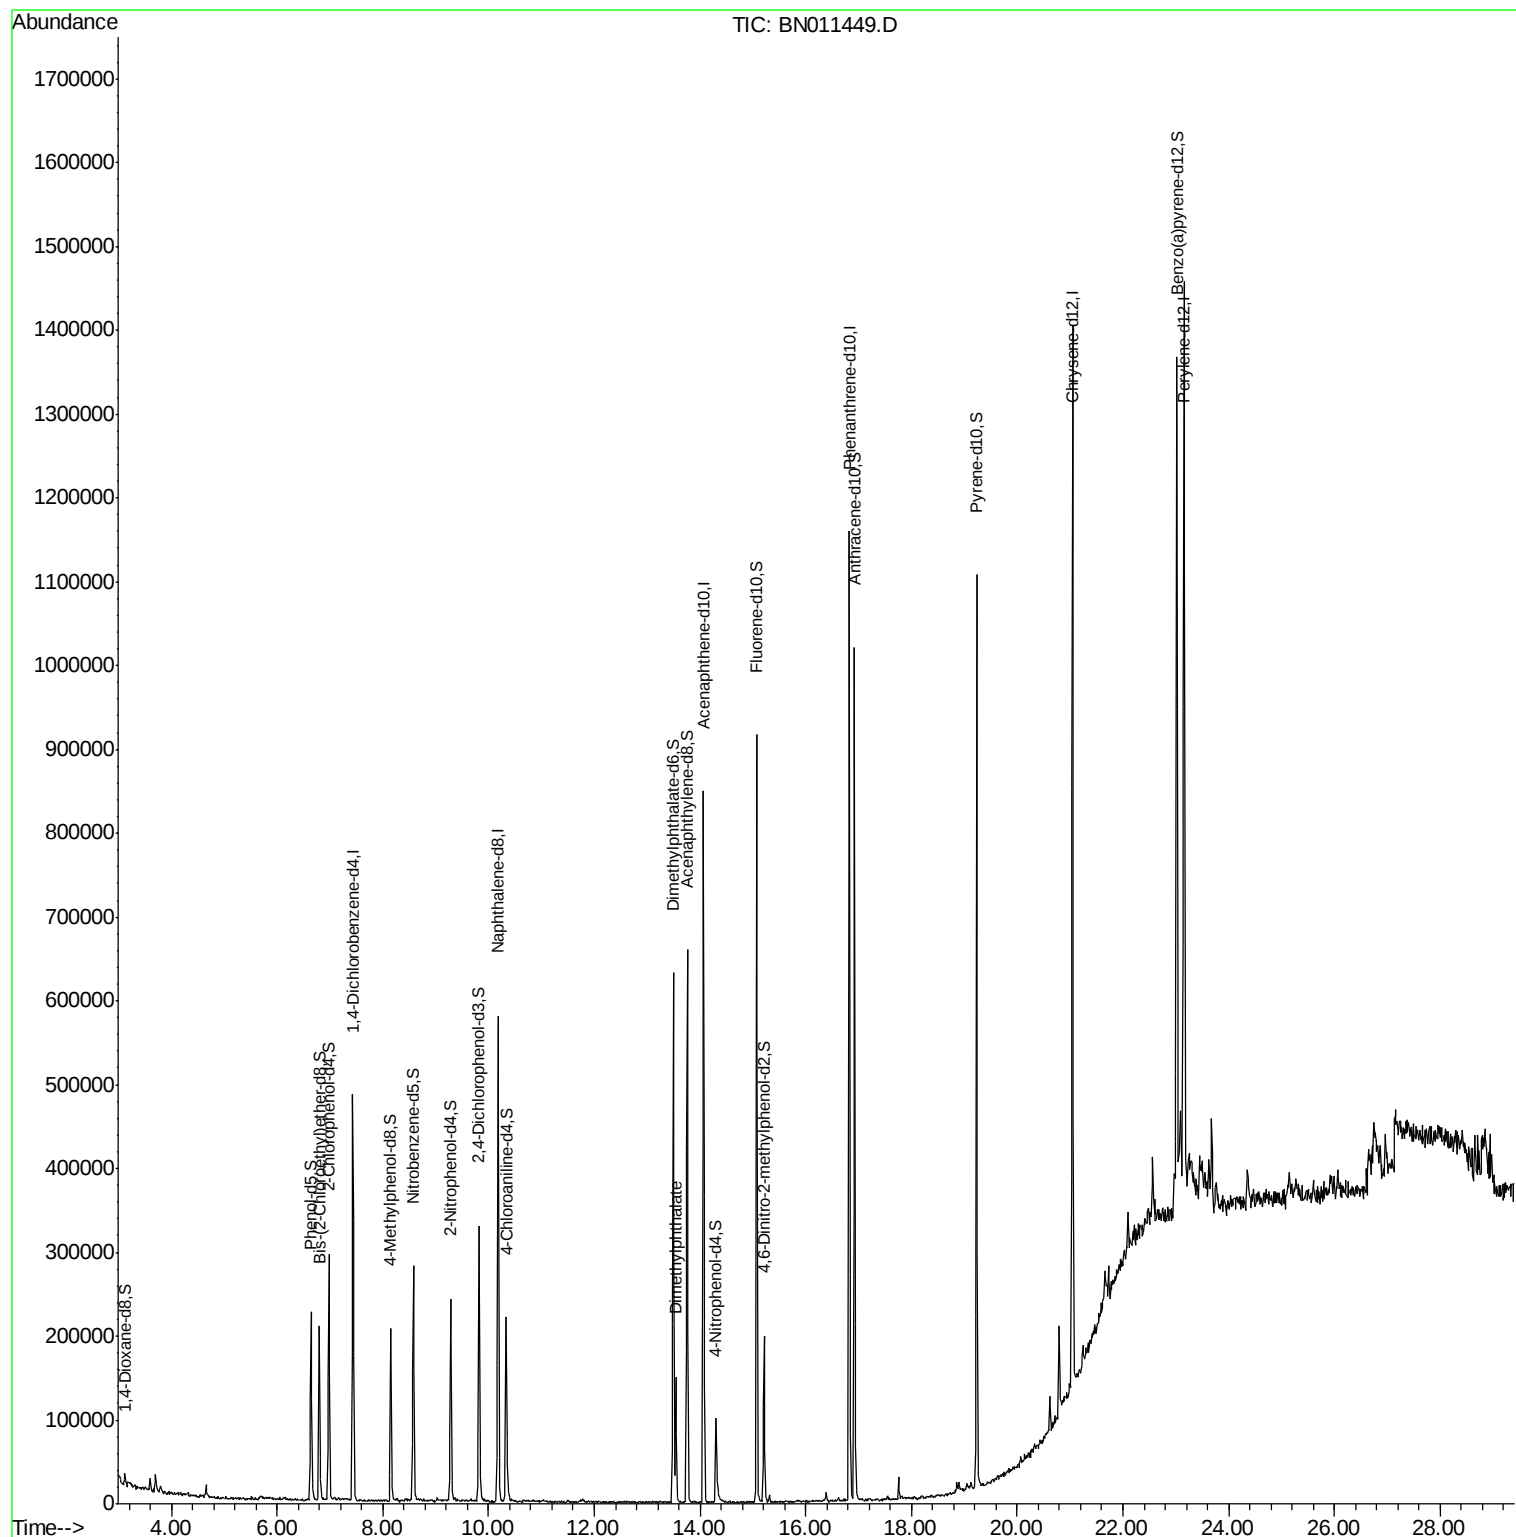

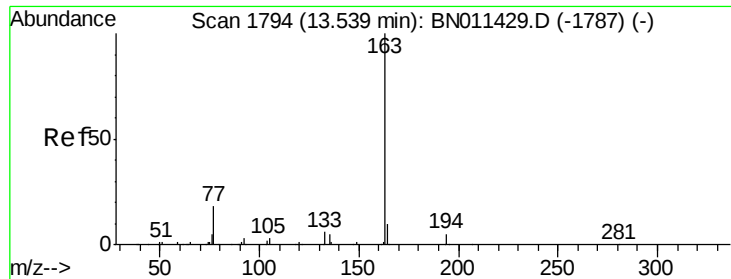

#45

Dimethylphthalate

Concen: 4.230 ng/ul

RT: 13.54 min Scan# 1794

Delta R.T. -0.01 min

Lab File: BN011449.D

Acq: 17 Aug 2020 12:30

Instrument :

BNA_N

ClientSampleId :

DBFL5

Tot Ion:163 Resp: 95217

Ion Ratio Lower Upper

163 100

194 3.7 3.8 5.6#

164 11.0 8.7 13.1

