

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011450.D
 Acq On : 17 Aug 2020 13:06
 Operator : CG/JU
 Sample : L3611-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFM2

Quant Time: Aug 17 14:05:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 14 15:37:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	131891	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	493493	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	288738	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	616182	20.00	ng/ul	0.00
78) Chrysene-d12	21.05	240	741758	20.00	ng/ul	0.00
86) Perylene-d12	23.16	264	698152	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	5314	1.93	ng/uL	0.00
5) Phenol-d5	6.64	99	85602	9.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	51930	10.92	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	82630	9.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	70598	9.32	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	40636	10.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	43583	10.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	80967	9.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	95833	9.86	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	293112	13.04	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	309921	11.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	24258	6.37	ng/ul	0.00
58) Fluorene-d10	15.07	176	240865	12.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.21	200	31453	7.70	ng/ul	0.00
71) Anthracene-d10	16.92	188	381709	12.97	ng/ul	0.00
79) Pyrene-d10	19.23	212	519780	13.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	506557	13.06	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.54	163	60054	2.602	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011450.D
Acq On : 17 Aug 2020 13:06
Operator : CG/JU
Sample : L3611-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFM2

Quant Time: Aug 17 14:05:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 14 15:37:33 2020
Response via : Initial Calibration

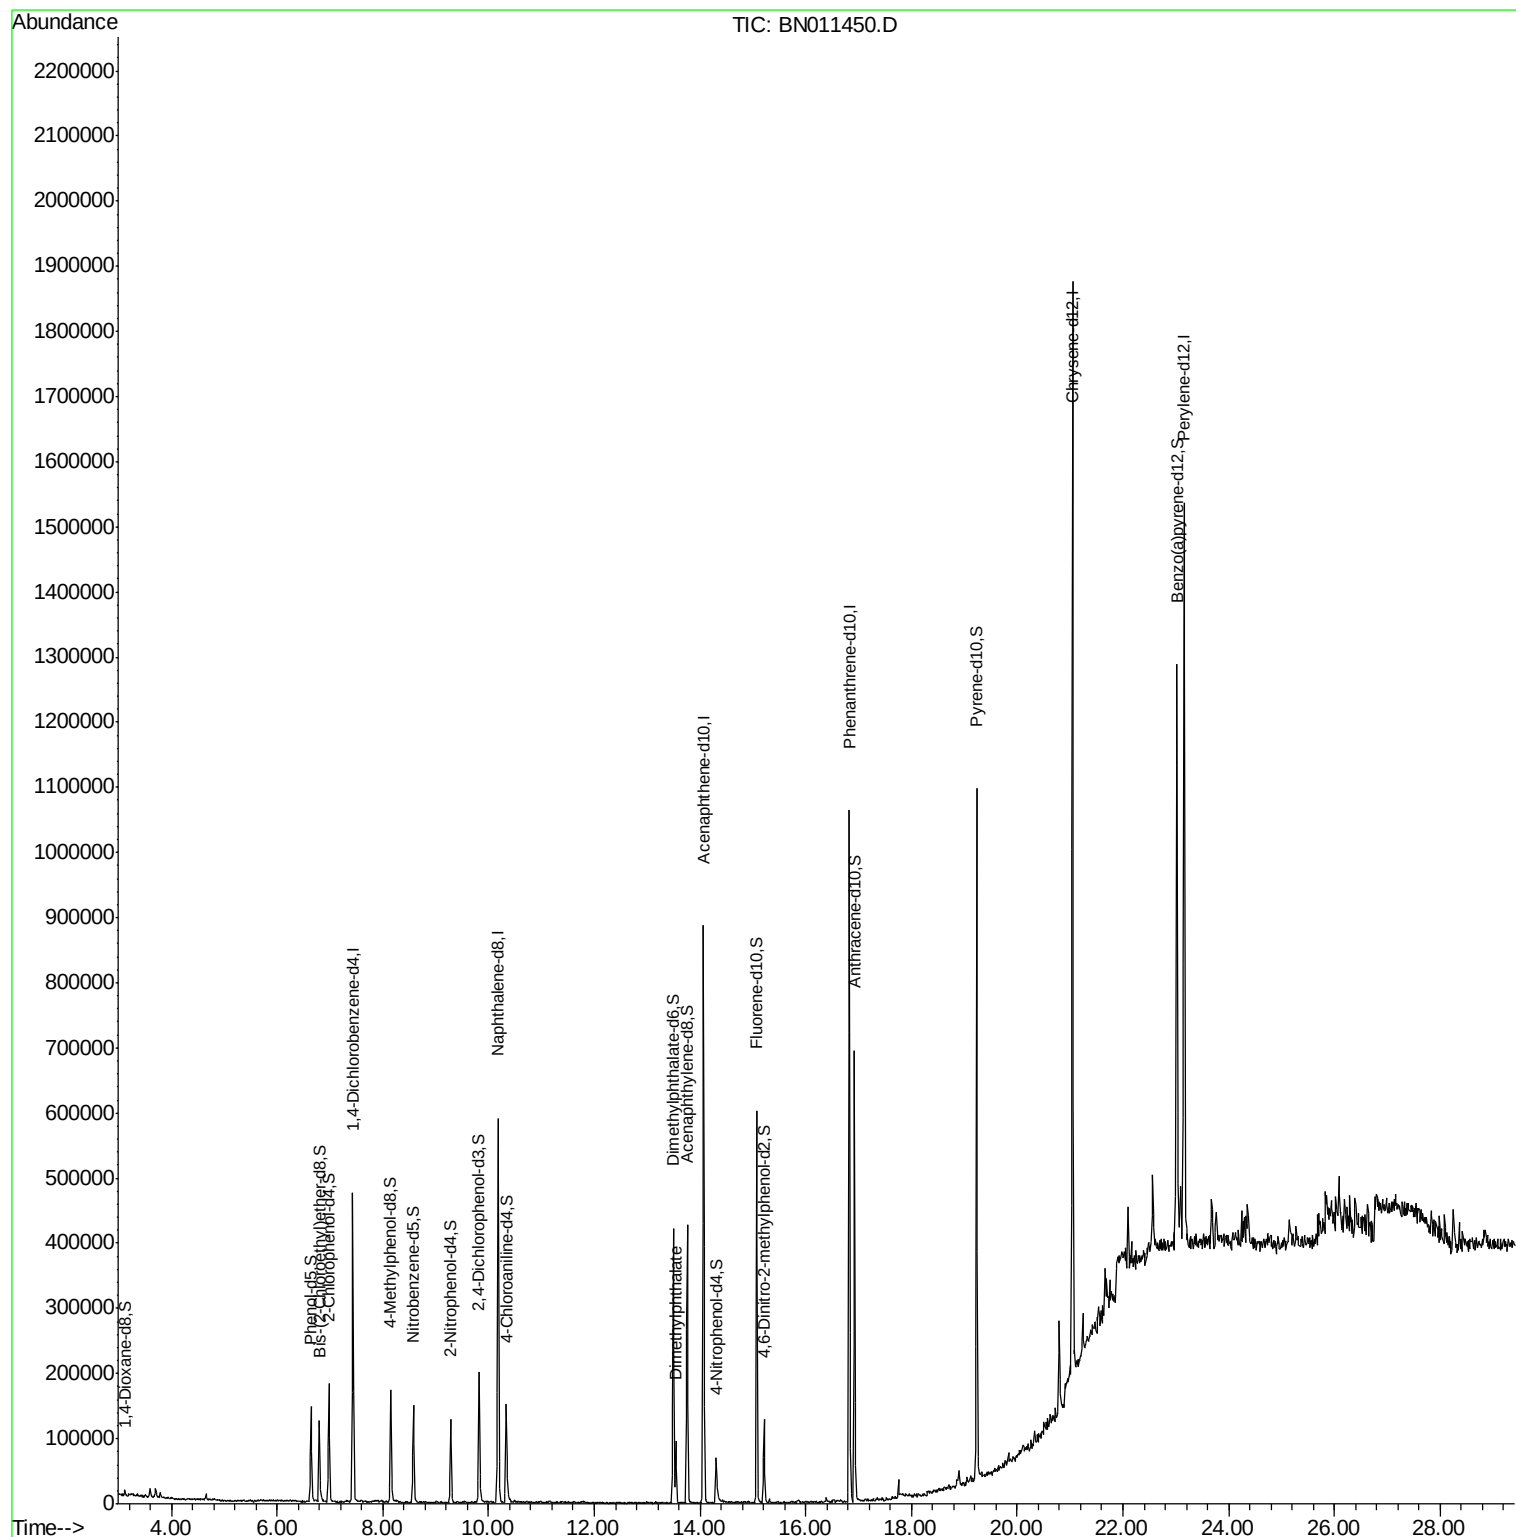

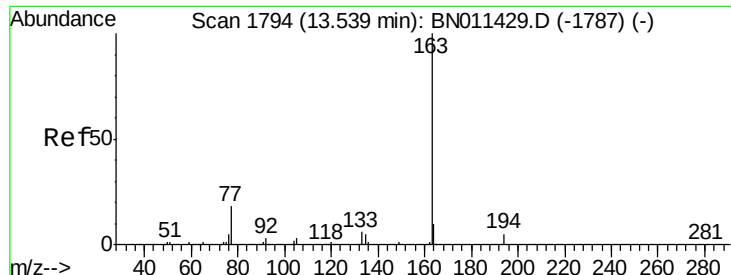

#45

Dimethylphthalate

Concen: 2.602 ng/ul

RT: 13.54 min Scan# 1794

Delta R.T. -0.01 min

Lab File: BN011450.D

Acq: 17 Aug 2020 13:06

Instrument :

BNA_N

ClientSampleId :

DBFM2


Tot Ion:163 Resp: 60054

Ion Ratio Lower Upper

163 100

194 4.6 3.8 5.6

164 11.0 8.7 13.1

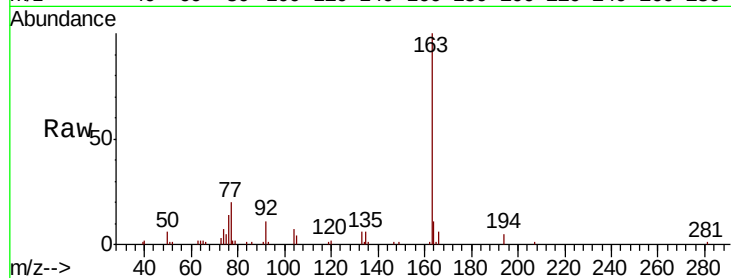

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

