

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011498.D
 Acq On : 18 Aug 2020 23:18
 Operator : CG/JU
 Sample : L3668-14
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW4

Quant Time: Aug 19 02:22:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 19 02:19:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	189731	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	637180	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	403397	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	867759	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	992662	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	916870	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	20909	5.29	ng/uL	0.00
5) Phenol-d5	6.63	99	83780	6.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	204193	29.86	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	277764	23.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.14	113	135735	12.46	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	145604	29.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	170324	30.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.81	165	296145	28.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	18801	1.50	ng/ul	0.01
44) Dimethylphthalate-d6	13.49	166	940729	29.95	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	1100765	29.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	23944	4.50	ng/ul	0.00
58) Fluorene-d10	15.07	176	879691	31.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	142689	24.79	ng/ul	0.00
71) Anthracene-d10	16.92	188	1428157	34.45	ng/ul	0.00
79) Pyrene-d10	19.23	212	1613928	31.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	1698946	33.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.54	163	142640	4.424	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011498.D
Acq On : 18 Aug 2020 23:18
Operator : CG/JU
Sample : L3668-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW4

Quant Time: Aug 19 02:22:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 19 02:19:14 2020
Response via : Initial Calibration

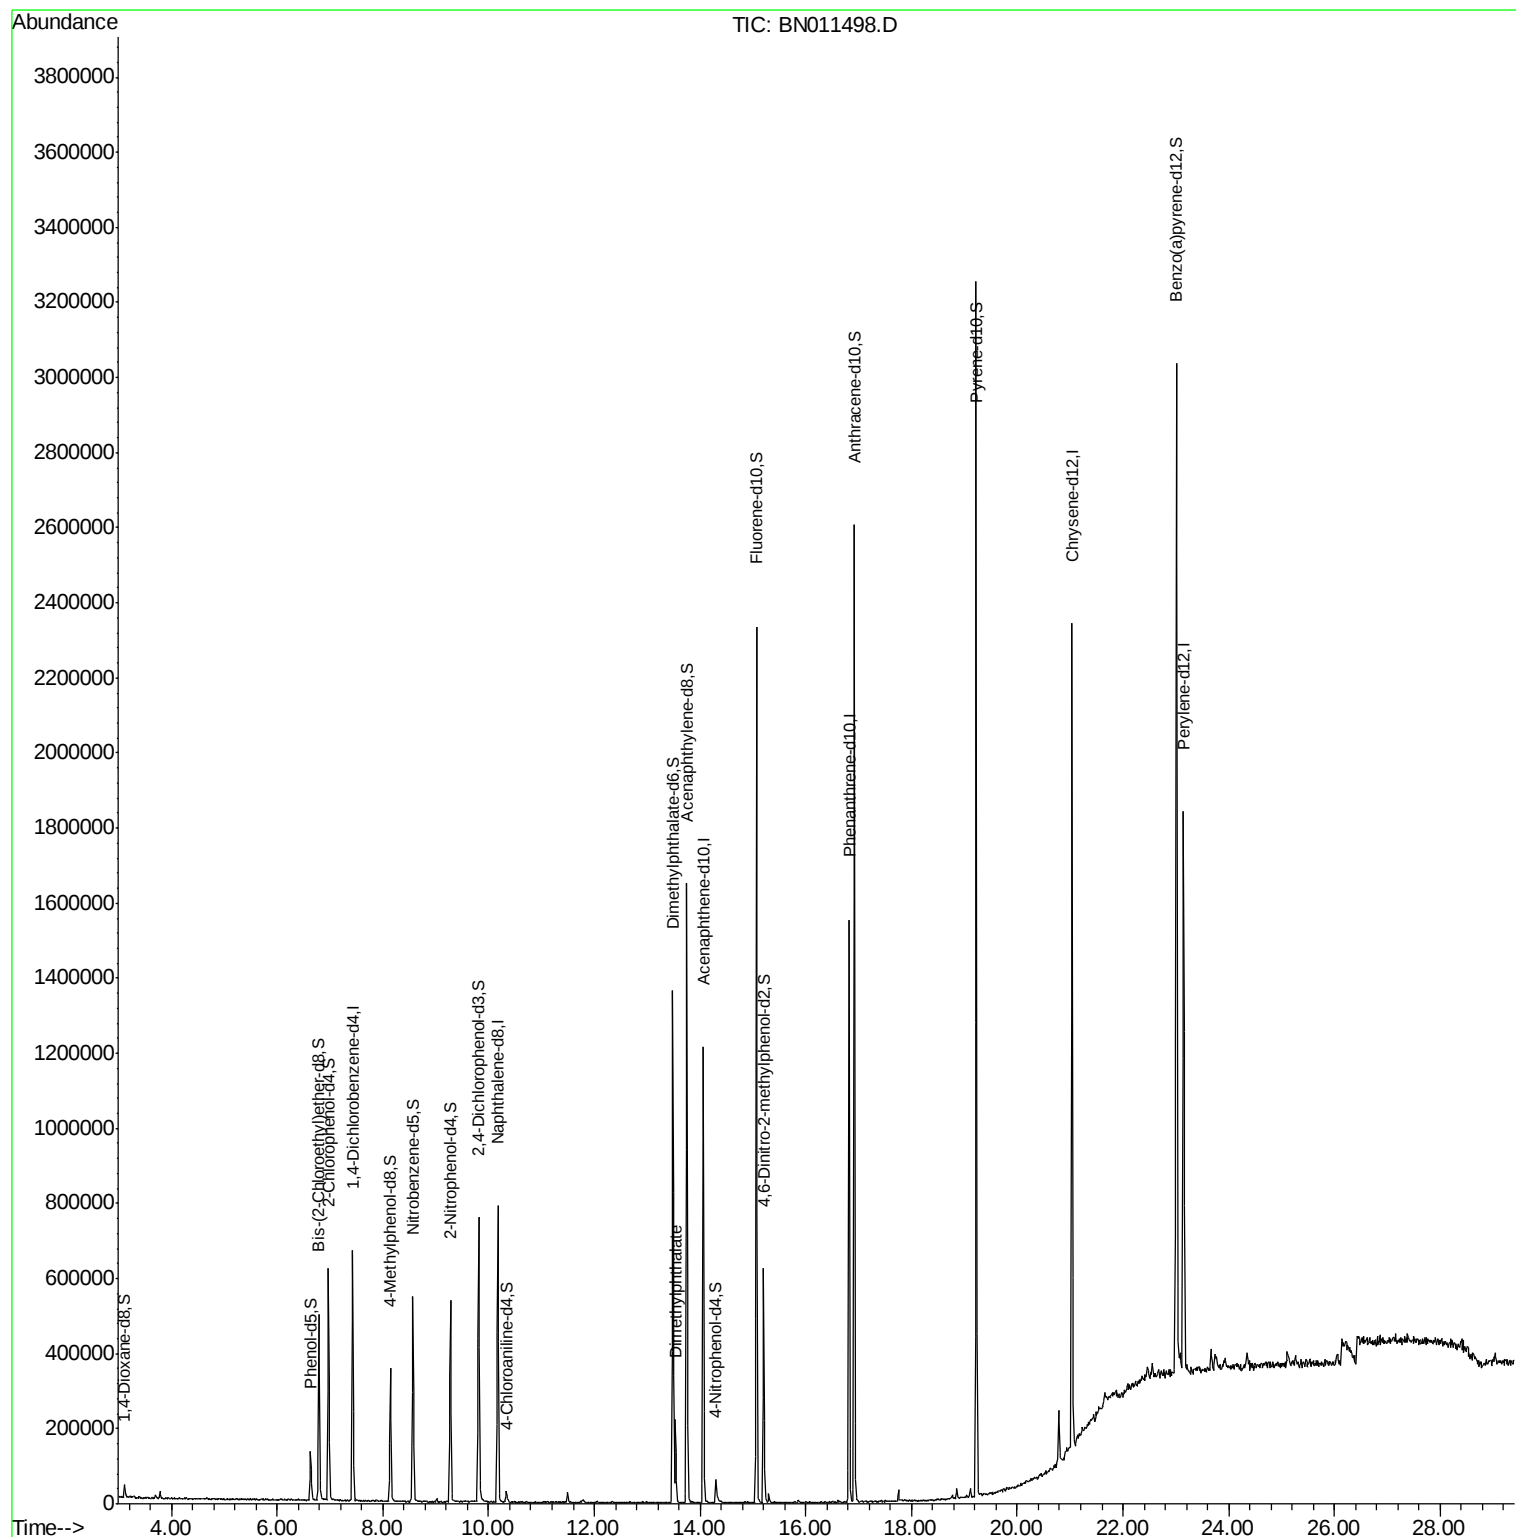


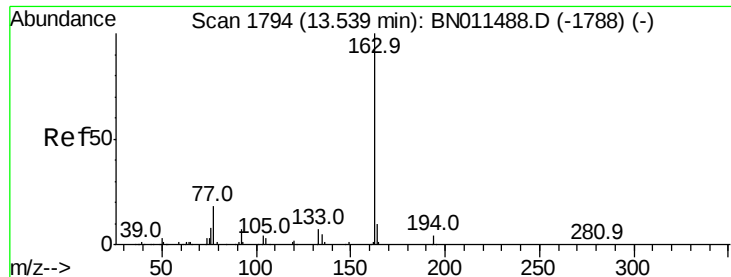

#45
 Dimethylphthalate
 Concen: 4.424 ng/ul
 RT: 13.54 min Scan# 1794
 Delta R.T. 0.00 min
 Lab File: BN011498.D
 Acq: 18 Aug 2020 23:18

Instrument :
 BNA_N
 ClientSampleId :
 DBFW4

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.8	5.6
164	8.5	8.7	13.1#

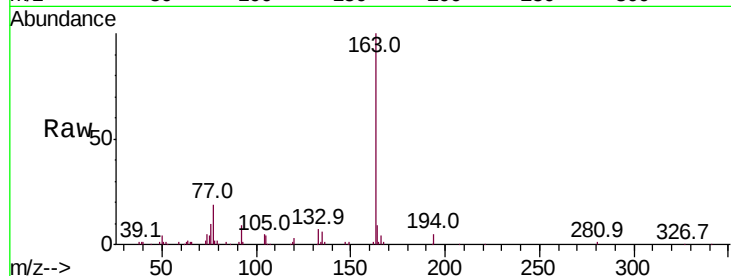

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

