

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011502.D
 Acq On : 19 Aug 2020 01:41
 Operator : CG/JU
 Sample : L3668-09
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFT4

Quant Time: Aug 19 02:22:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 19 02:19:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	158581	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	655870	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	380589	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	827105	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	977303	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	977572	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	18980	5.74	ng/uL	0.00
5) Phenol-d5	6.63	99	70148	6.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	189878	33.22	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	267912	26.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.14	113	141276	15.52	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	142555	28.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	162500	28.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.81	165	306186	28.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	26634	2.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	949652	32.05	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	1091417	30.60	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	25632	5.11	ng/ul	0.00
58) Fluorene-d10	15.07	176	925616	35.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	152642	27.83	ng/ul	0.00
71) Anthracene-d10	16.92	188	1313083	33.23	ng/ul	0.00
79) Pyrene-d10	19.23	212	1533768	30.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	1875690	34.55	ng/ul	0.00

Target Compounds


				Ovalue	
45) Dimethylphthalate	13.53	163	141740	4.660	ng/ul# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011502.D
Acq On : 19 Aug 2020 01:41
Operator : CG/JU
Sample : L3668-09
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFT4

Quant Time: Aug 19 02:22:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 19 02:19:14 2020
Response via : Initial Calibration

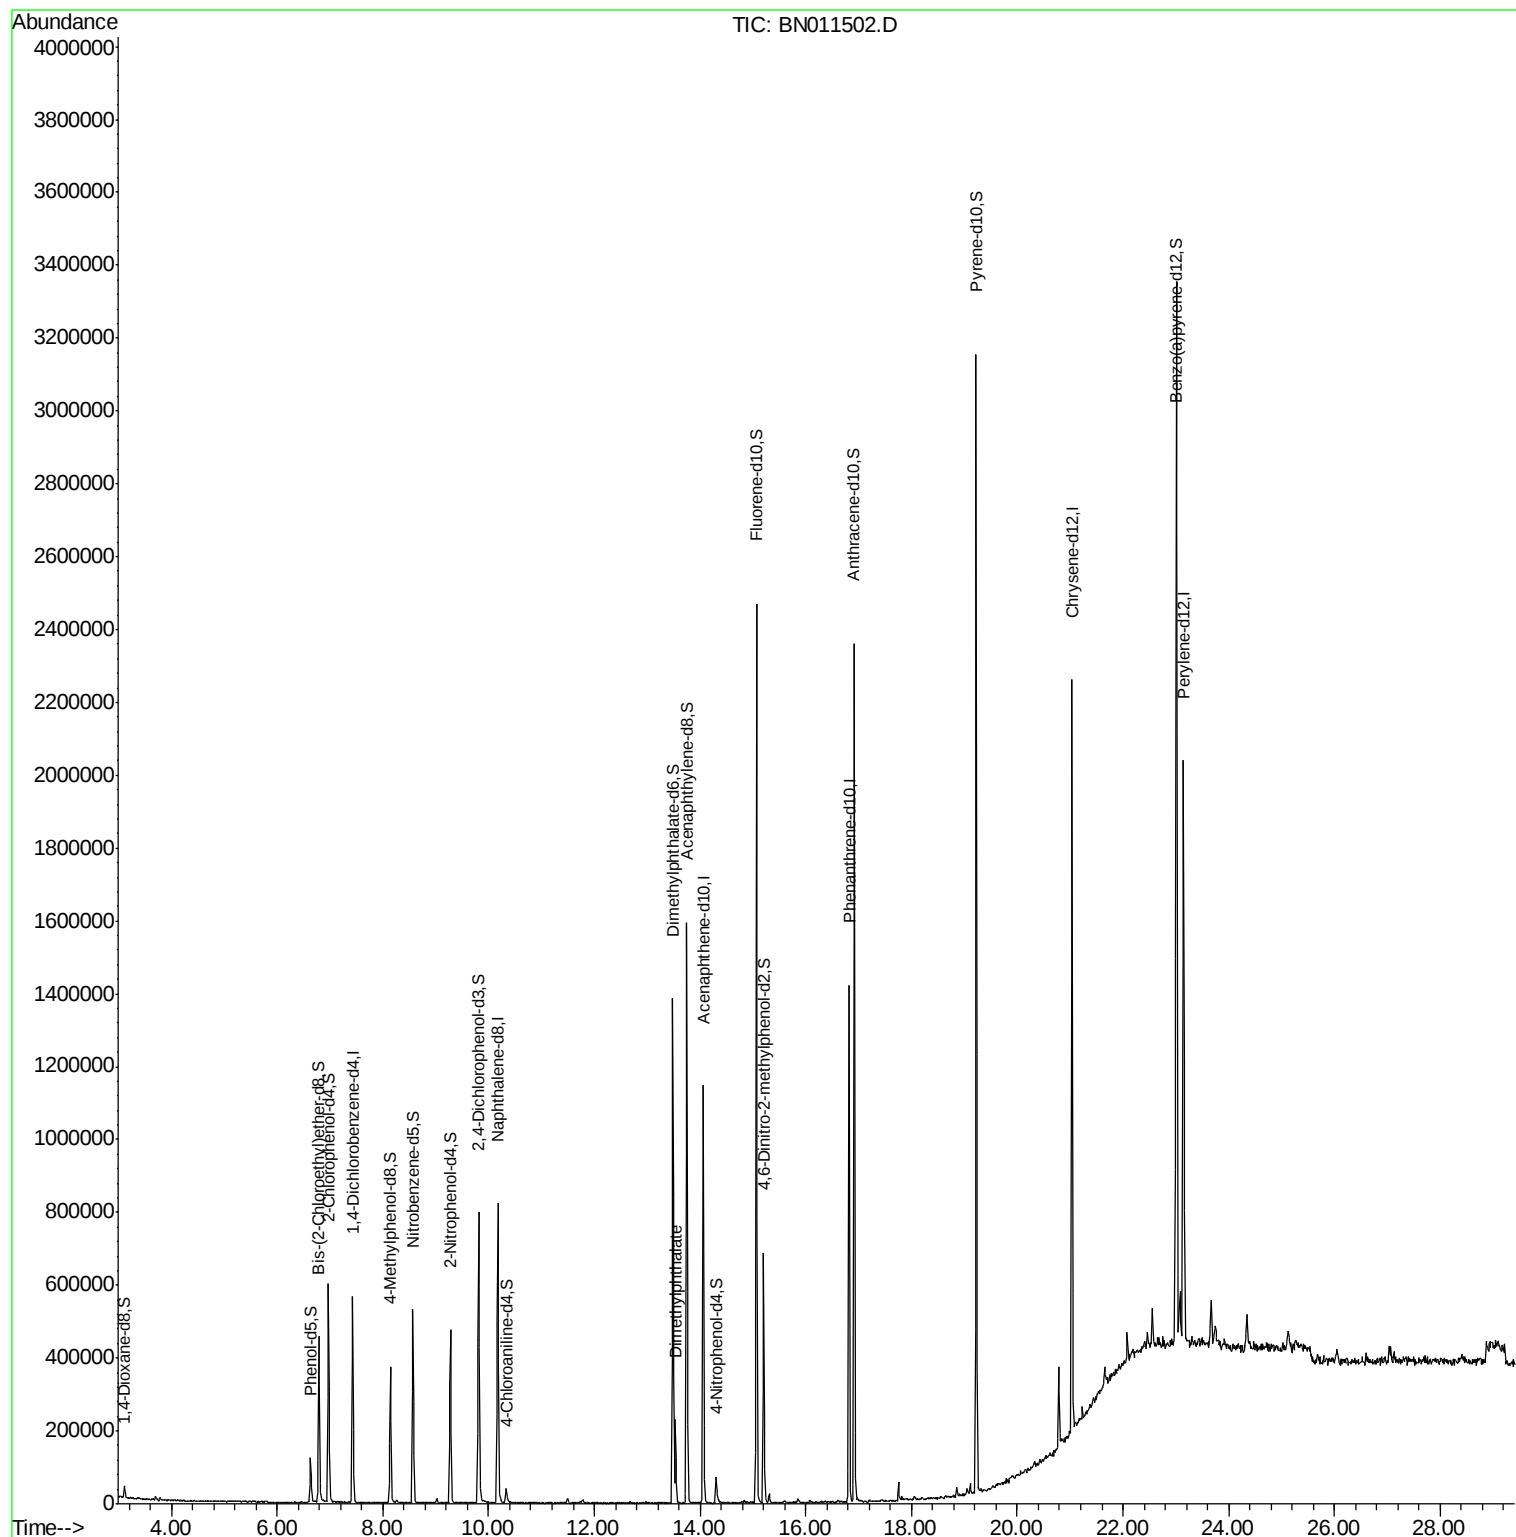

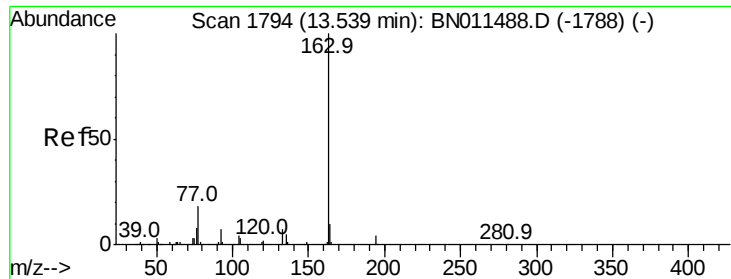

#45

Dimethylphthalate

Concen: 4.660 ng/ul

RT: 13.53 min Scan# 1793

Delta R.T. -0.01 min

Lab File: BN011502.D

Acq: 19 Aug 2020 01:41

Instrument :

BNA_N

ClientSampleId :

DBFT4


Tot Ion:163 Resp: 141740

Ion Ratio Lower Upper

163 100

194 3.5 3.8 5.6#

164 9.8 8.7 13.1

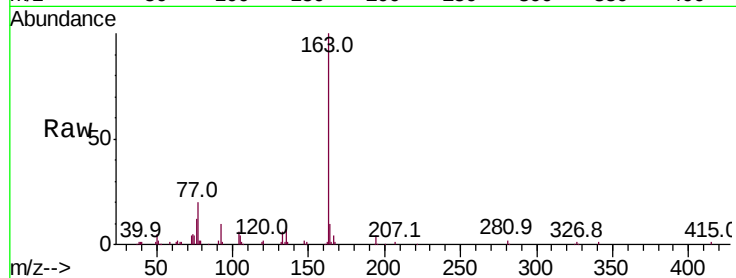

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

