

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011457.D
 Acq On : 17 Aug 2020 19:17
 Operator : CG/JU
 Sample : L3611-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFL6

Quant Time: Aug 18 05:23:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 18 04:25:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	148416	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	633470	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	392754	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	839848	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	854827	20.00	ng/ul	0.00
86) Perylene-d12	23.15	264	914734	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	7903	2.56	ng/uL	0.00
5) Phenol-d5	6.64	99	131213	12.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	76601	14.32	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	121915	12.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	83186	9.76	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	60832	12.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	68129	12.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	120018	11.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	144173	11.56	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	491006	16.06	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	515067	14.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	52895	10.21	ng/ul	0.00
58) Fluorene-d10	15.07	176	397349	14.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.21	200	57190	10.27	ng/ul	0.00
71) Anthracene-d10	16.92	188	616803	15.37	ng/ul	0.00
79) Pyrene-d10	19.23	212	762787	17.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	782859	15.41	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.54	163	98278	3.131 ng/ul# 97




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011457.D
Acq On : 17 Aug 2020 19:17
Operator : CG/JU
Sample : L3611-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFL6

Quant Time: Aug 18 05:23:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 18 04:25:59 2020
Response via : Initial Calibration

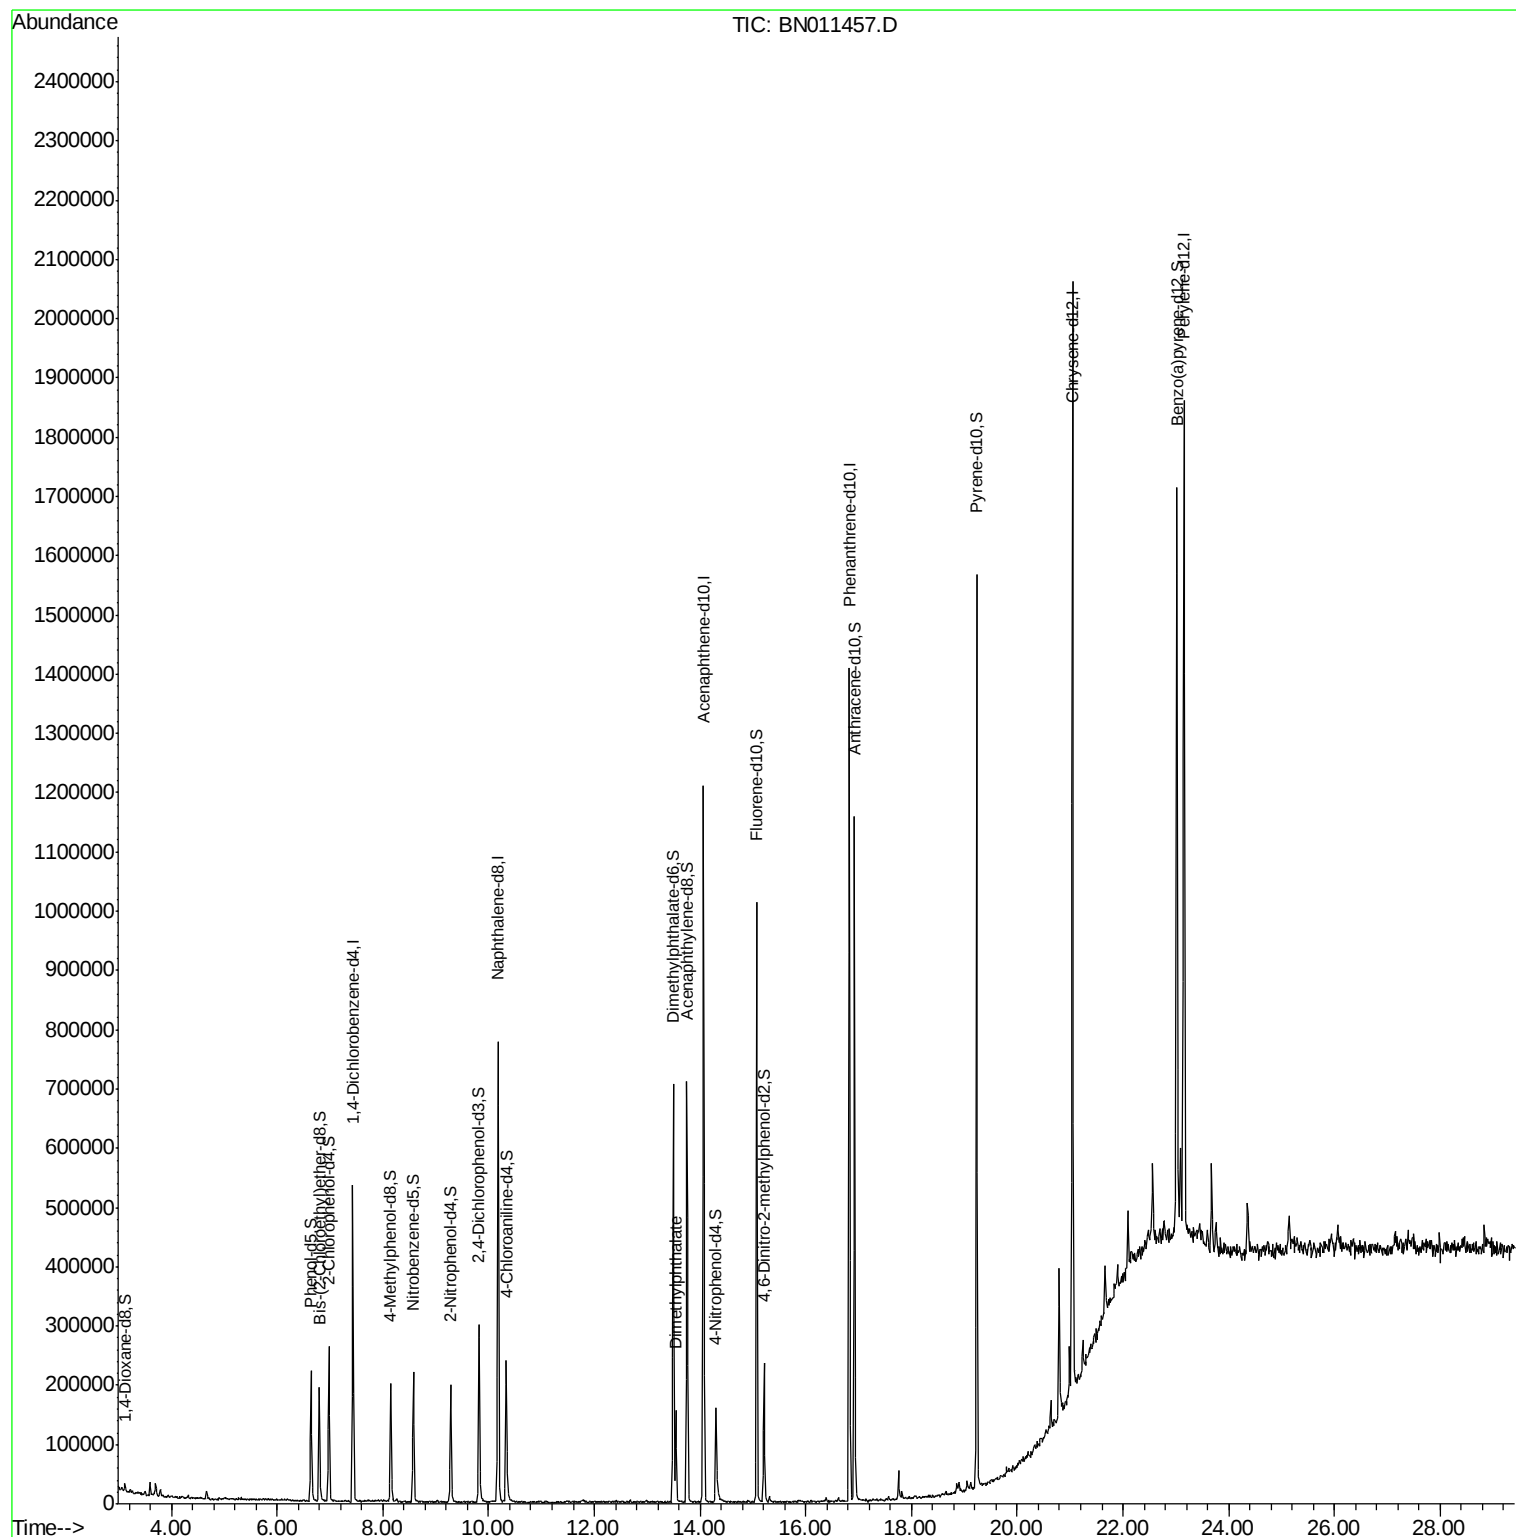

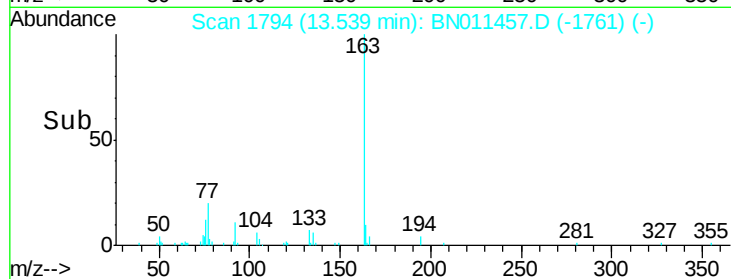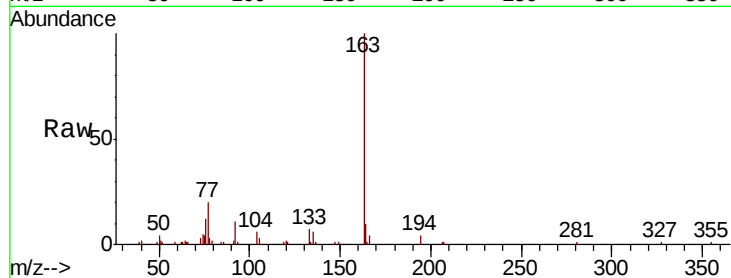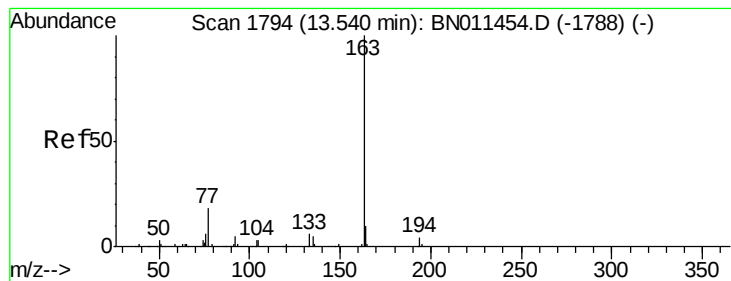

#45

Dimethylphthalate

Concen: 3.131 ng/ul

RT: 13.54 min Scan# 1794

Delta R.T. -0.01 min

Lab File: BN011457.D

Acq: 17 Aug 2020 19:17

Instrument :

BNA_N

ClientSampleId :

DBFL6

Tot Ion:163 Resp: 98278

Ion Ratio Lower Upper

163 100

194 3.7 3.8 5.6#

164 9.8 8.7 13.1

