

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011461.D
 Acq On : 17 Aug 2020 21:40
 Operator : CG/JU
 Sample : L3611-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFM1

Quant Time: Aug 18 06:20:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 18 04:25:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	189476	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	724147	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	391189	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	830856	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	841966	20.00	ng/ul	0.00
86) Perylene-d12	23.16	264	851329	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	18287	4.63	ng/uL	0.00
5) Phenol-d5	6.64	99	404659	30.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	213297	31.23	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	367575	30.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	312325	28.71	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	171915	30.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	192593	30.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	352369	29.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	449986	31.55	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	959915	31.51	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	1170634	31.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	112840	21.87	ng/ul	0.00
58) Fluorene-d10	15.07	176	811353	30.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.21	200	104910	19.04	ng/ul	0.00
71) Anthracene-d10	16.92	188	1229417	30.98	ng/ul	0.00
79) Pyrene-d10	19.23	212	1376406	31.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.03	264	1478590	31.27	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.55	163	200298	6.406	ng/ul 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011461.D
Acq On : 17 Aug 2020 21:40
Operator : CG/JU
Sample : L3611-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFM1

Quant Time: Aug 18 06:20:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 18 04:25:59 2020
Response via : Initial Calibration

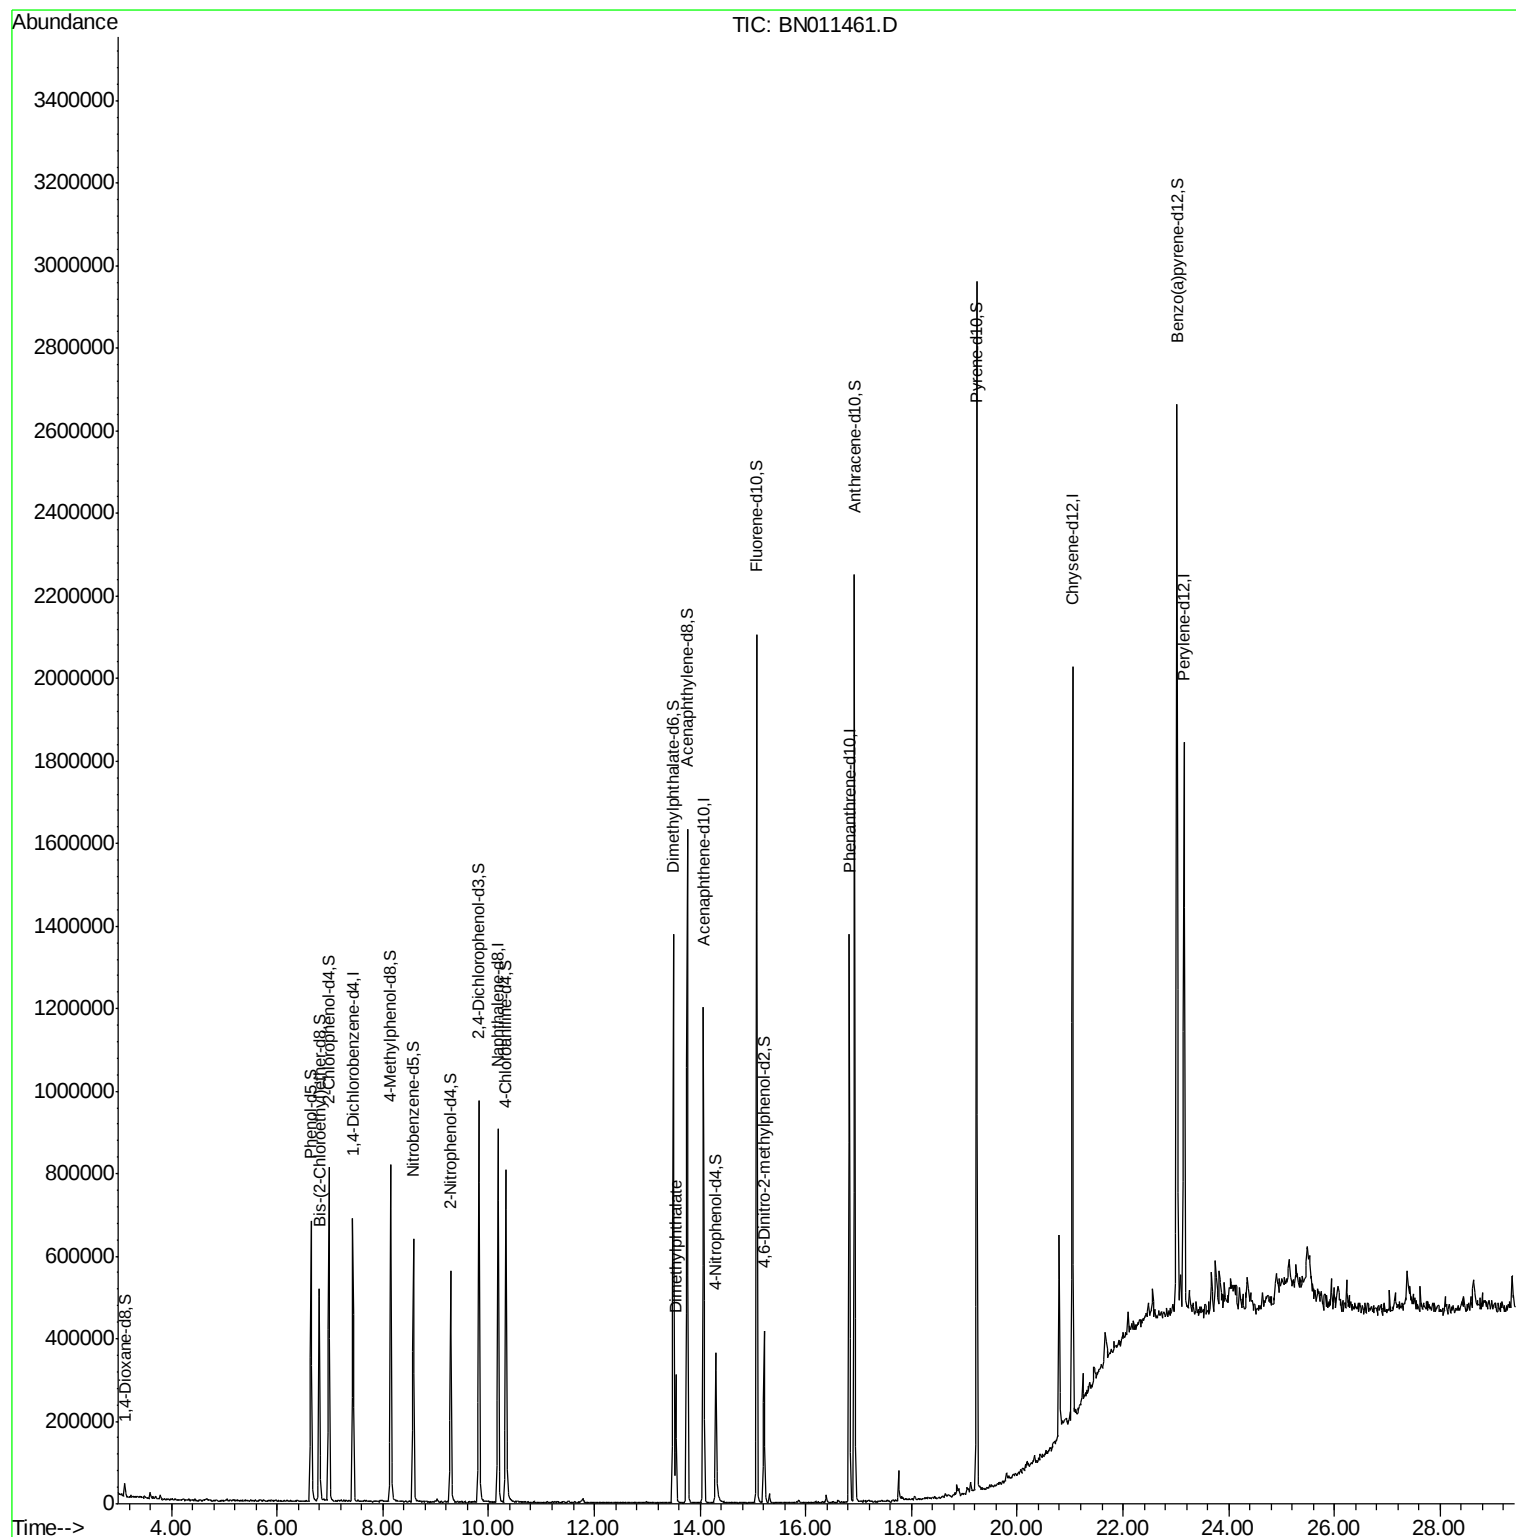

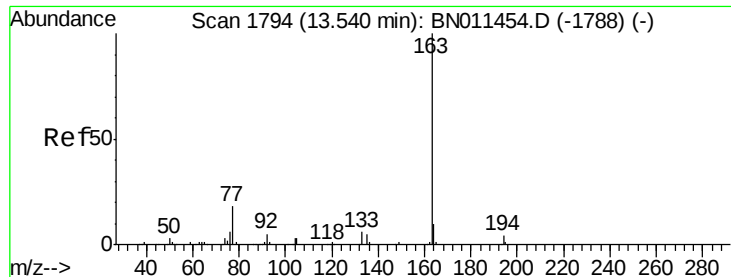

#45

Dimethylphthalate

Concen: 6.406 ng/ul

RT: 13.55 min Scan# 1795

Delta R.T. -0.00 min

Lab File: BN011461.D

Acq: 17 Aug 2020 21:40

Instrument :

BNA_N

ClientSampleId :

DBFM1


Tot Ion:163 Resp: 200298

Ion Ratio Lower Upper

163 100

194 4.2 3.8 5.6

164 8.8 8.7 13.1

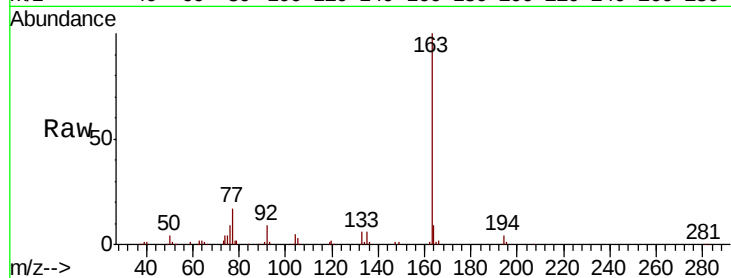

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

