

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011469.D
 Acq On : 18 Aug 2020 03:03
 Operator : CG/JU
 Sample : L3611-23
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFM8

Quant Time: Aug 18 06:49:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 18 06:41:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	192714	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	819661	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	503523	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	1018136	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	1009411	20.00	ng/ul	0.00
86) Perylene-d12	23.15	264	1062308	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	9972	2.48	ng/uL	0.00
5) Phenol-d5	6.64	99	194521	14.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	111390	16.04	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	164683	13.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	133497	12.06	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	79381	12.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	85502	11.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	175558	13.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	195821	12.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	548041	13.98	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	580997	12.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	56263	8.47	ng/ul	0.00
58) Fluorene-d10	15.07	176	504396	14.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	59630	8.83	ng/ul	0.00
71) Anthracene-d10	16.92	188	703941	14.47	ng/ul	0.00
79) Pyrene-d10	19.23	212	855782	16.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	900323	15.26	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.54	163	101699	2.527	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011469.D
Acq On : 18 Aug 2020 03:03
Operator : CG/JU
Sample : L3611-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFM8

Quant Time: Aug 18 06:49:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 18 06:41:47 2020
Response via : Initial Calibration

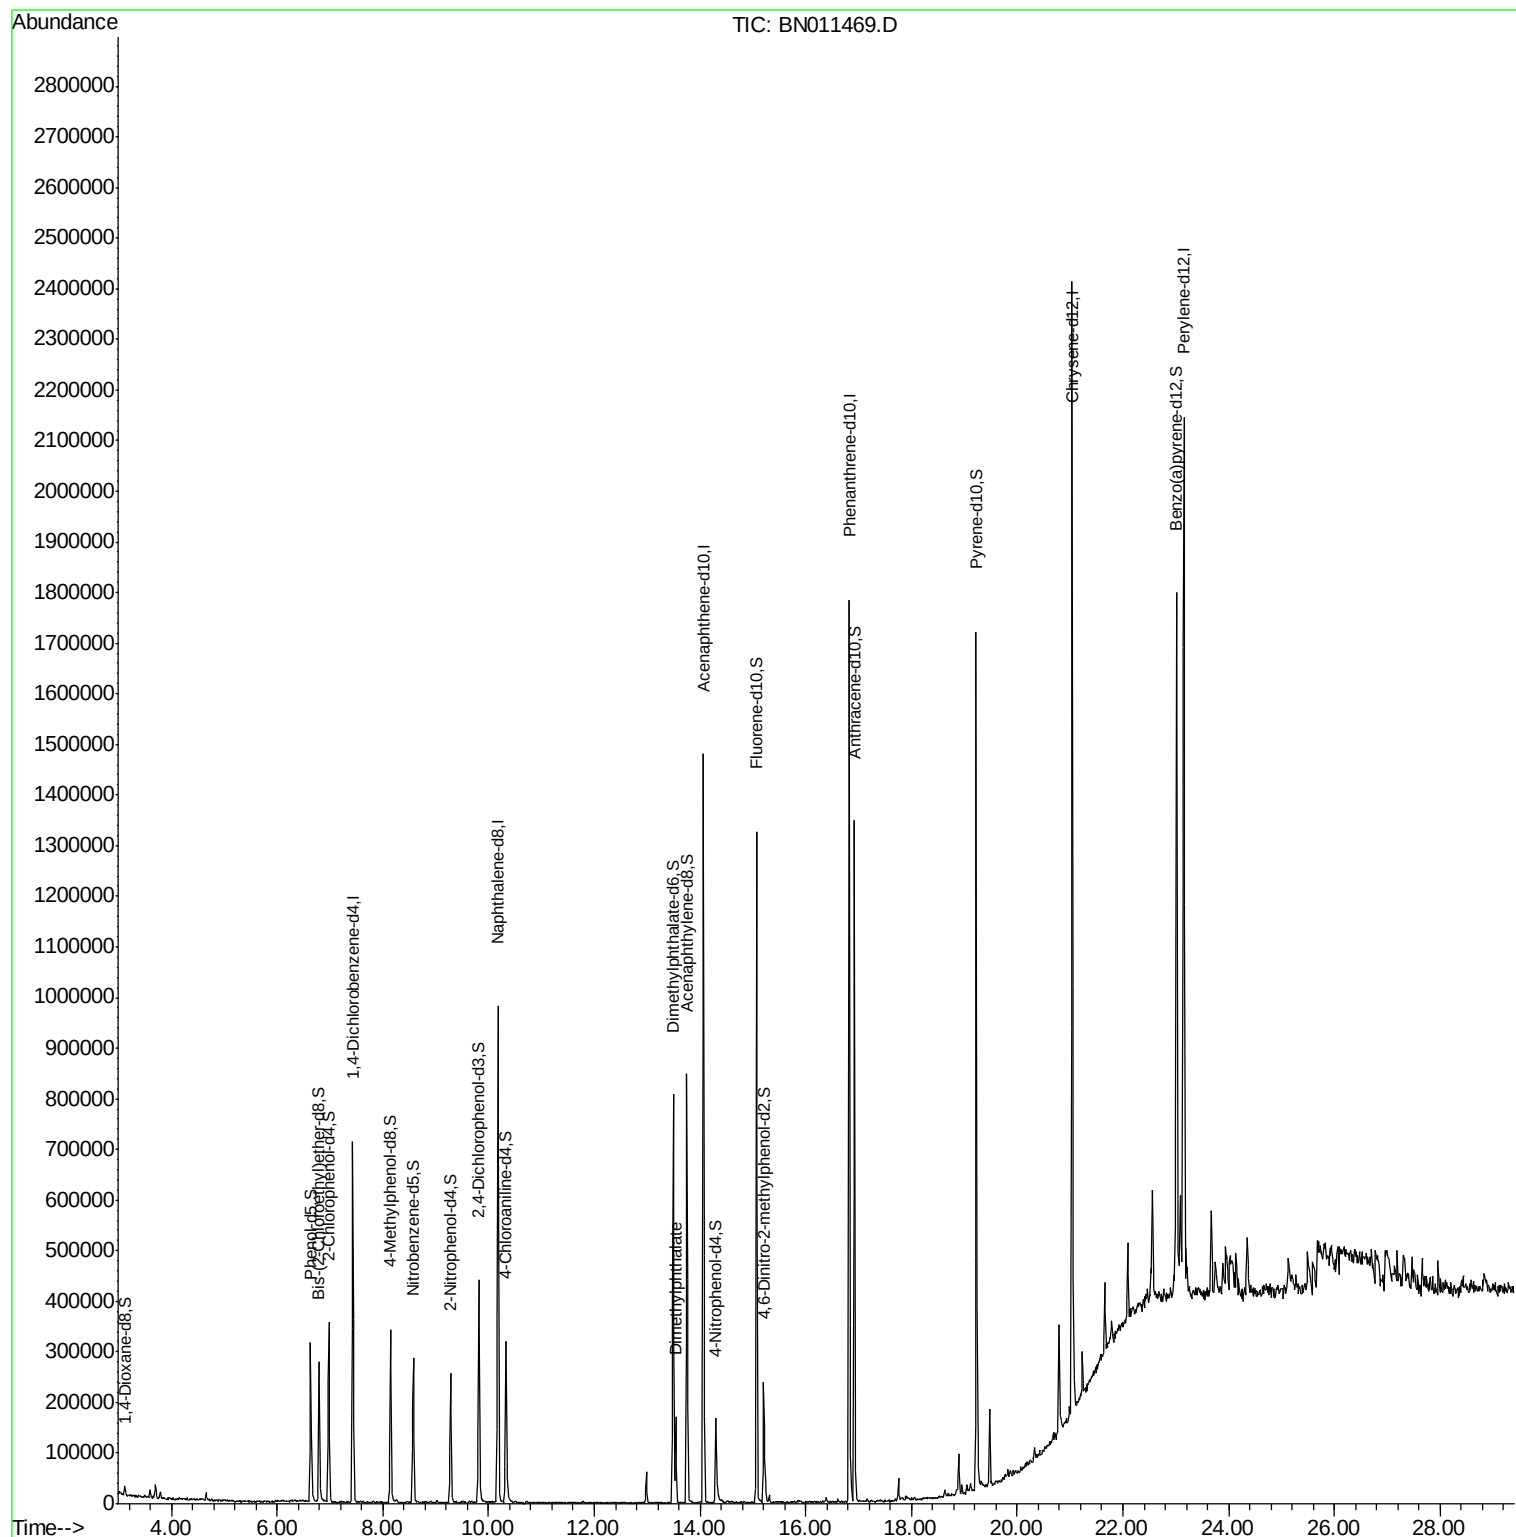

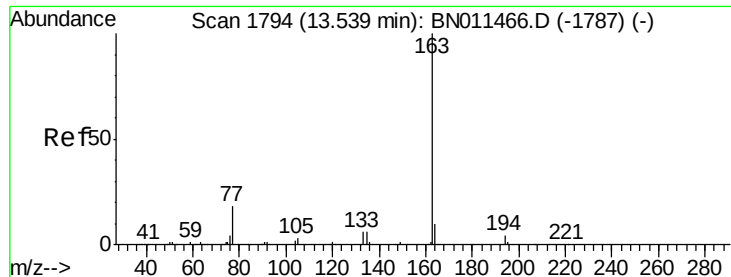

#45

Dimethylphthalate

Concen: 2.527 ng/ul

RT: 13.54 min Scan# 1794

Delta R.T. -0.01 min

Lab File: BN011469.D

Acq: 18 Aug 2020 03:03

Instrument :

BNA_N

ClientSampleId :

DBFM8


Tot Ion:163 Resp: 101699

Ion Ratio Lower Upper

163 100

194 4.8 3.8 5.6

164 9.2 8.7 13.1

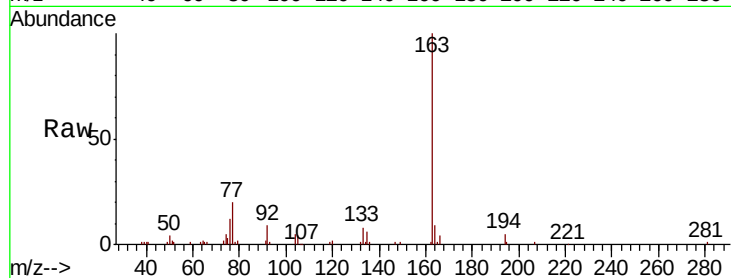

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

