

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011474.D
 Acq On : 18 Aug 2020 06:02
 Operator : CG/JU
 Sample : L3611-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFK9

Quant Time: Aug 18 07:06:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 18 06:41:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	198461	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	756006	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	427900	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	897278	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	1067032	20.00	ng/ul	0.00
86) Perylene-d12	23.15	264	927068	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	27925	6.75	ng/uL	0.00
5) Phenol-d5	6.64	99	507883	36.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	258198	36.09	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	466868	37.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	475231	41.70	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	217886	37.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	247375	37.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.81	165	459136	36.88	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.33	131	592897	39.82	ng/ul	0.00
44) Dimethylphthalate-d6	13.49	166	1529436	45.90	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	1813346	45.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	192004	34.01	ng/ul	0.00
58) Fluorene-d10	15.07	176	1172460	40.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	173897	29.22	ng/ul	0.00
71) Anthracene-d10	16.92	188	1756472	40.98	ng/ul	0.00
79) Pyrene-d10	19.23	212	2007137	36.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	2309805	44.86	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.66	94	22237	1.554	ng/ul 96
45) Dimethylphthalate	13.54	163	365369	10.683	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011474.D
Acq On : 18 Aug 2020 06:02
Operator : CG/JU
Sample : L3611-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFK9

Quant Time: Aug 18 07:06:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 18 06:41:47 2020
Response via : Initial Calibration

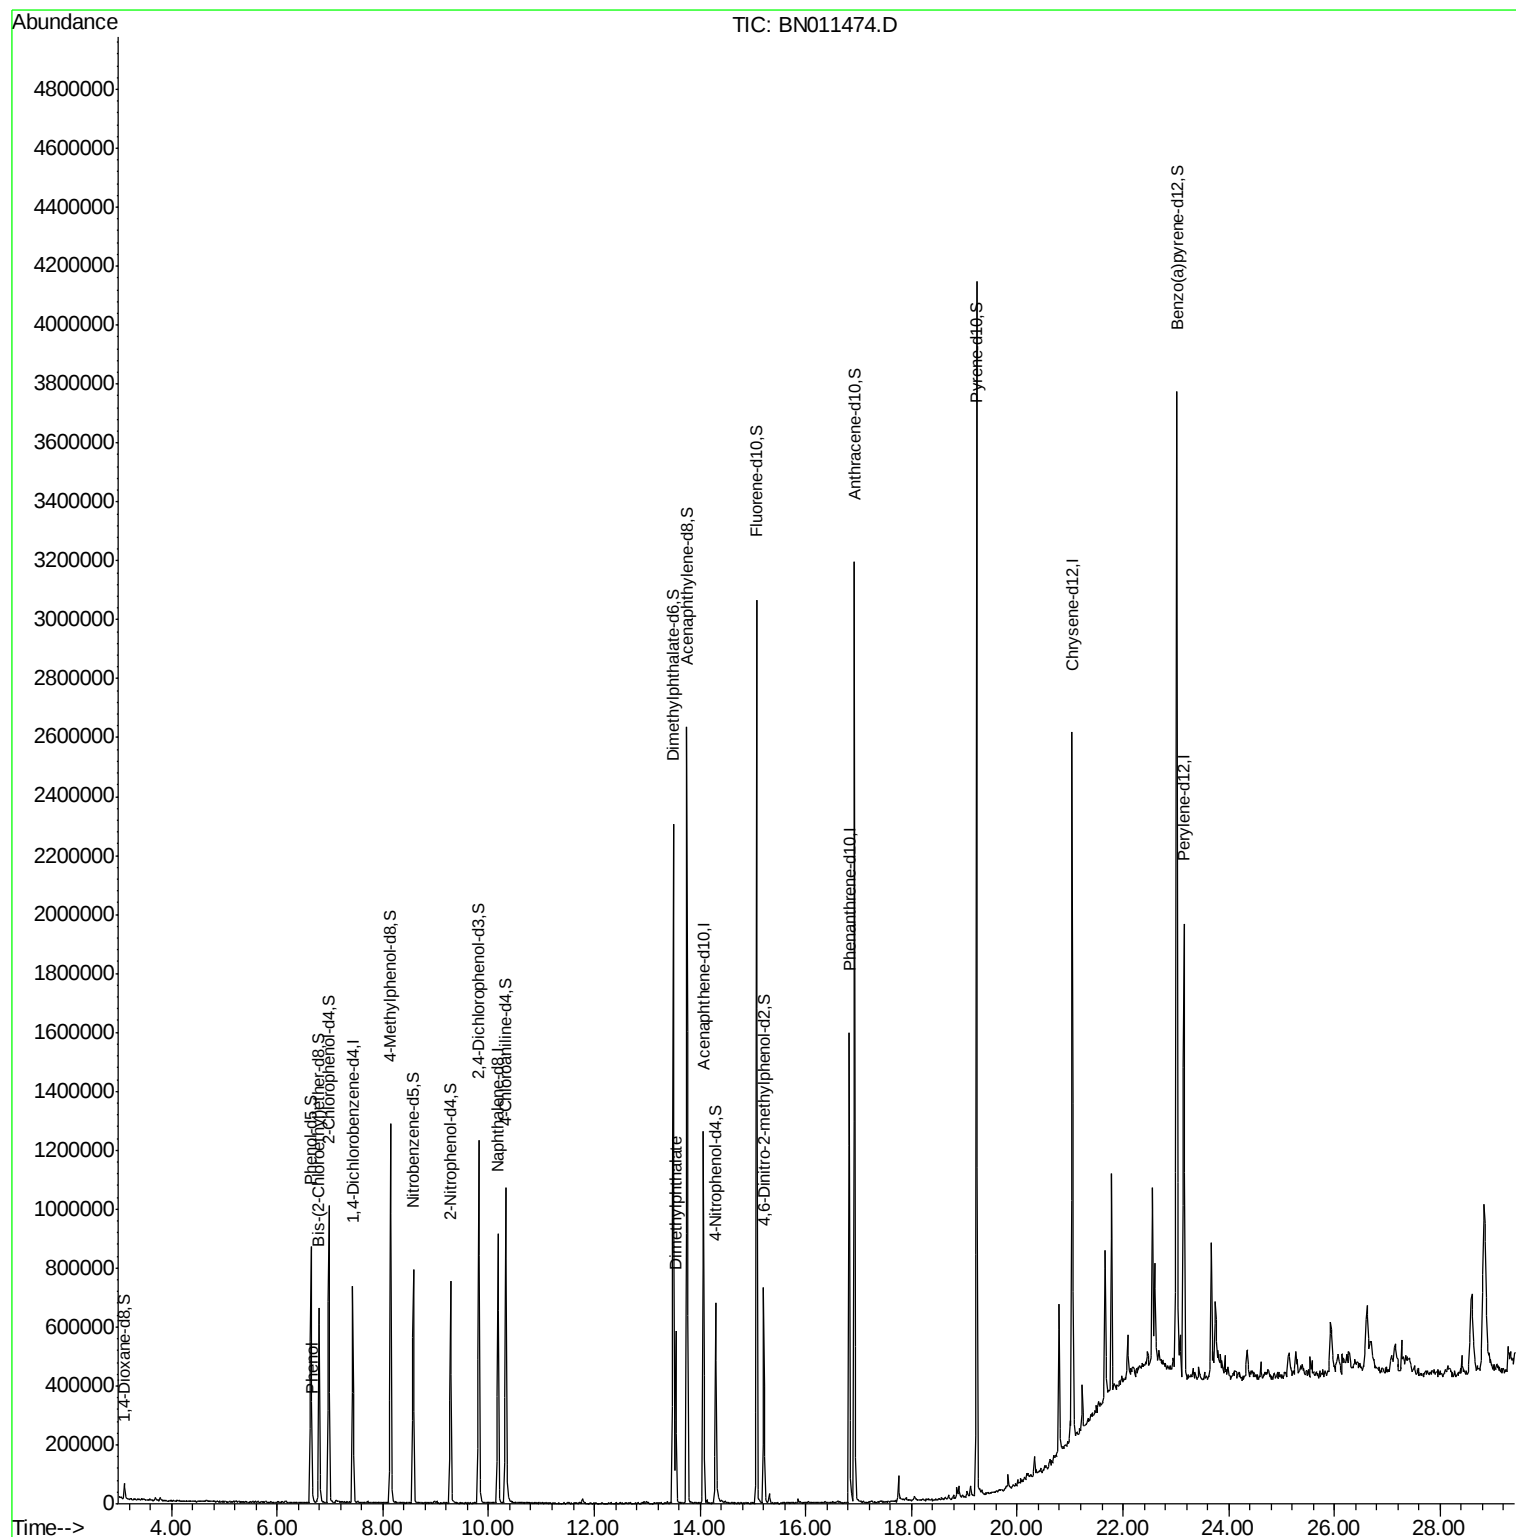

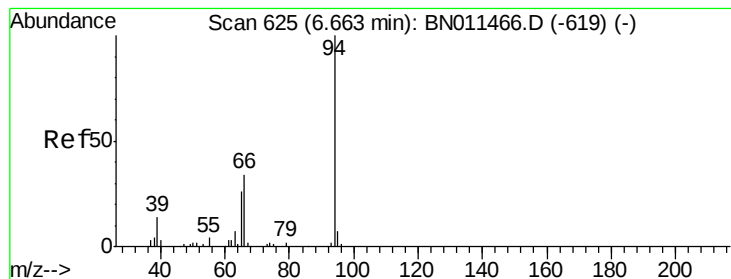





#6

Phenol

Concen: 1.554 ng/ul
 RT: 6.66 min Scan# 625
 Delta R.T. -0.01 min
 Lab File: BN011474.D
 Acq: 18 Aug 2020 06:02

Instrument :
 BNA_N
 ClientSampleId :
 DBFK9

Tot Ion	94	Resp	22237
Ion Ratio	Lower	Upper	
94	100		
65	27.6	22.1	33.1
66	44.3	32.1	48.1

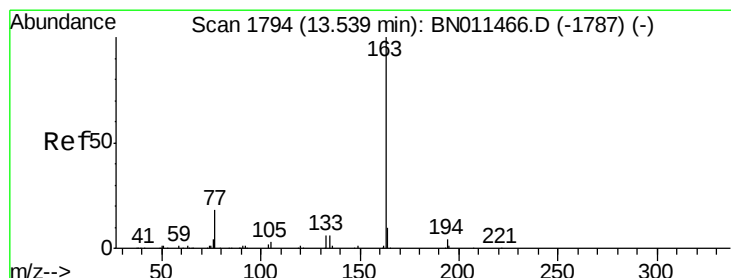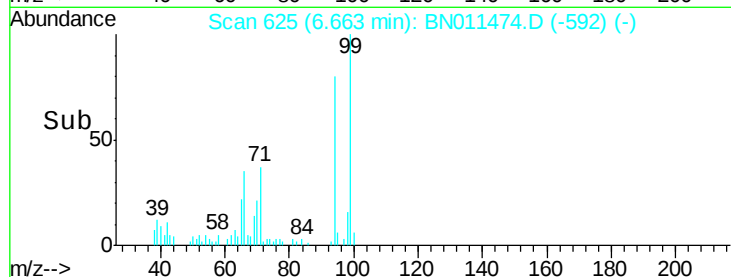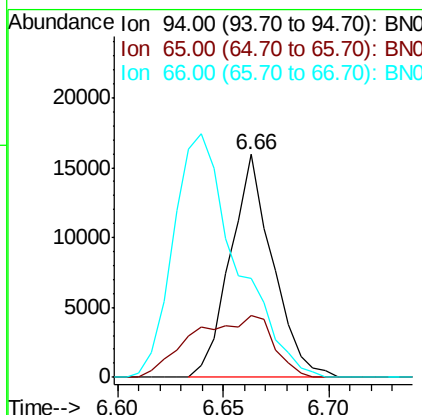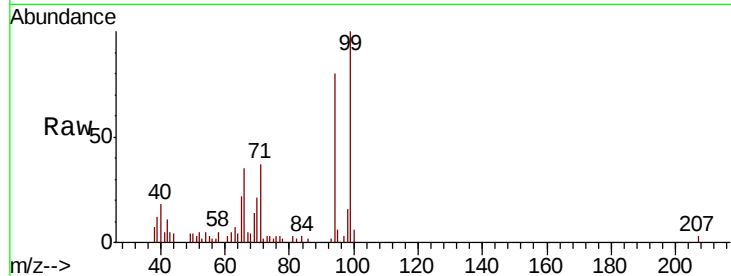

#45

Dimethylphthalate

Concen: 10.683 ng/ul
 RT: 13.54 min Scan# 1794
 Delta R.T. -0.01 min
 Lab File: BN011474.D
 Acq: 18 Aug 2020 06:02

Tgt Ion	163	Resp	365369
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.8	5.6
164	10.0	8.7	13.1

