

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011490.D
 Acq On : 18 Aug 2020 18:31
 Operator : CG/JU
 Sample : L3668-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS6

Quant Time: Aug 19 02:21:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 19 02:19:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	143472	20.00	ng/ul	0.00
18) Naphthalene-d8	10.17	136	539699	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	325844	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	703861	20.00	ng/ul	0.00
78) Chrysene-d12	21.04	240	780461	20.00	ng/ul	0.00
86) Perylene-d12	23.15	264	825949	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	14938	5.00	ng/uL	0.00
5) Phenol-d5	6.64	99	43101	4.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	108903	21.06	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	145123	15.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.14	113	80326	9.75	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	84955	20.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	88898	18.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.81	165	157420	17.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	14854	1.40	ng/ul	0.02
44) Dimethylphthalate-d6	13.49	166	553634	21.82	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	618853	20.27	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	10562	2.46	ng/ul	0.02
58) Fluorene-d10	15.07	176	473287	21.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	71919	15.41	ng/ul	0.00
71) Anthracene-d10	16.92	188	801452	23.84	ng/ul	0.00
79) Pyrene-d10	19.23	212	981939	24.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	1103959	24.07	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.54	163	243702	9.358	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011490.D
Acq On : 18 Aug 2020 18:31
Operator : CG/JU
Sample : L3668-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS6

Quant Time: Aug 19 02:21:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 19 02:19:14 2020
Response via : Initial Calibration

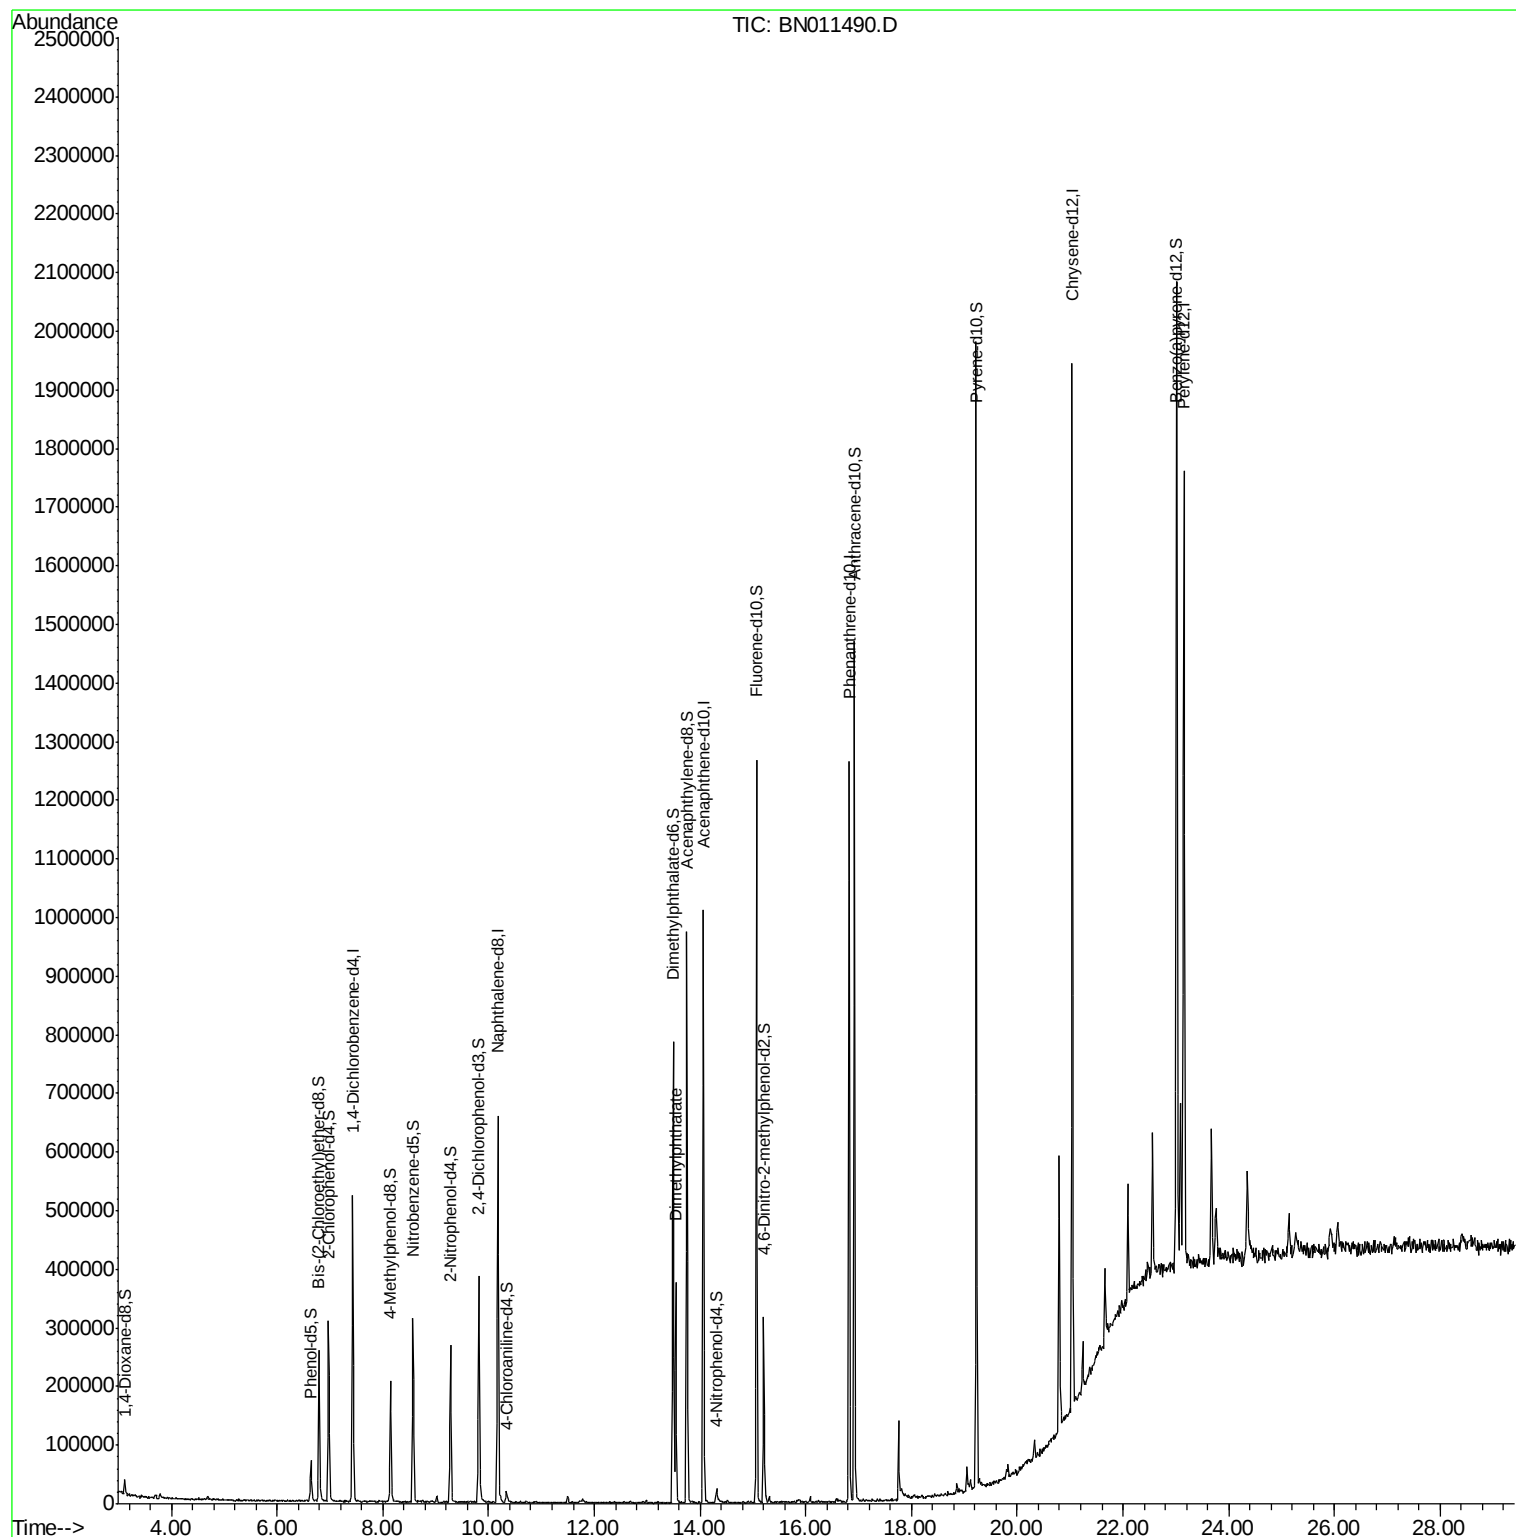

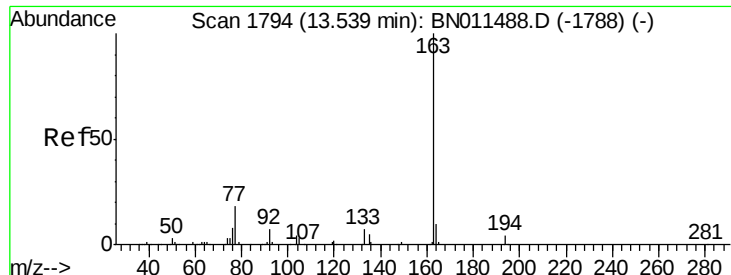

#45

Dimethylphthalate

Concen: 9.358 ng/ul

RT: 13.54 min Scan# 1794

Delta R.T. 0.00 min

Lab File: BN011490.D

Acq: 18 Aug 2020 18:31

Instrument :

BNA_N

ClientSampleId :

DBFS6


Tot Ion:163 Resp: 243702

Ion Ratio Lower Upper

163 100

194 4.4 3.8 5.6

164 10.2 8.7 13.1

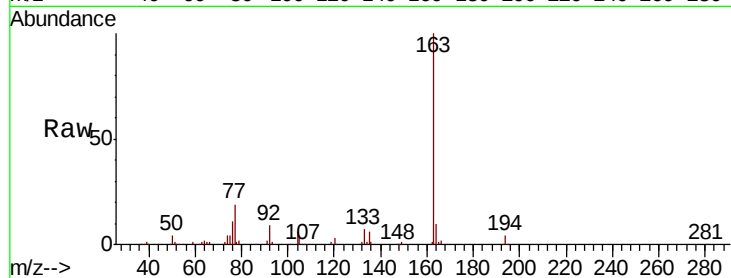

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

