

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011455.D
 Acq On : 17 Aug 2020 18:05
 Operator : CG/JU
 Sample : L3611-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	27	rVB2	16873	20963	0.75%	0.066%
2	3.505	85	88	91	rVB2	8717	9836	0.35%	0.031%
3	3.593	99	103	111	rVB	44918	58948	2.11%	0.186%
4	3.705	118	122	127	rVB2	22794	36276	1.30%	0.114%
5	3.787	132	136	139	rBV2	11951	17239	0.62%	0.054%
6	4.658	280	284	288	rBV	15672	23028	0.82%	0.073%
7	6.640	615	621	631	rBV	267080	426890	15.28%	1.346%
8	6.799	642	648	658	rBV	223524	363632	13.02%	1.147%
9	6.981	672	679	688	rVV	325182	505253	18.09%	1.593%
10	7.434	749	756	767	rVB	547398	853550	30.55%	2.691%
11	8.146	871	877	887	rBV	278673	443933	15.89%	1.400%
12	8.263	893	897	902	rBV4	4231	8703	0.31%	0.027%
13	8.575	944	950	958	rBV	277917	446451	15.98%	1.408%
14	9.028	1020	1027	1031	rBV4	3632	7741	0.28%	0.024%
15	9.287	1062	1071	1078	rBV	227539	383003	13.71%	1.208%
16	9.816	1155	1161	1174	rVV	355979	596997	21.37%	1.882%
17	10.181	1213	1223	1230	rBV	720841	1151311	41.21%	3.630%
18	10.234	1230	1232	1236	rVB3	10963	10804	0.39%	0.034%
19	10.334	1243	1249	1267	rBV	180871	379490	13.58%	1.197%
20	11.787	1491	1496	1500	rBV3	4257	7351	0.26%	0.023%
21	11.851	1502	1507	1514	rVB4	4059	7700	0.28%	0.024%
22	12.075	1540	1545	1550	rBV4	4028	6917	0.25%	0.022%
23	13.492	1779	1786	1791	rBV	658378	890383	31.87%	2.808%
24	13.540	1791	1794	1802	rVV	179702	253876	9.09%	0.801%
25	13.751	1824	1830	1843	rVB	713134	1093588	39.15%	3.448%
26	14.069	1877	1884	1891	rVV	939442	1387802	49.68%	4.376%
27	14.134	1891	1895	1900	rVB2	23760	31153	1.12%	0.098%
28	14.298	1918	1923	1940	rBV	138797	275759	9.87%	0.870%
29	14.481	1950	1954	1958	rBV	10971	16651	0.60%	0.053%
30	15.069	2048	2054	2060	rBV	933015	1302481	46.62%	4.107%
31	15.128	2060	2064	2072	rVB2	24153	42373	1.52%	0.134%
32	15.210	2072	2078	2089	rBV	225432	328016	11.74%	1.034%
33	15.310	2089	2095	2099	rVV5	9078	15354	0.55%	0.048%
34	15.428	2112	2115	2119	rBV2	8073	7934	0.28%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011455.D
 Acq On : 17 Aug 2020 18:05
 Operator : CG/JU
 Sample : L3611-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	15.575	2135	2140	2145	rVV3	4334	8970	0.32%	0.028%
36	16.375	2271	2276	2278	rBV2	4874	7390	0.26%	0.023%
37	16.404	2278	2281	2285	rVV4	6890	8105	0.29%	0.026%
38	16.486	2289	2295	2299	rBV3	12136	18096	0.65%	0.057%
39	16.610	2313	2316	2318	rVV3	6218	8101	0.29%	0.026%
40	16.645	2318	2322	2325	rVB	13083	16818	0.60%	0.053%
41	16.822	2346	2352	2356	rBV	1135402	1615727	57.84%	5.095%
42	16.863	2356	2359	2364	rVV	349917	473722	16.96%	1.494%
43	16.922	2364	2369	2382	rVV	955391	1387104	49.65%	4.374%
44	17.022	2382	2386	2391	rVB5	9525	13737	0.49%	0.043%
45	17.239	2413	2423	2427	rBV2	33921	56546	2.02%	0.178%
46	17.363	2438	2444	2446	rBV4	8054	13282	0.48%	0.042%
47	17.410	2449	2452	2455	rVB4	5027	6688	0.24%	0.021%
48	17.704	2497	2502	2505	rBV3	40289	53188	1.90%	0.168%
49	17.751	2505	2510	2517	rVV2	107750	152758	5.47%	0.482%
50	17.828	2519	2523	2528	rVV3	24642	42986	1.54%	0.136%
51	17.892	2529	2534	2538	rVV2	70162	115568	4.14%	0.364%
52	17.928	2538	2540	2549	rVB2	30340	46099	1.65%	0.145%
53	18.016	2551	2555	2557	rBV3	6764	9457	0.34%	0.030%
54	18.057	2558	2562	2568	rVV6	10001	14826	0.53%	0.047%
55	18.210	2585	2588	2592	rBV	35260	51142	1.83%	0.161%
56	18.251	2592	2595	2600	rVB2	41182	51288	1.84%	0.162%
57	18.457	2627	2630	2635	rVB4	12685	16545	0.59%	0.052%
58	18.510	2635	2639	2643	rBV4	14267	22466	0.80%	0.071%
59	18.551	2644	2646	2649	rVB4	7447	8957	0.32%	0.028%
60	18.639	2656	2661	2665	rBV5	41702	70632	2.53%	0.223%
61	18.698	2665	2671	2674	rBV8	22314	39234	1.40%	0.124%
62	18.775	2680	2684	2692	rBV2	29652	57615	2.06%	0.182%
63	18.892	2699	2704	2714	rVB	851576	1166865	41.77%	3.679%
64	18.975	2714	2718	2720	rBV3	10572	17876	0.64%	0.056%
65	19.051	2727	2731	2736	rVB2	37698	43803	1.57%	0.138%
66	19.098	2736	2739	2740	rBV3	14528	16543	0.59%	0.052%
67	19.127	2740	2744	2745	rBV4	17323	22084	0.79%	0.070%
68	19.233	2756	2762	2765	rBV	1520177	2295434	82.17%	7.238%
69	19.257	2765	2766	2775	rVV	777080	842635	30.16%	2.657%
70	19.339	2776	2780	2788	rVB4	41979	76106	2.72%	0.240%
71	19.398	2788	2790	2793	rVB4	9297	8103	0.29%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011455.D
 Acq On : 17 Aug 2020 18:05
 Operator : CG/JU
 Sample : L3611-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

72	19.451	2793	2799	2803	rBV	53022	84565	3.03%	0.267%
73	19.510	2806	2809	2814	rVB5	37515	58815	2.11%	0.185%
74	19.604	2814	2825	2830	rBV6	58923	159533	5.71%	0.503%
75	19.651	2831	2833	2837	rVB5	16925	16078	0.58%	0.051%
76	19.739	2843	2848	2849	rBV3	42719	66643	2.39%	0.210%
77	19.769	2849	2853	2856	rVB2	100594	141986	5.08%	0.448%
78	19.827	2861	2863	2866	rBV4	34329	38332	1.37%	0.121%
79	19.869	2867	2870	2874	rVB	61655	74223	2.66%	0.234%
80	19.927	2875	2880	2884	rBV3	72288	111114	3.98%	0.350%
81	20.016	2892	2895	2899	rVB6	19411	21268	0.76%	0.067%
82	20.069	2900	2904	2907	rVB	37006	46848	1.68%	0.148%
83	20.116	2908	2912	2917	rBV3	42609	68462	2.45%	0.216%
84	20.198	2923	2926	2930	rBV3	55849	64960	2.33%	0.205%
85	20.333	2946	2949	2953	rBV6	38908	48145	1.72%	0.152%
86	20.522	2978	2981	2989	rVB2	65228	98725	3.53%	0.311%
87	20.686	3006	3009	3013	rVB	72341	82303	2.95%	0.260%
88	20.727	3013	3016	3019	rBV	64937	69133	2.47%	0.218%
89	20.792	3023	3027	3030	rBV4	130211	187596	6.72%	0.592%
90	20.992	3058	3061	3063	rBV	99098	110771	3.97%	0.349%
91	21.045	3063	3070	3073	rVV2	1788518	2793538	100.00%	8.809%
92	21.080	3073	3076	3084	rVB	482382	626483	22.43%	1.975%
93	21.192	3092	3095	3100	rBV3	81554	140463	5.03%	0.443%
94	21.239	3100	3103	3109	rVV7	98344	156574	5.60%	0.494%
95	22.092	3246	3248	3256	rVB4	116465	179394	6.42%	0.566%
96	22.539	3319	3324	3327	rBV	477262	910779	32.60%	2.872%
97	22.980	3395	3399	3402	rBV	207040	327749	11.73%	1.033%
98	23.021	3402	3406	3411	rVV	1034436	1706693	61.09%	5.382%
99	23.063	3411	3413	3422	rVV3	343638	623647	22.32%	1.966%
100	23.151	3423	3428	3443	rVB2	1305557	2411352	86.32%	7.603%


Sum of corrected areas: 31714054

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011455.D
Acq On : 17 Aug 2020 18:05
Operator : CG/JU
Sample : L3611-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

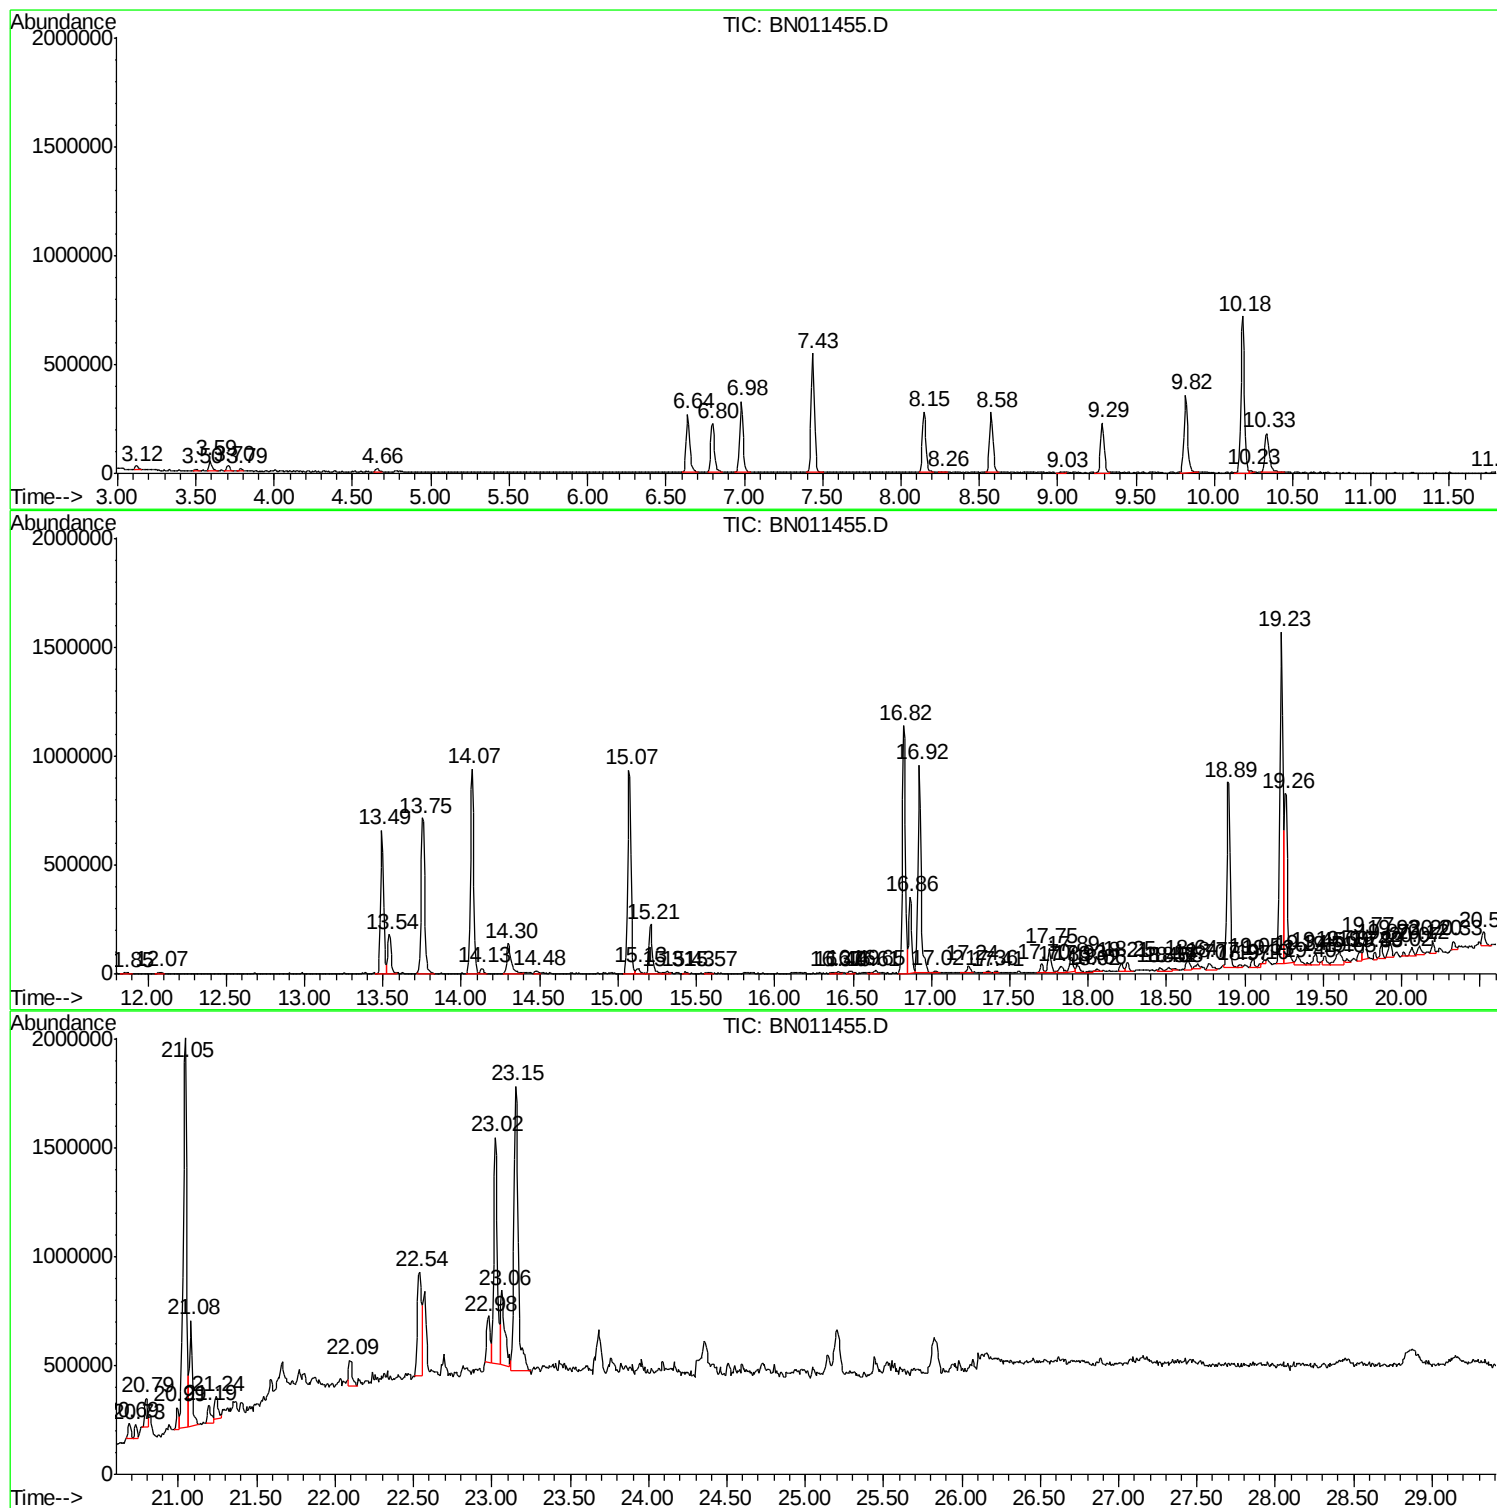

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011455.D
Acq On : 17 Aug 2020 18:05
Operator : CG/JU
Sample : L3611-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011455.D
Acq On : 17 Aug 2020 18:05
Operator : CG/JU
Sample : L3611-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFL3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc