

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011481.D
 Acq On : 18 Aug 2020 10:52
 Operator : CG/JU
 Sample : L3668-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	29	rVB	27270	34660	0.87%	0.100%
2	3.246	42	44	49	rVB4	2986	4314	0.11%	0.012%
3	3.364	61	64	67	rVB4	3950	3980	0.10%	0.012%
4	3.699	117	121	127	rBV4	7121	12676	0.32%	0.037%
5	3.787	133	136	140	rVB5	10320	13294	0.34%	0.038%
6	6.452	582	589	592	rBV3	2144	4164	0.11%	0.012%
7	6.640	615	621	629	rBV	101643	165730	4.18%	0.480%
8	6.793	641	647	660	rBV	368611	584254	14.75%	1.692%
9	6.975	672	678	693	rVB	454762	733909	18.53%	2.125%
10	7.075	693	695	698	rBV3	3603	5121	0.13%	0.015%
11	7.434	749	756	768	rVB	550823	860503	21.72%	2.491%
12	8.146	871	877	886	rBV	328181	514950	13.00%	1.491%
13	8.569	943	949	958	rBV	484796	786082	19.84%	2.276%
14	8.716	972	974	979	rBV4	2917	5137	0.13%	0.015%
15	9.022	1021	1026	1032	rVB5	7615	10562	0.27%	0.031%
16	9.281	1064	1070	1082	rBV	485041	768995	19.41%	2.226%
17	9.810	1153	1160	1175	rBV	714037	1257389	31.74%	3.641%
18	10.175	1215	1222	1228	rBV	757572	1239611	31.29%	3.589%
19	10.228	1228	1231	1236	rVB2	27027	40761	1.03%	0.118%
20	10.340	1244	1250	1262	rBV4	31992	68768	1.74%	0.199%
21	11.498	1443	1447	1450	rBV3	6906	8517	0.21%	0.025%
22	11.781	1491	1495	1498	rBV2	6345	9523	0.24%	0.028%
23	13.492	1780	1786	1791	rBV	1228274	1715323	43.30%	4.966%
24	13.539	1791	1794	1801	rVB	172141	229314	5.79%	0.664%
25	13.751	1822	1830	1842	rBV	1446764	2151729	54.32%	6.230%
26	14.063	1877	1883	1892	rBV	1034099	1533907	38.72%	4.441%
27	14.304	1917	1924	1935	rBV2	49546	106821	2.70%	0.309%
28	15.069	2048	2054	2070	rVB	2290599	3084163	77.85%	8.930%
29	15.204	2072	2077	2091	rVV	595190	828947	20.92%	2.400%
30	15.310	2091	2095	2100	rVB2	24933	30731	0.78%	0.089%
31	15.857	2185	2188	2195	rVB2	6614	8671	0.22%	0.025%
32	16.075	2221	2225	2229	rBV4	5893	7745	0.20%	0.022%
33	16.557	2302	2307	2308	rBV3	3114	3999	0.10%	0.012%
34	16.610	2314	2316	2322	rVB4	4155	5324	0.13%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011481.D
 Acq On : 18 Aug 2020 10:52
 Operator : CG/JU
 Sample : L3668-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	16.822	2346	2352	2360	rBV	1351248	1812025	45.74%	5.246%
36	16.922	2362	2369	2377	rVV2	2324891	3246143	81.94%	9.399%
37	16.992	2380	2381	2385	rVB3	4669	4322	0.11%	0.013%
38	17.098	2396	2399	2403	rBV4	5068	6415	0.16%	0.019%
39	17.498	2465	2467	2471	rBV4	3449	4729	0.12%	0.014%
40	17.627	2485	2489	2491	rBV2	4114	6857	0.17%	0.020%
41	17.751	2506	2510	2519	rBV6	29653	47407	1.20%	0.137%
42	17.898	2530	2535	2536	rBV5	4397	5549	0.14%	0.016%
43	18.010	2549	2554	2556	rBV4	2867	4277	0.11%	0.012%
44	18.222	2587	2590	2591	rBV3	3516	4235	0.11%	0.012%
45	18.375	2613	2616	2619	rVB5	3743	4843	0.12%	0.014%
46	18.680	2666	2668	2674	rBV6	4276	7293	0.18%	0.021%
47	18.863	2693	2699	2702	rBV	25377	34239	0.86%	0.099%
48	19.057	2728	2732	2737	rVB6	5139	6934	0.18%	0.020%
49	19.110	2738	2741	2746	rVB2	17708	23362	0.59%	0.068%
50	19.227	2755	2761	2773	rBV	2864113	3873290	97.77%	11.214%
51	19.392	2787	2789	2794	rBV5	4582	5411	0.14%	0.016%
52	19.745	2847	2849	2850	rBV	6244	4348	0.11%	0.013%
53	19.827	2861	2863	2864	rBV2	6691	4069	0.10%	0.012%
54	19.910	2875	2877	2879	rBV3	8542	8524	0.22%	0.025%
55	20.792	3023	3027	3034	rBV3	147513	208544	5.26%	0.604%
56	21.045	3064	3070	3077	rBV	1623769	2126496	53.68%	6.157%
57	23.021	3400	3406	3414	rBV	2317116	3961542	100.00%	11.470%
58	23.151	3423	3428	3437	rVB2	1255397	2150588	54.29%	6.227%
59	29.027	4424	4427	4429	rBV	91045	137768	3.48%	0.399%


Sum of corrected areas: 34538784

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011481.D
Acq On : 18 Aug 2020 10:52
Operator : CG/JU
Sample : L3668-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

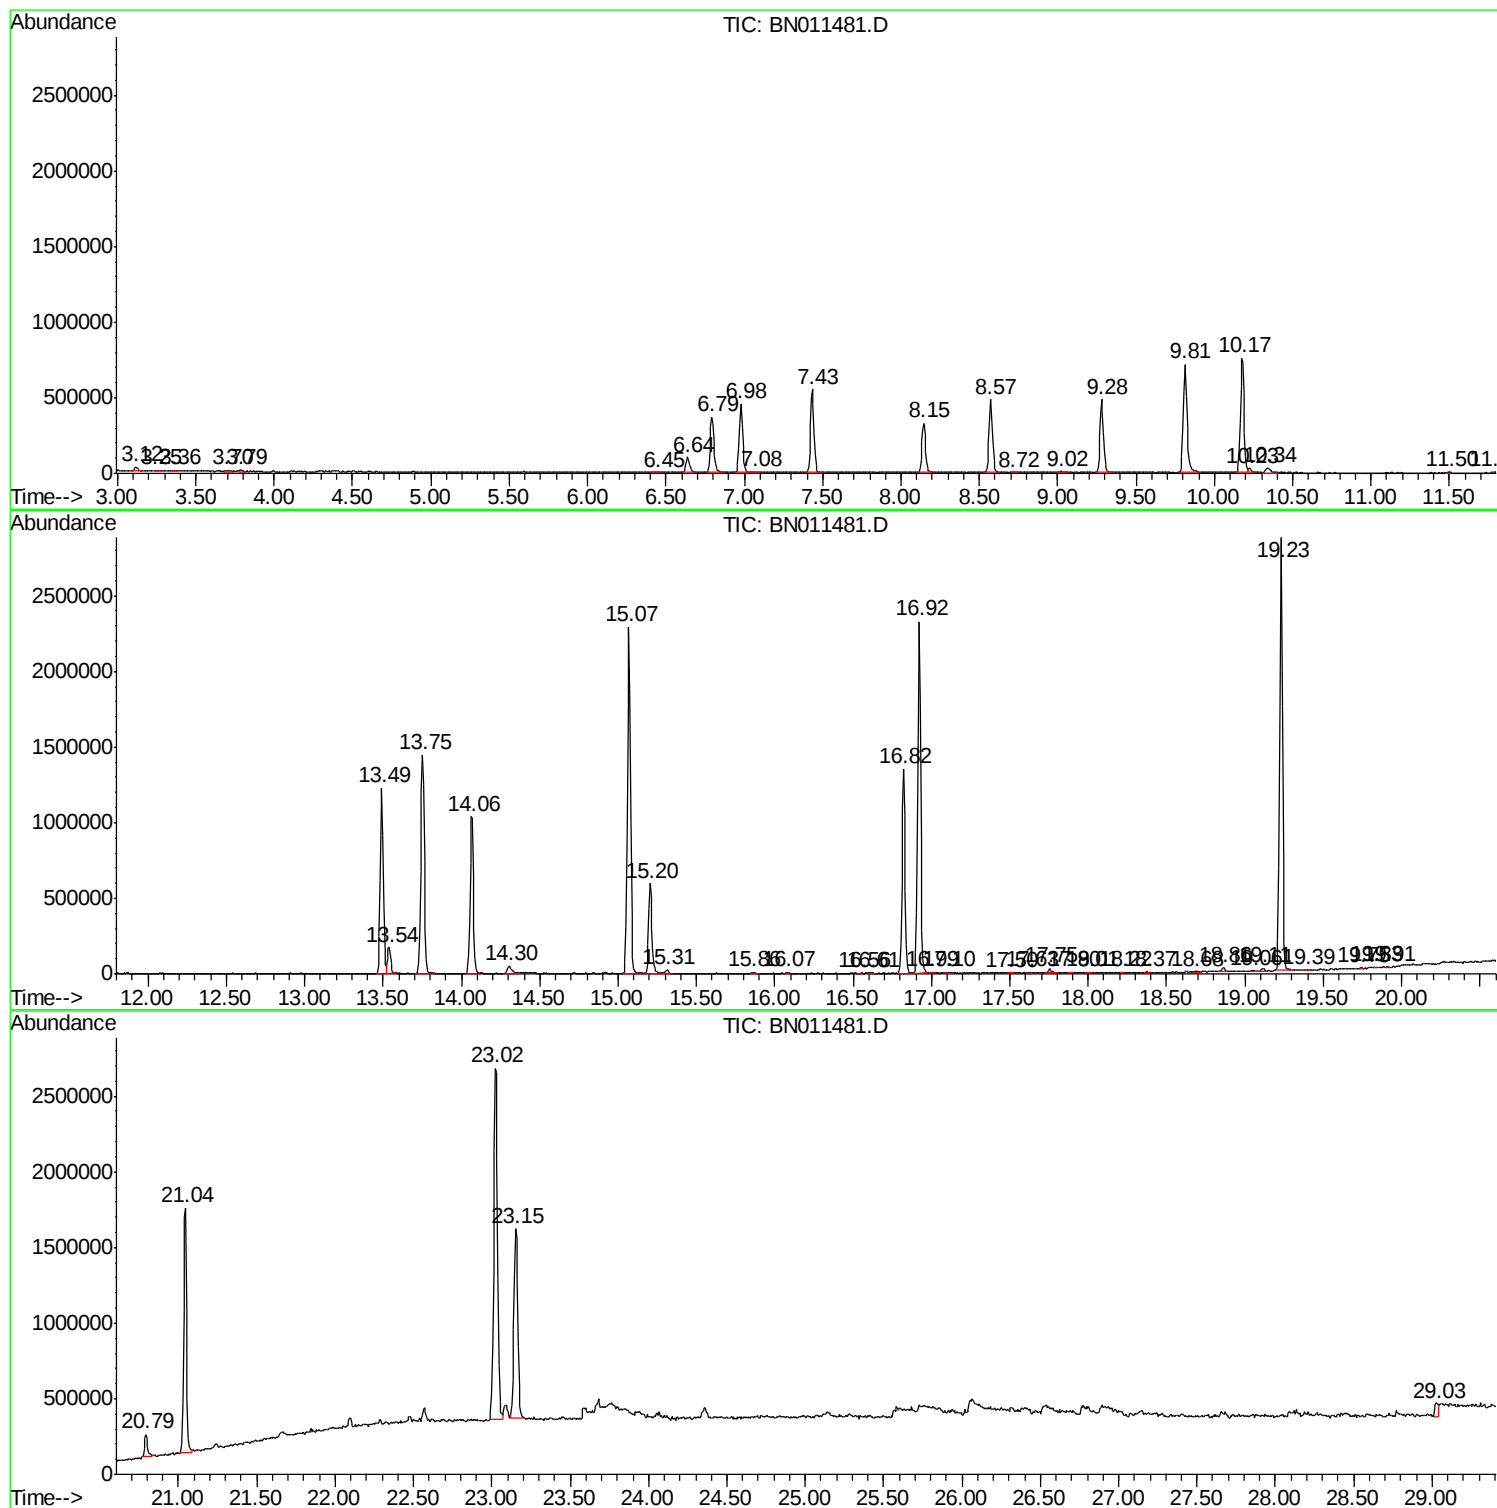

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011481.D
Acq On : 18 Aug 2020 10:52
Operator : CG/JU
Sample : L3668-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011481.D
Acq On : 18 Aug 2020 10:52
Operator : CG/JU
Sample : L3668-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
