

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011492.D
 Acq On : 18 Aug 2020 19:43
 Operator : CG/JU
 Sample : L3611-20
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	21	22	26	rBV2	7412	7458	0.24%	0.027%
2	3.511	86	89	92	rVB3	5119	5593	0.18%	0.021%
3	3.593	99	103	107	rBV2	12802	17578	0.57%	0.065%
4	3.658	111	114	116	rBV3	3100	3718	0.12%	0.014%
5	3.705	118	122	127	rVB2	19136	27528	0.90%	0.101%
6	3.781	133	135	139	rBV3	8742	11701	0.38%	0.043%
7	3.952	162	164	168	rBV3	3890	3858	0.13%	0.014%
8	3.993	168	171	177	rBV2	17071	29844	0.97%	0.110%
9	4.234	208	212	215	rBV4	4415	4708	0.15%	0.017%
10	4.387	234	238	243	rBV4	10503	17569	0.57%	0.064%
11	4.658	280	284	289	rVB2	16806	24580	0.80%	0.090%
12	5.193	373	375	378	rBV3	2704	3207	0.10%	0.012%
13	5.587	438	442	445	rBV6	2683	4272	0.14%	0.016%
14	5.999	509	512	514	rBV3	4384	4452	0.15%	0.016%
15	6.634	615	620	633	rVB	244409	387101	12.62%	1.421%
16	6.793	642	647	656	rBV	197860	298824	9.74%	1.097%
17	6.975	672	678	686	rBV	278399	429460	14.00%	1.576%
18	7.434	749	756	765	rBV	586078	911170	29.70%	3.344%
19	8.140	870	876	892	rBV	302408	510604	16.64%	1.874%
20	8.258	892	896	901	rVB4	5510	8239	0.27%	0.030%
21	8.569	944	949	958	rBV	234461	392426	12.79%	1.440%
22	9.011	1021	1024	1026	rBV2	3143	3568	0.12%	0.013%
23	9.281	1063	1070	1081	rBV	212974	351601	11.46%	1.290%
24	9.810	1154	1160	1170	rBV	330627	569454	18.56%	2.090%
25	10.175	1213	1222	1229	rBV	795676	1257319	40.98%	4.615%
26	10.328	1242	1248	1263	rBV	247944	492123	16.04%	1.806%
27	11.781	1492	1495	1499	rVB5	2003	3183	0.10%	0.012%
28	11.857	1505	1508	1511	rBV2	2629	3111	0.10%	0.011%
29	13.493	1780	1786	1791	rBV	652180	938657	30.59%	3.445%
30	13.540	1791	1794	1804	rVB	72966	102024	3.33%	0.374%
31	13.751	1823	1830	1839	rBV	719671	1074699	35.03%	3.944%
32	14.063	1876	1883	1890	rBV	1202321	1703823	55.53%	6.253%
33	14.134	1893	1895	1899	rVB4	5359	4955	0.16%	0.018%
34	14.299	1917	1923	1935	rBV	157953	308257	10.05%	1.131%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011492.D
 Acq On : 18 Aug 2020 19:43
 Operator : CG/JU
 Sample : L3611-20
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	14.522	1957	1961	1964	rVB4	2519	4107	0.13%	0.015%
36	15.069	2047	2054	2062	rBV	1006173	1391202	45.34%	5.106%
37	15.122	2062	2063	2068	rVV4	7547	7321	0.24%	0.027%
38	15.204	2072	2077	2087	rVV	225108	320062	10.43%	1.175%
39	15.316	2090	2096	2099	rVB4	8000	13065	0.43%	0.048%
40	15.569	2134	2139	2144	rVB5	2209	4206	0.14%	0.015%
41	15.816	2177	2181	2184	rBV2	2951	3927	0.13%	0.014%
42	16.075	2221	2225	2228	rVB5	3507	5731	0.19%	0.021%
43	16.363	2269	2274	2278	rBV3	3215	5620	0.18%	0.021%
44	16.487	2290	2295	2299	rVB3	4269	7424	0.24%	0.027%
45	16.610	2311	2316	2320	rBV2	6646	9803	0.32%	0.036%
46	16.822	2345	2352	2356	rBV	1546105	2077570	67.71%	7.625%
47	16.863	2356	2359	2363	rVV	121515	158596	5.17%	0.582%
48	16.922	2363	2369	2381	rVV2	996803	1486390	48.44%	5.455%
49	17.022	2383	2386	2388	rVV3	6626	7122	0.23%	0.026%
50	17.234	2418	2422	2431	rVB	12235	21307	0.69%	0.078%
51	17.304	2431	2434	2438	rVB3	2986	4151	0.14%	0.015%
52	17.351	2438	2442	2444	rBV4	5135	5780	0.19%	0.021%
53	17.392	2448	2449	2453	rBV2	3225	4822	0.16%	0.018%
54	17.534	2471	2473	2475	rBV2	3788	3075	0.10%	0.011%
55	17.698	2496	2501	2505	rBV	16286	23578	0.77%	0.087%
56	17.751	2505	2510	2514	rVV	36054	48614	1.58%	0.178%
57	17.834	2519	2524	2527	rVV4	6285	11578	0.38%	0.042%
58	17.887	2527	2533	2538	rVV4	23851	41991	1.37%	0.154%
59	17.928	2538	2540	2545	rVB4	11382	14290	0.47%	0.052%
60	18.057	2559	2562	2563	rBV3	4875	4369	0.14%	0.016%
61	18.210	2584	2588	2591	rBV3	13296	18793	0.61%	0.069%
62	18.245	2591	2594	2599	rVB2	21780	28251	0.92%	0.104%
63	18.392	2616	2619	2620	rBV2	3819	3147	0.10%	0.012%
64	18.516	2637	2640	2642	rVB3	5602	5369	0.17%	0.020%
65	18.545	2642	2645	2649	rBV6	4425	5951	0.19%	0.022%
66	18.639	2655	2661	2664	rBV6	17015	24776	0.81%	0.091%
67	18.698	2668	2671	2674	rVB4	9466	10915	0.36%	0.040%
68	18.728	2674	2676	2678	rVB3	6420	5613	0.18%	0.021%
69	18.775	2678	2684	2686	rBV5	15668	26664	0.87%	0.098%
70	18.828	2691	2693	2695	rVB2	3978	3388	0.11%	0.012%
71	18.892	2695	2704	2710	rBV	390675	541494	17.65%	1.987%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
 Data File : BN011492.D
 Acq On : 18 Aug 2020 19:43
 Operator : CG/JU
 Sample : L3611-20
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

72	18.969	2714	2717	2721	rBV6	8408	12668	0.41%	0.046%
73	19.045	2727	2730	2733	rBV4	9302	13163	0.43%	0.048%
74	19.116	2738	2742	2744	rBV4	10802	14418	0.47%	0.053%
75	19.228	2755	2761	2765	rBV	1485173	2080092	67.79%	7.634%
76	19.445	2795	2798	2801	rBV2	13788	18019	0.59%	0.066%
77	19.604	2817	2825	2830	rBV8	24627	63288	2.06%	0.232%
78	19.686	2837	2839	2841	rBV3	8832	7719	0.25%	0.028%
79	19.728	2844	2846	2848	rVV3	21794	22241	0.72%	0.082%
80	19.763	2850	2852	2856	rVV2	33887	47734	1.56%	0.175%
81	19.828	2860	2863	2865	rBV4	13515	16751	0.55%	0.061%
82	19.863	2867	2869	2873	rVB3	24262	27202	0.89%	0.100%
83	19.922	2875	2879	2883	rBV5	34155	48552	1.58%	0.178%
84	20.069	2900	2904	2906	rBV5	19838	25803	0.84%	0.095%
85	20.681	3006	3008	3012	rVB3	42296	51803	1.69%	0.190%
86	20.786	3024	3026	3030	rBV5	49010	52901	1.72%	0.194%
87	21.039	3063	3069	3073	rBV	2361370	3068329	100.00%	11.261%
88	21.075	3073	3075	3085	rVB	269622	302245	9.85%	1.109%
89	22.527	3318	3322	3325	rBV	258024	423087	13.79%	1.553%
90	23.016	3400	3405	3410	rBV2	1097255	1759757	57.35%	6.459%
91	23.145	3421	3427	3439	rVB2	1614034	2913712	94.96%	10.694%


Sum of corrected areas: 27246210

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011492.D
Acq On : 18 Aug 2020 19:43
Operator : CG/JU
Sample : L3611-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFM5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

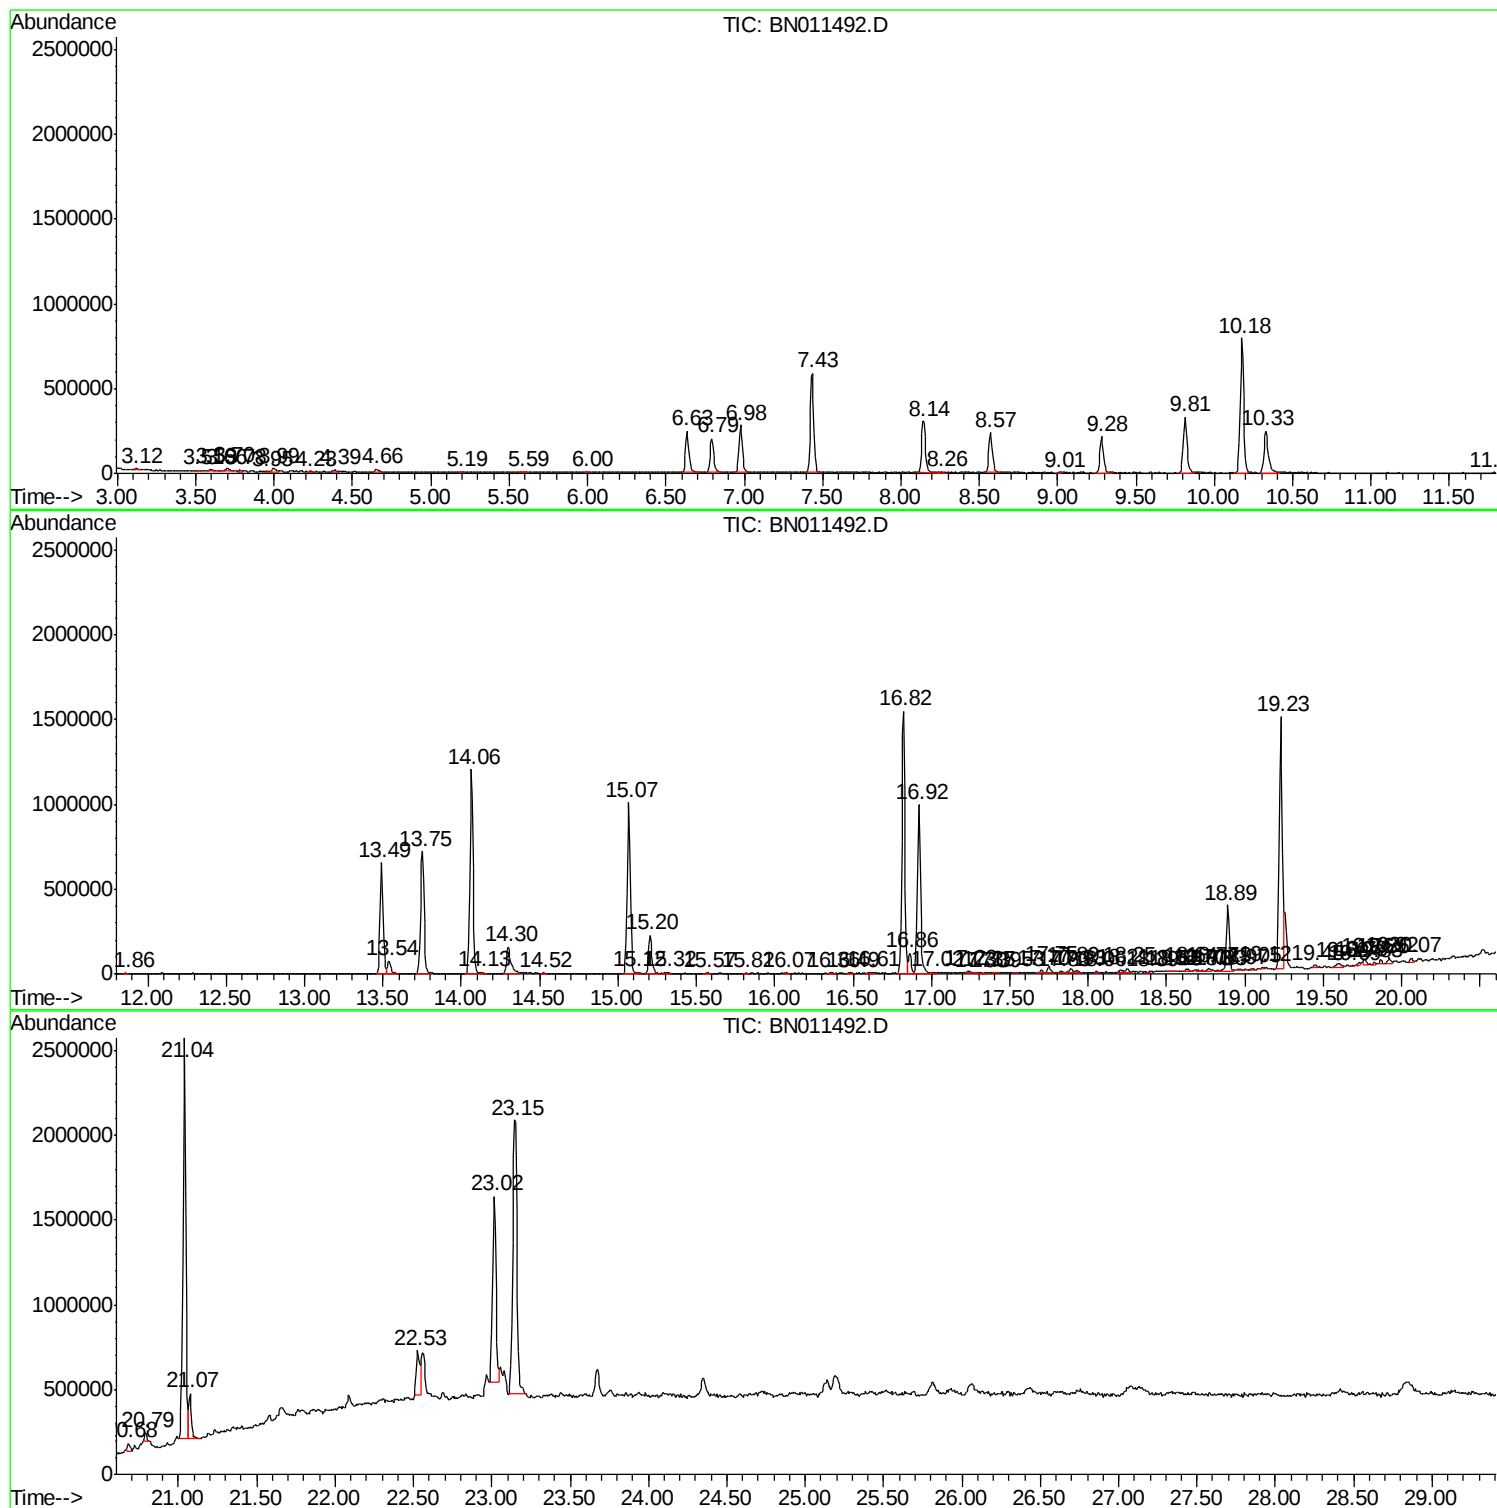

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011492.D
Acq On : 18 Aug 2020 19:43
Operator : CG/JU
Sample : L3611-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFM5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011492.D
Acq On : 18 Aug 2020 19:43
Operator : CG/JU
Sample : L3611-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFM5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
