

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011504.D
 Acq On : 19 Aug 2020 02:52
 Operator : CG/JU
 Sample : L3668-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFT2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	19	21	33	rVB	34472	57277	1.30%	0.149%
2	3.370	61	65	71	rVB4	8264	14785	0.34%	0.038%
3	3.705	118	122	127	rBV3	8139	11185	0.25%	0.029%
4	3.787	132	136	143	rVB3	10780	15781	0.36%	0.041%
5	4.005	171	173	177	rVB2	3428	4525	0.10%	0.012%
6	4.111	186	191	192	rBV4	3421	4719	0.11%	0.012%
7	4.622	273	278	282	rBV5	2833	4837	0.11%	0.013%
8	6.634	613	620	632	rVB	119222	194765	4.42%	0.506%
9	6.793	639	647	660	rBV	401823	656586	14.90%	1.706%
10	6.975	672	678	688	rBV	552564	850435	19.30%	2.210%
11	7.364	741	744	749	rVB2	6186	8781	0.20%	0.023%
12	7.428	749	755	767	rBV	600800	948178	21.52%	2.464%
13	7.775	811	814	820	rVB4	3964	4635	0.11%	0.012%
14	8.140	870	876	884	rBV	364139	576662	13.09%	1.498%
15	8.199	884	886	892	rVV5	4922	6699	0.15%	0.017%
16	8.275	895	899	903	rVV3	3802	4718	0.11%	0.012%
17	8.569	942	949	957	rBV	520785	848905	19.27%	2.206%
18	9.016	1020	1025	1029	rBV7	5585	8183	0.19%	0.021%
19	9.275	1063	1069	1083	rBV	491589	825037	18.73%	2.144%
20	9.810	1152	1160	1171	rBV	720850	1247112	28.31%	3.240%
21	10.175	1214	1222	1227	rBV	759763	1238051	28.10%	3.217%
22	10.222	1227	1230	1239	rVB	63217	97393	2.21%	0.253%
23	10.340	1241	1250	1254	rBV2	32815	64366	1.46%	0.167%
24	11.493	1442	1446	1452	rVB2	11085	17834	0.40%	0.046%
25	11.775	1489	1494	1498	rBV3	7814	13759	0.31%	0.036%
26	11.852	1504	1507	1514	rVB2	3675	5433	0.12%	0.014%
27	12.069	1541	1544	1551	rBV3	2737	4842	0.11%	0.013%
28	12.887	1679	1683	1690	rBV3	7955	12645	0.29%	0.033%
29	12.969	1693	1697	1698	rBV	3821	5085	0.12%	0.013%
30	13.487	1779	1785	1790	rBV	1445097	1964170	44.59%	5.104%
31	13.534	1790	1793	1800	rVB	262914	356884	8.10%	0.927%
32	13.751	1823	1830	1841	rBV	1603975	2409199	54.69%	6.260%
33	14.063	1876	1883	1890	rBV2	1123594	1630787	37.02%	4.237%
34	14.122	1890	1893	1901	rVB5	5783	9967	0.23%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011504.D
 Acq On : 19 Aug 2020 02:52
 Operator : CG/JU
 Sample : L3668-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFT2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	14.204	1901	1907	1917	rVB	31675	47266	1.07%	0.123%
36	14.298	1917	1923	1932	rBV	68358	136827	3.11%	0.356%
37	14.381	1932	1937	1940	rVB4	12155	18084	0.41%	0.047%
38	14.469	1947	1952	1959	rVB	36388	48315	1.10%	0.126%
39	14.628	1972	1979	1982	rBV4	8224	12927	0.29%	0.034%
40	15.069	2044	2054	2060	rBV	1923178	2789715	63.33%	7.249%
41	15.122	2060	2063	2071	rVV2	16895	24967	0.57%	0.065%
42	15.198	2071	2076	2089	rVV	570693	837245	19.01%	2.175%
43	15.310	2091	2095	2100	rVB2	23620	33230	0.75%	0.086%
44	15.692	2158	2160	2166	rVB4	12349	14162	0.32%	0.037%
45	15.863	2184	2189	2191	rBV3	7009	8016	0.18%	0.021%
46	15.987	2207	2210	2213	rBV4	3239	4837	0.11%	0.013%
47	16.081	2222	2226	2228	rVB4	8252	10151	0.23%	0.026%
48	16.116	2228	2232	2236	rVB4	6095	9069	0.21%	0.024%
49	16.357	2269	2273	2276	rVB3	4063	5585	0.13%	0.015%
50	16.439	2281	2287	2291	rVV6	54395	93105	2.11%	0.242%
51	16.481	2291	2294	2300	rVB3	66592	95167	2.16%	0.247%
52	16.575	2305	2310	2313	rBV4	5501	6770	0.15%	0.018%
53	16.604	2313	2315	2320	rBV3	4735	8125	0.18%	0.021%
54	16.704	2328	2332	2335	rBV4	3956	4456	0.10%	0.012%
55	16.816	2345	2351	2357	rBV	1501016	2003162	45.47%	5.205%
56	16.916	2362	2368	2379	rBV	2298361	3227093	73.25%	8.385%
57	17.087	2388	2397	2404	rBV7	51850	116259	2.64%	0.302%
58	17.234	2416	2422	2428	rVB	79802	119330	2.71%	0.310%
59	17.287	2428	2431	2434	rBV4	3994	5767	0.13%	0.015%
60	17.457	2458	2460	2465	rVB3	11926	12422	0.28%	0.032%
61	17.681	2494	2498	2501	rBV5	5169	8222	0.19%	0.021%
62	17.751	2503	2510	2518	rBV2	71579	111072	2.52%	0.289%
63	17.822	2518	2522	2529	rVV2	39497	60861	1.38%	0.158%
64	17.898	2532	2535	2538	rVB5	6673	6960	0.16%	0.018%
65	18.010	2549	2554	2559	rVV2	65700	105481	2.39%	0.274%
66	18.051	2559	2561	2566	rVB4	10272	11296	0.26%	0.029%
67	18.251	2591	2595	2600	rVV7	5068	7624	0.17%	0.020%
68	18.298	2600	2603	2608	rVV6	2665	4734	0.11%	0.012%
69	18.428	2622	2625	2628	rBV5	3850	6126	0.14%	0.016%
70	18.481	2630	2634	2637	rVB3	14612	17703	0.40%	0.046%
71	18.551	2641	2646	2650	rBV2	36993	57602	1.31%	0.150%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
 Data File : BN011504.D
 Acq On : 19 Aug 2020 02:52
 Operator : CG/JU
 Sample : L3668-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFT2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

72	18.710	2672	2673	2676	rBV3	4441	4986	0.11%	0.013%
73	18.857	2690	2698	2704	rBV2	29386	54406	1.24%	0.141%
74	19.045	2727	2730	2734	rBV4	22193	26938	0.61%	0.070%
75	19.116	2738	2742	2745	rBV	19982	23326	0.53%	0.061%
76	19.228	2755	2761	2768	rBV	3148755	4123345	93.60%	10.714%
77	19.439	2796	2797	2798	rBV	10165	6229	0.14%	0.016%
78	20.439	2965	2967	2971	rBV4	20965	33327	0.76%	0.087%
79	20.786	3022	3026	3033	rBV2	225657	322826	7.33%	0.839%
80	21.033	3063	3068	3075	rBV	2040042	2548831	57.86%	6.623%
81	23.010	3398	3404	3411	rBV	2630597	4405338	100.00%	11.447%
82	23.139	3420	3426	3434	rVB	1551919	2616044	59.38%	6.797%
83	27.845	4224	4226	4229	rBV3	79767	106758	2.42%	0.277%


Sum of corrected areas: 38486307

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011504.D
Acq On : 19 Aug 2020 02:52
Operator : CG/JU
Sample : L3668-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFT2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

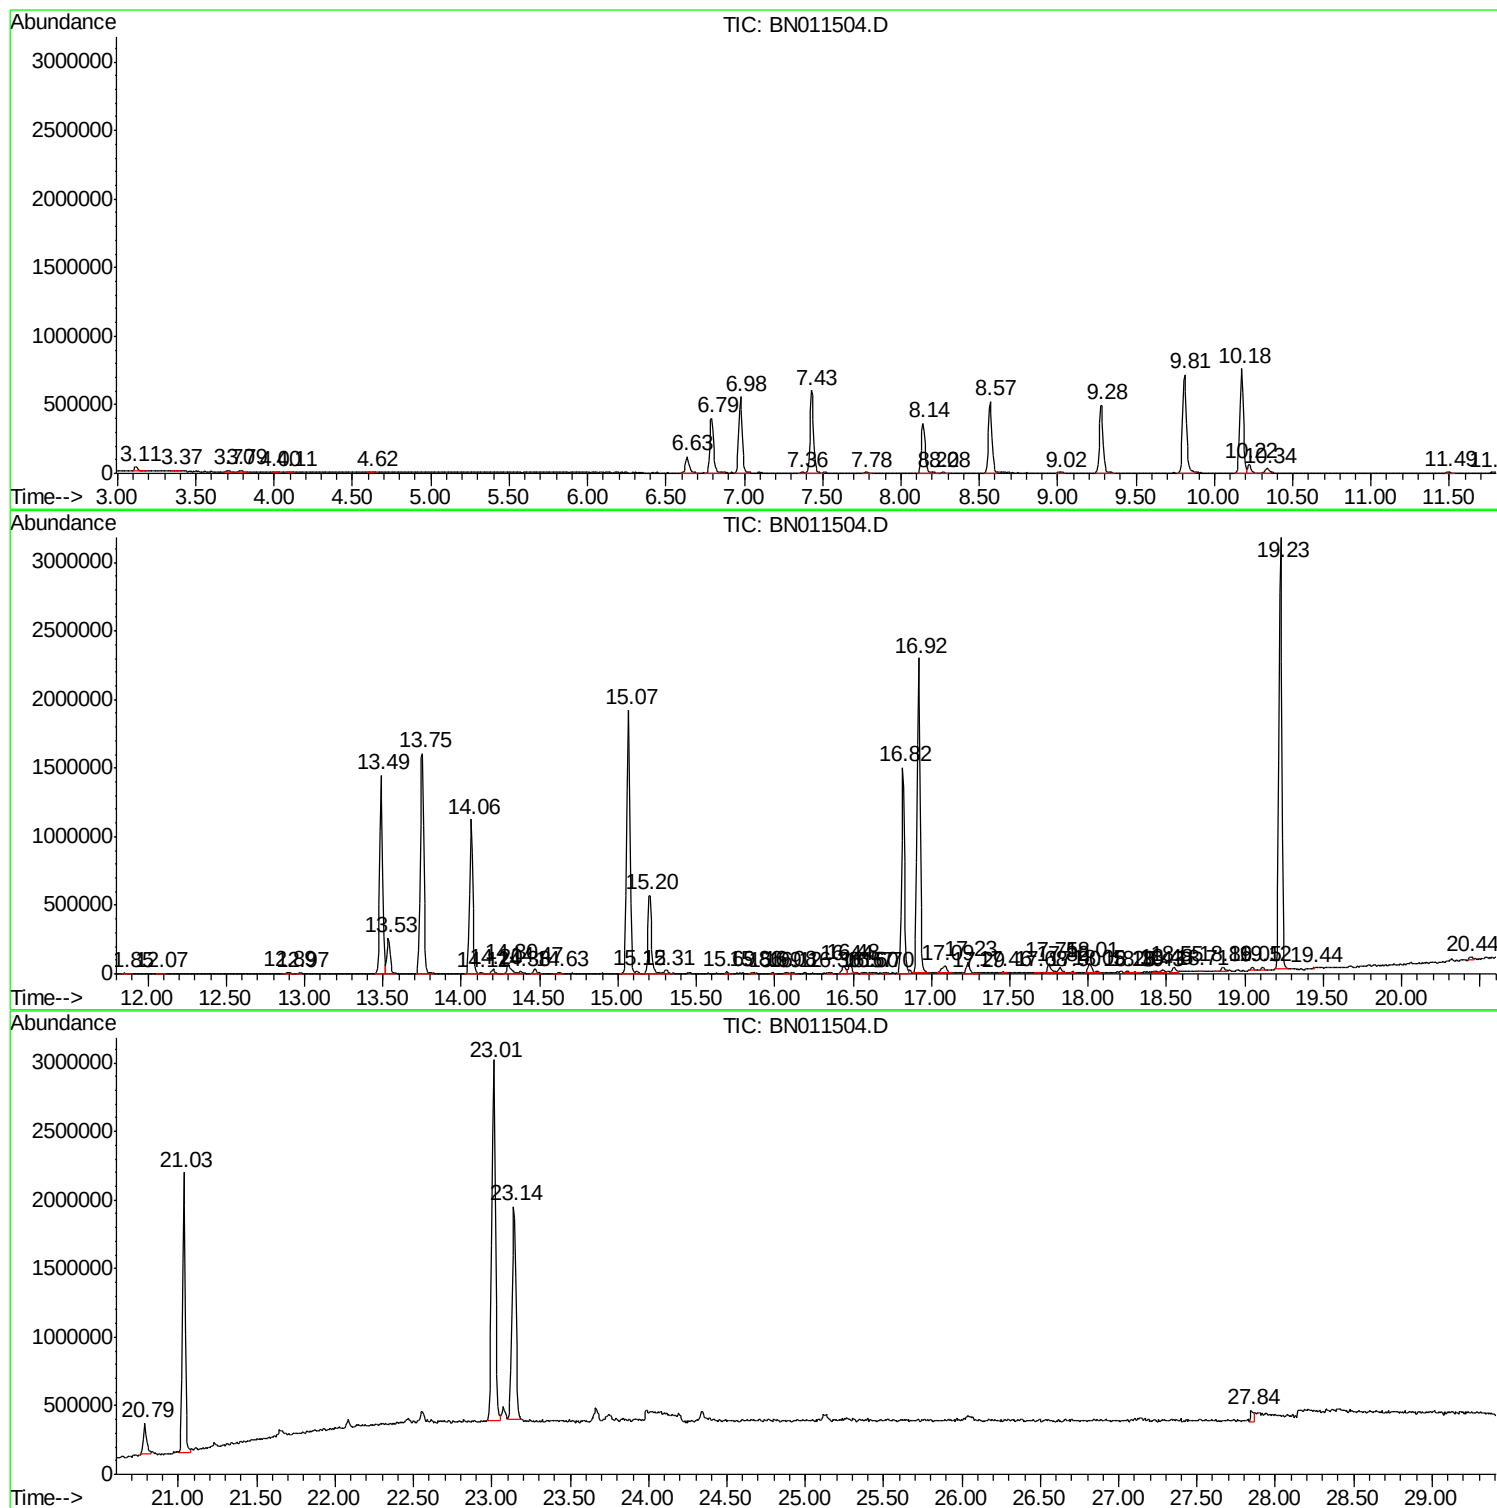

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081720\
Data File : BN011504.D
Acq On : 19 Aug 2020 02:52
Operator : CG/JU
Sample : L3668-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFT2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.79	2.53 ng/ul	322826	Chrysene-d12	21.03

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Eicosene, (E)-			280	C20H40	074685-33-9	98
2	Cyclopentadecane			210	C15H30	000295-48-7	96
3	1-Nonadecene			266	C19H38	018435-45-5	95
4	1-Heptacosanol			396	C27H56O	002004-39-9	91
5	Chloroacetic acid, pentadecyl ester			304	C17H33ClO2	070301-47-2	87

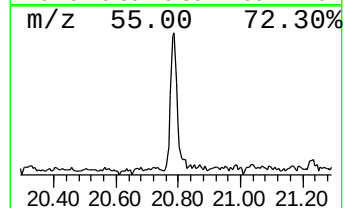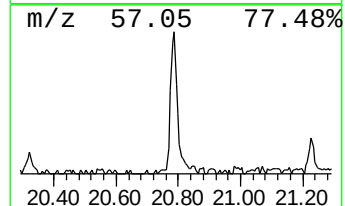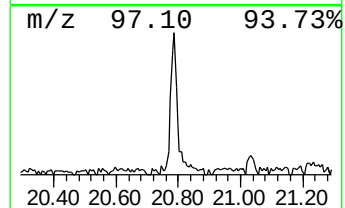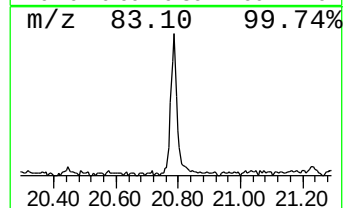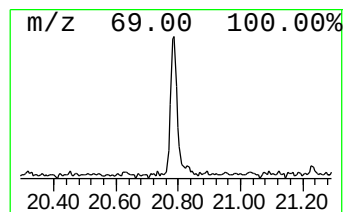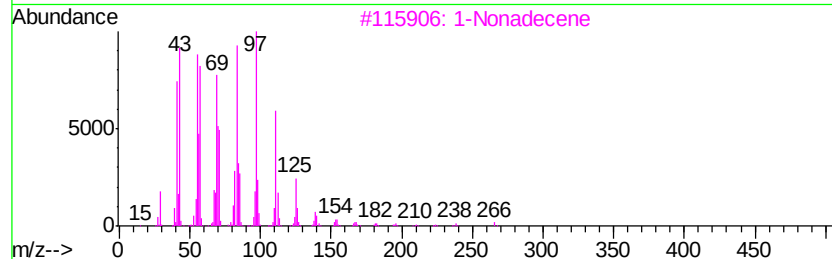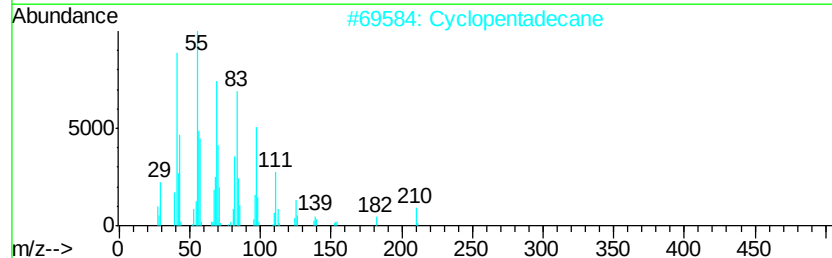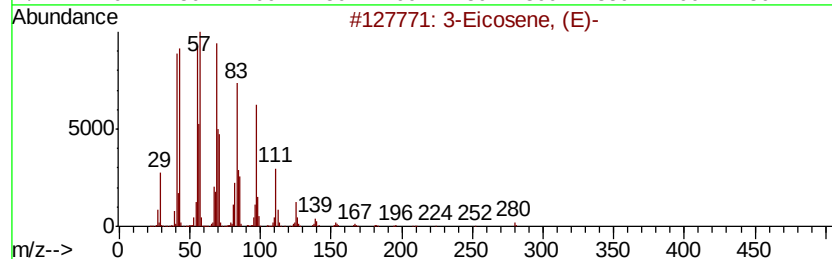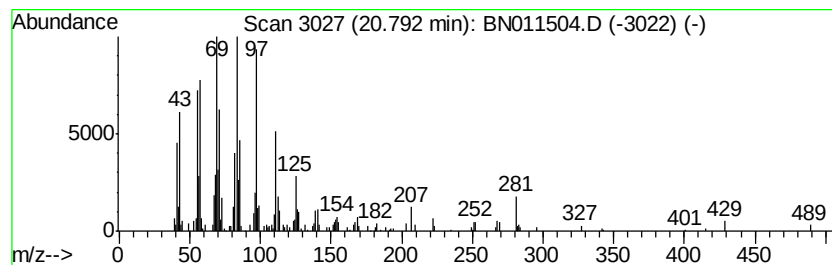

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081720\
Data File : BN011504.D
Acq On : 19 Aug 2020 02:52
Operator : CG/JU
Sample : L3668-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFT2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc

(DEL) Alkane: Str...	20.79	2.5	ng/ul	322826	5	21.03	2548830	20.0