

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
 Data File : BN021276.D
 Acq On : 17 Aug 2022 09:37
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Aug 18 06:40:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 16 09:19:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.783	152	3560	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	11607	0.400	ng	-0.01
13) Acenaphthene-d10	14.429	164	6967	0.400	ng	0.00
19) Phenanthrene-d10	17.182	188	13259	0.400	ng	0.00
29) Chrysene-d12	21.386	240	7922	0.400	ng	0.00
35) Perylene-d12	23.723	264	6140	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.371	112	3459	0.389	ng	0.00
5) Phenol-d6	6.974	99	4169	0.402	ng	0.00
8) Nitrobenzene-d5	8.948	82	3072	0.420	ng	-0.01
11) 2-Methylnaphthalene-d10	12.179	152	7266	0.360	ng	0.00
14) 2,4,6-Tribromophenol	15.941	330	652	0.286	ng	0.00
15) 2-Fluorobiphenyl	13.060	172	10864	0.392	ng	0.00
27) Fluoranthene-d10	19.223	212	13362	0.371	ng	0.00
31) Terphenyl-d14	19.830	244	8721	0.404	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.226	88	1874	0.377	ng	97
3) n-Nitrosodimethylamine	3.587	42	1297	0.398	ng	# 95
6) bis(2-Chloroethyl)ether	7.213	93	3880	0.443	ng	93
9) Naphthalene	10.624	128	13932	0.397	ng	100
10) Hexachlorobutadiene	10.912	225	2379	0.378	ng	# 100
12) 2-Methylnaphthalene	12.255	142	8341	0.348	ng	99
16) Acenaphthylene	14.151	152	10968	0.328	ng	99
17) Acenaphthene	14.493	154	8096	0.352	ng	99
18) Fluorene	15.487	166	10362	0.354	ng	99
20) 4,6-Dinitro-2-methylph...	15.615	198	251	0.371	ng	95
21) 4-Bromophenyl-phenylether	16.382	248	3072	0.377	ng	# 89
22) Hexachlorobenzene	16.495	284	3522	0.384	ng	97
23) Atrazine	16.659	200	1736	0.331	ng	98
24) Pentachlorophenol	16.854	266	708	0.343	ng	96
25) Phenanthrene	17.223	178	16738	0.379	ng	99
26) Anthracene	17.315	178	13024	0.353	ng	99
28) Fluoranthene	19.252	202	17182	0.372	ng	99
30) Pyrene	19.619	202	17154	0.420	ng	100
32) Benzo(a)anthracene	21.377	228	9443	0.366	ng	100
33) Chrysene	21.422	228	12967	0.405	ng	99
34) Bis(2-ethylhexyl)phtha...	21.305	149	6276	0.356	ng	100
36) Indeno(1,2,3-cd)pyrene	26.126	276	9758	0.359	ng	97
37) Benzo(b)fluoranthene	23.015	252	9765	0.381	ng	96
38) Benzo(k)fluoranthene	23.062	252	9984	0.386	ng	99
39) Benzo(a)pyrene	23.620	252	8025	0.376	ng	# 93
40) Dibenzo(a,h)anthracene	26.143	278	7582	0.361	ng	98
41) Benzo(g,h,i)perylene	26.860	276	9441	0.387	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
 Data File : BN021276.D
 Acq On : 17 Aug 2022 09:37
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Aug 18 06:40:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 16 09:19:59 2022
 Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.783 min Scan# 665
 Delta R.T. 0.000 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDC0.4

Tgt Ion:152 Resp: 3560
 Ion Ratio Lower Upper
 152 100
 150 152.6 123.1 184.7
 115 62.7 52.2 78.4



#2
 1,4-Dioxane
 Concen: 0.377 ng
 RT: 3.226 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37

Tgt Ion: 88 Resp: 1874
 Ion Ratio Lower Upper
 88 100
 43 35.4 28.6 42.8
 58 89.9 74.5 111.7









#3
n-Nitrosodimethylamine
Concen: 0.398 ng
RT: 3.587 min Scan# 84
Delta R.T. -0.007 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 1297
Ion Ratio Lower Upper
42 100
74 108.6 82.4 123.6
44 4.9 2.7 4.1#

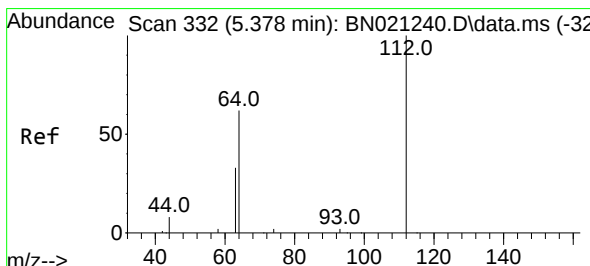

#4
2-Fluorophenol
Concen: 0.389 ng
RT: 5.371 min Scan# 331
Delta R.T. -0.007 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion: 112 Resp: 3459
Ion Ratio Lower Upper
112 100
64 64.8 52.0 78.0
63 33.8 27.5 41.3









#5
Phenol-d6
Concen: 0.402 ng
RT: 6.974 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 4169
Ion Ratio Lower Upper
99 100
42 24.1 19.1 28.7
71 35.2 28.9 43.3



#6
bis(2-Chloroethyl)ether
Concen: 0.443 ng
RT: 7.213 min Scan# 586
Delta R.T. -0.007 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion: 93 Resp: 3880
Ion Ratio Lower Upper
93 100
63 77.7 67.8 101.8
95 33.8 28.7 43.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	11607
Ion Ratio	Lower	Upper	
136	100		
137	11.6	9.6	14.4
54	12.1	8.2	12.2
68	7.7	5.3	7.9



#8
Nitrobenzene-d5
Concen: 0.420 ng
RT: 8.948 min Scan# 798
Delta R.T. -0.010 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:	82	Resp:	3072
Ion Ratio	Lower	Upper	
82	100		
128	37.9	33.6	50.4
54	64.2	50.2	75.2









#9
Naphthalene
Concen: 0.397 ng
RT: 10.624 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	128	Resp:	13932
Ion Ratio	Lower	Upper	
128	100		
129	11.7	9.4	14.0
127	13.7	11.0	16.6



#10
Hexachlorobutadiene
Concen: 0.378 ng
RT: 10.912 min Scan# 982
Delta R.T. -0.011 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:	225	Resp:	2379
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.4	50.9	76.3









#11
2-Methylnaphthalene-d10
Concen: 0.360 ng
RT: 12.179 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 7266
Ion Ratio Lower Upper
152 100
151 20.1 15.8 23.8



#12
2-Methylnaphthalene
Concen: 0.348 ng
RT: 12.255 min Scan# 1235
Delta R.T. -0.004 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:142 Resp: 8341
Ion Ratio Lower Upper
142 100
141 88.5 71.0 106.6
115 38.5 31.3 46.9








#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.429 min Scan# 1481
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:164 Resp: 6967
Ion Ratio Lower Upper
164 100
162 101.9 83.8 125.6
160 46.7 39.8 59.6



#14
2,4,6-Tribromophenol
Concen: 0.286 ng
RT: 15.941 min Scan# 1623
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:330 Resp: 652
Ion Ratio Lower Upper
330 100
332 94.3 78.1 117.1
141 53.8 45.4 68.0








#15
2-Fluorobiphenyl
Concen: 0.392 ng
RT: 13.060 min Scan# 1353
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	10864
Ion Ratio	Lower	Upper	
172	100		
171	34.2	28.4	42.6
170	23.2	19.0	28.6



#16
Acenaphthylene
Concen: 0.328 ng
RT: 14.151 min Scan# 1455
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:	152	Resp:	10968
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.8	23.6
153	13.0	10.4	15.6









#17
Acenaphthene
Concen: 0.352 ng
RT: 14.493 min Scan# 1487
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 8096
Ion Ratio Lower Upper
154 100
153 115.3 91.5 137.3
152 56.5 45.2 67.8



#18
Fluorene
Concen: 0.354 ng
RT: 15.487 min Scan# 1580
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:166 Resp: 10362
Ion Ratio Lower Upper
166 100
165 99.0 78.8 118.2
167 13.4 11.0 16.4









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.182 min Scan# 1744
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 13259
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.1 11.8 17.6



#20
4,6-Dinitro-2-methylphenol
Concen: 0.371 ng
RT: 15.615 min Scan# 1592
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:198 Resp: 251
Ion Ratio Lower Upper
198 100
182 45.8 33.9 50.9
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.377 ng
RT: 16.382 min Scan# 1666
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 3072
Ion Ratio Lower Upper
248 100
250 98.9 78.6 117.8
141 62.9 66.8 100.2#



#22
Hexachlorobenzene
Concen: 0.384 ng
RT: 16.495 min Scan# 1677
Delta R.T. -0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:284 Resp: 3522
Ion Ratio Lower Upper
284 100
142 47.7 36.0 54.0
249 32.6 27.0 40.6









#23
 Atrazine
 Concen: 0.331 ng
 RT: 16.659 min Scan# 1693
 Delta R.T. 0.000 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:200 Resp: 1736
 Ion Ratio Lower Upper
 200 100
 173 31.6 26.0 39.0
 215 46.7 38.2 57.4



#24
 Pentachlorophenol
 Concen: 0.343 ng
 RT: 16.854 min Scan# 1712
 Delta R.T. -0.010 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37

Tgt Ion:266 Resp: 708
 Ion Ratio Lower Upper
 266 100
 264 61.9 50.0 75.0
 268 63.8 47.1 70.7









#25
Phenanthrene
Concen: 0.379 ng
RT: 17.223 min Scan# 1748
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 16738
Ion Ratio Lower Upper
178 100
176 19.2 15.6 23.4
179 15.1 12.2 18.4



#26
Anthracene
Concen: 0.353 ng
RT: 17.315 min Scan# 1757
Delta R.T. -0.010 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:178 Resp: 13024
Ion Ratio Lower Upper
178 100
176 18.8 14.6 22.0
179 15.3 11.7 17.5







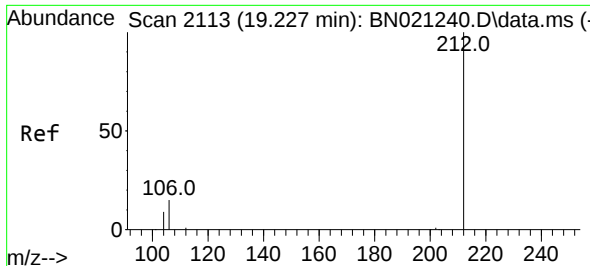

#27
Fluoranthene-d10
Concen: 0.371 ng
RT: 19.223 min Scan# 2112
Delta R.T. -0.004 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 13362
Ion Ratio Lower Upper
212 100
106 16.8 12.6 18.8
104 9.8 7.2 10.8

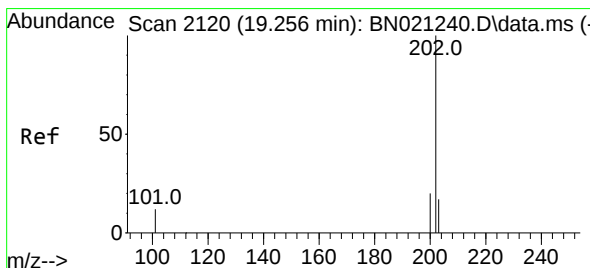

#28
Fluoranthene
Concen: 0.372 ng
RT: 19.252 min Scan# 2119
Delta R.T. -0.004 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:202 Resp: 17182
Ion Ratio Lower Upper
202 100
101 13.1 10.1 15.1
203 16.6 13.3 19.9





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.386 min Scan# 2452

Delta R.T. 0.000 min

Lab File: BN021276.D

Acq: 17 Aug 2022 09:37

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:240 Resp: 7922

Ion Ratio Lower Upper

240 100

120 18.6 13.4 20.2

236 28.6 22.6 33.8



#30

Pyrene

Concen: 0.420 ng

RT: 19.619 min Scan# 2206

Delta R.T. 0.000 min

Lab File: BN021276.D

Acq: 17 Aug 2022 09:37




Tgt Ion:202 Resp: 17154

Ion Ratio Lower Upper

202 100

200 20.8 16.8 25.2

203 17.7 14.2 21.4









#31
 Terphenyl-d14
 Concen: 0.404 ng
 RT: 19.830 min Scan# 211
 Delta R.T. 0.000 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 8721
 Ion Ratio Lower Upper
 244 100
 212 9.7 8.3 12.5
 122 0.0 0.0 0.0



#32
 Benzo(a)anthracene
 Concen: 0.366 ng
 RT: 21.377 min Scan# 2451
 Delta R.T. 0.000 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37

Tgt Ion:228 Resp: 9443
 Ion Ratio Lower Upper
 228 100
 226 28.1 22.4 33.6
 229 20.6 16.6 24.8



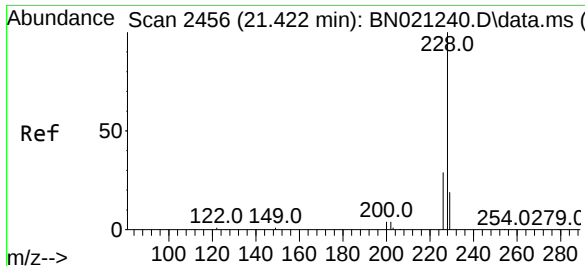

#33

Chrysene

Concen: 0.405 ng

RT: 21.422 min Scan# 2456

Delta R.T. 0.000 min

Lab File: BN021276.D

Acq: 17 Aug 2022 09:37

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 12967

Ion Ratio Lower Upper

228 100

226 30.9 23.8 35.8

229 19.8 15.9 23.9

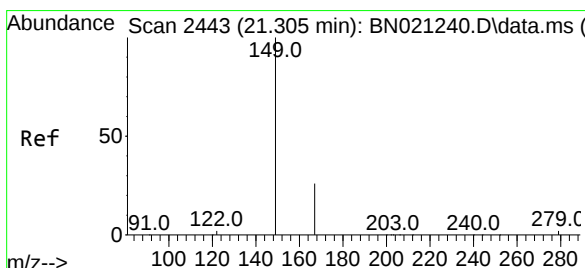

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.356 ng

RT: 21.305 min Scan# 2443

Delta R.T. 0.000 min

Lab File: BN021276.D

Acq: 17 Aug 2022 09:37




Tgt Ion:149 Resp: 6276


Ion Ratio Lower Upper

149 100

167 25.7 20.6 31.0

279 2.7 2.4 3.6









#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.723 min Scan# 3016
 Delta R.T. 0.003 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:264 Resp: 6140
 Ion Ratio Lower Upper
 264 100
 260 26.6 21.4 32.2
 265 41.1 34.3 51.5



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.359 ng
 RT: 26.126 min Scan# 3838
 Delta R.T. -0.003 min
 Lab File: BN021276.D
 Acq: 17 Aug 2022 09:37

Tgt Ion:276 Resp: 9758
 Ion Ratio Lower Upper
 276 100
 138 32.7 24.2 36.2
 277 24.9 19.1 28.7









#37
Benzo(b)fluoranthene
Concen: 0.381 ng
RT: 23.015 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 9765
Ion Ratio Lower Upper
252 100
253 25.6 21.4 32.0
125 16.3 15.3 22.9



#38
Benzo(k)fluoranthene
Concen: 0.386 ng
RT: 23.062 min Scan# 2790
Delta R.T. 0.003 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Tgt Ion:252 Resp: 9984
Ion Ratio Lower Upper
252 100
253 25.9 21.4 32.2
125 15.6 12.6 18.8









#39
Benzo(a)pyrene
Concen: 0.376 ng
RT: 23.620 min Scan# 2981
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 8025
Ion Ratio Lower Upper
252 100
253 30.6 24.8 37.2
125 22.0 23.8 35.6#



#40
Dibenzo(a,h)anthracene
Concen: 0.361 ng
RT: 26.143 min Scan# 3844
Delta R.T. -0.003 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37


Tgt Ion:278 Resp: 7582
Ion Ratio Lower Upper
278 100
139 26.1 20.5 30.7
279 28.6 23.8 35.8





#41
Benzo(g,h,i)perylene
Concen: 0.387 ng
RT: 26.860 min Scan# 4089
Delta R.T. 0.000 min
Lab File: BN021276.D
Acq: 17 Aug 2022 09:37

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion:276 Resp: 9441
Ion Ratio Lower Upper
276 100
277 25.5 21.0 31.4
138 30.7 23.8 35.6

