
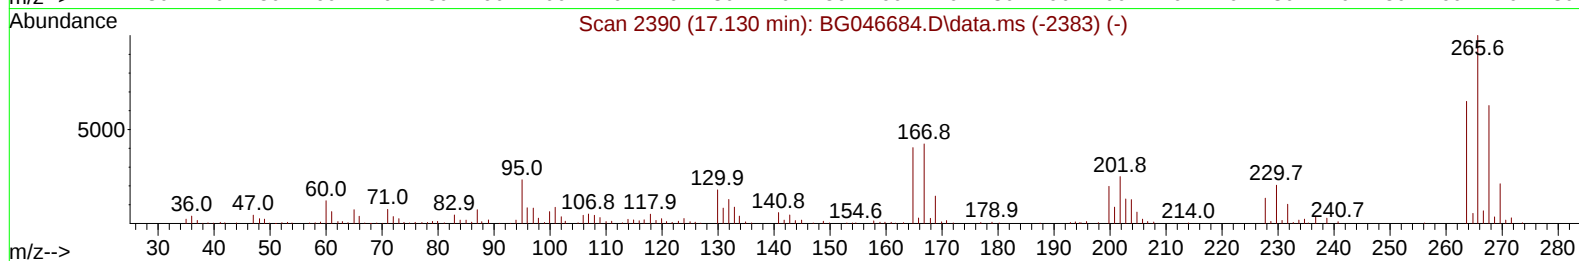
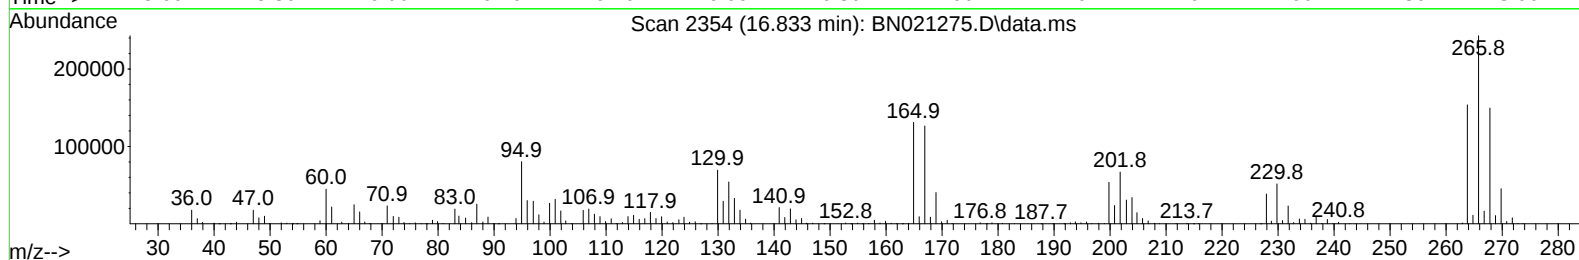


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
Data File : BN021275.D
Acq On : 17 Aug 2022 09:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 08:43:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 08:42:23 2022
Response via : Initial Calibration

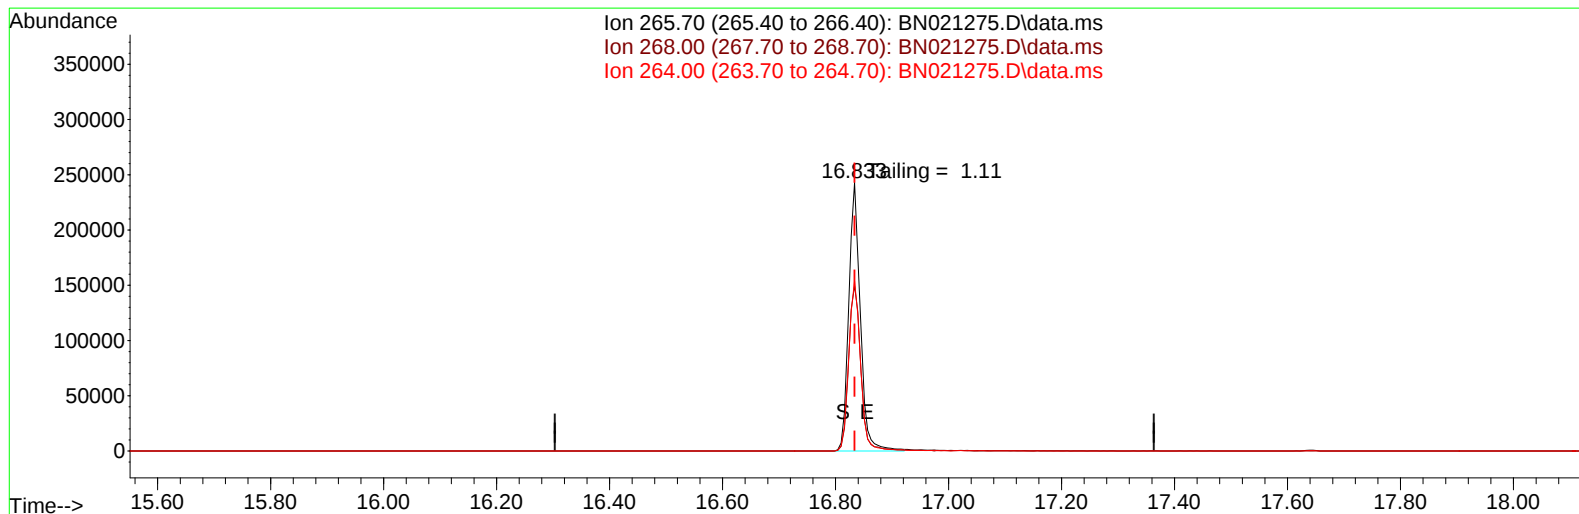

TIC: BN021275.D\data.ms

(70) Pentachlorophenol (C)




16.833min (0.000) 18764.82 ng

response 349010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.55
264.00	61.60	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
Data File : BN021275.D
Acq On : 17 Aug 2022 09:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 08:43:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 08:42:23 2022
Response via : Initial Calibration

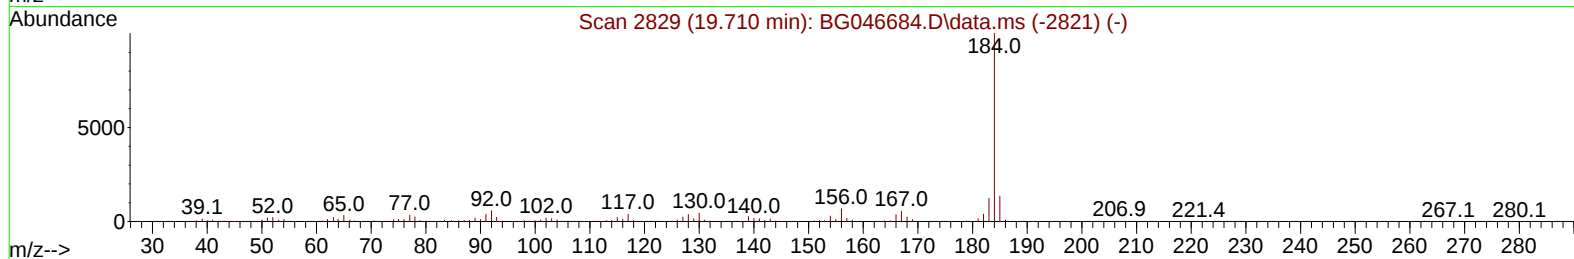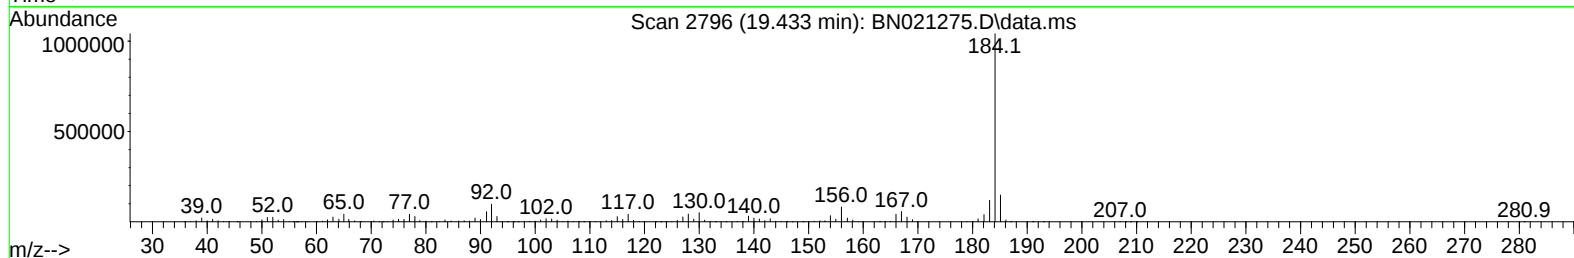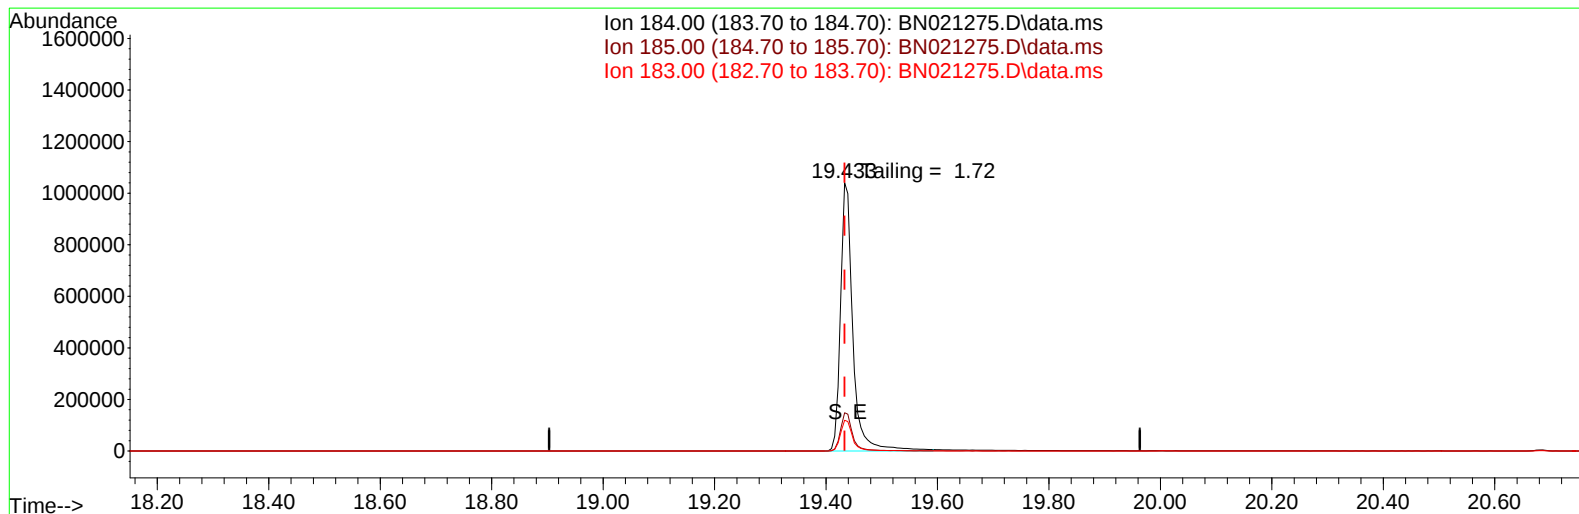

TIC: BN021275.D\data.ms

(77) Benzidine

19.433min (0.000) 0.00 ng

response 1642165

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	11.44
0.00	0.00	0.00