


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
 Data File : BN021275.D
 Acq On : 17 Aug 2022 09:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 16 09:19:59 2022

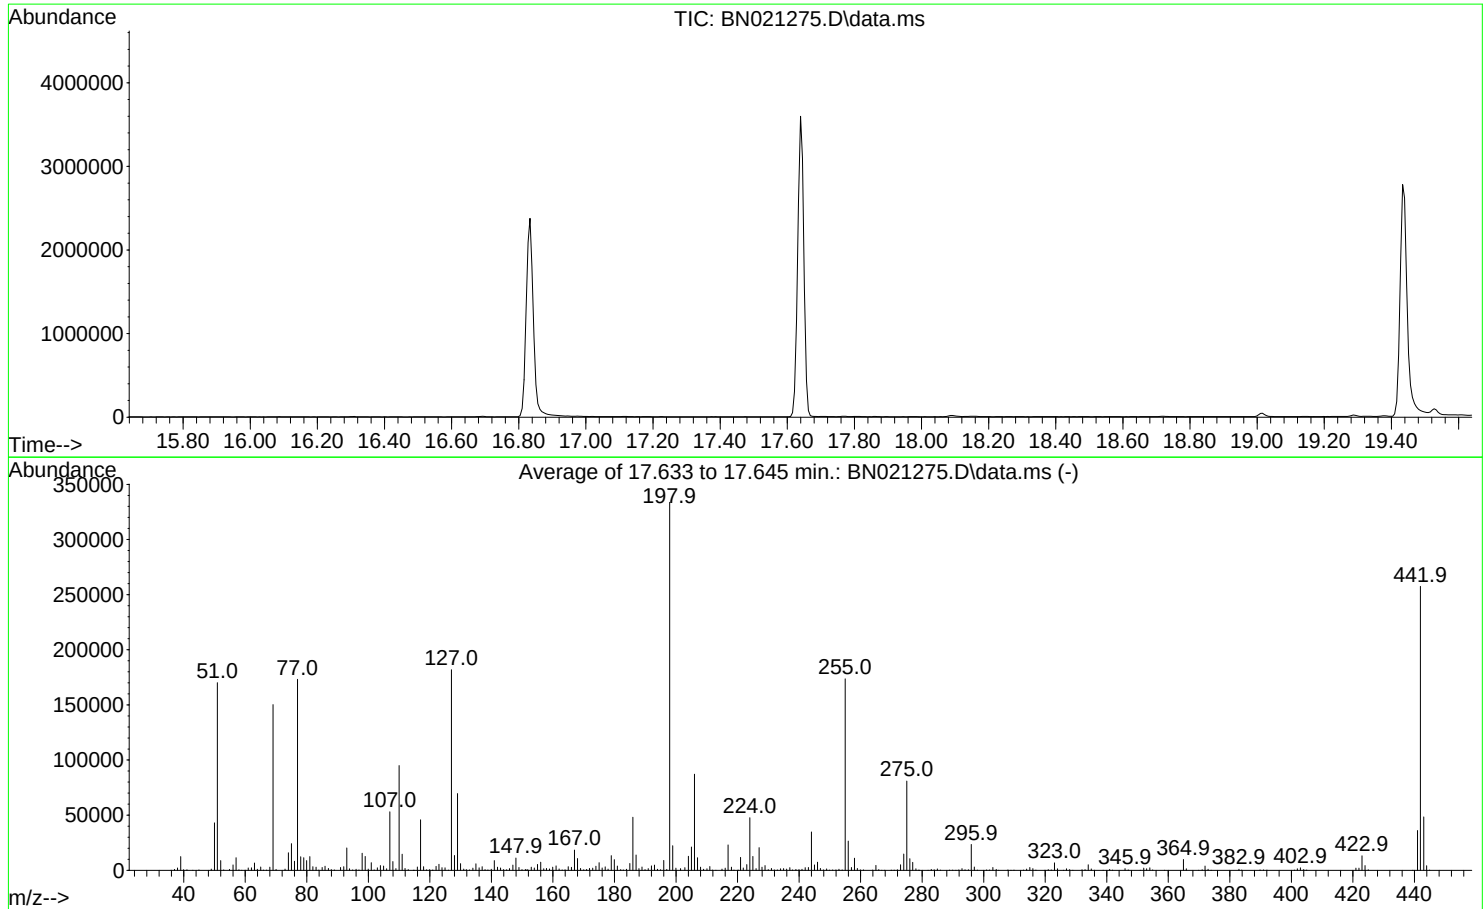




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	170158	PASS
68	69	0.00	2	1.9	2790	PASS
69	198	0.00	100	45.0	150208	PASS
70	69	0.00	2	0.5	798	PASS
127	198	10	80	54.5	181952	PASS
197	198	0.00	2	0.3	846	PASS
198	198	100	100	100.0	333632	PASS
199	198	5	9	6.7	22317	PASS
275	198	10	60	24.3	80925	PASS
365	198	1	100	3.0	9844	PASS
441	198	0.01	100	10.8	36141	PASS
442	442	50	100	100.0	257536	PASS
443	442	15	24	18.8	48363	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
Data File : BN021275.D
Acq On : 17 Aug 2022 09:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 18 08:43:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 08:42:23 2022
Response via : Initial Calibration

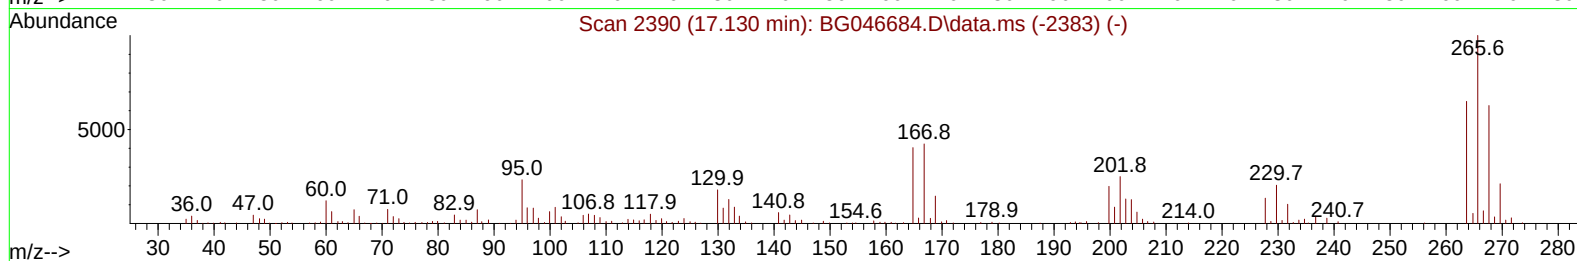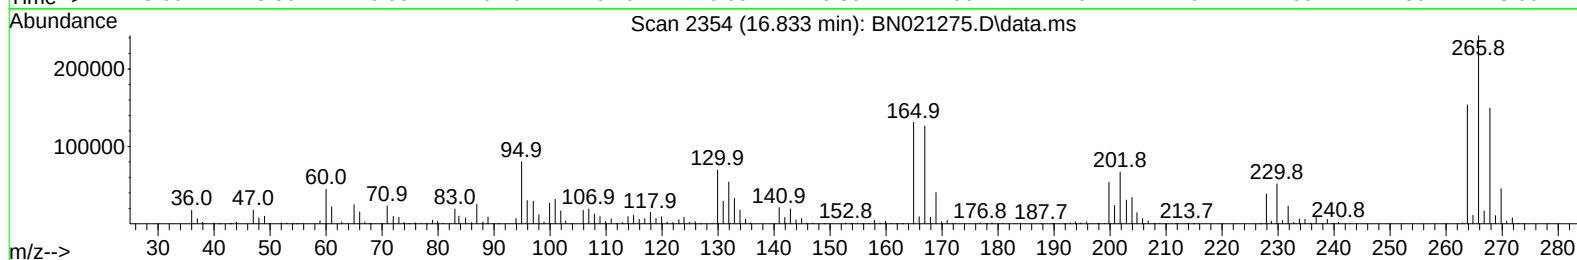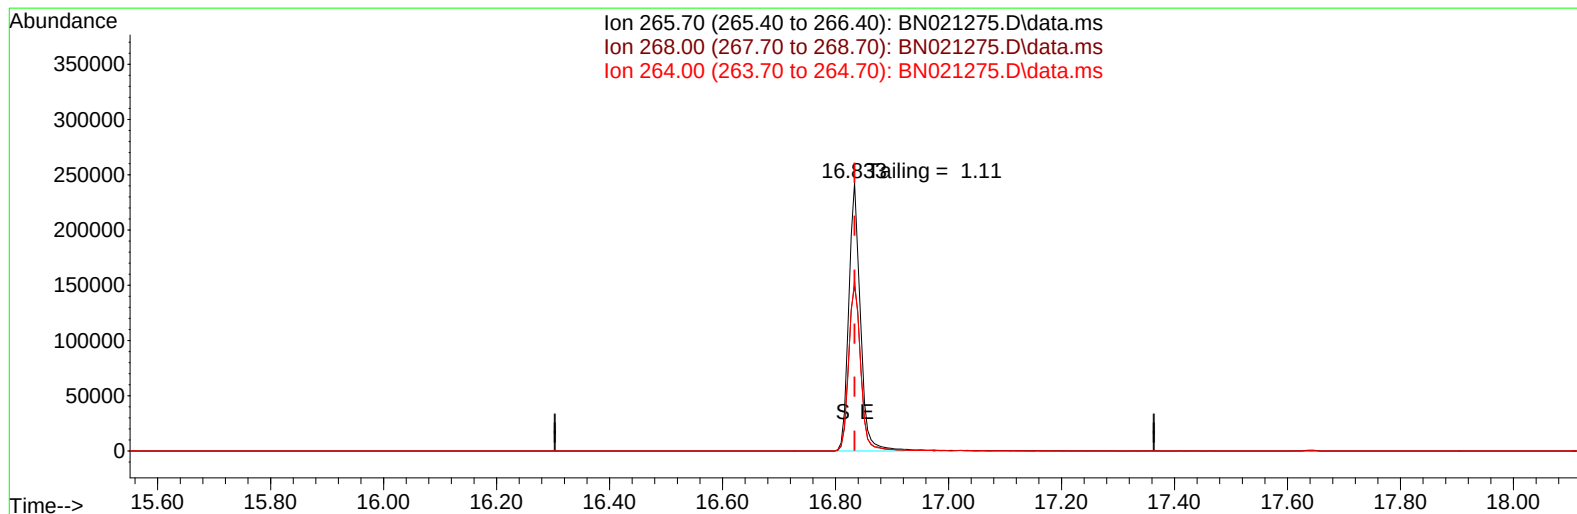

TIC: BN021275.D\data.ms

(70) Pentachlorophenol (C)

16.833min (0.000) 18764.82 ng




response 349010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.55
264.00	61.60	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081722\
Data File : BN021275.D
Acq On : 17 Aug 2022 09:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 18 08:43:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 08:42:23 2022
Response via : Initial Calibration

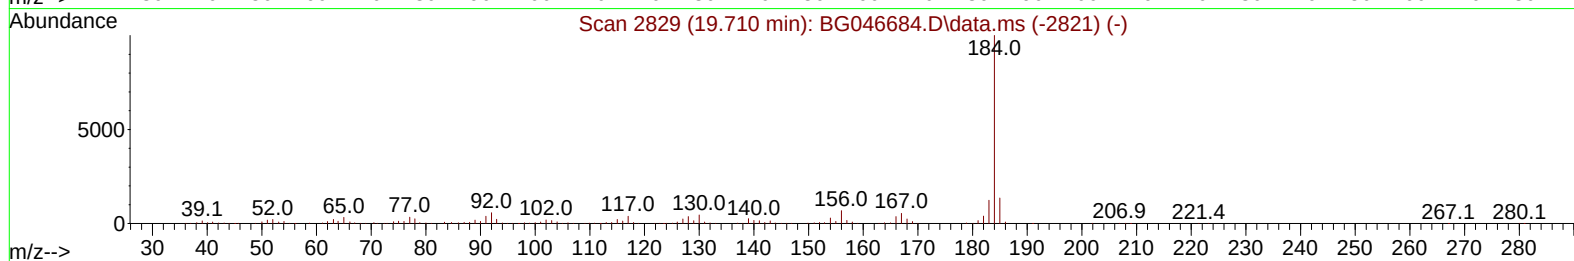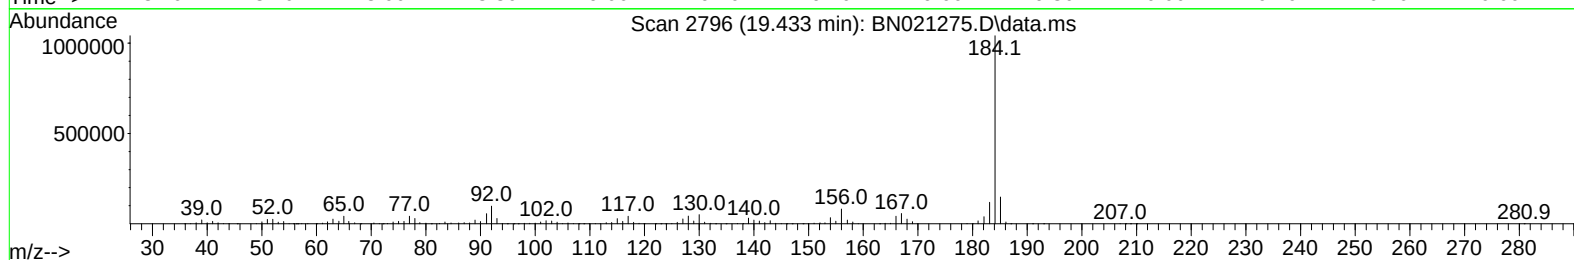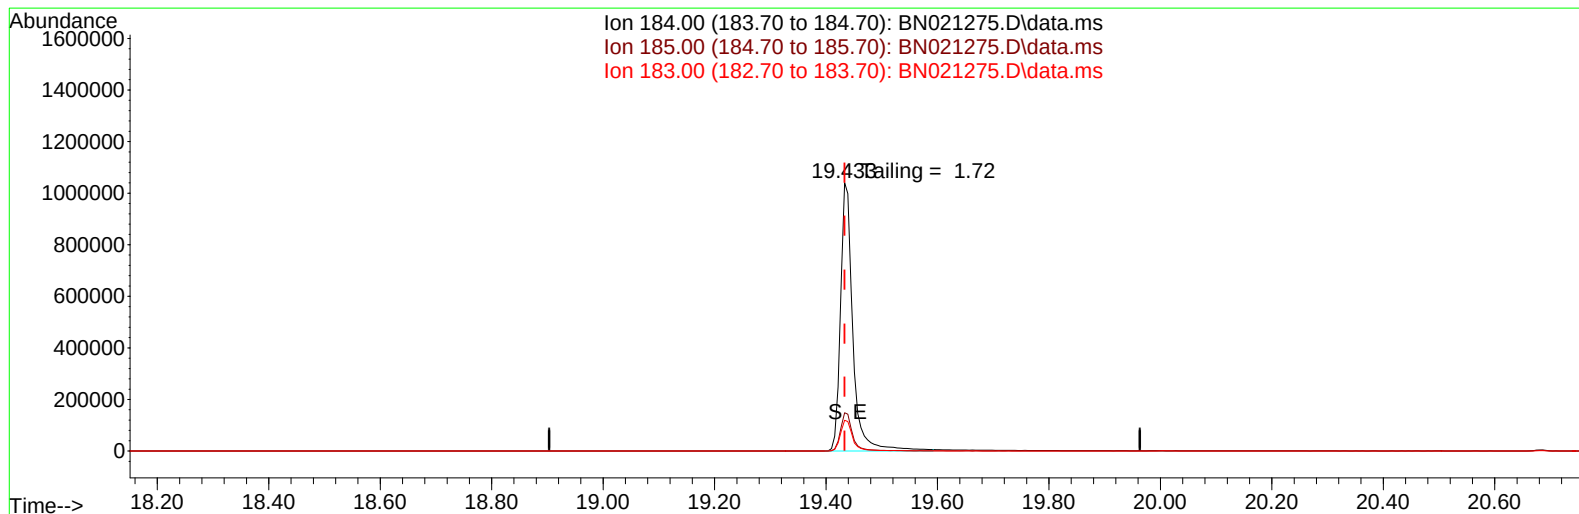

TIC: BN021275.D\data.ms

(77) Benzidine

19.433min (0.000) 0.00 ng

response 1642165

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2022	BNA_N	<u>BN021275.D</u>
Compound Name	Response	Retention Time
DDT	1061237	20.686
DDD	66177	20.239
DDE	4689	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
70866	1132103	6.26

Instrument :
BNA_N
ClientSampleId :
DFTPP