
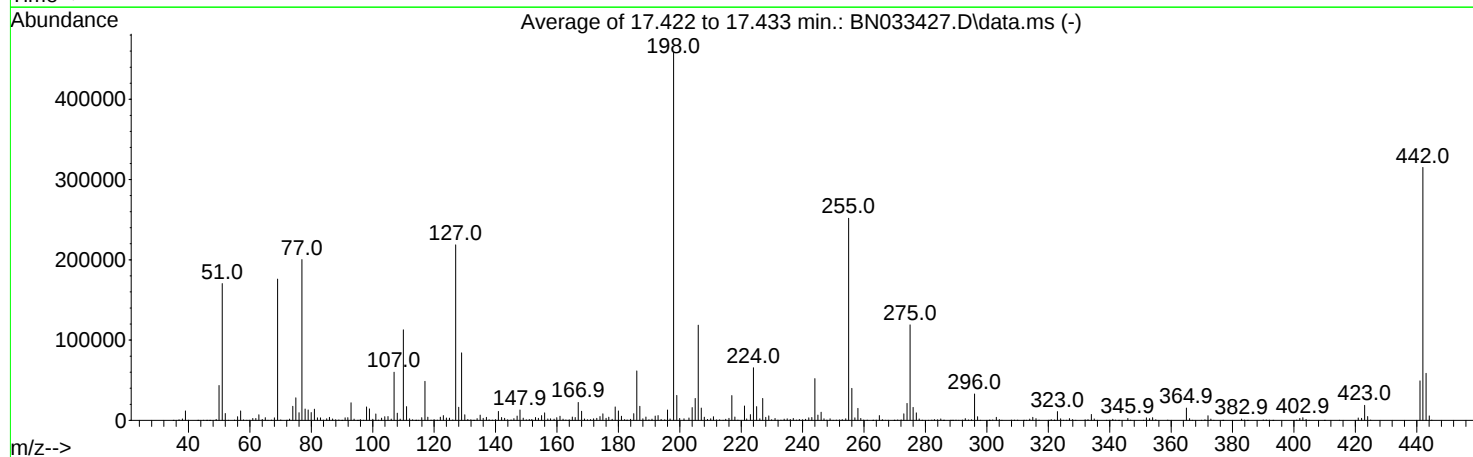


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081724\
Data File : BN033427.D
Acq On : 16 Aug 2024 12:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 16 04:44:11 2024

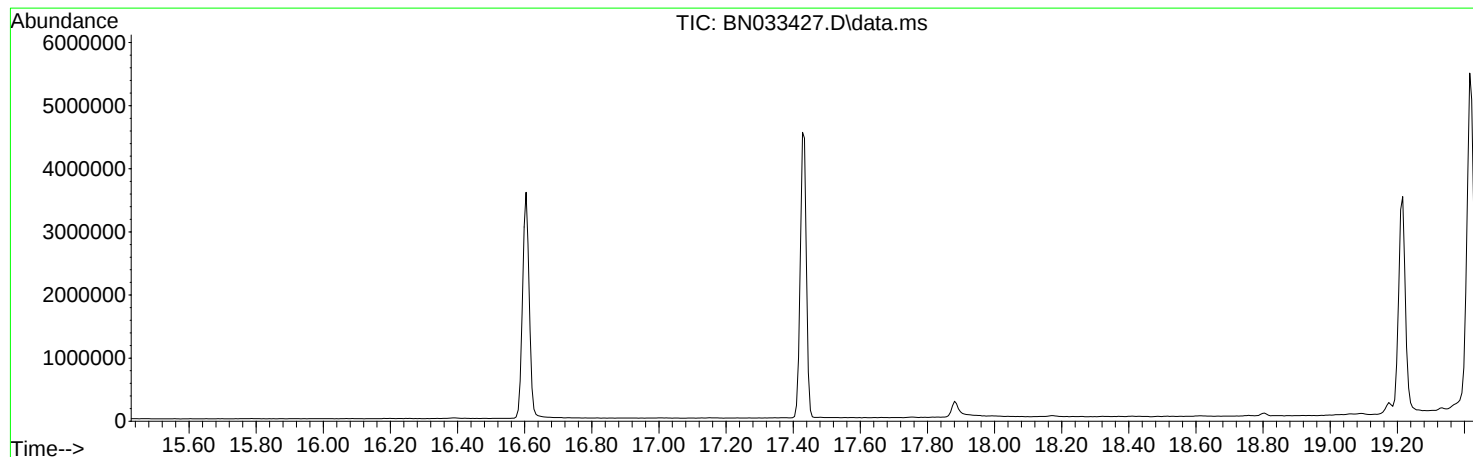

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	170491	PASS
68	69	0.00	2	1.8	3158	PASS
69	198	0.00	100	38.4	175968	PASS
70	69	0.00	2	0.3	564	PASS
127	198	10	80	47.7	218645	PASS
197	198	0.00	2	0.4	1784	PASS
198	198	100	100	100.0	458283	PASS
199	198	5	9	6.8	31059	PASS
275	198	10	60	25.9	118923	PASS
365	198	1	100	3.3	15294	PASS
441	198	0.01	100	10.7	49232	PASS
442	442	50	100	100.0	315072	PASS
443	442	15	24	18.6	58544	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/17/2024	BNA_N	<u>BN033427.D</u>
Compound Name	Response	Retention Time
DDT	1407924	20.469
DDD	113057	20.021
DDE	4154	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
117211	1525135	7.69

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081724\
Data File : BN033427.D
Acq On : 16 Aug 2024 12:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 03:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 17 03:18:59 2024
Response via : Initial Calibration

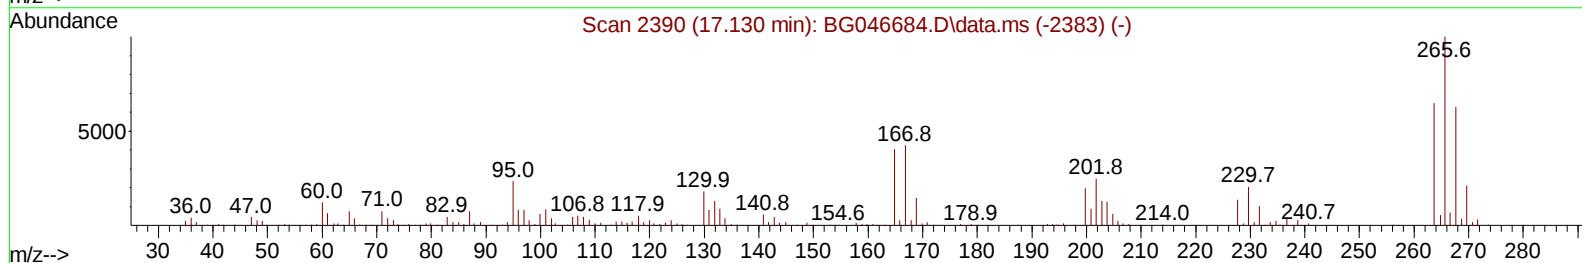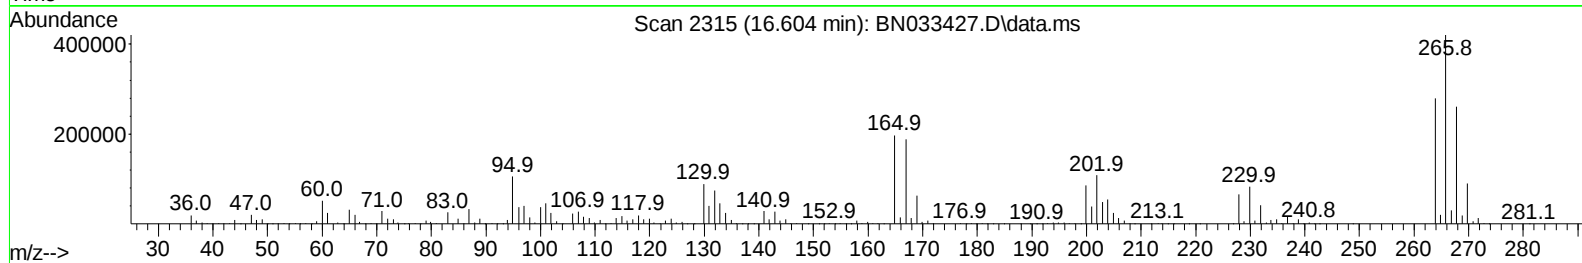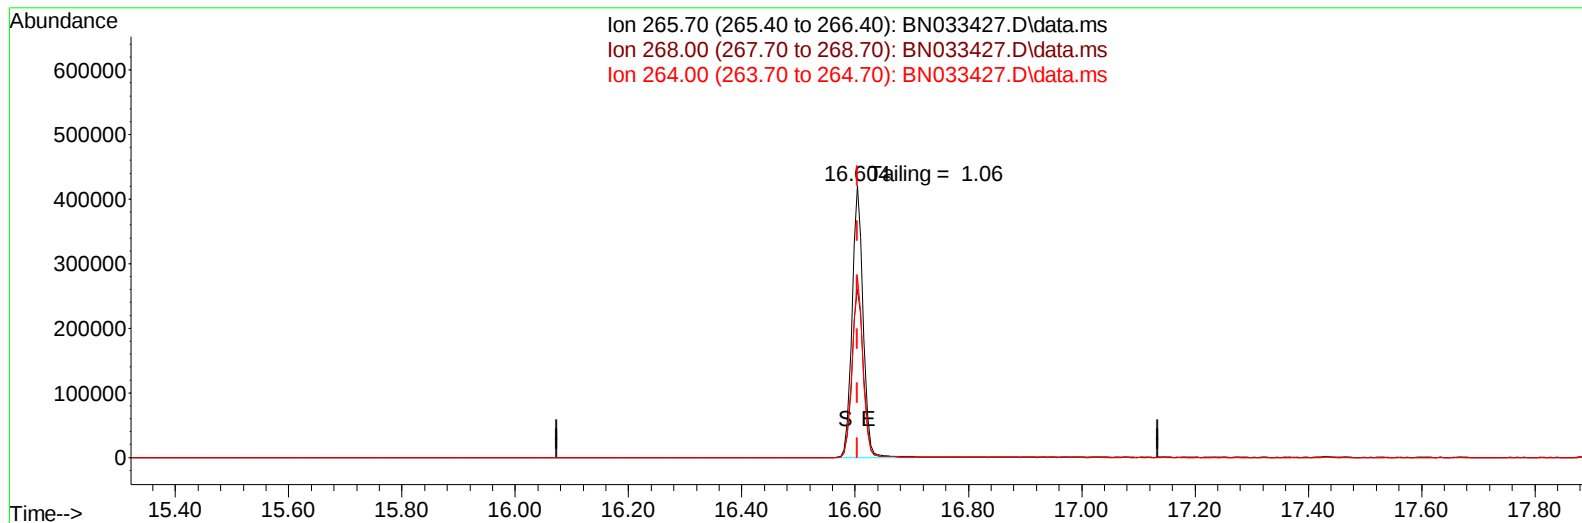

TIC: BN033427.D\data.ms

(70) Pentachlorophenol (C)

16.604min (0.000) 25557.41 ng




response 574427

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.98
264.00	61.60	66.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081724\
Data File : BN033427.D
Acq On : 16 Aug 2024 12:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 17 03:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 17 03:18:59 2024
Response via : Initial Calibration

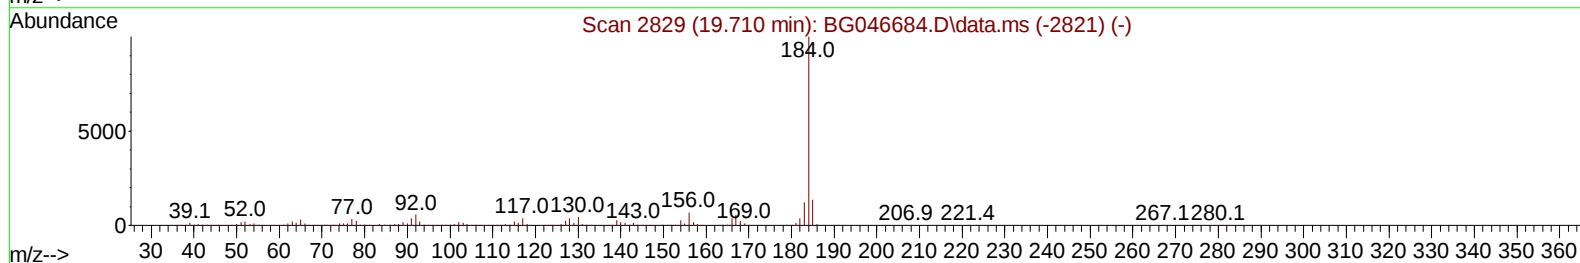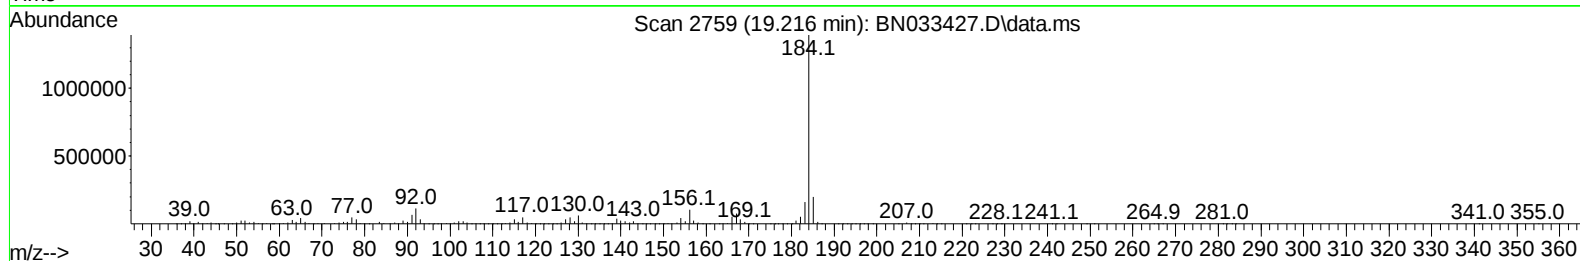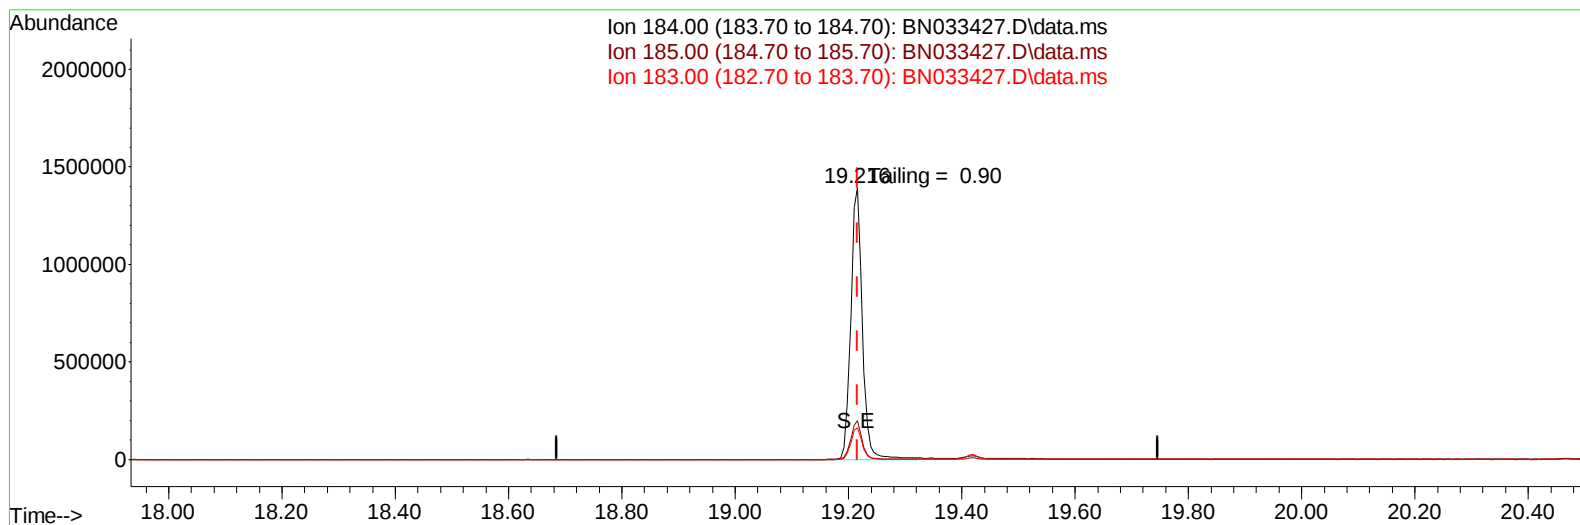

TIC: BN033427.D\data.ms

(77) Benzidine

19.216min (0.000) 1181394.59 ng

response 2002931

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.18
183.00	13.20	11.59
0.00	0.00	0.00