

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081822\
 Data File : BN021285.D
 Acq On : 18 Aug 2022 18:10
 Operator : CG/JU
 Sample : SSTD01024
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010225

Quant Time: Aug 18 19:42:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 18 19:40:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	113219	20.000	ng/u1	0.00
20) Naphthalene-d8	10.934	136	457821	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.757	164	260001	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.510	188	510147	20.000	ng/u1	0.00
79) Chrysene-d12	21.704	240	476159	20.000	ng/u1	0.00
88) Perylene-d12	24.245	264	485264	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	12563	4.806	ng/uL	0.00
4) Pyridine-d5	3.823	84	78843	11.035	ng/u1	0.00
7) Phenol-d5	7.246	99	93737	10.006	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	58506	9.995	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	73180	9.614	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	68157	8.409	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	27165	7.799	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	21637	5.853	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	61553	9.539	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	97862	9.365	ng/u1	0.00
46) Dimethylphthalate-d6	14.169	166	170702	9.023	ng/u1	0.00
49) Acenaphthylene-d8	14.451	160	215099	9.804	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	21478	5.666	ng/u1	0.00
60) Fluorene-d10	15.745	176	152791	9.760	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	10357	3.505	ng/u1	0.00
73) Anthracene-d10	17.604	188	232680	10.451	ng/u1	0.00
81) Pyrene-d10	19.898	212	244595	9.475	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.080	264	233646	9.841	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	13646	4.945	ng/uL#	89
5) Pyridine	3.840	79	79563	10.622	ng/u1	88
6) Benzaldehyde	7.222	77	43971	9.961	ng/u1	95
8) Phenol	7.269	94	96959	9.719	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.516	93	79208	10.144	ng/u1	93
12) 2-Chlorophenol	7.652	128	78256	9.835	ng/u1	96
13) 2-Methylphenol	8.546	108	71885	9.373	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.634	45	63558	5.191	ng/u1	95
16) Acetophenone	8.934	105	113671	9.222	ng/u1	92
17) N-Nitroso-di-n-propyla...	8.916	70	55080	8.747	ng/u1	94
18) 4-Methylphenol	8.875	108	75660	8.938	ng/u1	98
19) Hexachloroethane	9.199	117	33306	10.403	ng/u1	91
22) Nitrobenzene	9.316	77	70255	8.699	ng/u1	99
23) Isophorone	9.846	82	153984	9.657	ng/u1	99
25) 2-Nitrophenol	10.040	139	25536	6.252	ng/u1	94
26) 2,4-Dimethylphenol	10.093	107	80457	9.508	ng/u1	92
27) Bis(2-Chloroethoxy)met...	10.340	93	98217	10.065	ng/u1	99
29) 2,4-Dichlorophenol	10.575	162	62803	9.409	ng/u1	99
30) Naphthalene	10.987	128	243720	10.272	ng/u1	98
32) 4-Chloroaniline	11.093	127	99952	9.563	ng/u1	98
33) Hexachlorobutadiene	11.269	225	39248	10.241	ng/u1	99
34) Caprolactam	11.840	113	17431	6.687	ng/u1	88
35) 4-Chloro-3-methylphenol	12.210	107	64245	8.151	ng/u1	94
36) 2-Methylnaphthalene	12.593	142	157297	9.806	ng/u1	94

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081822\
 Data File : BN021285.D
 Acq On : 18 Aug 2022 18:10
 Operator : CG/JU
 Sample : SSTD01024
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010225

Quant Time: Aug 18 19:42:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 18 19:40:32 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.810	142	158763	9.699	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.951	216	72788	10.977	ng/ul	94
40) Hexachlorocyclopentadiene	12.934	237	40615	10.069	ng/ul#	91
41) 2,4,6-Trichlorophenol	13.193	196	41004	8.968	ng/ul	94
42) 2,4,5-Trichlorophenol	13.257	196	42921	8.476	ng/ul	99
43) 1,1'-Biphenyl	13.593	154	201708	10.477	ng/ul	99
44) 2-Chloronaphthalene	13.640	162	152507	10.442	ng/ul	98
45) 2-Nitroaniline	13.834	65	25388	5.587	ng/ul	93
47) Dimethylphthalate	14.210	163	180693	9.488	ng/ul	99
48) 2,6-Dinitrotoluene	14.328	165	21137	5.677	ng/ul#	94
50) Acenaphthylene	14.481	152	249640	10.277	ng/ul	99
51) 3-Nitroaniline	14.657	138	21604	5.488	ng/ul#	94
52) Acenaphthene	14.822	153	162063	10.214	ng/ul	99
53) 2,4-Dinitrophenol	14.857	184	6980	2.928	ng/ul	99
55) 4-Nitrophenol	14.963	109	19593	6.055	ng/ul	95
56) Dibenzofuran	15.151	168	223497	9.999	ng/ul	99
57) 2,4-Dinitrotoluene	15.110	165	28631	5.193	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	15.375	232	30068	7.564	ng/ul#	89
59) Diethylphthalate	15.575	149	179829	9.171	ng/ul	99
61) Fluorene	15.804	166	182034	10.466	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.798	204	84422	10.539	ng/ul	98
63) 4-Nitroaniline	15.816	138	21302	5.791	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.869	198	11250	3.755	ng/ul#	85
67) N-Nitrosodiphenylamine	16.010	169	152184	10.406	ng/ul	99
68) 4-Bromophenyl-phenylether	16.692	248	47331	10.654	ng/ul	92
69) Hexachlorobenzene	16.804	284	55727	10.912	ng/ul	90
70) Atrazine	16.963	200	50420	9.881	ng/ul	95
71) Pentachlorophenol	17.151	266	22372	7.034	ng/ul	92
72) Phenanthrene	17.551	178	276634	10.275	ng/ul	97
74) Anthracene	17.639	178	280548	10.363	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.557	216	74856	10.958	ng/uL	89
76) Pentachlorobenzene	15.069	250	69941	11.584	ng/uL	100
77) Carbazole	17.910	167	256803	10.427	ng/ul	98
78) Di-n-butylphthalate	18.481	149	294930	9.658	ng/ul	99
80) Fluoranthene	19.563	202	306529	9.832	ng/ul#	95
82) Pyrene	19.928	202	325071	10.163	ng/ul#	92
83) Butylbenzylphthalate	20.833	149	111805	7.767	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.616	252	93361	10.266	ng/ul#	94
85) Benzo(a)anthracene	21.686	228	287562	9.564	ng/ul	93
86) Bis(2-ethylhexyl)phtha...	21.616	149	189617	9.336	ng/ul	99
87) Chrysene	21.739	228	292702	9.950	ng/ul	94
89) Di-n-octyl phthalate	22.598	149	319376	8.086	ng/ul	100
90) Benzo(b)fluoranthene	23.463	252	310811	10.205	ng/ul#	96
91) Benzo(k)fluoranthene	23.516	252	278183	9.595	ng/ul	95
93) Benzo(a)pyrene	24.133	252	296344	10.052	ng/ul#	95
94) Indeno(1,2,3-cd)pyrene	26.927	276	344550	11.359	ng/ul	98
95) Dibenzo(a,h)anthracene	26.968	278	294106	11.352	ng/ul	98
96) Benzo(g,h,i)perylene	27.768	276	302265	11.801	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

BNA N

ClientSampleId :
SSTD010225





[illegible]



#2
1,4-Dioxane
Concen: 4.945 ng/uL
RT: 3.428 min Scan# 24
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion: 88 Resp: 13646
Ion Ratio Lower Upper
88 100
43 36.8 22.4 33.6#
58 69.1 61.0 91.4



#5
Pyridine
Concen: 10.622 ng/uL
RT: 3.840 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion: 79 Resp: 79563
Ion Ratio Lower Upper
79 100
52 71.1 65.0 97.4
51 31.9 31.6 47.4




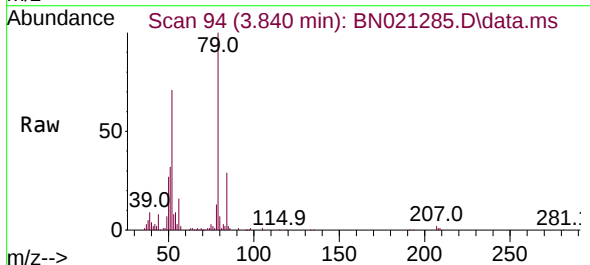




#6
Benzaldehyde
Concen: 9.961 ng/ul
RT: 7.222 min Scan# 669
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion: 77 Resp: 43971
Ion Ratio Lower Upper
77 100
105 96.3 74.7 112.1
106 93.9 70.2 105.4

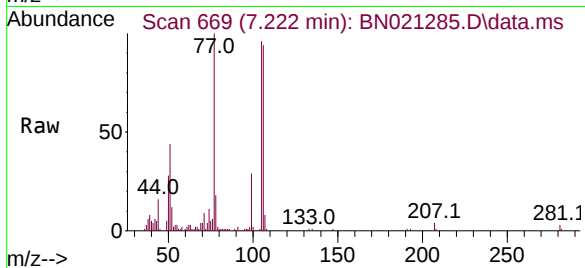

#8
Phenol
Concen: 9.719 ng/ul
RT: 7.269 min Scan# 677
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion: 94 Resp: 96959
Ion Ratio Lower Upper
94 100
65 27.2 23.6 35.4
66 34.0 31.2 46.8


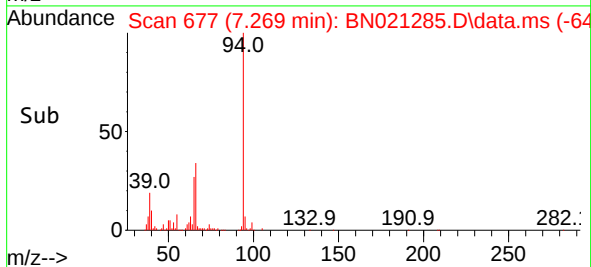

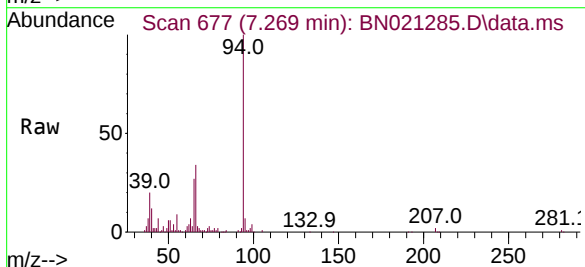




#10
Bis(2-Chloroethyl)ether
Concen: 10.144 ng/ul
RT: 7.516 min Scan# 719
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion: 93 Resp: 79208
Ion Ratio Lower Upper
93 100
63 70.3 63.4 95.0
95 32.8 26.2 39.2

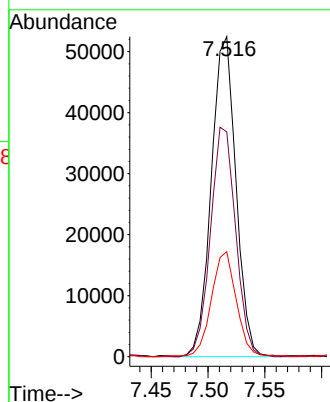

#12
2-Chlorophenol
Concen: 9.835 ng/ul
RT: 7.652 min Scan# 742
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:128 Resp: 78256
Ion Ratio Lower Upper
128 100
64 45.4 38.6 57.8
130 33.3 25.0 37.4

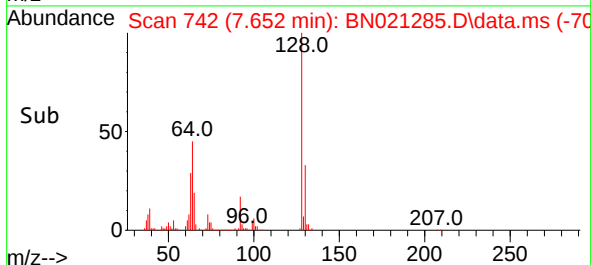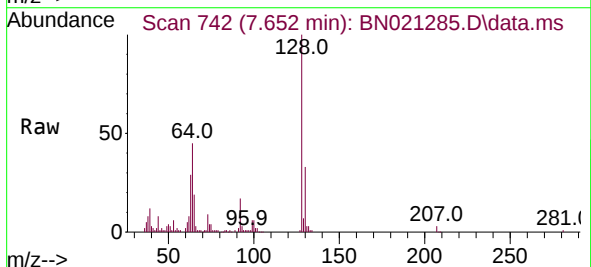



#13

2-Methylphenol

Concen: 9.373 ng/ul

RT: 8.546 min Scan# 894

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Instrument :

BNA_N

ClientSampleId :





SSTD010225

Tgt Ion:108 Resp: 71885

Ion Ratio Lower Upper

108 100

107 85.8 71.5 107.3

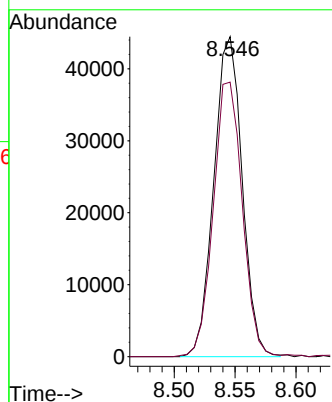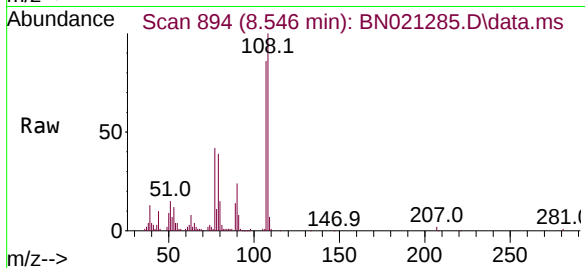

#14

2,2'-oxybis(1-Chloropropane)

Concen: 5.191 ng/ul

RT: 8.634 min Scan# 909

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10




Tgt Ion: 45 Resp: 63558


Ion Ratio Lower Upper

45 100

77 16.3 10.9 16.3

79 11.9 8.6 13.0


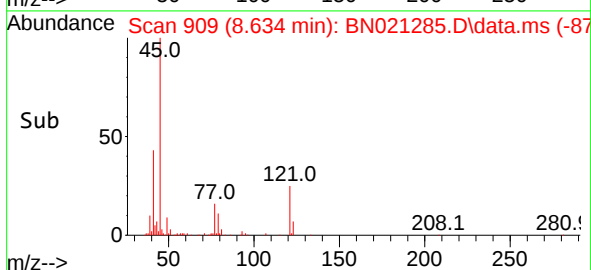

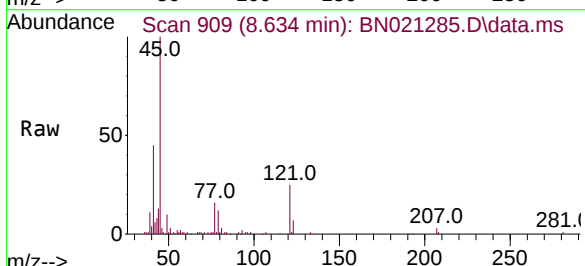




#16
 Acetophenone
 Concen: 9.222 ng/ul
 RT: 8.934 min Scan# 910
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10




Instrument :
 BNA_N
 ClientSampleId :
 SST010225


Tgt Ion:105 Resp: 113671
 Ion Ratio Lower Upper
 105 100
 77 73.0 63.5 95.3
 51 24.5 23.5 35.3

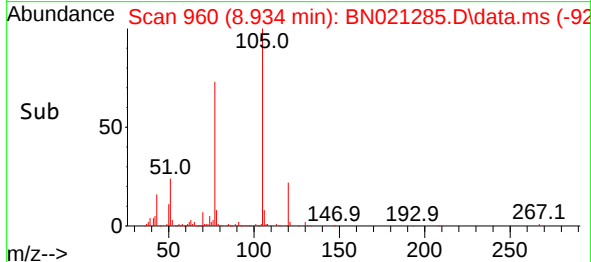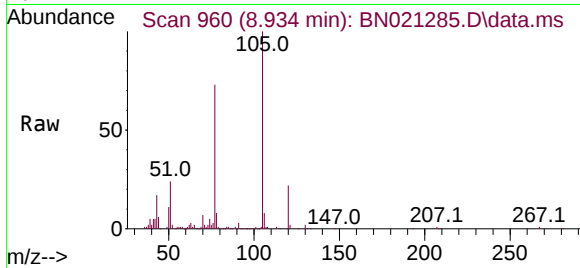

#17
 N-Nitroso-di-n-propylamine
 Concen: 8.747 ng/ul
 RT: 8.916 min Scan# 957
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10

Tgt Ion: 70 Resp: 55080
 Ion Ratio Lower Upper
 70 100
 42 53.7 47.8 71.6
 101 10.1 7.8 11.6
 130 21.8 15.8 23.8


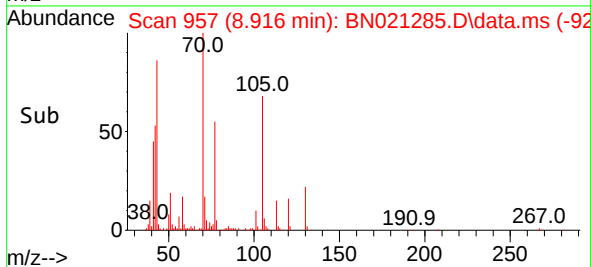

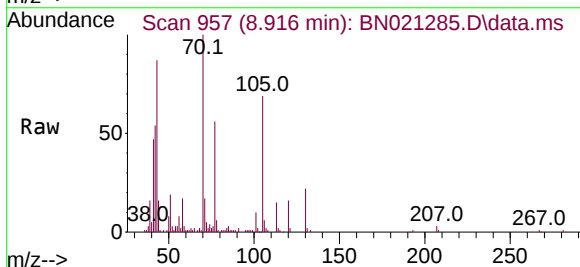




#18
4-Methylphenol
Concen: 8.938 ng/ul
RT: 8.875 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:108 Resp: 75660
Ion Ratio Lower Upper
108 100
107 108.2 88.0 132.0

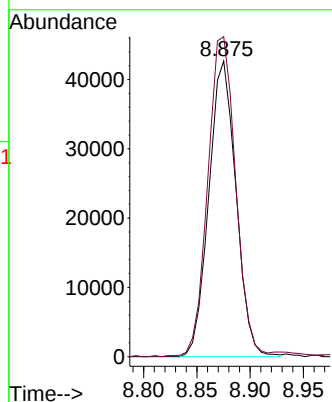

#19
Hexachloroethane
Concen: 10.403 ng/ul
RT: 9.199 min Scan# 1005
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:117 Resp: 33306
Ion Ratio Lower Upper
117 100
201 92.8 83.2 124.8
199 58.4 50.2 75.4


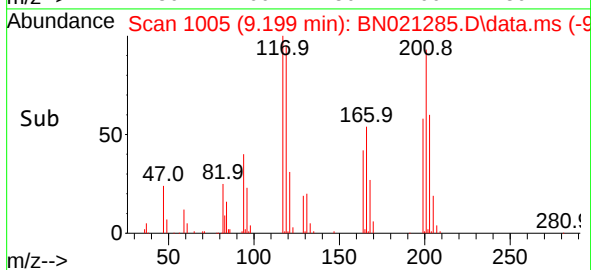




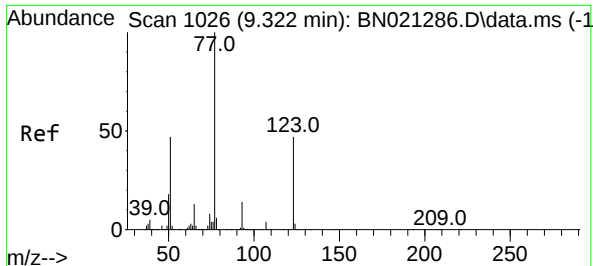

#22
Nitrobenzene
Concen: 8.699 ng/ul
RT: 9.316 min Scan# 1025
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion: 77 Resp: 70255
Ion Ratio Lower Upper
77 100
123 43.1 34.5 51.7
65 12.1 11.1 16.7

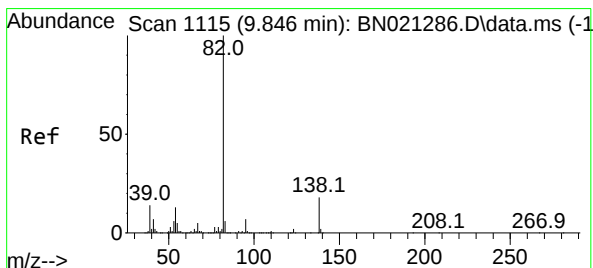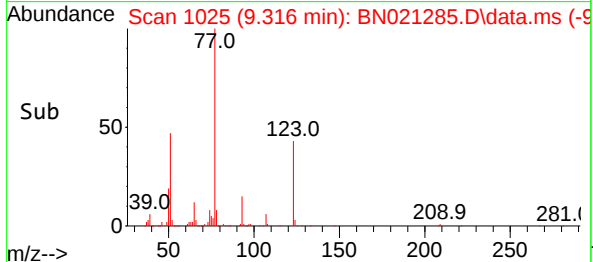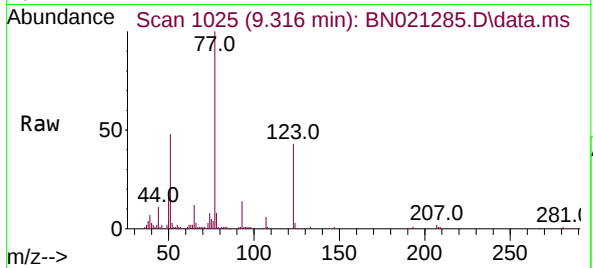

#23
Isophorone
Concen: 9.657 ng/ul
RT: 9.846 min Scan# 1115
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion: 82 Resp: 153984
Ion Ratio Lower Upper
82 100
95 6.6 5.8 8.8
138 17.6 13.8 20.8


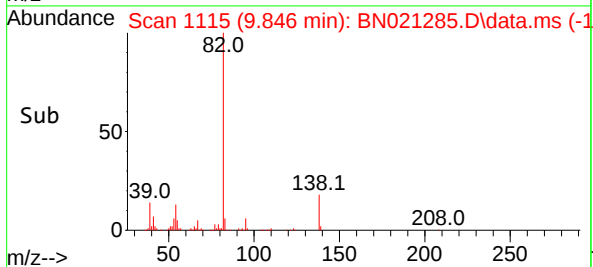

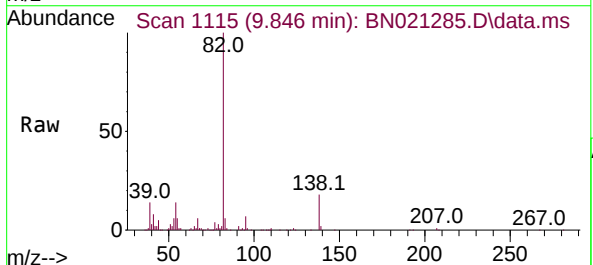


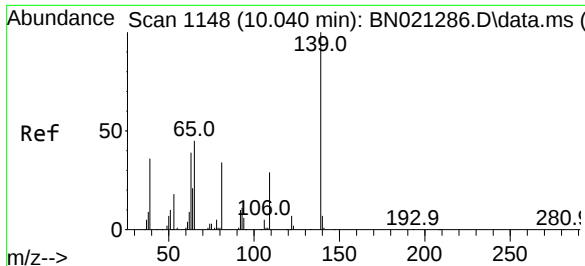

#25
2-Nitrophenol
Concen: 6.252 ng/ul
RT: 10.040 min Scan# 1148
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:139 Resp: 25536
Ion Ratio Lower Upper
139 100
65 49.3 43.7 65.5
109 29.8 25.8 38.6

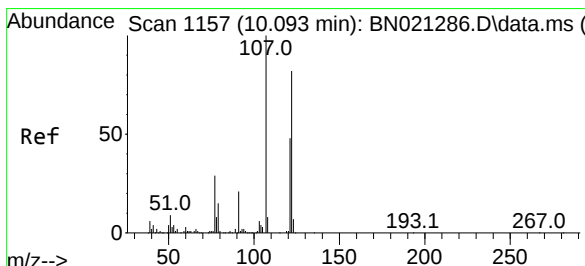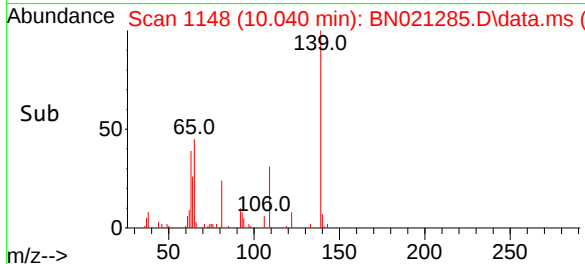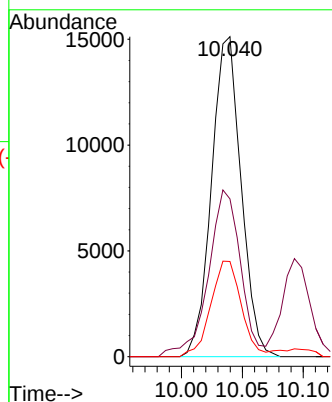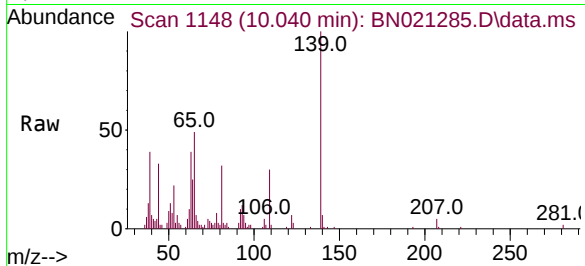

#26
2,4-Dimethylphenol
Concen: 9.508 ng/ul
RT: 10.093 min Scan# 1157
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:107 Resp: 80457
Ion Ratio Lower Upper
107 100
121 51.7 38.3 57.5
122 90.7 66.3 99.5


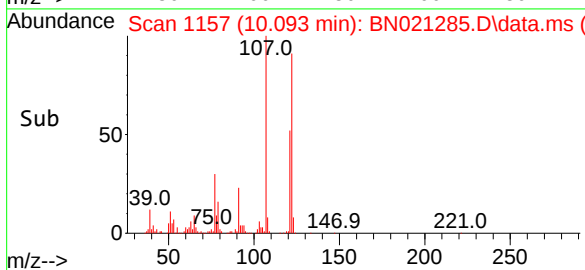

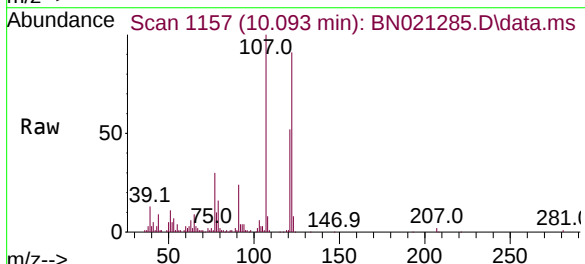




#27
 Bis(2-Chloroethoxy)methane
 Concen: 10.065 ng/ul
 RT: 10.340 min Scan# 1199
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010225


Tgt Ion: 93 Resp: 98217
 Ion Ratio Lower Upper
 93 100
 95 30.9 25.4 38.0
 123 11.0 8.3 12.5

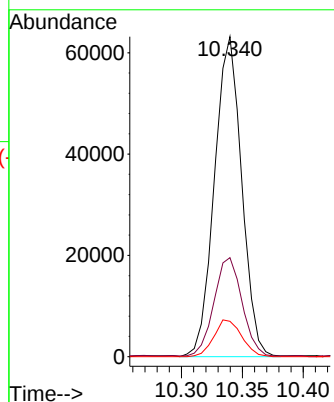

#29
 2,4-Dichlorophenol
 Concen: 9.409 ng/ul
 RT: 10.575 min Scan# 1239
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10

Tgt Ion: 162 Resp: 62803
 Ion Ratio Lower Upper
 162 100
 164 66.8 52.9 79.3
 98 38.2 29.8 44.8



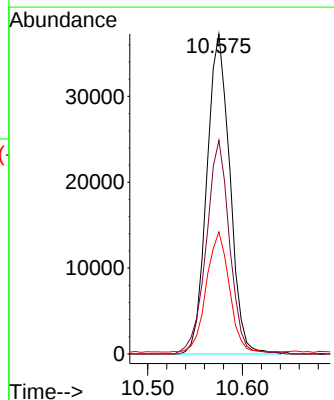





#30
Naphthalene
Concen: 10.272 ng/ul
RT: 10.987 min Scan# 1309
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:128 Resp: 243720
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 12.0 10.6 16.0

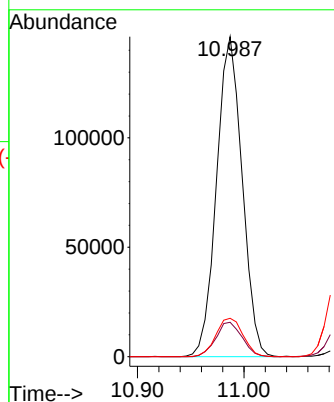

#32
4-Chloroaniline
Concen: 9.563 ng/ul
RT: 11.093 min Scan# 1327
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:127 Resp: 99952
Ion Ratio Lower Upper
127 100
129 31.2 26.1 39.1


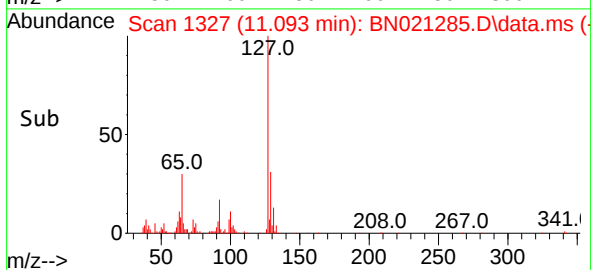
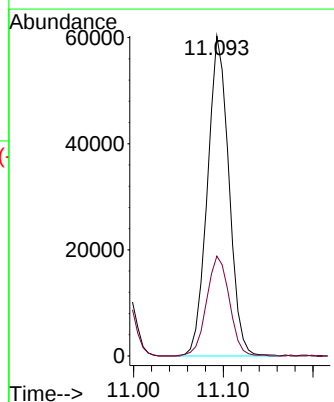





#33
Hexachlorobutadiene
Concen: 10.241 ng/ul
RT: 11.269 min Scan# 111
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:225 Resp: 39248
Ion Ratio Lower Upper
225 100
223 64.5 51.8 77.6
227 64.4 50.6 76.0

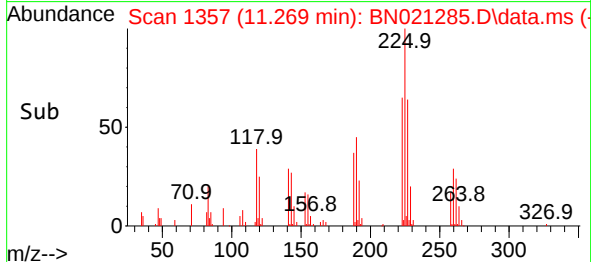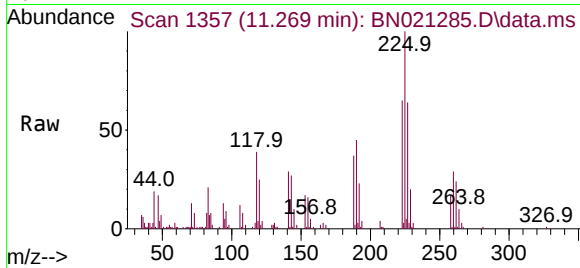

#34
Caprolactam
Concen: 6.687 ng/ul
RT: 11.840 min Scan# 1454
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:113 Resp: 17431
Ion Ratio Lower Upper
113 100
55 160.7 145.5 218.3
56 123.6 106.5 159.7


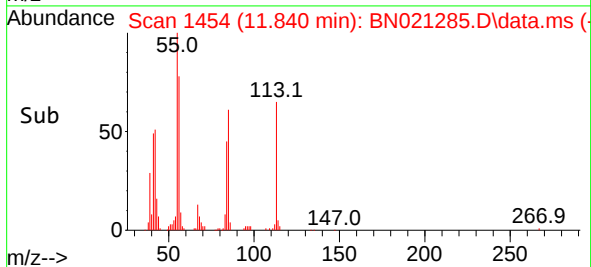

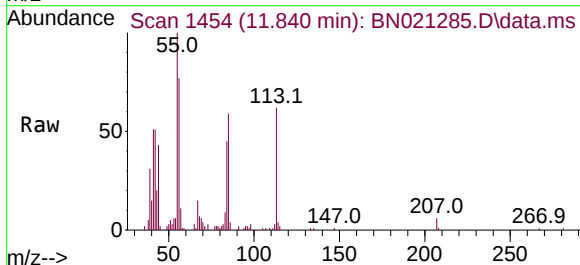




#35
4-Chloro-3-methylphenol
Concen: 8.151 ng/ul
RT: 12.210 min Scan# 1517
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:107 Resp: 64245
Ion Ratio Lower Upper
107 100
144 27.2 20.6 31.0
142 83.8 62.2 93.4

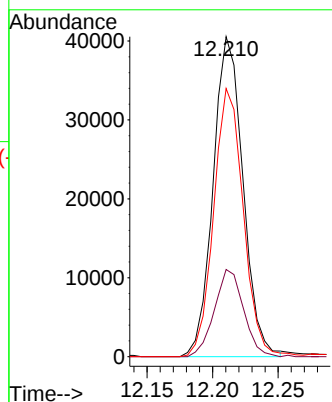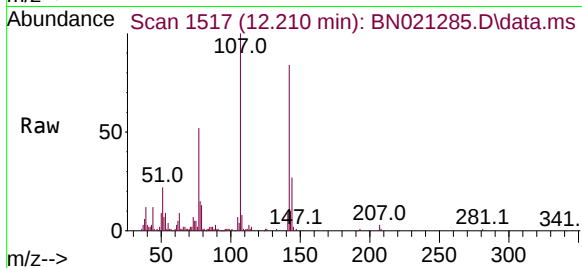

#36
2-Methylnaphthalene
Concen: 9.806 ng/ul
RT: 12.593 min Scan# 1582
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:142 Resp: 157297
Ion Ratio Lower Upper
142 100
141 82.8 70.6 105.8


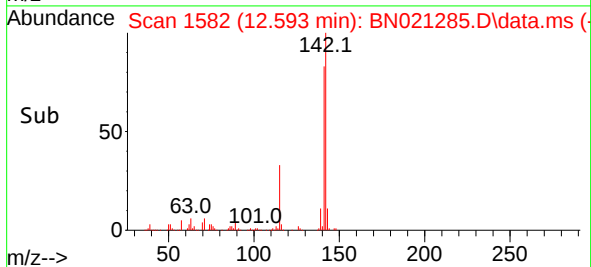
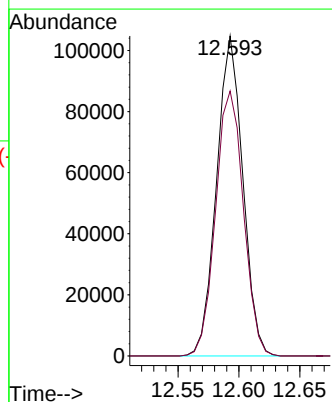
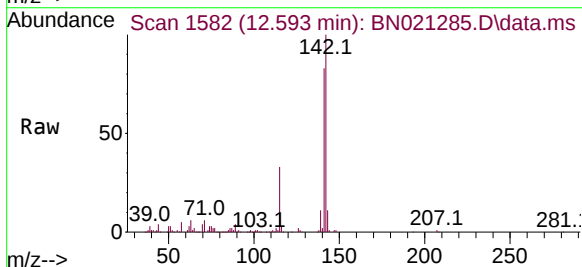




#37
1-Methylnaphthalene
Concen: 9.699 ng/ul
RT: 12.810 min Scan# 1619
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:142 Resp: 158763
Ion Ratio Lower Upper
142 100
141 92.5 70.9 106.3
116 4.0 3.1 4.7

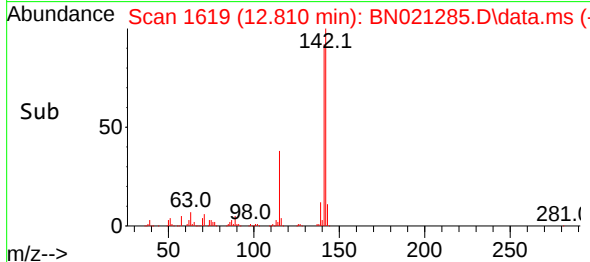

#39
1,2,4,5-Tetrachlorobenzene
Concen: 10.977 ng/ul
RT: 12.951 min Scan# 1643
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:216 Resp: 72788
Ion Ratio Lower Upper
216 100
214 73.5 63.4 95.0
179 19.6 17.8 26.8
108 18.4 15.1 22.7


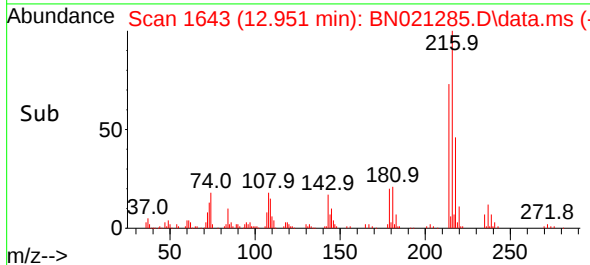






#40
Hexachlorocyclopentadiene
Concen: 10.069 ng/ul
RT: 12.934 min Scan# 1640
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:237 Resp: 40615
Ion Ratio Lower Upper
237 100
235 67.9 48.8 73.2
272 14.3 9.3 13.9#

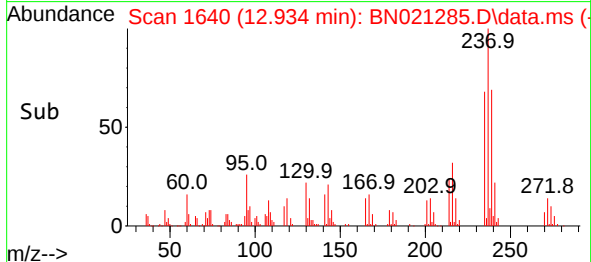

#41
2,4,6-Trichlorophenol
Concen: 8.968 ng/ul
RT: 13.193 min Scan# 1684
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:196 Resp: 41004
Ion Ratio Lower Upper
196 100
198 93.1 79.8 119.8
200 30.0 25.0 37.6


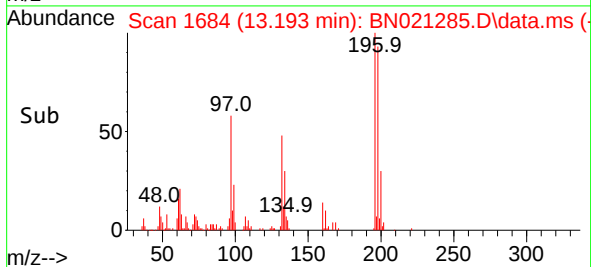

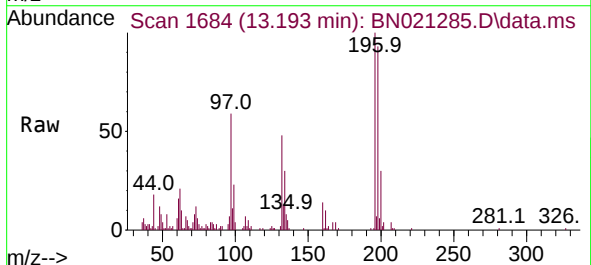




#42
2,4,5-Trichlorophenol
Concen: 8.476 ng/ul
RT: 13.257 min Scan# 1695
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:196 Resp: 42921
Ion Ratio Lower Upper
196 100
198 97.7 77.6 116.4
200 29.4 24.4 36.6



#43
1,1'-Biphenyl
Concen: 10.477 ng/ul
RT: 13.593 min Scan# 1752
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:154 Resp: 201708
Ion Ratio Lower Upper
154 100
153 40.4 31.5 47.3
76 13.5 10.5 15.7









#44
2-Chloronaphthalene
Concen: 10.442 ng/ul
RT: 13.640 min Scan# 1760
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:162 Resp: 152507
Ion Ratio Lower Upper
162 100
164 31.3 25.8 38.6
127 40.3 31.4 47.2

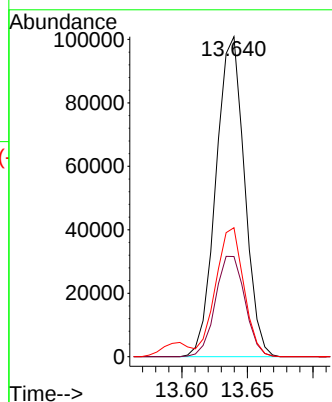

#45
2-Nitroaniline
Concen: 5.587 ng/ul
RT: 13.834 min Scan# 1793
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion: 65 Resp: 25388
Ion Ratio Lower Upper
65 100
92 70.4 54.1 81.1
138 105.1 77.0 115.4









#47
Dimethylphthalate
Concen: 9.488 ng/ul
RT: 14.210 min Scan# 1857
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:163 Resp: 180693
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.0
164 9.8 7.7 11.5

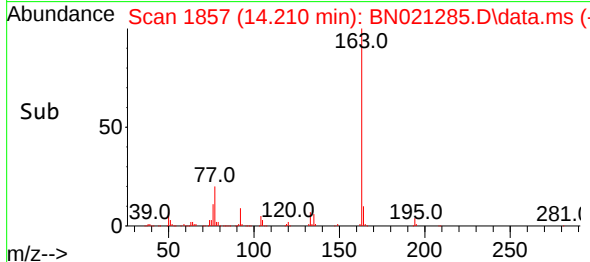

#48
2,6-Dinitrotoluene
Concen: 5.677 ng/ul
RT: 14.328 min Scan# 1877
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:165 Resp: 21137
Ion Ratio Lower Upper
165 100
89 66.7 50.6 75.8
121 27.8 17.9 26.9#





#50

Acenaphthylene

Concen: 10.277 ng/ul

RT: 14.481 min Scan# 1903

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Instrument :

BNA_N

ClientSampleId :

SSTD010225





Tgt Ion:152 Resp: 249640

Ion Ratio Lower Upper

152 100

151 19.5 16.0 24.0

153 13.5 10.7 16.1

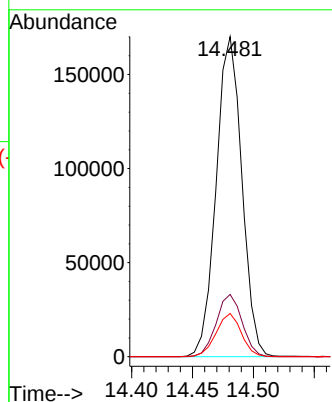

#51

3-Nitroaniline

Concen: 5.488 ng/ul

RT: 14.657 min Scan# 1933

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10




Tgt Ion:138 Resp: 21604


Ion Ratio Lower Upper

138 100

108 26.3 8.6 12.8#

92 113.6 92.9 139.3









#52
Acenaphthene
Concen: 10.214 ng/ul
RT: 14.822 min Scan# 1961
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:153 Resp: 162063
Ion Ratio Lower Upper
153 100
152 46.9 38.4 57.6
154 88.4 69.7 104.5

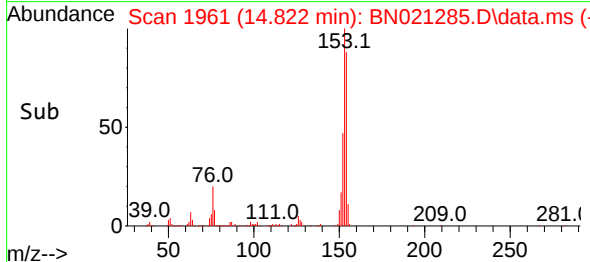

#53
2,4-Dinitrophenol
Concen: 2.928 ng/ul
RT: 14.857 min Scan# 1967
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:184 Resp: 6980
Ion Ratio Lower Upper
184 100
63 69.2 55.9 83.9
154 64.7 53.1 79.7




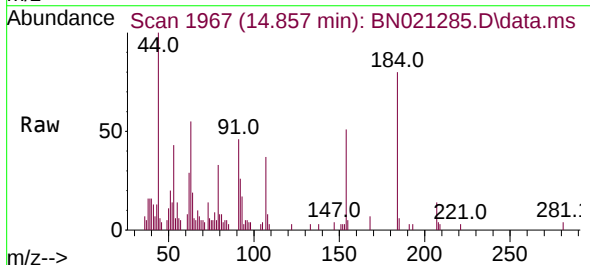




#55
4-Nitrophenol
Concen: 6.055 ng/ul
RT: 14.963 min Scan# 1984
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:109 Resp: 19593
Ion Ratio Lower Upper
109 100
139 129.7 100.1 150.1
65 124.2 104.6 157.0



#56
Dibenzofuran
Concen: 9.999 ng/ul
RT: 15.151 min Scan# 2017
Delta R.T. -0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:168 Resp: 223497
Ion Ratio Lower Upper
168 100
139 38.1 31.1 46.7


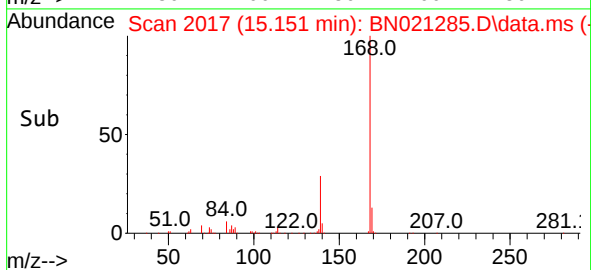






#57
2,4-Dinitrotoluene
Concen: 5.193 ng/ul
RT: 15.110 min Scan# 2010
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:165 Resp: 28631
Ion Ratio Lower Upper
165 100
63 48.1 36.3 54.5
182 2.9 2.3 3.5

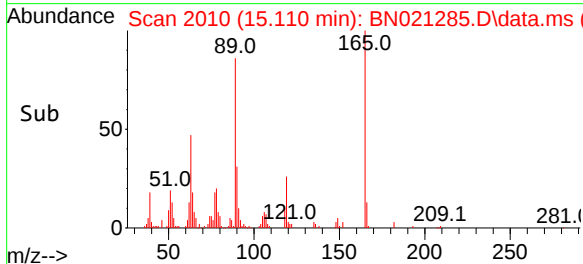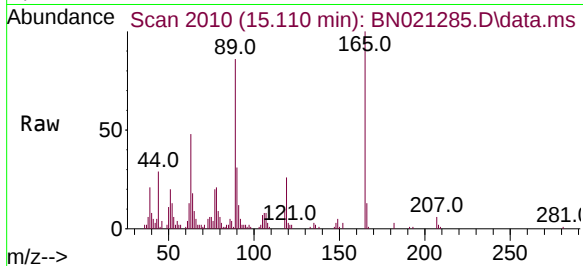

#58
2,3,4,6-Tetrachlorophenol
Concen: 7.564 ng/ul
RT: 15.375 min Scan# 2055
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:232 Resp: 30068
Ion Ratio Lower Upper
232 100
131 56.3 38.5 57.7
130 3.7 2.2 3.2#
166 37.6 25.8 38.8


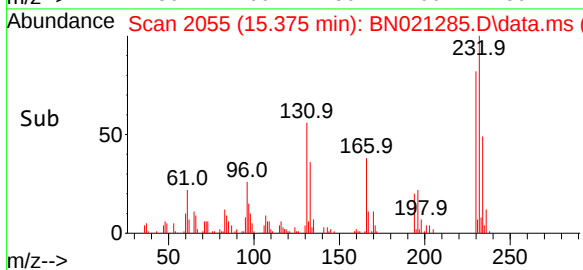

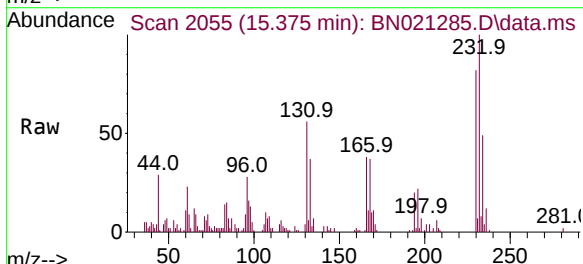




#59
Diethylphthalate
Concen: 9.171 ng/ul
RT: 15.575 min Scan# 2089
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:149 Resp: 179829
Ion Ratio Lower Upper
149 100
177 22.5 17.8 26.8
150 12.8 10.5 15.7

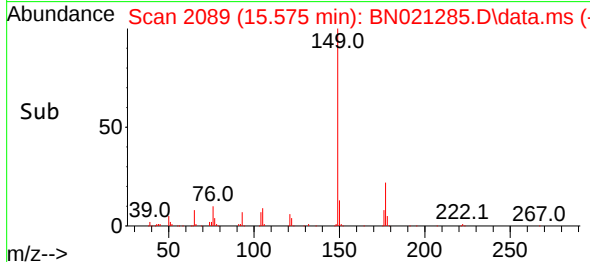

#61
Fluorene
Concen: 10.466 ng/ul
RT: 15.804 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:166 Resp: 182034
Ion Ratio Lower Upper
166 100
165 97.6 77.7 116.5
167 12.8 11.1 16.7




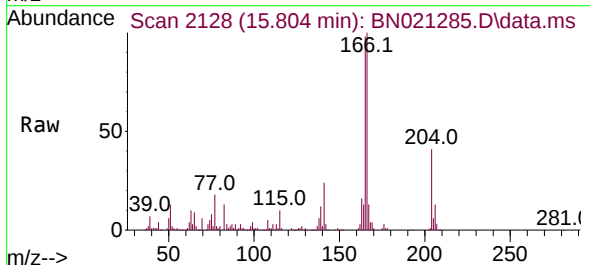




#62
4-Chlorophenyl-phenylether
Concen: 10.539 ng/ul
RT: 15.798 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:204 Resp: 84422
Ion Ratio Lower Upper
204 100
206 35.5 26.7 40.1
141 61.5 50.2 75.2

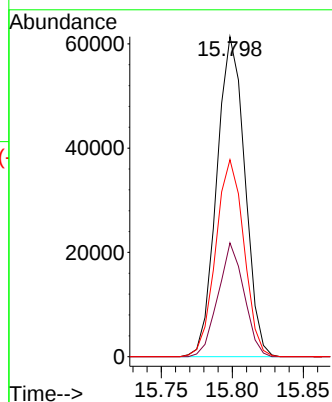

#63
4-Nitroaniline
Concen: 5.791 ng/ul
RT: 15.816 min Scan# 2130
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:138 Resp: 21302
Ion Ratio Lower Upper
138 100
92 50.5 41.0 61.6
108 84.6 65.3 97.9









#66
 4,6-Dinitro-2-methylphenol
 Concen: 3.755 ng/ul
 RT: 15.869 min Scan# 2139
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10




Instrument :
 BNA_N
 ClientSampleId :
 SST010225


Tgt Ion:198 Resp: 11250
 Ion Ratio Lower Upper
 198 100
 182 5.7 3.0 4.4#
 77 33.4 20.1 30.1#



#67
 N-Nitrosodiphenylamine
 Concen: 10.406 ng/ul
 RT: 16.010 min Scan# 2163
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10

Tgt Ion:169 Resp: 152184
 Ion Ratio Lower Upper
 169 100
 168 66.1 52.4 78.6
 167 34.6 27.5 41.3


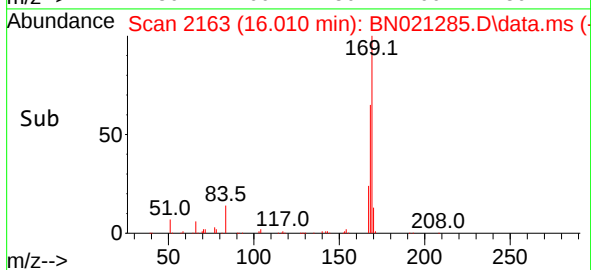






#68
4-Bromophenyl-phenylether
Concen: 10.654 ng/ul
RT: 16.692 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:248 Resp: 47331
Ion Ratio Lower Upper
248 100
250 95.7 77.8 116.8
141 91.1 62.6 93.8



#69
Hexachlorobenzene
Concen: 10.912 ng/ul
RT: 16.804 min Scan# 2298
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:284 Resp: 55727
Ion Ratio Lower Upper
284 100
142 41.0 27.8 41.8
249 27.3 25.7 38.5









#70
Atrazine
Concen: 9.881 ng/ul
RT: 16.963 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:200 Resp: 50420
Ion Ratio Lower Upper
200 100
173 28.3 20.5 30.7
215 45.7 38.9 58.3

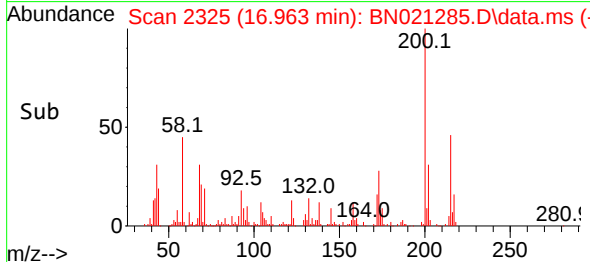

#71
Pentachlorophenol
Concen: 7.034 ng/ul
RT: 17.151 min Scan# 2357
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:266 Resp: 22372
Ion Ratio Lower Upper
266 100
264 58.5 50.2 75.2
268 53.3 49.3 73.9




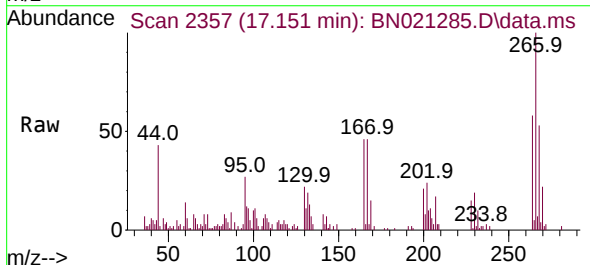




#72
Phenanthrene
Concen: 10.275 ng/ul
RT: 17.551 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:178 Resp: 276634
Ion Ratio Lower Upper
178 100
179 14.4 12.2 18.4
176 20.4 15.2 22.8

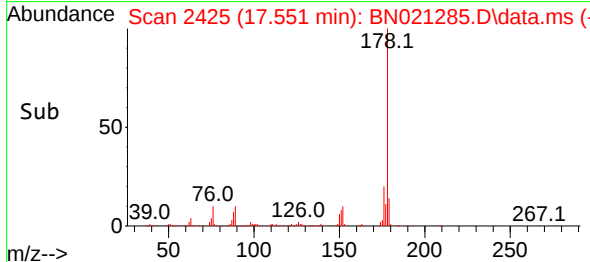

#74
Anthracene
Concen: 10.363 ng/ul
RT: 17.639 min Scan# 2440
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:178 Resp: 280548
Ion Ratio Lower Upper
178 100
179 14.3 13.0 19.4
176 18.6 15.5 23.3

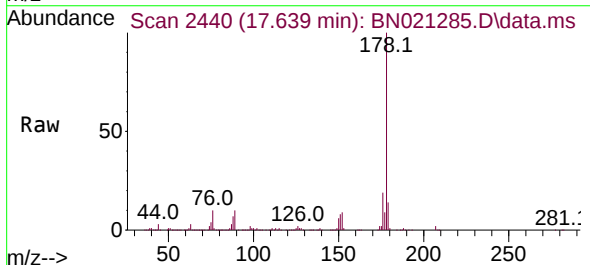



#75

1,2,3,4-Tetrachlorobenzene

Concen: 10.958 ng/uL

RT: 13.557 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Instrument :

BNA_N

ClientSampleId :

SSTD010225





Tgt Ion:216 Resp: 74856

Ion Ratio Lower Upper

216 100

214 65.3 63.2 94.8

218 44.4 37.9 56.9

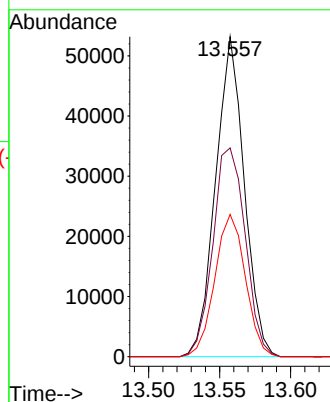

#76

Pentachlorobenzene

Concen: 11.584 ng/uL

RT: 15.069 min Scan# 2003

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10




Tgt Ion:250 Resp: 69941


Ion Ratio Lower Upper

250 100

248 66.0 53.0 79.4

252 66.6 53.4 80.2









#77
 Carbazole
 Concen: 10.427 ng/ul
 RT: 17.910 min Scan# 2486
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010225

Tgt Ion:167 Resp: 256803




Ion	Ratio	Lower	Upper
167	100		
166	21.2	16.1	24.1
139	13.4	10.2	15.2

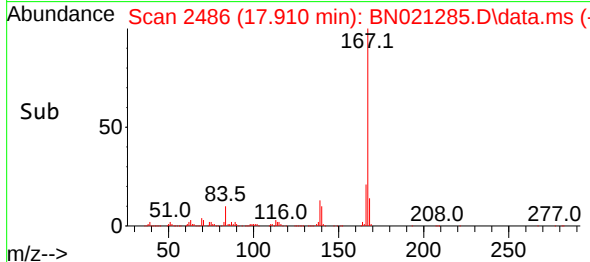


#78
 Di-n-butylphthalate
 Concen: 9.658 ng/ul
 RT: 18.481 min Scan# 2583
 Delta R.T. -0.000 min
 Lab File: BN021285.D
 Acq: 18 Aug 2022 18:10

Tgt Ion:149 Resp: 294930

Ion	Ratio	Lower	Upper
149	100		
150	9.2	7.1	10.7
104	5.3	4.1	6.1




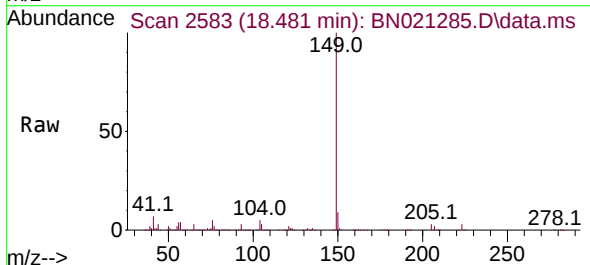




#80
Fluoranthene
Concen: 9.832 ng/ul
RT: 19.563 min Scan# 2767
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:202 Resp: 306529
Ion Ratio Lower Upper
202 100
101 13.1 8.9 13.3
100 10.2 6.7 10.1#



#82
Pyrene
Concen: 10.163 ng/ul
RT: 19.928 min Scan# 2829
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:202 Resp: 325071
Ion Ratio Lower Upper
202 100
101 15.8 9.7 14.5#
100 12.2 8.0 12.0#









#83
Butylbenzylphthalate
Concen: 7.767 ng/ul
RT: 20.833 min Scan# 2983
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:149 Resp: 111805
Ion Ratio Lower Upper
149 100
91 71.9 58.8 88.2
206 19.8 18.1 27.1

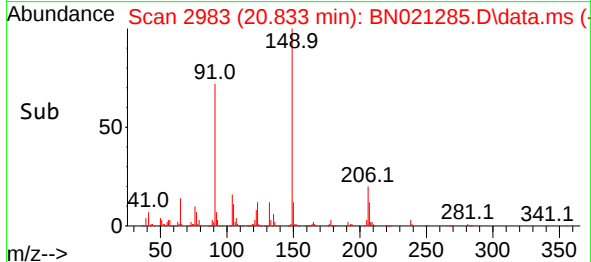

#84
3,3'-Dichlorobenzidine
Concen: 10.266 ng/ul
RT: 21.616 min Scan# 3116
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:252 Resp: 93361
Ion Ratio Lower Upper
252 100
254 67.3 50.8 76.2
126 14.1 8.2 12.4#

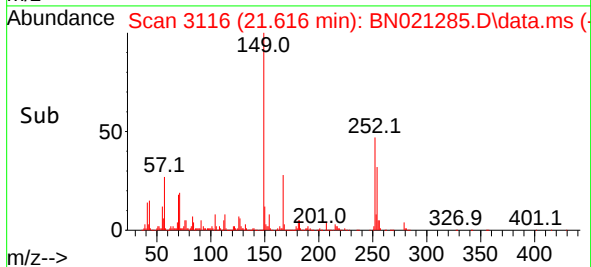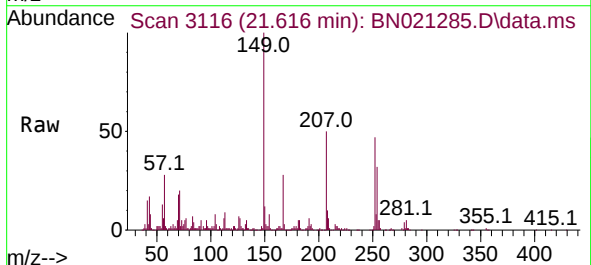



#85

Benzo(a)anthracene

Concen: 9.564 ng/ul

RT: 21.686 min Scan# 3127

Delta R.T. 0.006 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Instrument :

BNA_N

ClientSampleId :

SSTD010225





Tgt Ion:228 Resp: 287562

Ion Ratio Lower Upper

228 100

229 17.4 16.3 24.5

226 25.1 23.2 34.8

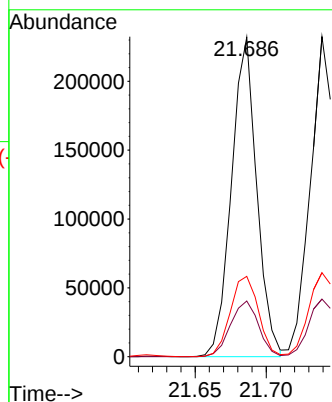

#86

Bis(2-ethylhexyl)phthalate

Concen: 9.336 ng/ul

RT: 21.616 min Scan# 3116

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10




Tgt Ion:149 Resp: 189617


Ion Ratio Lower Upper

149 100

167 27.6 22.5 33.7

279 3.7 3.5 5.3









#87
Chrysene
Concen: 9.950 ng/ul
RT: 21.739 min Scan# 3137
Delta R.T. -0.000 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:228 Resp: 292702
Ion Ratio Lower Upper
228 100
226 26.3 24.2 36.2
229 18.0 16.2 24.2

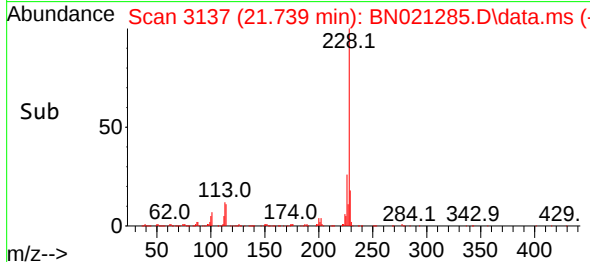

#89
Di-n-octyl phthalate
Concen: 8.086 ng/ul
RT: 22.598 min Scan# 3283
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:149 Resp: 319376




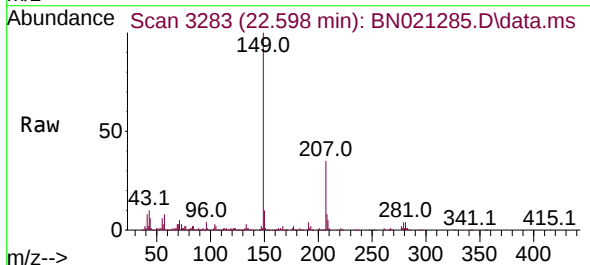




#90
Benzo(b)fluoranthene
Concen: 10.205 ng/ul
RT: 23.463 min Scan# 3429
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10




Instrument :
BNA_N
ClientSampleId :
SSTD010225


Tgt Ion:252 Resp: 310811
Ion Ratio Lower Upper
252 100
253 21.8 16.5 24.7
125 12.7 7.8 11.8#

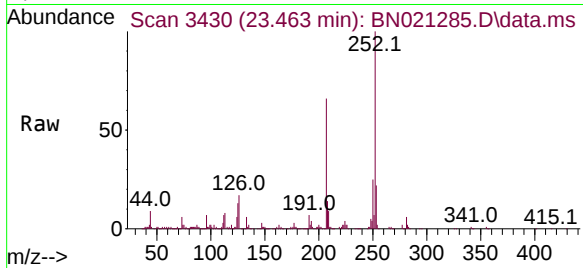

#91
Benzo(k)fluoranthene
Concen: 9.595 ng/ul
RT: 23.516 min Scan# 3439
Delta R.T. 0.006 min
Lab File: BN021285.D
Acq: 18 Aug 2022 18:10

Tgt Ion:252 Resp: 278183
Ion Ratio Lower Upper
252 100
253 20.0 18.2 27.4
125 11.9 8.2 12.4

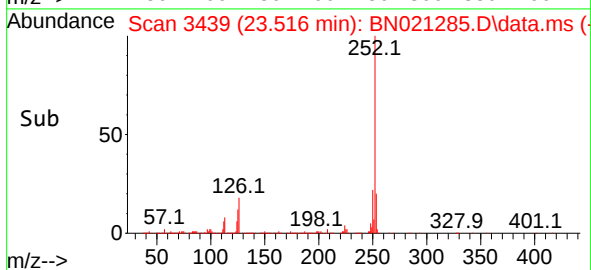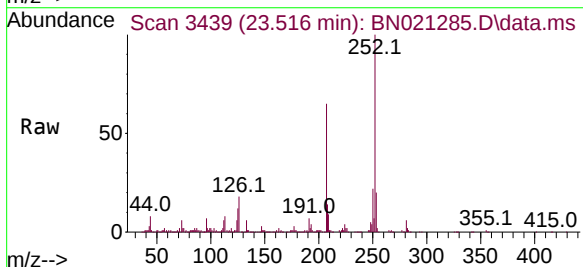



#93

Benzo(a)pyrene

Concen: 10.052 ng/ul

RT: 24.133 min Scan# 3544

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Instrument :

BNA_N

ClientSampleId :

SSTD010225





Tgt Ion:252 Resp: 296344

Ion Ratio Lower Upper

252 100

253 21.7 18.7 28.1

125 14.8 9.2 13.8#



#94

Indeno(1,2,3-cd)pyrene

Concen: 11.359 ng/ul

RT: 26.927 min Scan# 4019

Delta R.T. -0.000 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10




Tgt Ion:276 Resp: 344550


Ion Ratio Lower Upper

276 100

138 24.1 19.5 29.3

277 25.4 21.4 32.0

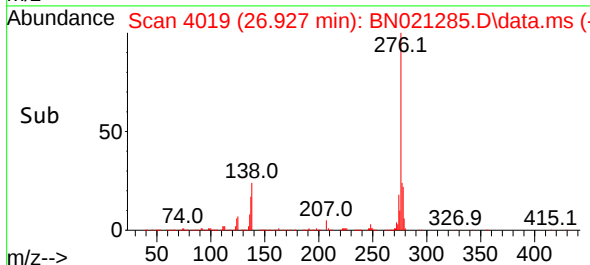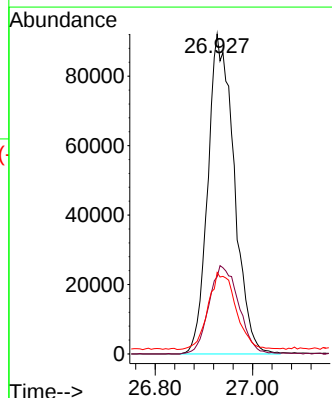



#95

Dibenzo(a,h)anthracene

Concen: 11.352 ng/ul

RT: 26.968 min Scan# 4025

Delta R.T. 0.006 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Instrument :

BNA_N

ClientSampleId :

SSTD010225





Tgt Ion:278 Resp: 294106

Ion Ratio Lower Upper

278 100

139 18.6 13.8 20.8

279 23.4 18.3 27.5

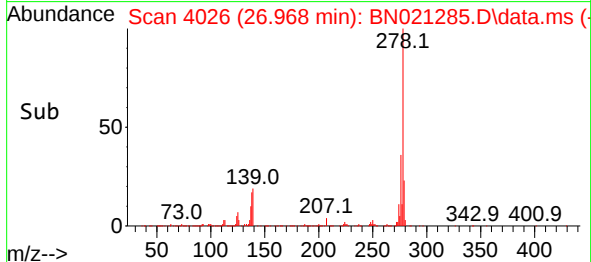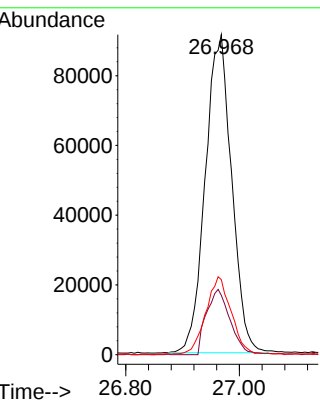

#96

Benzo(g,h,i)perylene

Concen: 11.801 ng/ul

RT: 27.768 min Scan# 4162

Delta R.T. 0.012 min

Lab File: BN021285.D

Acq: 18 Aug 2022 18:10

Tgt Ion:276 Resp: 302265

Ion Ratio Lower Upper

276 100

138 23.6 17.0 25.6

277 25.5 17.8 26.6

