

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081822\
 Data File : BN021290.D
 Acq On : 18 Aug 2022 21:51
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SICV230

Quant Time: Aug 18 22:19:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 18 21:26:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	131747	20.000	ng/u1	0.00
20) Naphthalene-d8	10.934	136	538693	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.751	164	308426	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.504	188	593958	20.000	ng/u1	0.00
79) Chrysene-d12	21.698	240	556263	20.000	ng/u1	0.00
88) Perylene-d12	24.233	264	576416	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	28413	7.959	ng/uL	0.00
4) Pyridine-d5	3.817	84	182618	19.387	ng/u1	0.00
7) Phenol-d5	7.240	99	208398	18.688	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	129507	19.344	ng/u1	0.00
11) 2-Chlorophenol-d4	7.616	132	167242	19.630	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	154411	18.780	ng/u1	0.00
21) Nitrobenzene-d5	9.269	128	71788	20.651	ng/u1	0.00
24) 2-Nitrophenol-d4	10.004	143	62972	21.065	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	142902	19.365	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	218029	19.167	ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	389315	18.975	ng/u1	0.00
49) Acenaphthylene-d8	14.451	160	488503	19.311	ng/u1	0.00
54) 4-Nitrophenol-d4	14.939	143	67127	18.924	ng/u1	0.00
60) Fluorene-d10	15.745	176	345720	19.131	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	36118	17.907	ng/u1	0.00
73) Anthracene-d10	17.604	188	502201	19.177	ng/u1	0.00
81) Pyrene-d10	19.892	212	549522	19.414	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.068	264	549458	19.443	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	29367	7.671	ng/uL	92
5) Pyridine	3.840	79	183387	19.429	ng/u1#	84
6) Benzaldehyde	7.222	77	103815	21.600	ng/u1	92
8) Phenol	7.269	94	218029	19.179	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.510	93	176963	19.227	ng/u1	93
12) 2-Chlorophenol	7.652	128	176922	19.577	ng/u1	96
13) 2-Methylphenol	8.540	108	161580	19.005	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.634	45	220253	19.459	ng/u1	96
16) Acetophenone	8.928	105	249516	19.441	ng/u1	94
17) N-Nitroso-di-n-propyla...	8.910	70	121972	19.239	ng/u1	95
18) 4-Methylphenol	8.869	108	170099	19.003	ng/u1	98
19) Hexachloroethane	9.193	117	72941	19.293	ng/u1	95
22) Nitrobenzene	9.316	77	175723	20.341	ng/u1	93
23) Isophorone	9.846	82	338802	18.730	ng/u1	98
25) 2-Nitrophenol	10.034	139	77085	21.744	ng/u1	93
26) 2,4-Dimethylphenol	10.093	107	180537	19.279	ng/u1	93
27) Bis(2-Chloroethoxy)met...	10.334	93	217071	19.178	ng/u1	99
29) 2,4-Dichlorophenol	10.569	162	148179	19.632	ng/u1	99
30) Naphthalene	10.981	128	540870	19.604	ng/u1	99
32) 4-Chloroaniline	11.093	127	221974	19.076	ng/u1	100
33) Hexachlorobutadiene	11.269	225	90939	19.799	ng/u1	99
34) Caprolactam	11.840	113	44851	18.176	ng/u1	83
35) 4-Chloro-3-methylphenol	12.210	107	151950	19.225	ng/u1	98
36) 2-Methylnaphthalene	12.587	142	345319	19.112	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081822\
 Data File : BN021290.D
 Acq On : 18 Aug 2022 21:51
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SICV230


Quant Time: Aug 18 22:19:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 18 21:26:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.804	142	347044	19.200	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.945	216	170378	20.050	ng/ul	95
40) Hexachlorocyclopentadiene	12.934	237	95649	18.206	ng/ul	99
41) 2,4,6-Trichlorophenol	13.187	196	98310	19.346	ng/ul	98
42) 2,4,5-Trichlorophenol	13.257	196	107862	19.528	ng/ul	100
43) 1,1'-Biphenyl	13.592	154	442447	18.862	ng/ul	99
44) 2-Chloronaphthalene	13.634	162	339467	19.192	ng/ul	97
45) 2-Nitroaniline	13.834	65	77644	21.212	ng/ul	89
47) Dimethylphthalate	14.210	163	407601	19.258	ng/ul	98
48) 2,6-Dinitrotoluene	14.328	165	65300	21.030	ng/ul	98
50) Acenaphthylene	14.475	152	549819	19.103	ng/ul	98
51) 3-Nitroaniline	14.651	138	69095	19.070	ng/ul#	96
52) Acenaphthene	14.816	153	360859	19.619	ng/ul	98
53) 2,4-Dinitrophenol	14.857	184	23475	16.611	ng/ul	91
55) 4-Nitrophenol	14.951	109	54956	18.966	ng/ul	91
56) Dibenzofuran	15.151	168	504858	19.404	ng/ul	95
57) 2,4-Dinitrotoluene	15.110	165	94230	22.016	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.375	232	78777	19.838	ng/ul	99
59) Diethylphthalate	15.569	149	402078	18.935	ng/ul	96
61) Fluorene	15.798	166	393372	19.136	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.798	204	185195	19.589	ng/ul	94
63) 4-Nitroaniline	15.816	138	63633	19.258	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.869	198	38725	17.988	ng/ul	93
67) N-Nitrosodiphenylamine	16.004	169	335831	19.390	ng/ul	97
68) 4-Bromophenyl-phenylether	16.692	248	112640	20.367	ng/ul	99
69) Hexachlorobenzene	16.798	284	126110	19.597	ng/ul	94
70) Atrazine	16.957	200	116003	19.649	ng/ul	97
71) Pentachlorophenol	17.145	266	61433	18.325	ng/ul	99
72) Phenanthrene	17.545	178	617280	19.794	ng/ul	100
74) Anthracene	17.639	178	618588	19.549	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.557	216	167686	19.760	ng/ul	98
76) Pentachlorobenzene	15.063	250	155221	20.181	ng/ul	94
77) Carbazole	17.910	167	578755	20.048	ng/ul	98
78) Di-n-butylphthalate	18.475	149	686766	19.613	ng/ul	100
80) Fluoranthene	19.563	202	687723	19.717	ng/ul	97
82) Pyrene	19.922	202	715073	19.817	ng/ul#	93
83) Butylbenzylphthalate	20.822	149	287562	20.467	ng/ul#	97
84) 3,3'-Dichlorobenzidine	21.610	252	229299	21.224	ng/ul#	95
85) Benzo(a)anthracene	21.674	228	675456	19.954	ng/ul	93
86) Bis(2-ethylhexyl)phtha...	21.610	149	446810	20.038	ng/ul	98
87) Chrysene	21.733	228	650078	19.835	ng/ul	99
89) Di-n-octyl phthalate	22.586	149	767210	19.566	ng/ul	100
90) Benzo(b)fluoranthene	23.457	252	712831	19.810	ng/ul	98
91) Benzo(k)fluoranthene	23.457	252	712831	21.491	ng/ul	96
93) Benzo(a)pyrene	24.121	252	675963	19.529	ng/ul	95
94) Indeno(1,2,3-cd)pyrene	26.915	276	794462	19.404	ng/ul	96
95) Dibenzo(a,h)anthracene	26.945	278	690771	19.783	ng/ul	97
96) Benzo(g,h,i)perylene	27.745	276	698966	19.633	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

BNA N





ClientSampleId :
SICV230



#2
 1,4-Dioxane
 Concen: 7.671 ng/uL
 RT: 3.422 min Scan# 21
 Delta R.T. -0.007 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51




Instrument :
 BNA_N
 ClientSampleId :
 SICV230


Tgt Ion: 88 Resp: 29367
 Ion Ratio Lower Upper
 88 100
 43 27.9 22.4 33.6
 58 66.9 61.0 91.4



#5
 Pyridine
 Concen: 19.429 ng/uL
 RT: 3.840 min Scan# 94
 Delta R.T. -0.000 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Tgt Ion: 79 Resp: 183387
 Ion Ratio Lower Upper
 79 100
 52 65.3 65.0 97.4
 51 31.6 31.6 47.4#









#6
Benzaldehyde
Concen: 21.600 ng/ul
RT: 7.222 min Scan# 669
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion: 77 Resp: 103815
Ion Ratio Lower Upper
77 100
105 101.8 74.7 112.1
106 94.8 70.2 105.4



#8
Phenol
Concen: 19.179 ng/ul
RT: 7.269 min Scan# 677
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion: 94 Resp: 218029
Ion Ratio Lower Upper
94 100
65 26.2 23.6 35.4
66 34.3 31.2 46.8









#10
 Bis(2-Chloroethyl)ether
 Concen: 19.227 ng/ul
 RT: 7.510 min Scan# 718
 Delta R.T. -0.006 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51




Instrument :
 BNA_N
 ClientSampleId :
 SICV230


Tgt Ion: 93 Resp: 176963
 Ion Ratio Lower Upper
 93 100
 63 71.5 63.4 95.0
 95 31.6 26.2 39.2



#12
 2-Chlorophenol
 Concen: 19.577 ng/ul
 RT: 7.652 min Scan# 742
 Delta R.T. -0.000 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Tgt Ion:128 Resp: 176922
 Ion Ratio Lower Upper
 128 100
 64 45.8 38.6 57.8
 130 34.3 25.0 37.4





#13

2-Methylphenol

Concen: 19.005 ng/ul

RT: 8.540 min Scan# 894

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :





SICV230

Tgt Ion:108 Resp: 161580

Ion Ratio Lower Upper

108 100

107 88.0 71.5 107.3



#14

2,2'-oxybis(1-Chloropropane)

Concen: 19.459 ng/ul

RT: 8.634 min Scan# 909

Delta R.T. -0.000 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion: 45 Resp: 220253


Ion Ratio Lower Upper

45 100

77 15.5 10.9 16.3

79 11.6 8.6 13.0









#16
 Acetophenone
 Concen: 19.441 ng/ul
 RT: 8.928 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51




Instrument :
 BNA_N
 ClientSampleId :
 SICV230


Tgt Ion:105 Resp: 249516
 Ion Ratio Lower Upper
 105 100
 77 74.7 63.5 95.3
 51 24.9 23.5 35.3



#17
 N-Nitroso-di-n-propylamine
 Concen: 19.239 ng/ul
 RT: 8.910 min Scan# 956
 Delta R.T. -0.006 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Tgt Ion: 70 Resp: 121972
 Ion Ratio Lower Upper
 70 100
 42 55.8 47.8 71.6
 101 10.0 7.8 11.6
 130 22.0 15.8 23.8









#18
4-Methylphenol
Concen: 19.003 ng/ul
RT: 8.869 min Scan# 949
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:108 Resp: 170099
Ion Ratio Lower Upper
108 100
107 111.7 88.0 132.0



#19
Hexachloroethane
Concen: 19.293 ng/ul
RT: 9.193 min Scan# 1004
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:117 Resp: 72941
Ion Ratio Lower Upper
117 100
201 99.9 83.2 124.8
199 57.7 50.2 75.4



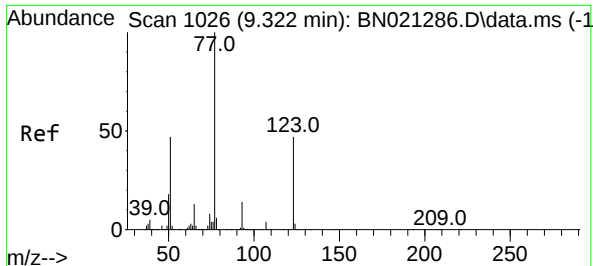

#22

Nitrobenzene

Concen: 20.341 ng/ul

RT: 9.316 min Scan# 1026

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion: 77 Resp: 175723

Ion Ratio Lower Upper

77 100

123 48.5 34.5 51.7

65 13.5 11.1 16.7



#23

Isophorone

Concen: 18.730 ng/ul

RT: 9.846 min Scan# 1115

Delta R.T. -0.000 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion: 82 Resp: 338802


Ion Ratio Lower Upper

82 100

95 7.0 5.8 8.8

138 18.1 13.8 20.8







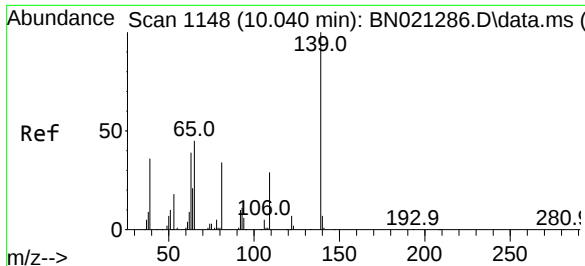

#25
2-Nitrophenol
Concen: 21.744 ng/ul
RT: 10.034 min Scan# 1147
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:139 Resp: 77085
Ion Ratio Lower Upper
139 100
65 48.9 43.7 65.5
109 28.4 25.8 38.6

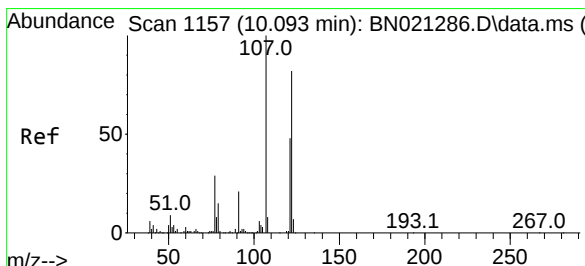

#26
2,4-Dimethylphenol
Concen: 19.279 ng/ul
RT: 10.093 min Scan# 1157
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:107 Resp: 180537
Ion Ratio Lower Upper
107 100
121 51.5 38.3 57.5
122 89.9 66.3 99.5









#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.178 ng/ul
 RT: 10.334 min Scan# 1199
 Delta R.T. -0.006 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51




Instrument :
 BNA_N
 ClientSampleId :
 SICV230


Tgt Ion: 93 Resp: 217071
 Ion Ratio Lower Upper
 93 100
 95 31.9 25.4 38.0
 123 11.5 8.3 12.5



#29
 2,4-Dichlorophenol
 Concen: 19.632 ng/ul
 RT: 10.569 min Scan# 1238
 Delta R.T. -0.006 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Tgt Ion:162 Resp: 148179
 Ion Ratio Lower Upper
 162 100
 164 66.0 52.9 79.3
 98 35.7 29.8 44.8









#30
Naphthalene
Concen: 19.604 ng/ul
RT: 10.981 min Scan# 11
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:128 Resp: 540870
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 12.8 10.6 16.0



#32
4-Chloroaniline
Concen: 19.076 ng/ul
RT: 11.093 min Scan# 1327
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:127 Resp: 221974
Ion Ratio Lower Upper
127 100
129 32.9 26.1 39.1









#33
Hexachlorobutadiene
Concen: 19.799 ng/ul
RT: 11.269 min Scan# 11
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:225 Resp: 90939
Ion Ratio Lower Upper
225 100
223 64.1 51.8 77.6
227 64.5 50.6 76.0



#34
Caprolactam
Concen: 18.176 ng/ul
RT: 11.840 min Scan# 1454
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:113 Resp: 44851
Ion Ratio Lower Upper
113 100
55 157.4 145.5 218.3
56 114.7 106.5 159.7









#35
4-Chloro-3-methylphenol
Concen: 19.225 ng/ul
RT: 12.210 min Scan# 1517
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:107 Resp: 151950
Ion Ratio Lower Upper
107 100
144 26.3 20.6 31.0
142 79.4 62.2 93.4



#36
2-Methylnaphthalene
Concen: 19.112 ng/ul
RT: 12.587 min Scan# 1581
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:142 Resp: 345319
Ion Ratio Lower Upper
142 100
141 89.2 70.6 105.8









#37
1-Methylnaphthalene
Concen: 19.200 ng/ul
RT: 12.804 min Scan# 1619
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:142 Resp: 347044
Ion Ratio Lower Upper
142 100
141 90.9 70.9 106.3
116 4.0 3.1 4.7



#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.050 ng/ul
RT: 12.945 min Scan# 1642
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:216 Resp: 170378
Ion Ratio Lower Upper
216 100
214 73.2 63.4 95.0
179 20.6 17.8 26.8
108 19.0 15.1 22.7









#40
Hexachlorocyclopentadiene
Concen: 18.206 ng/ul
RT: 12.934 min Scan# 1640
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:237 Resp: 95649
Ion Ratio Lower Upper
237 100
235 61.0 48.8 73.2
272 13.2 9.3 13.9



#41
2,4,6-Trichlorophenol
Concen: 19.346 ng/ul
RT: 13.187 min Scan# 1683
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:196 Resp: 98310
Ion Ratio Lower Upper
196 100
198 98.6 79.8 119.8
200 32.7 25.0 37.6









#42
2,4,5-Trichlorophenol
Concen: 19.528 ng/ul
RT: 13.257 min Scan# 1695
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:196 Resp: 107862
Ion Ratio Lower Upper
196 100
198 97.4 77.6 116.4
200 30.1 24.4 36.6



#43
1,1'-Biphenyl
Concen: 18.862 ng/ul
RT: 13.592 min Scan# 1752
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:154 Resp: 442447
Ion Ratio Lower Upper
154 100
153 39.0 31.5 47.3
76 13.7 10.5 15.7









#44
2-Chloronaphthalene
Concen: 19.192 ng/ul
RT: 13.634 min Scan# 1759
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:162 Resp: 339467
Ion Ratio Lower Upper
162 100
164 33.6 25.8 38.6
127 41.5 31.4 47.2



#45
2-Nitroaniline
Concen: 21.212 ng/ul
RT: 13.834 min Scan# 1793
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion: 65 Resp: 77644
Ion Ratio Lower Upper
65 100
92 71.1 54.1 81.1
138 111.3 77.0 115.4









#47
Dimethylphthalate
Concen: 19.258 ng/ul
RT: 14.210 min Scan# 1857
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:163 Resp: 407601
Ion Ratio Lower Upper
163 100
194 3.9 3.4 5.0
164 10.4 7.7 11.5



#48
2,6-Dinitrotoluene
Concen: 21.030 ng/ul
RT: 14.328 min Scan# 1877
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:165 Resp: 65300
Ion Ratio Lower Upper
165 100
89 61.5 50.6 75.8
121 23.7 17.9 26.9









#50
Acenaphthylene
Concen: 19.103 ng/ul
RT: 14.475 min Scan# 1902
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:152 Resp: 549819
Ion Ratio Lower Upper
152 100
151 18.9 16.0 24.0
153 13.3 10.7 16.1



#51
3-Nitroaniline
Concen: 19.070 ng/ul
RT: 14.651 min Scan# 1932
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:138 Resp: 69095
Ion Ratio Lower Upper
138 100
108 15.2 8.6 12.8#
92 120.0 92.9 139.3









#52
Acenaphthene
Concen: 19.619 ng/ul
RT: 14.816 min Scan# 1960
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:153 Resp: 360859
Ion Ratio Lower Upper
153 100
152 46.3 38.4 57.6
154 86.1 69.7 104.5



#53
2,4-Dinitrophenol
Concen: 16.611 ng/ul
RT: 14.857 min Scan# 1967
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:184 Resp: 23475
Ion Ratio Lower Upper
184 100
63 62.6 55.9 83.9
154 59.1 53.1 79.7









#55
4-Nitrophenol
Concen: 18.966 ng/ul
RT: 14.951 min Scan# 1983
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:109 Resp: 54956
Ion Ratio Lower Upper
109 100
139 142.8 100.1 150.1
65 134.3 104.6 157.0



#56
Dibenzofuran
Concen: 19.404 ng/ul
RT: 15.151 min Scan# 2017
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:168 Resp: 504858
Ion Ratio Lower Upper
168 100
139 35.9 31.1 46.7





#57

2,4-Dinitrotoluene

Concen: 22.016 ng/ul

RT: 15.110 min Scan# 2010

Delta R.T. -0.000 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:165 Resp: 94230

Ion Ratio Lower Upper

165 100

63 44.3 36.3 54.5

182 3.0 2.3 3.5



#58

2,3,4,6-Tetrachlorophenol

Concen: 19.838 ng/ul

RT: 15.375 min Scan# 2055

Delta R.T. -0.000 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Tgt Ion:232 Resp: 78777




Ion Ratio Lower Upper


232 100

131 48.4 38.5 57.7

130 2.5 2.2 3.2

166 31.9 25.8 38.8









#59
Diethylphthalate
Concen: 18.935 ng/ul
RT: 15.569 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:149 Resp: 402078
Ion Ratio Lower Upper
149 100
177 20.5 17.8 26.8
150 11.4 10.5 15.7



#61
Fluorene
Concen: 19.136 ng/ul
RT: 15.798 min Scan# 2127
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:166 Resp: 393372
Ion Ratio Lower Upper
166 100
165 97.5 77.7 116.5
167 13.1 11.1 16.7









#62
4-Chlorophenyl-phenylether
Concen: 19.589 ng/ul
RT: 15.798 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:204 Resp: 185195
Ion Ratio Lower Upper
204 100
206 30.4 26.7 40.1
141 58.1 50.2 75.2



#63
4-Nitroaniline
Concen: 19.258 ng/ul
RT: 15.816 min Scan# 2130
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:138 Resp: 63633
Ion Ratio Lower Upper
138 100
92 50.5 41.0 61.6
108 77.4 65.3 97.9









#66
 4,6-Dinitro-2-methylphenol
 Concen: 17.988 ng/ul
 RT: 15.869 min Scan# 2139
 Delta R.T. -0.000 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51




Instrument :
 BNA_N
 ClientSampleId :
 SICV230


Tgt Ion:198 Resp: 38725
 Ion Ratio Lower Upper
 198 100
 182 4.4 3.0 4.4
 77 29.0 20.1 30.1



#67
 N-Nitrosodiphenylamine
 Concen: 19.390 ng/ul
 RT: 16.004 min Scan# 2162
 Delta R.T. -0.006 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Tgt Ion:169 Resp: 335831
 Ion Ratio Lower Upper
 169 100
 168 68.8 52.4 78.6
 167 35.5 27.5 41.3









#68
4-Bromophenyl-phenylether
Concen: 20.367 ng/ul
RT: 16.692 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:248 Resp: 112640
Ion Ratio Lower Upper
248 100
250 95.2 77.8 116.8
141 78.0 62.6 93.8



#69
Hexachlorobenzene
Concen: 19.597 ng/ul
RT: 16.798 min Scan# 2297
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:284 Resp: 126110
Ion Ratio Lower Upper
284 100
142 40.3 27.8 41.8
249 30.9 25.7 38.5





#70

Atrazine

Concen: 19.649 ng/ul

RT: 16.957 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:200 Resp: 116003

Ion Ratio Lower Upper

200 100

173 27.0 20.5 30.7

215 46.1 38.9 58.3



#71

Pentachlorophenol

Concen: 18.325 ng/ul

RT: 17.145 min Scan# 2356

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion:266 Resp: 61433


Ion Ratio Lower Upper

266 100

264 64.0 50.2 75.2

268 61.3 49.3 73.9









#72
Phenanthrene
Concen: 19.794 ng/ul
RT: 17.545 min Scan# 2425
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:178 Resp: 617280
Ion Ratio Lower Upper
178 100
179 15.3 12.2 18.4
176 19.2 15.2 22.8



#74
Anthracene
Concen: 19.549 ng/ul
RT: 17.639 min Scan# 2440
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:178 Resp: 618588
Ion Ratio Lower Upper
178 100
179 15.5 13.0 19.4
176 18.2 15.5 23.3









#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.760 ng/uL
RT: 13.557 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:216 Resp: 167686
Ion Ratio Lower Upper
216 100
214 76.7 63.2 94.8
218 47.5 37.9 56.9



#76
Pentachlorobenzene
Concen: 20.181 ng/uL
RT: 15.063 min Scan# 2002
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:250 Resp: 155221
Ion Ratio Lower Upper
250 100
248 61.5 53.0 79.4
252 62.7 53.4 80.2





#77

Carbazole

Concen: 20.048 ng/ul

RT: 17.910 min Scan# 2486

Delta R.T. -0.000 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:167 Resp: 578755

Ion Ratio Lower Upper

167 100

166 20.7 16.1 24.1

139 13.6 10.2 15.2



#78

Di-n-butylphthalate

Concen: 19.613 ng/ul

RT: 18.475 min Scan# 2582

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion:149 Resp: 686766


Ion Ratio Lower Upper

149 100

150 9.0 7.1 10.7

104 5.1 4.1 6.1









#80
Fluoranthene
Concen: 19.717 ng/ul
RT: 19.563 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:202 Resp: 687723
Ion Ratio Lower Upper
202 100
101 12.3 8.9 13.3
100 9.4 6.7 10.1



#82
Pyrene
Concen: 19.817 ng/ul
RT: 19.922 min Scan# 2828
Delta R.T. -0.006 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:202 Resp: 715073
Ion Ratio Lower Upper
202 100
101 15.0 9.7 14.5#
100 12.4 8.0 12.0#





#83

Butylbenzylphthalate

Concen: 20.467 ng/ul

RT: 20.822 min Scan# 2981

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:149 Resp: 287562

Ion Ratio Lower Upper

149 100

91 74.1 58.8 88.2

206 17.4 18.1 27.1#



#84

3,3'-Dichlorobenzidine

Concen: 21.224 ng/ul

RT: 21.610 min Scan# 3115

Delta R.T. -0.000 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion:252 Resp: 229299


Ion Ratio Lower Upper

252 100

254 67.4 50.8 76.2

126 13.4 8.2 12.4#





#85

Benzo(a)anthracene

Concen: 19.954 ng/ul

RT: 21.674 min Scan# 3127

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:228 Resp: 675456

Ion Ratio Lower Upper

228 100

229 18.5 16.3 24.5

226 24.3 23.2 34.8



#86

Bis(2-ethylhexyl)phthalate

Concen: 20.038 ng/ul

RT: 21.610 min Scan# 3115

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion:149 Resp: 446810


Ion Ratio Lower Upper

149 100

167 27.2 22.5 33.7

279 4.1 3.5 5.3





#87

Chrysene

Concen: 19.835 ng/ul

RT: 21.733 min Scan# 3137

Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:228 Resp: 650078

Ion Ratio Lower Upper

228 100

226 31.0 24.2 36.2

229 20.0 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 19.566 ng/ul




RT: 22.586 min Scan# 3281


Delta R.T. -0.006 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Tgt Ion:149 Resp: 767210









#90
Benzo(b)fluoranthene
Concen: 19.810 ng/ul
RT: 23.457 min Scan# 3429
Delta R.T. -0.000 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51




Instrument :
BNA_N
ClientSampleId :
SICV230


Tgt Ion:252 Resp: 712831
Ion Ratio Lower Upper
252 100
253 20.7 16.5 24.7
125 11.6 7.8 11.8



#91
Benzo(k)fluoranthene
Concen: 21.491 ng/ul
RT: 23.457 min Scan# 3429
Delta R.T. -0.053 min
Lab File: BN021290.D
Acq: 18 Aug 2022 21:51

Tgt Ion:252 Resp: 712831
Ion Ratio Lower Upper
252 100
253 20.7 18.2 27.4
125 11.6 8.2 12.4





#93

Benzo(a)pyrene

Concen: 19.529 ng/ul

RT: 24.121 min Scan# 3542

Delta R.T. -0.012 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51

Instrument :

BNA_N

ClientSampleId :

SICV230





Tgt Ion:252 Resp: 675963

Ion Ratio Lower Upper

252 100

253 20.5 18.7 28.1

125 13.2 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.404 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. -0.012 min

Lab File: BN021290.D

Acq: 18 Aug 2022 21:51




Tgt Ion:276 Resp: 794462


Ion Ratio Lower Upper

276 100

138 27.3 19.5 29.3

277 25.2 21.4 32.0









#95
 Dibenzo(a,h)anthracene
 Concen: 19.783 ng/ul
 RT: 26.945 min Scan# 4158
 Delta R.T. -0.018 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Instrument :
 BNA_N
 ClientSampleId :
 SICV230

Tgt Ion:278 Resp: 690771
 Ion Ratio Lower Upper
 278 100
 139 19.1 13.8 20.8
 279 23.7 18.3 27.5



#96
 Benzo(g,h,i)perylene
 Concen: 19.633 ng/ul
 RT: 27.745 min Scan# 4158
 Delta R.T. -0.012 min
 Lab File: BN021290.D
 Acq: 18 Aug 2022 21:51

Tgt Ion:276 Resp: 698966
 Ion Ratio Lower Upper
 276 100
 138 24.6 17.0 25.6
 277 24.9 17.8 26.6

