
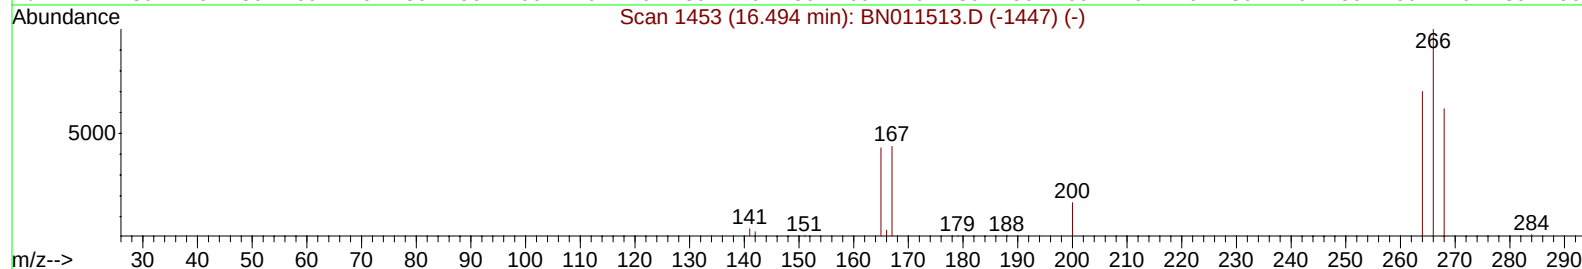
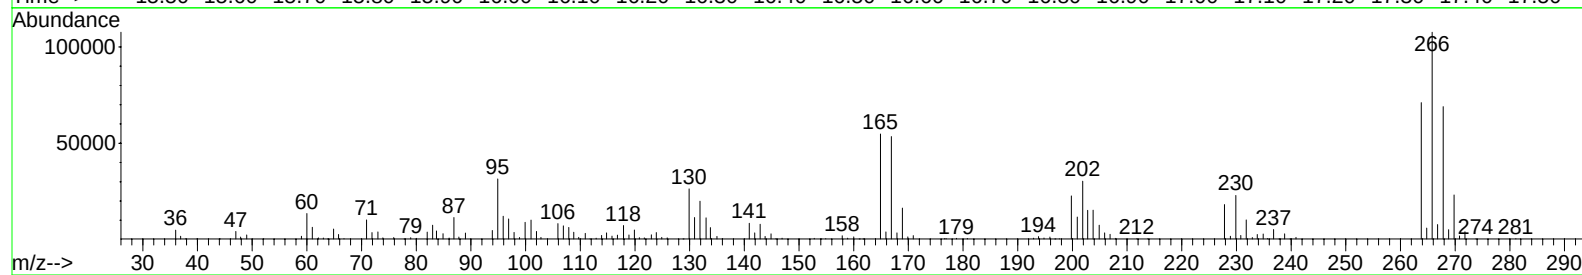


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081920\
 Data File : BN011509.D
 Acq On : 19 Aug 2020 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 18:19:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 19 15:54:57 2020
 Response via : Initial Calibration

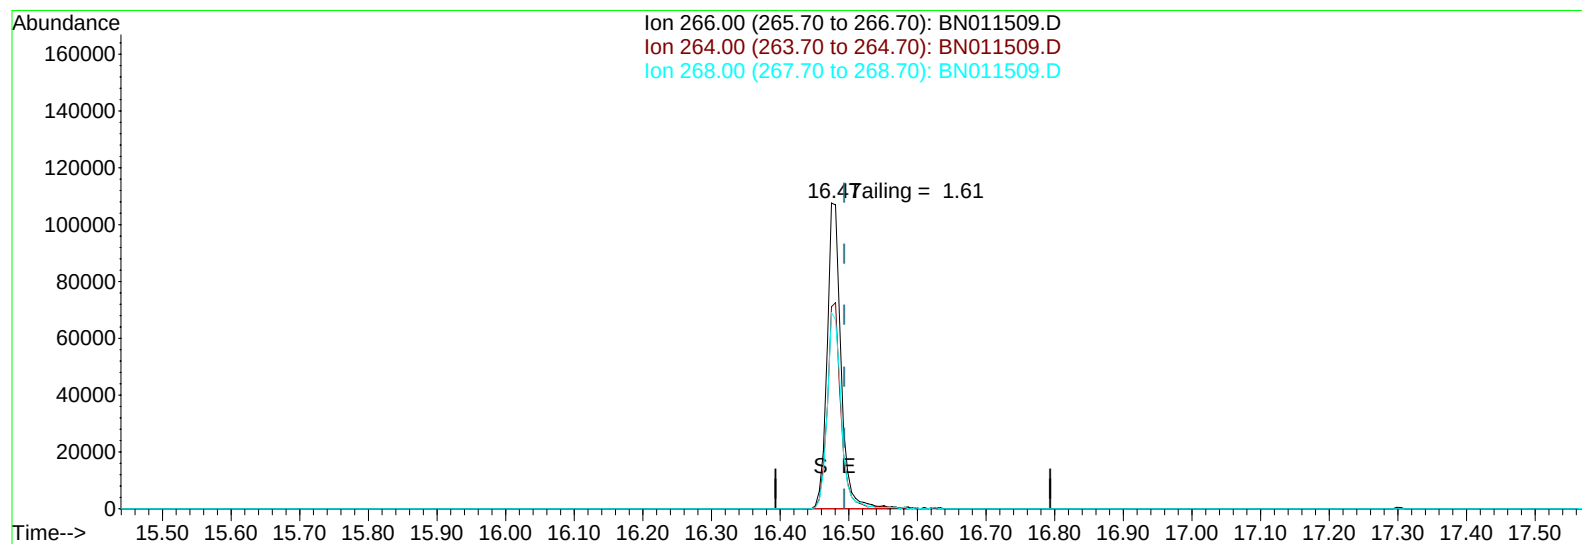

TIC: BN011509.D

(24) Pentachlorophenol

16.475min (-0.019) 1034.35ng

response 152048

Ion	Exp%	Act%
266.00	100	100
264.00	67.10	65.90
268.00	66.20	64.61
0.00	0.00	0.00