


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081920\
 Data File : BN011509.D
 Acq On : 19 Aug 2020 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 19 15:54:57 2020

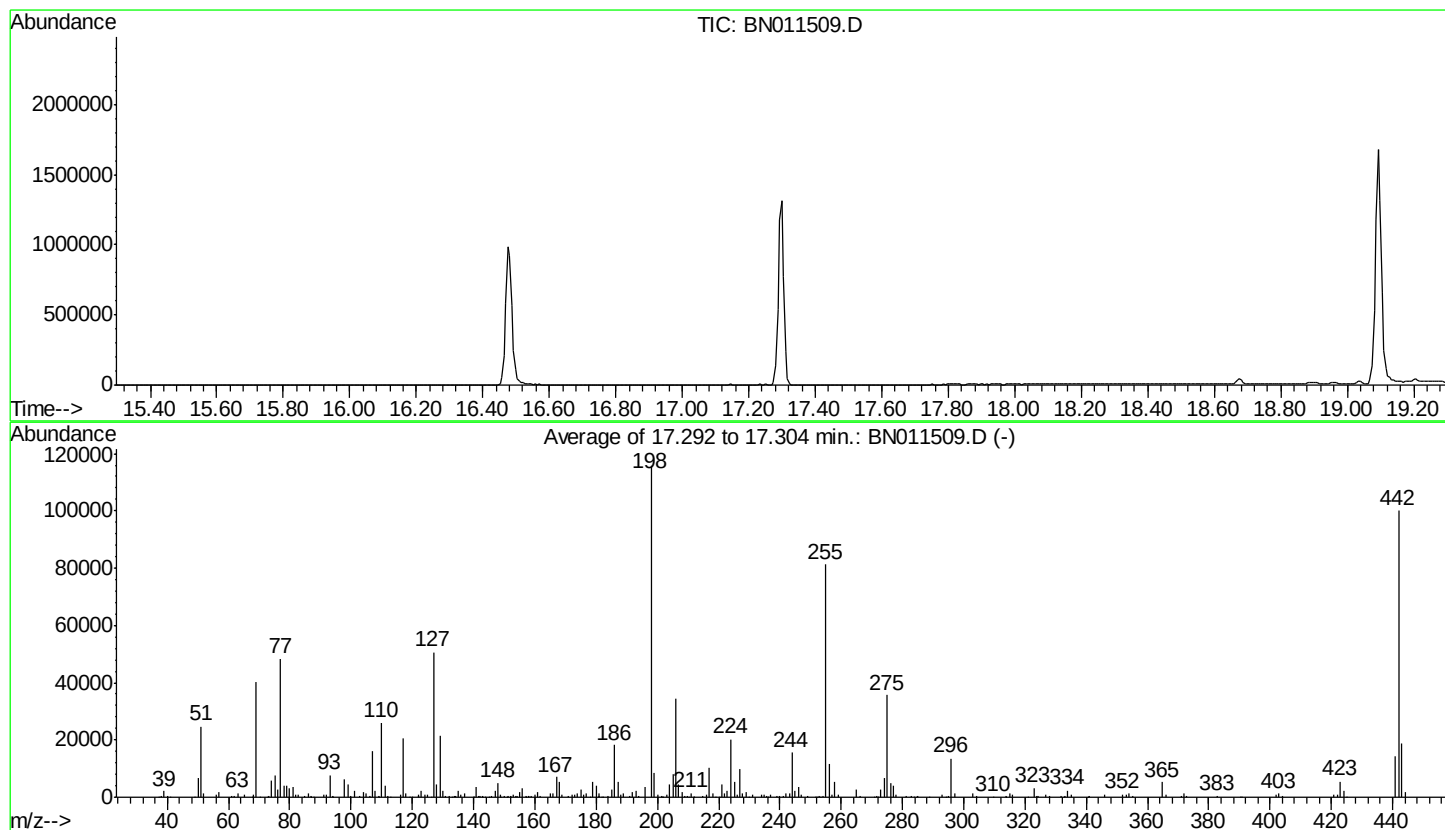

AutoFind: Scans 2432, 2433, 2434; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	24808	PASS
68	69	0.00	2	2.0	789	PASS
69	198	0.00	100	34.8	40352	PASS
70	69	0.00	2	0.4	156	PASS
127	198	10	80	43.7	50549	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115800	PASS
199	198	5	9	7.2	8332	PASS
275	198	10	60	30.9	35728	PASS
365	198	1	100	4.6	5286	PASS
441	198	0.01	100	12.4	14320	PASS
442	198	50	100	86.4	100072	PASS
443	442	15	24	18.9	18909	PASS