

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081922\
 Data File : BN021292.D
 Acq On : 19 Aug 2022 11:43
 Operator : CG/JU
 Sample : SSTD00523
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231

Quant Time: Aug 19 15:37:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 15:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	117385	20.000	ng/u1	0.00
20) Naphthalene-d8	10.934	136	532884	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.751	164	349946	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.504	188	744694	20.000	ng/u1	0.00
79) Chrysene-d12	21.698	240	800706	20.000	ng/u1	0.00
88) Perylene-d12	24.239	264	885366	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	6112	1.922	ng/uL	0.00
4) Pyridine-d5	3.822	84	34301	4.087	ng/u1	0.00
7) Phenol-d5	7.240	99	42454	4.273	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	28811	4.830	ng/u1	0.00
11) 2-Chlorophenol-d4	7.616	132	33127	4.364	ng/u1	0.00
15) 4-Methylphenol-d8	8.805	113	33053	4.512	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	14187	4.126	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	11762	3.977	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	29698	4.068	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	54430	4.837	ng/u1	0.00
46) Dimethylphthalate-d6	14.157	166	107229	4.606	ng/u1	0.00
49) Acenaphthylene-d8	14.445	160	122372	4.264	ng/u1	0.00
54) 4-Nitrophenol-d4	14.934	143	14033	3.487	ng/u1	0.00
60) Fluorene-d10	15.745	176	98160	4.787	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	7903	3.125	ng/u1	0.00
73) Anthracene-d10	17.598	188	149900	4.565	ng/u1	0.00
81) Pyrene-d10	19.892	212	171802	4.217	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.068	264	184842	4.258	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.423	88	5719	1.677	ng/uL	94
5) Pyridine	3.840	79	37873	4.503	ng/u1	95
6) Benzaldehyde	7.222	77	21714	5.071	ng/u1	95
8) Phenol	7.269	94	45361	4.478	ng/u1	92
10) Bis(2-Chloroethyl)ether	7.511	93	39231	4.784	ng/u1	95
12) 2-Chlorophenol	7.652	128	36515	4.535	ng/u1	94
13) 2-Methylphenol	8.540	108	34087	4.500	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.628	45	50984	5.056	ng/u1	95
16) Acetophenone	8.928	105	61685	5.394	ng/u1	95
17) N-Nitroso-di-n-propyla...	8.910	70	28810	5.100	ng/u1	96
18) 4-Methylphenol	8.869	108	36594	4.588	ng/u1	91
19) Hexachloroethane	9.193	117	14888	4.420	ng/u1	91
22) Nitrobenzene	9.316	77	37641	4.405	ng/u1	97
23) Isophorone	9.840	82	80584	4.504	ng/u1	98
25) 2-Nitrophenol	10.034	139	13028	3.715	ng/u1	99
26) 2,4-Dimethylphenol	10.093	107	41535	4.484	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.334	93	52754	4.712	ng/u1	96
29) 2,4-Dichlorophenol	10.569	162	31861	4.267	ng/u1	97
30) Naphthalene	10.981	128	130947	4.798	ng/u1	99
32) 4-Chloroaniline	11.093	127	58179	5.054	ng/u1	99
33) Hexachlorobutadiene	11.269	225	20635	4.542	ng/u1	94
34) Caprolactam	11.840	113	9874	4.045	ng/u1	87
35) 4-Chloro-3-methylphenol	12.204	107	35172	4.498	ng/u1	98
36) 2-Methylnaphthalene	12.587	142	86473	4.838	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081922\
 Data File : BN021292.D
 Acq On : 19 Aug 2022 11:43
 Operator : CG/JU
 Sample : SST00523
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SST005231

Quant Time: Aug 19 15:37:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 15:36:45 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.804	142	86757	4.852	ng/ul	92
39) 1,2,4,5-Tetrachloroben...	12.946	216	41435	4.297	ng/ul	97
40) Hexachlorocyclopentadiene	12.928	237	21586	3.621	ng/ul#	85
41) 2,4,6-Trichlorophenol	13.187	196	22451	3.894	ng/ul	94
42) 2,4,5-Trichlorophenol	13.257	196	23903	3.814	ng/ul	93
43) 1,1'-Biphenyl	13.593	154	118660	4.459	ng/ul	96
44) 2-Chloronaphthalene	13.634	162	90335	4.501	ng/ul	99
45) 2-Nitroaniline	13.834	65	17191	4.139	ng/ul	88
47) Dimethylphthalate	14.204	163	110854	4.616	ng/ul	98
48) 2,6-Dinitrotoluene	14.322	165	14456	4.103	ng/ul	91
50) Acenaphthylene	14.475	152	146503	4.486	ng/ul	99
51) 3-Nitroaniline	14.651	138	14823	3.606	ng/ul#	97
52) Acenaphthene	14.816	153	97795	4.686	ng/ul	99
53) 2,4-Dinitrophenol	14.851	184	4826	3.010	ng/ul	97
55) 4-Nitrophenol	14.945	109	12891	3.921	ng/ul	98
56) Dibenzofuran	15.151	168	140936	4.774	ng/ul	99
57) 2,4-Dinitrotoluene	15.104	165	20264	4.173	ng/ul#	97
58) 2,3,4,6-Tetrachlorophenol	15.369	232	17929	3.979	ng/ul	93
59) Diethylphthalate	15.569	149	108099	4.487	ng/ul	99
61) Fluorene	15.798	166	112845	4.838	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.792	204	51863	4.835	ng/ul	98
63) 4-Nitroaniline	15.810	138	14741	3.932	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.863	198	7772	2.879	ng/ul#	85
67) N-Nitrosodiphenylamine	16.004	169	96269	4.433	ng/ul	96
68) 4-Bromophenyl-phenylether	16.692	248	29253	4.219	ng/ul	96
69) Hexachlorobenzene	16.792	284	35397	4.387	ng/ul	91
70) Atrazine	16.951	200	29562	3.994	ng/ul	96
71) Pentachlorophenol	17.145	266	13361	3.179	ng/ul	94
72) Phenanthrene	17.545	178	183790	4.701	ng/ul	99
74) Anthracene	17.634	178	180138	4.541	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.551	216	42421	3.987	ng/ul	95
76) Pentachlorobenzene	15.063	250	43729	4.535	ng/ul	93
77) Carbazole	17.904	167	170311	4.705	ng/ul	98
78) Di-n-butylphthalate	18.475	149	167682	3.819	ng/ul	99
80) Fluoranthene	19.557	202	204009	4.063	ng/ul#	95
82) Pyrene	19.922	202	223262	4.299	ng/ul#	92
83) Butylbenzylphthalate	20.827	149	64432	3.186	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.610	252	64012	4.116	ng/ul#	96
85) Benzo(a)anthracene	21.680	228	218684	4.488	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.610	149	117038	3.646	ng/ul#	98
87) Chrysene	21.733	228	219627	4.655	ng/ul	96
89) Di-n-octyl phthalate	22.586	149	194821	3.235	ng/ul	100
90) Benzo(b)fluoranthene	23.451	252	243310	4.402	ng/ul#	96
91) Benzo(k)fluoranthene	23.504	252	222196	4.361	ng/ul	98
93) Benzo(a)pyrene	24.121	252	230437	4.334	ng/ul#	97
94) Indeno(1,2,3-cd)pyrene	26.915	276	278943	4.436	ng/ul	95
95) Dibenzo(a,h)anthracene	26.939	278	243227	4.535	ng/ul	97
96) Benzo(g,h,i)perylene	27.739	276	248826	4.550	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed






#2
1,4-Dioxane
Concen: 1.677 ng/uL
RT: 3.423 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Instrument :
BNA_N
ClientSampleId :
SSTD005231







Tgt Ion: 88 Resp: 5719
Ion Ratio Lower Upper
88 100
43 32.2 22.4 33.6
58 71.5 61.0 91.4



#5
Pyridine
Concen: 4.503 ng/uL
RT: 3.840 min Scan# 94
Delta R.T. 0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion: 79 Resp: 37873
Ion Ratio Lower Upper
79 100
52 74.4 65.0 97.4
51 39.8 31.6 47.4









#6
Benzaldehyde
Concen: 5.071 ng/ul
RT: 7.222 min Scan# 669
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion: 77 Resp: 21714
Ion Ratio Lower Upper
77 100
105 97.7 74.7 112.1
106 93.1 70.2 105.4



#8
Phenol
Concen: 4.478 ng/ul
RT: 7.269 min Scan# 677
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion: 94 Resp: 45361
Ion Ratio Lower Upper
94 100
65 26.0 23.6 35.4
66 33.0 31.2 46.8









#10
 Bis(2-Chloroethyl)ether
 Concen: 4.784 ng/ul
 RT: 7.511 min Scan# 718
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231

Tgt Ion: 93 Resp: 39231




Ion	Ratio	Lower	Upper
93	100		
63	73.1	63.4	95.0
95	32.3	26.2	39.2




#12
 2-Chlorophenol
 Concen: 4.535 ng/ul
 RT: 7.652 min Scan# 742
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion: 128 Resp: 36515

Ion	Ratio	Lower	Upper
128	100		
64	43.6	38.6	57.8
130	34.4	25.0	37.4





#13

2-Methylphenol

Concen: 4.500 ng/ul

RT: 8.540 min Scan# 893

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Instrument :

BNA_N

ClientSampleId :





SSTD005231

Tgt Ion:108 Resp: 34087

Ion Ratio Lower Upper

108 100

107 87.6 71.5 107.3



#14

2,2'-oxybis(1-Chloropropane)

Concen: 5.056 ng/ul

RT: 8.628 min Scan# 908

Delta R.T. -0.006 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43




Tgt Ion: 45 Resp: 50984


Ion Ratio Lower Upper

45 100

77 16.1 10.9 16.3

79 11.9 8.6 13.0









#16
 Acetophenone
 Concen: 5.394 ng/ul
 RT: 8.928 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231


Tgt Ion:	105	Resp:	61685
Ion Ratio	Lower	Upper	
105	100		
77	76.4	63.5	95.3
51	25.3	23.5	35.3



#17
 N-Nitroso-di-n-propylamine
 Concen: 5.100 ng/ul
 RT: 8.910 min Scan# 956
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:	70	Resp:	28810
Ion Ratio	Lower	Upper	
70	100		
42	56.2	47.8	71.6
101	10.4	7.8	11.6
130	21.3	15.8	23.8









#18
4-Methylphenol
Concen: 4.588 ng/ul
RT: 8.869 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:108 Resp: 36594
Ion Ratio Lower Upper
108 100
107 119.8 88.0 132.0



#19
Hexachloroethane
Concen: 4.420 ng/ul
RT: 9.193 min Scan# 1004
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:117 Resp: 14888
Ion Ratio Lower Upper
117 100
201 92.7 83.2 124.8
199 58.0 50.2 75.4









#22
Nitrobenzene
Concen: 4.405 ng/ul
RT: 9.316 min Scan# 1025
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion: 77 Resp: 37641
Ion Ratio Lower Upper
77 100
123 41.0 34.5 51.7
65 12.7 11.1 16.7



#23
Isophorone
Concen: 4.504 ng/ul
RT: 9.840 min Scan# 1114
Delta R.T. -0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion: 82 Resp: 80584
Ion Ratio Lower Upper
82 100
95 7.0 5.8 8.8
138 18.3 13.8 20.8









#25
2-Nitrophenol
Concen: 3.715 ng/ul
RT: 10.034 min Scan# 1147
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:139 Resp: 13028
Ion Ratio Lower Upper
139 100
65 54.1 43.7 65.5
109 32.8 25.8 38.6



#26
2,4-Dimethylphenol
Concen: 4.484 ng/ul
RT: 10.093 min Scan# 1157
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:107 Resp: 41535
Ion Ratio Lower Upper
107 100
121 48.6 38.3 57.5
122 82.2 66.3 99.5









#27
 Bis(2-Chloroethoxy)methane
 Concen: 4.712 ng/ul
 RT: 10.334 min Scan# 1198
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231


Tgt Ion:	93	Resp:	52754
Ion	Ratio	Lower	Upper
93	100		
95	33.8	25.4	38.0
123	11.8	8.3	12.5



#29
 2,4-Dichlorophenol
 Concen: 4.267 ng/ul
 RT: 10.569 min Scan# 1238
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:	162	Resp:	31861
Ion	Ratio	Lower	Upper
162	100		
164	62.9	52.9	79.3
98	35.8	29.8	44.8









#30
Naphthalene
Concen: 4.798 ng/ul
RT: 10.981 min Scan# 1308
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:128 Resp: 130947
Ion Ratio Lower Upper
128 100
129 10.6 8.7 13.1
127 13.0 10.6 16.0



#32
4-Chloroaniline
Concen: 5.054 ng/ul
RT: 11.093 min Scan# 1327
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:127 Resp: 58179
Ion Ratio Lower Upper
127 100
129 32.0 26.1 39.1









#33
Hexachlorobutadiene
Concen: 4.542 ng/ul
RT: 11.269 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:225 Resp: 20635
Ion Ratio Lower Upper
225 100
223 58.9 51.8 77.6
227 66.3 50.6 76.0



#34
Caprolactam
Concen: 4.045 ng/ul
RT: 11.840 min Scan# 1454
Delta R.T. -0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:113 Resp: 9874
Ion Ratio Lower Upper
113 100
55 163.1 145.5 218.3
56 116.7 106.5 159.7









#35
4-Chloro-3-methylphenol
Concen: 4.498 ng/ul
RT: 12.204 min Scan# 1516
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:107 Resp: 35172
Ion Ratio Lower Upper
107 100
144 26.6 20.6 31.0
142 79.5 62.2 93.4



#36
2-Methylnaphthalene
Concen: 4.838 ng/ul
RT: 12.587 min Scan# 1581
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:142 Resp: 86473
Ion Ratio Lower Upper
142 100
141 89.4 70.6 105.8





#37

1-Methylnaphthalene

Concen: 4.852 ng/ul

RT: 12.804 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Instrument :

BNA_N

ClientSampleId :

SSTD005231





Tgt Ion:142 Resp: 86757

Ion Ratio Lower Upper

142 100

141 96.5 70.9 106.3

116 3.8 3.1 4.7



#39

1,2,4,5-Tetrachlorobenzene

Concen: 4.297 ng/ul

RT: 12.946 min Scan# 1642

Delta R.T. -0.006 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Tgt Ion:216 Resp: 41435




Ion Ratio Lower Upper


216 100

214 75.8 63.4 95.0

179 22.0 17.8 26.8

108 21.1 15.1 22.7









#40
Hexachlorocyclopentadiene
Concen: 3.621 ng/ul
RT: 12.928 min Scan# 1639
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:237 Resp: 21586
Ion Ratio Lower Upper
237 100
235 74.0 48.8 73.2#
272 13.6 9.3 13.9



#41
2,4,6-Trichlorophenol
Concen: 3.894 ng/ul
RT: 13.187 min Scan# 1683
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:196 Resp: 22451
Ion Ratio Lower Upper
196 100
198 92.1 79.8 119.8
200 32.0 25.0 37.6









#42
2,4,5-Trichlorophenol
Concen: 3.814 ng/ul
RT: 13.257 min Scan# 1695
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:196 Resp: 23903
Ion Ratio Lower Upper
196 100
198 88.6 77.6 116.4
200 32.4 24.4 36.6



#43
1,1'-Biphenyl
Concen: 4.459 ng/ul
RT: 13.593 min Scan# 1752
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:154 Resp: 118660
Ion Ratio Lower Upper
154 100
153 41.7 31.5 47.3
76 14.4 10.5 15.7





#44

2-Chloronaphthalene

Concen: 4.501 ng/ul

RT: 13.634 min Scan# 1759

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Instrument :

BNA_N

ClientSampleId :

SSTD005231





Tgt Ion:162 Resp: 90335

Ion Ratio Lower Upper

162 100

164 32.9 25.8 38.6

127 38.9 31.4 47.2



#45

2-Nitroaniline

Concen: 4.139 ng/ul

RT: 13.834 min Scan# 1793

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43




Tgt Ion: 65 Resp: 17191


Ion Ratio Lower Upper

65 100

92 71.6 54.1 81.1

138 112.7 77.0 115.4









#47
Dimethylphthalate
Concen: 4.616 ng/ul
RT: 14.204 min Scan# 1856
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:163 Resp: 110854
Ion Ratio Lower Upper
163 100
194 3.5 3.4 5.0
164 10.5 7.7 11.5



#48
2,6-Dinitrotoluene
Concen: 4.103 ng/ul
RT: 14.322 min Scan# 1876
Delta R.T. -0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:165 Resp: 14456
Ion Ratio Lower Upper
165 100
89 70.4 50.6 75.8
121 25.7 17.9 26.9









#50
Acenaphthylene
Concen: 4.486 ng/ul
RT: 14.475 min Scan# 1902
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:152 Resp: 146503
Ion Ratio Lower Upper
152 100
151 20.3 16.0 24.0
153 13.1 10.7 16.1



#51
3-Nitroaniline
Concen: 3.606 ng/ul
RT: 14.651 min Scan# 1932
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:138 Resp: 14823
Ion Ratio Lower Upper
138 100
108 17.1 8.6 12.8#
92 113.7 92.9 139.3









#52
Acenaphthene
Concen: 4.686 ng/ul
RT: 14.816 min Scan# 1960
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:153 Resp: 97795
Ion Ratio Lower Upper
153 100
152 47.4 38.4 57.6
154 86.7 69.7 104.5



#53
2,4-Dinitrophenol
Concen: 3.010 ng/ul
RT: 14.851 min Scan# 1966
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:184 Resp: 4826
Ion Ratio Lower Upper
184 100
63 73.7 55.9 83.9
154 65.4 53.1 79.7









#55
4-Nitrophenol
Concen: 3.921 ng/ul
RT: 14.945 min Scan# 1982
Delta R.T. -0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:109 Resp: 12891
Ion Ratio Lower Upper
109 100
139 130.4 100.1 150.1
65 130.9 104.6 157.0



#56
Dibenzofuran
Concen: 4.774 ng/ul
RT: 15.151 min Scan# 2017
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:168 Resp: 140936
Ion Ratio Lower Upper
168 100
139 38.5 31.1 46.7









#57
2,4-Dinitrotoluene
Concen: 4.173 ng/ul
RT: 15.104 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:165 Resp: 20264
Ion Ratio Lower Upper
165 100
63 47.5 36.3 54.5
182 2.3 2.3 3.5#



#58
2,3,4,6-Tetrachlorophenol
Concen: 3.979 ng/ul
RT: 15.369 min Scan# 2054
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:232 Resp: 17929
Ion Ratio Lower Upper
232 100
131 52.0 38.5 57.7
130 2.9 2.2 3.2
166 36.8 25.8 38.8









#59
 Diethylphthalate
 Concen: 4.487 ng/ul
 RT: 15.569 min Scan# 2088
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231


Tgt Ion:149 Resp: 108099
 Ion Ratio Lower Upper
 149 100
 177 22.7 17.8 26.8
 150 13.0 10.5 15.7



#61
 Fluorene
 Concen: 4.838 ng/ul
 RT: 15.798 min Scan# 2127
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:166 Resp: 112845
 Ion Ratio Lower Upper
 166 100
 165 96.3 77.7 116.5
 167 13.1 11.1 16.7









#62
4-Chlorophenyl-phenylether
Concen: 4.835 ng/ul
RT: 15.792 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:204 Resp: 51863
Ion Ratio Lower Upper
204 100
206 34.6 26.7 40.1
141 64.4 50.2 75.2



#63
4-Nitroaniline
Concen: 3.932 ng/ul
RT: 15.810 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:138 Resp: 14741
Ion Ratio Lower Upper
138 100
92 56.3 41.0 61.6
108 75.5 65.3 97.9









#66
 4,6-Dinitro-2-methylphenol
 Concen: 2.879 ng/ul
 RT: 15.863 min Scan# 2138
 Delta R.T. -0.006 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231


Tgt Ion:198 Resp: 7772
 Ion Ratio Lower Upper
 198 100
 182 9.1 3.0 4.4#
 77 32.6 20.1 30.1#



#67
 N-Nitrosodiphenylamine
 Concen: 4.433 ng/ul
 RT: 16.004 min Scan# 2162
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:169 Resp: 96269
 Ion Ratio Lower Upper
 169 100
 168 68.9 52.4 78.6
 167 36.8 27.5 41.3









#68
4-Bromophenyl-phenylether
Concen: 4.219 ng/ul
RT: 16.692 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:248 Resp: 29253
Ion Ratio Lower Upper
248 100
250 92.4 77.8 116.8
141 80.0 62.6 93.8



#69
Hexachlorobenzene
Concen: 4.387 ng/ul
RT: 16.792 min Scan# 2296
Delta R.T. -0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:284 Resp: 35397
Ion Ratio Lower Upper
284 100
142 41.5 27.8 41.8
249 28.1 25.7 38.5









#70
Atrazine
Concen: 3.994 ng/ul
RT: 16.951 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:200 Resp: 29562
Ion Ratio Lower Upper
200 100
173 28.5 20.5 30.7
215 46.3 38.9 58.3



#71
Pentachlorophenol
Concen: 3.179 ng/ul
RT: 17.145 min Scan# 2356
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:266 Resp: 13361
Ion Ratio Lower Upper
266 100
264 59.9 50.2 75.2
268 55.3 49.3 73.9









#72
Phenanthrene
Concen: 4.701 ng/ul
RT: 17.545 min Scan# 2424
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:178 Resp: 183790
Ion Ratio Lower Upper
178 100
179 15.4 12.2 18.4
176 18.0 15.2 22.8



#74
Anthracene
Concen: 4.541 ng/ul
RT: 17.634 min Scan# 2439
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:178 Resp: 180138
Ion Ratio Lower Upper
178 100
179 16.2 13.0 19.4
176 18.9 15.5 23.3









#75
 1,2,3,4-Tetrachlorobenzene
 Concen: 3.987 ng/uL
 RT: 13.551 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SST005231


Tgt Ion:	216	Resp:	42421
Ion Ratio	Lower	Upper	
216	100		
214	83.0	63.2	94.8
218	50.7	37.9	56.9

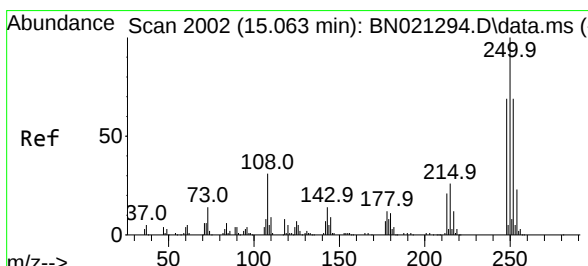

#76
 Pentachlorobenzene
 Concen: 4.535 ng/uL
 RT: 15.063 min Scan# 2002
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:	250	Resp:	43729
Ion Ratio	Lower	Upper	
250	100		
248	59.7	53.0	79.4
252	62.0	53.4	80.2









#77
 Carbazole
 Concen: 4.705 ng/ul
 RT: 17.904 min Scan# 2485
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231


Tgt Ion:167 Resp: 170311
 Ion Ratio Lower Upper
 167 100
 166 21.5 16.1 24.1
 139 12.7 10.2 15.2



#78
 Di-n-butylphthalate
 Concen: 3.819 ng/ul
 RT: 18.475 min Scan# 2582
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:149 Resp: 167682
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.1 10.7
 104 5.6 4.1 6.1









#80
Fluoranthene
Concen: 4.063 ng/u1
RT: 19.557 min Scan# 2766
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:202 Resp: 204009
Ion Ratio Lower Upper
202 100
101 13.2 8.9 13.3
100 10.1 6.7 10.1#



#82
Pyrene
Concen: 4.299 ng/u1
RT: 19.922 min Scan# 2828
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:202 Resp: 223262
Ion Ratio Lower Upper
202 100
101 15.3 9.7 14.5#
100 12.8 8.0 12.0#









#83
Butylbenzylphthalate
Concen: 3.186 ng/ul
RT: 20.827 min Scan# 2981
Delta R.T. 0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:149 Resp: 64432
Ion Ratio Lower Upper
149 100
91 72.9 58.8 88.2
206 19.0 18.1 27.1



#84
3,3'-Dichlorobenzidine
Concen: 4.116 ng/ul
RT: 21.610 min Scan# 3115
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:252 Resp: 64012
Ion Ratio Lower Upper
252 100
254 60.7 50.8 76.2
126 12.4 8.2 12.4#









#85
 Benzo(a)anthracene
 Concen: 4.488 ng/ul
 RT: 21.680 min Scan# 3127
 Delta R.T. 0.000 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43




Instrument :
 BNA_N
 ClientSampleId :
 SSTD005231


Tgt Ion:228 Resp: 218684
 Ion Ratio Lower Upper
 228 100
 229 20.1 16.3 24.5
 226 29.2 23.2 34.8



#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.646 ng/ul
 RT: 21.610 min Scan# 3115
 Delta R.T. 0.006 min
 Lab File: BN021292.D
 Acq: 19 Aug 2022 11:43

Tgt Ion:149 Resp: 117038
 Ion Ratio Lower Upper
 149 100
 167 26.9 22.5 33.7
 279 3.4 3.5 5.3#









#87
Chrysene
Concen: 4.655 ng/ul
RT: 21.733 min Scan# 3136
Delta R.T. 0.000 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43




Instrument :
BNA_N
ClientSampleId :
SSTD005231


Tgt Ion:228 Resp: 219627
Ion Ratio Lower Upper
228 100
226 28.5 24.2 36.2
229 18.2 16.2 24.2



#89
Di-n-octyl phthalate
Concen: 3.235 ng/ul
RT: 22.586 min Scan# 3281
Delta R.T. 0.006 min
Lab File: BN021292.D
Acq: 19 Aug 2022 11:43

Tgt Ion:149 Resp: 194821





#90

Benzo(b)fluoranthene

Concen: 4.402 ng/ul

RT: 23.451 min Scan# 3428

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Instrument :

BNA_N

ClientSampleId :

SSTD005231





Tgt Ion:252 Resp: 243310

Ion Ratio Lower Upper

252 100

253 22.1 16.5 24.7

125 11.9 7.8 11.8#



#91

Benzo(k)fluoranthene

Concen: 4.361 ng/ul

RT: 23.504 min Scan# 3437

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43




Tgt Ion:252 Resp: 222196


Ion Ratio Lower Upper

252 100

253 22.3 18.2 27.4

125 12.3 8.2 12.4





#93

Benzo(a)pyrene

Concen: 4.334 ng/ul

RT: 24.121 min Scan# 3542

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Instrument :

BNA_N

ClientSampleId :

SSTD005231





Tgt Ion:252 Resp: 230437

Ion Ratio Lower Upper

252 100

253 22.6 18.7 28.1

125 13.9 9.2 13.8#



#94

Indeno(1,2,3-cd)pyrene

Concen: 4.436 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. 0.006 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43




Tgt Ion:276 Resp: 278943


Ion Ratio Lower Upper

276 100

138 26.4 19.5 29.3

277 23.3 21.4 32.0





#95

Dibenzo(a,h)anthracene

Concen: 4.535 ng/ul

RT: 26.939 min Scan# 4022

Delta R.T. -0.006 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Instrument :

BNA_N

ClientSampleId :

SSTD005231





Tgt Ion:278 Resp: 243227

Ion Ratio Lower Upper

278 100

139 18.5 13.8 20.8

279 24.3 18.3 27.5



#96

Benzo(g,h,i)perylene

Concen: 4.550 ng/ul

RT: 27.739 min Scan# 4157

Delta R.T. 0.000 min

Lab File: BN021292.D

Acq: 19 Aug 2022 11:43

Tgt Ion:276 Resp: 248826

Ion Ratio Lower Upper

276 100

138 25.0 17.0 25.6

277 21.2 17.8 26.6

