

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081922\
 Data File : BN021293.D
 Acq On : 19 Aug 2022 12:20
 Operator : CG/JU
 Sample : SSTD01024
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232

Quant Time: Aug 19 15:38:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 15:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	84424	20.000	ng/u1	0.00
20) Naphthalene-d8	10.934	136	389051	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.751	164	254403	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.504	188	529102	20.000	ng/u1	0.00
79) Chrysene-d12	21.692	240	587804	20.000	ng/u1	0.00
88) Perylene-d12	24.233	264	626169	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	9199	4.021	ng/uL	0.00
4) Pyridine-d5	3.817	84	57213	9.479	ng/u1	0.00
7) Phenol-d5	7.240	99	69287	9.696	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	46994	10.954	ng/u1	0.00
11) 2-Chlorophenol-d4	7.616	132	53066	9.720	ng/u1	0.00
15) 4-Methylphenol-d8	8.805	113	54648	10.372	ng/u1	0.00
21) Nitrobenzene-d5	9.269	128	24654	9.820	ng/u1	0.00
24) 2-Nitrophenol-d4	9.999	143	19791	9.167	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	49641	9.314	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	88576	10.782	ng/u1	0.00
46) Dimethylphthalate-d6	14.157	166	169785	10.032	ng/u1	0.00
49) Acenaphthylene-d8	14.445	160	203034	9.731	ng/u1	0.00
54) 4-Nitrophenol-d4	14.934	143	26007	8.889	ng/u1	0.00
60) Fluorene-d10	15.745	176	152473	10.229	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	13863	7.716	ng/u1	0.00
73) Anthracene-d10	17.598	188	240453	10.307	ng/u1	0.00
81) Pyrene-d10	19.892	212	269543	9.011	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.063	264	296157	9.647	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.417	88	9831	4.008	ng/uL	90
5) Pyridine	3.834	79	58226	9.626	ng/u1	92
6) Benzaldehyde	7.222	77	34354	11.154	ng/u1	93
8) Phenol	7.263	94	74062	10.167	ng/u1	94
10) Bis(2-Chloroethyl)ether	7.510	93	63188	10.714	ng/u1	96
12) 2-Chlorophenol	7.652	128	58049	10.024	ng/u1	93
13) 2-Methylphenol	8.540	108	55104	10.114	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.634	45	80245	11.064	ng/u1	97
16) Acetophenone	8.928	105	97143	11.812	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.910	70	46872	11.537	ng/u1	95
18) 4-Methylphenol	8.869	108	61872	10.787	ng/u1	97
19) Hexachloroethane	9.193	117	23547	9.720	ng/u1	91
22) Nitrobenzene	9.316	77	63010	10.099	ng/u1	99
23) Isophorone	9.840	82	130700	10.005	ng/u1	98
25) 2-Nitrophenol	10.034	139	23632	9.230	ng/u1	95
26) 2,4-Dimethylphenol	10.093	107	67627	9.999	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.334	93	85104	10.411	ng/u1	99
29) 2,4-Dichlorophenol	10.569	162	52475	9.627	ng/u1	100
30) Naphthalene	10.981	128	210551	10.567	ng/u1	98
32) 4-Chloroaniline	11.093	127	93619	11.140	ng/u1	99
33) Hexachlorobutadiene	11.269	225	32372	9.759	ng/u1	98
34) Caprolactam	11.840	113	16646	9.340	ng/u1	89
35) 4-Chloro-3-methylphenol	12.204	107	58480	10.245	ng/u1	98
36) 2-Methylnaphthalene	12.587	142	139442	10.686	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081922\
 Data File : BN021293.D
 Acq On : 19 Aug 2022 12:20
 Operator : CG/JU
 Sample : SSTD01024
 Misc :
 ALS Vial : 3 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232


Quant Time: Aug 19 15:38:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 15:36:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.804	142	141534	10.842	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.945	216	65918	9.404	ng/ul	96
40) Hexachlorocyclopentadiene	12.928	237	36037	8.316	ng/ul	92
41) 2,4,6-Trichlorophenol	13.187	196	37513	8.950	ng/ul	88
42) 2,4,5-Trichlorophenol	13.257	196	39858	8.748	ng/ul	98
43) 1,1'-Biphenyl	13.592	154	189665	9.803	ng/ul	99
44) 2-Chloronaphthalene	13.634	162	143947	9.867	ng/ul	99
45) 2-Nitroaniline	13.834	65	29520	9.777	ng/ul	91
47) Dimethylphthalate	14.204	163	178498	10.224	ng/ul	98
48) 2,6-Dinitrotoluene	14.322	165	25257	9.861	ng/ul	97
50) Acenaphthylene	14.475	152	239021	10.068	ng/ul	99
51) 3-Nitroaniline	14.651	138	24912	8.336	ng/ul#	94
52) Acenaphthene	14.816	153	156947	10.345	ng/ul	99
53) 2,4-Dinitrophenol	14.851	184	8666	7.434	ng/ul	94
55) 4-Nitrophenol	14.951	109	22888	9.576	ng/ul	93
56) Dibenzofuran	15.151	168	223301	10.405	ng/ul	98
57) 2,4-Dinitrotoluene	15.104	165	36574	10.360	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.369	232	30838	9.415	ng/ul	96
59) Diethylphthalate	15.563	149	175918	10.043	ng/ul	97
61) Fluorene	15.798	166	178770	10.543	ng/ul	95
62) 4-Chlorophenyl-phenyle...	15.792	204	83758	10.741	ng/ul	97
63) 4-Nitroaniline	15.810	138	26706	9.799	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.863	198	14722	7.677	ng/ul#	82
67) N-Nitrosodiphenylamine	16.004	169	155035	10.048	ng/ul	99
68) 4-Bromophenyl-phenylether	16.686	248	47065	9.553	ng/ul	97
69) Hexachlorobenzene	16.792	284	56797	9.908	ng/ul	93
70) Atrazine	16.951	200	49857	9.480	ng/ul	95
71) Pentachlorophenol	17.145	266	22994	7.700	ng/ul	94
72) Phenanthrene	17.545	178	292112	10.515	ng/ul	97
74) Anthracene	17.633	178	289281	10.263	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.551	216	69471	9.190	ng/ul	99
76) Pentachlorobenzene	15.063	250	66961	9.773	ng/ul	96
77) Carbazole	17.904	167	270949	10.536	ng/ul	97
78) Di-n-butylphthalate	18.475	149	277273	8.889	ng/ul	99
80) Fluoranthene	19.557	202	327613	8.889	ng/ul#	92
82) Pyrene	19.922	202	352650	9.249	ng/ul#	95
83) Butylbenzylphthalate	20.822	149	107739	7.257	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.610	252	108267	9.484	ng/ul#	95
85) Benzo(a)anthracene	21.680	228	352756	9.862	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.610	149	188492	8.000	ng/ul	97
87) Chrysene	21.733	228	348997	10.077	ng/ul	98
89) Di-n-octyl phthalate	22.586	149	316800	7.437	ng/ul	100
90) Benzo(b)fluoranthene	23.451	252	381286	9.754	ng/ul#	97
91) Benzo(k)fluoranthene	23.504	252	341667	9.482	ng/ul#	95
93) Benzo(a)pyrene	24.121	252	374541	9.961	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.915	276	443103	9.962	ng/ul	97
95) Dibenzo(a,h)anthracene	26.939	278	381780	10.065	ng/ul	95
96) Benzo(g,h,i)perylene	27.727	276	189828	4.908	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 19 15:38:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 19 15:36:45 2022
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 4.008 ng/uL
 RT: 3.417 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232


Tgt Ion: 88 Resp: 9831
 Ion Ratio Lower Upper
 88 100
 43 30.3 22.4 33.6
 58 66.2 61.0 91.4



#5
 Pyridine
 Concen: 9.626 ng/uL
 RT: 3.834 min Scan# 93
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion: 79 Resp: 58226
 Ion Ratio Lower Upper
 79 100
 52 75.4 65.0 97.4
 51 33.6 31.6 47.4









#6
Benzaldehyde
Concen: 11.154 ng/ul
RT: 7.222 min Scan# 669
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion: 77 Resp: 34354
Ion Ratio Lower Upper
77 100
105 100.0 74.7 112.1
106 94.4 70.2 105.4

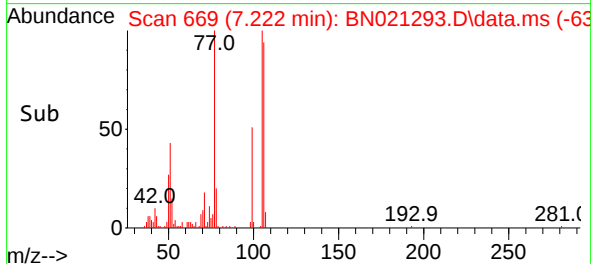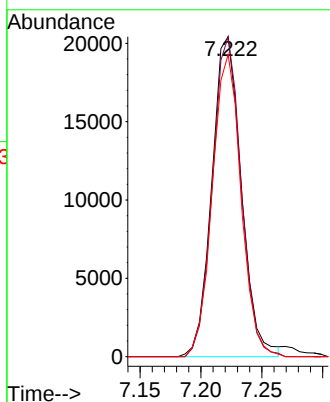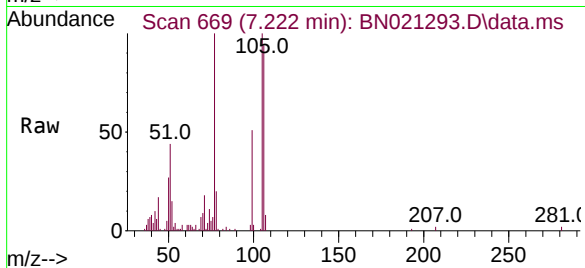

#8
Phenol
Concen: 10.167 ng/ul
RT: 7.263 min Scan# 676
Delta R.T. -0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion: 94 Resp: 74062
Ion Ratio Lower Upper
94 100
65 26.6 23.6 35.4
66 34.8 31.2 46.8



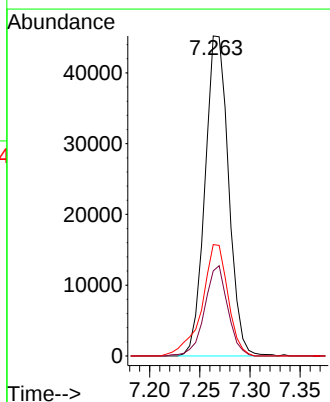
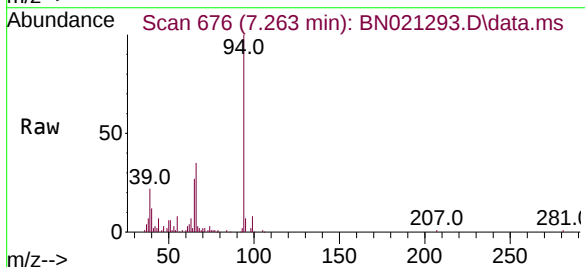




#10
Bis(2-Chloroethyl)ether
Concen: 10.714 ng/ul
RT: 7.510 min Scan# 718
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion: 93 Resp: 63188
Ion Ratio Lower Upper
93 100
63 74.8 63.4 95.0
95 32.4 26.2 39.2

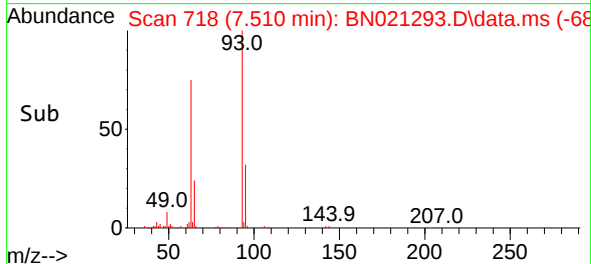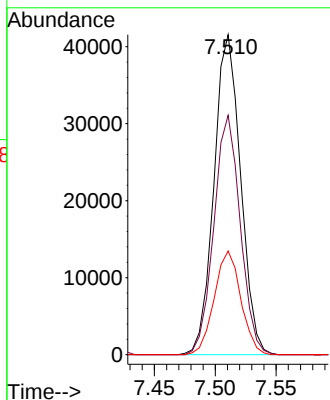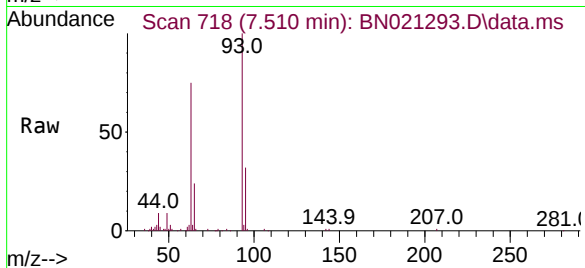

#12
2-Chlorophenol
Concen: 10.024 ng/ul
RT: 7.652 min Scan# 742
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:128 Resp: 58049
Ion Ratio Lower Upper
128 100
64 42.0 38.6 57.8
130 32.6 25.0 37.4

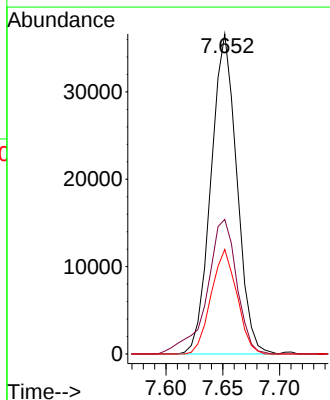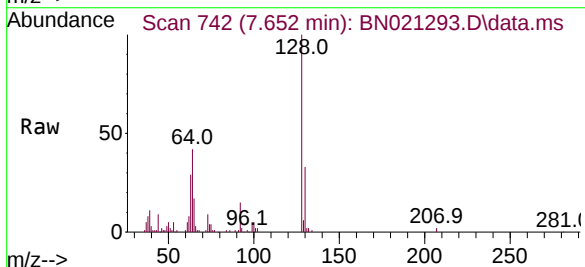



#13

2-Methylphenol

Concen: 10.114 ng/ul

RT: 8.540 min Scan# 893

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Instrument :

BNA_N

ClientSampleId :





SSTD010232

Tgt Ion:108 Resp: 55104

Ion Ratio Lower Upper

108 100

107 88.9 71.5 107.3

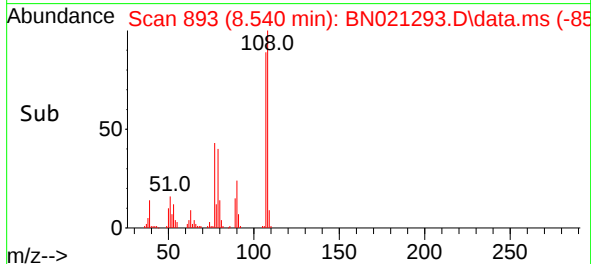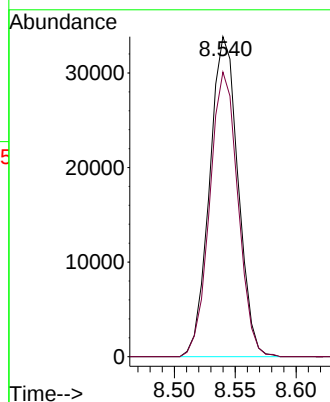

#14

2,2'-oxybis(1-Chloropropane)

Concen: 11.064 ng/ul

RT: 8.634 min Scan# 909

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20




Tgt Ion: 45 Resp: 80245


Ion Ratio Lower Upper

45 100

77 14.8 10.9 16.3

79 11.6 8.6 13.0



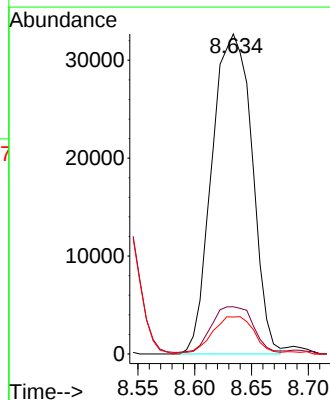





#16
Acetophenone
Concen: 11.812 ng/ul
RT: 8.928 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:105 Resp: 97143
Ion Ratio Lower Upper
105 100
77 79.2 63.5 95.3
51 25.7 23.5 35.3

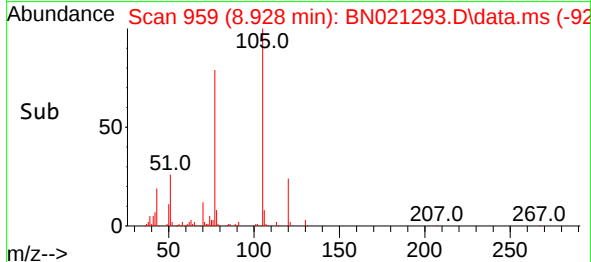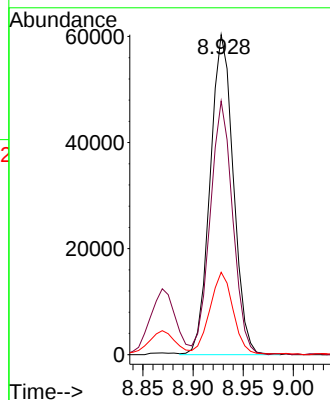

#17
N-Nitroso-di-n-propylamine
Concen: 11.537 ng/ul
RT: 8.910 min Scan# 956
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion: 70 Resp: 46872
Ion Ratio Lower Upper
70 100
42 55.5 47.8 71.6
101 10.2 7.8 11.6
130 21.4 15.8 23.8


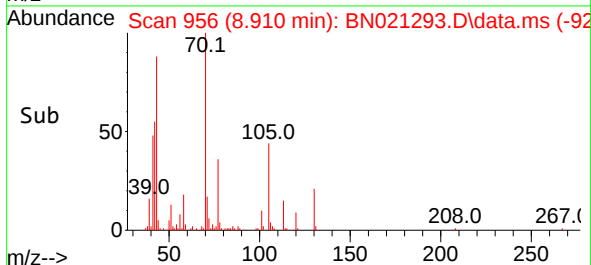
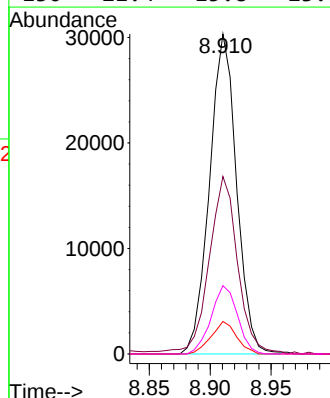
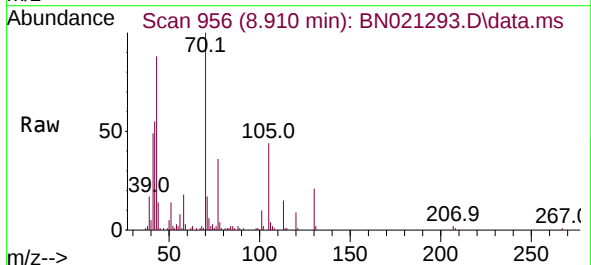




#18
4-Methylphenol
Concen: 10.787 ng/ul
RT: 8.869 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:108 Resp: 61872
Ion Ratio Lower Upper
108 100
107 112.9 88.0 132.0

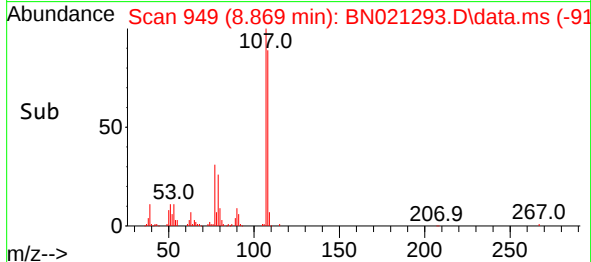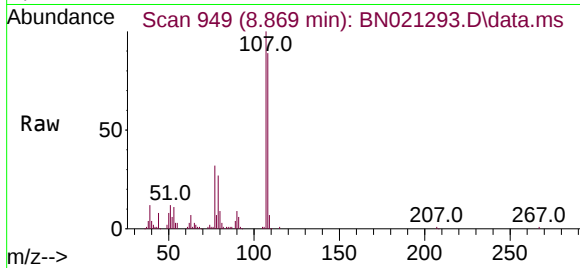

#19
Hexachloroethane
Concen: 9.720 ng/ul
RT: 9.193 min Scan# 1004
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:117 Resp: 23547
Ion Ratio Lower Upper
117 100
201 95.6 83.2 124.8
199 54.4 50.2 75.4




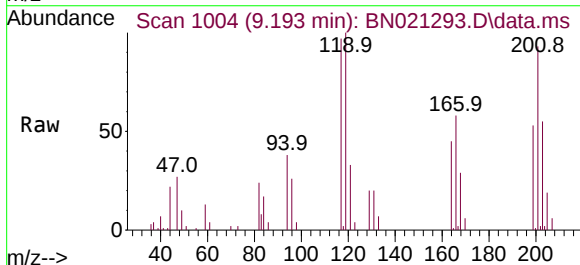




#22
Nitrobenzene
Concen: 10.099 ng/ul
RT: 9.316 min Scan# 1025
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion: 77 Resp: 63010
Ion Ratio Lower Upper
77 100
123 43.4 34.5 51.7
65 12.9 11.1 16.7

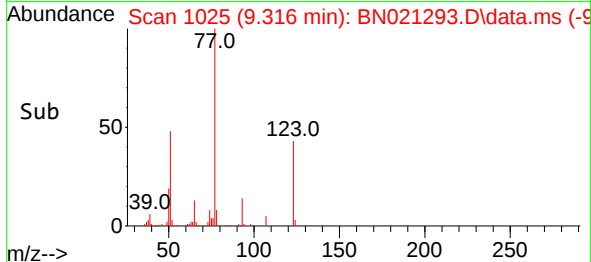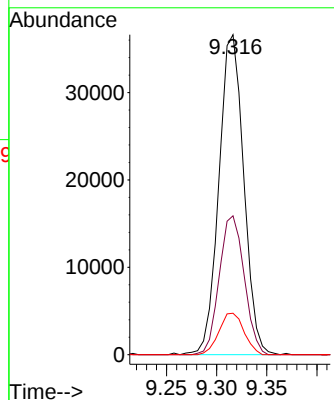

#23
Isophorone
Concen: 10.005 ng/ul
RT: 9.840 min Scan# 1114
Delta R.T. -0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion: 82 Resp: 130700
Ion Ratio Lower Upper
82 100
95 6.8 5.8 8.8
138 16.6 13.8 20.8



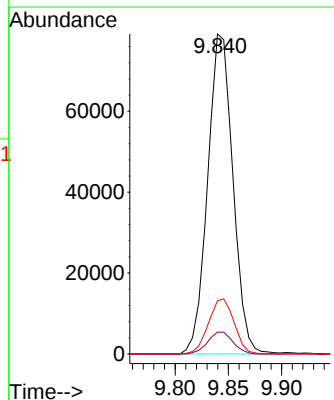
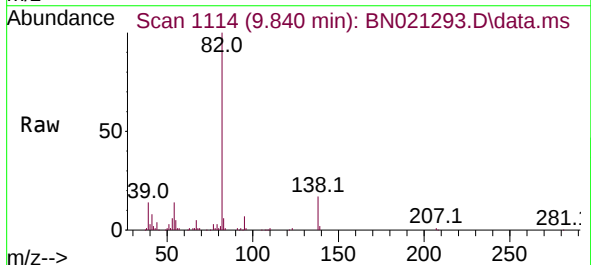


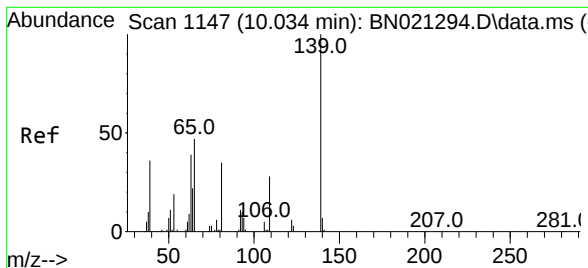

#25
2-Nitrophenol
Concen: 9.230 ng/ul
RT: 10.034 min Scan# 1147
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:139 Resp: 23632
Ion Ratio Lower Upper
139 100
65 51.1 43.7 65.5
109 29.0 25.8 38.6

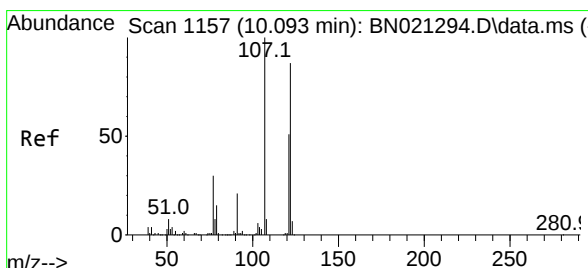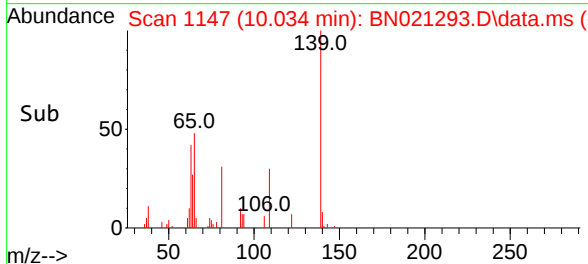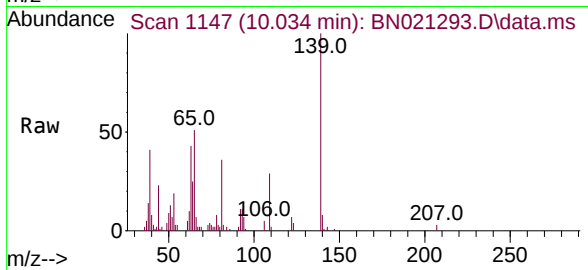

#26
2,4-Dimethylphenol
Concen: 9.999 ng/ul
RT: 10.093 min Scan# 1157
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:107 Resp: 67627
Ion Ratio Lower Upper
107 100
121 52.4 38.3 57.5
122 86.4 66.3 99.5


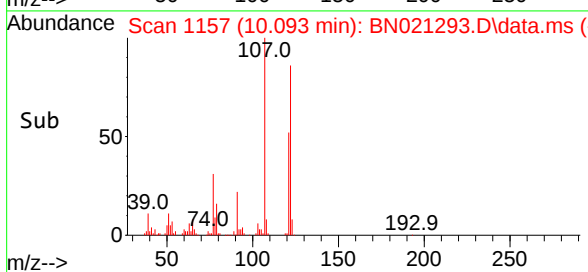

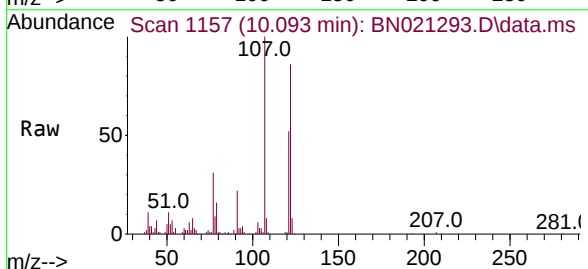




#27
 Bis(2-Chloroethoxy)methane
 Concen: 10.411 ng/ul
 RT: 10.334 min Scan# 1198
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SST010232


Tgt Ion: 93 Resp: 85104
 Ion Ratio Lower Upper
 93 100
 95 32.0 25.4 38.0
 123 11.4 8.3 12.5

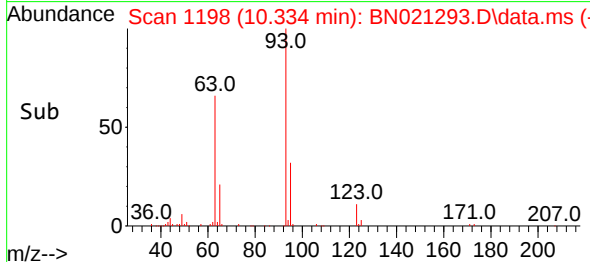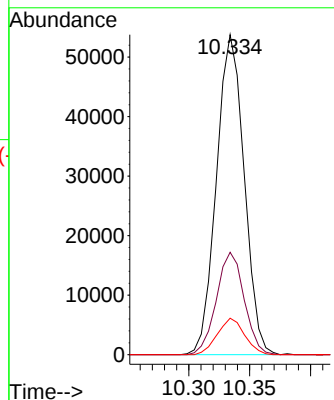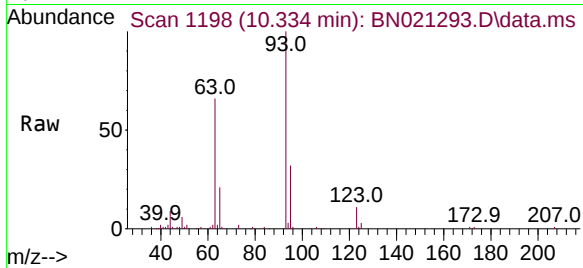

#29
 2,4-Dichlorophenol
 Concen: 9.627 ng/ul
 RT: 10.569 min Scan# 1238
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion: 162 Resp: 52475
 Ion Ratio Lower Upper
 162 100
 164 65.8 52.9 79.3
 98 36.9 29.8 44.8



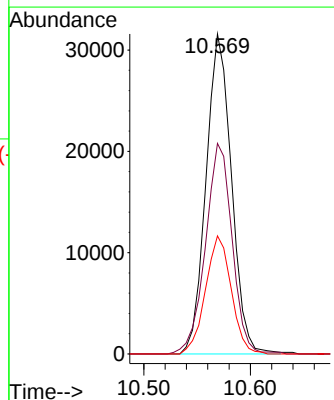
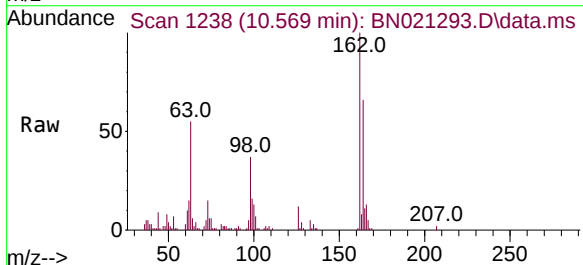




#30
Naphthalene
Concen: 10.567 ng/ul
RT: 10.981 min Scan# 1308
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:128 Resp: 210551
Ion Ratio Lower Upper
128 100
129 10.7 8.7 13.1
127 12.3 10.6 16.0

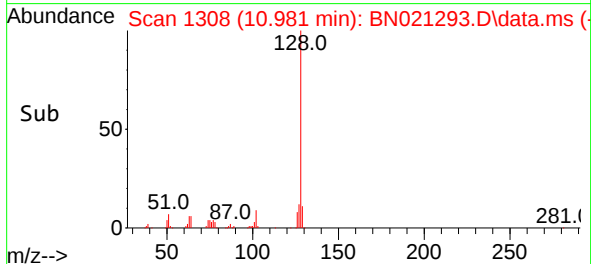

#32
4-Chloroaniline
Concen: 11.140 ng/ul
RT: 11.093 min Scan# 1327
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:127 Resp: 93619
Ion Ratio Lower Upper
127 100
129 32.9 26.1 39.1


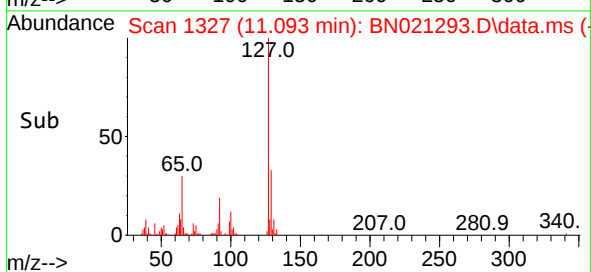

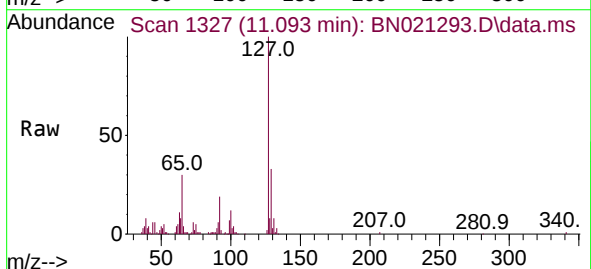




#33
Hexachlorobutadiene
Concen: 9.759 ng/ul
RT: 11.269 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:225 Resp: 32372
Ion Ratio Lower Upper
225 100
223 62.1 51.8 77.6
227 62.5 50.6 76.0

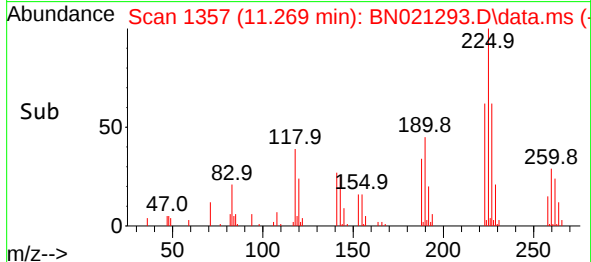

#34
Caprolactam
Concen: 9.340 ng/ul
RT: 11.840 min Scan# 1454
Delta R.T. -0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:113 Resp: 16646
Ion Ratio Lower Upper
113 100
55 164.4 145.5 218.3
56 122.8 106.5 159.7




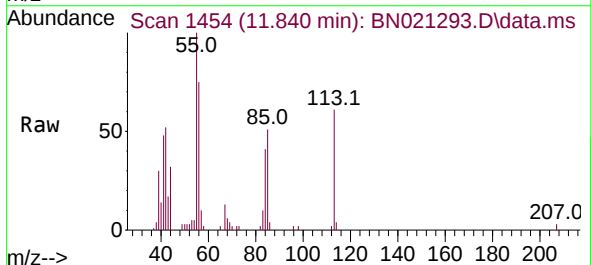




#35
4-Chloro-3-methylphenol
Concen: 10.245 ng/ul
RT: 12.204 min Scan# 1516
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:107 Resp: 58480
Ion Ratio Lower Upper
107 100
144 26.7 20.6 31.0
142 79.1 62.2 93.4



#36
2-Methylnaphthalene
Concen: 10.686 ng/ul
RT: 12.587 min Scan# 1581
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:142 Resp: 139442
Ion Ratio Lower Upper
142 100
141 88.5 70.6 105.8

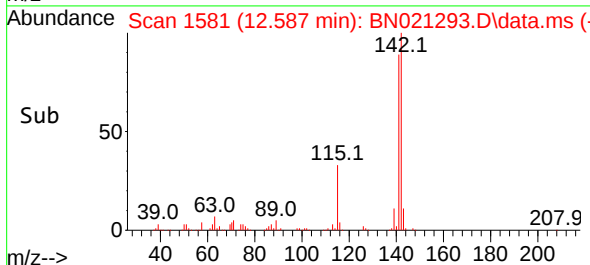



#37

1-Methylnaphthalene

Concen: 10.842 ng/ul

RT: 12.804 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Instrument :

BNA_N

ClientSampleId :

SSTD010232





Tgt Ion:142 Resp: 141534

Ion Ratio Lower Upper

142 100

141 92.1 70.9 106.3

116 3.8 3.1 4.7



#39

1,2,4,5-Tetrachlorobenzene

Concen: 9.404 ng/ul

RT: 12.945 min Scan# 1642

Delta R.T. -0.006 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Tgt Ion:216 Resp: 65918




Ion Ratio Lower Upper


216 100

214 75.3 63.4 95.0

179 20.9 17.8 26.8

108 19.4 15.1 22.7



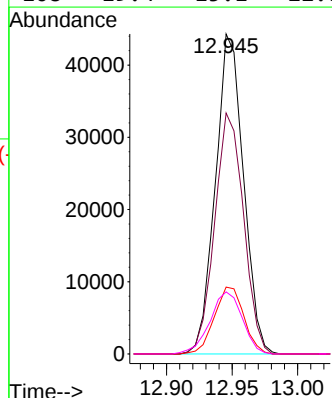





#40
Hexachlorocyclopentadiene
Concen: 8.316 ng/ul
RT: 12.928 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:237	Resp:	36037
Ion Ratio	Lower	Upper
237	100	
235	67.2	48.8 73.2
272	13.7	9.3 13.9

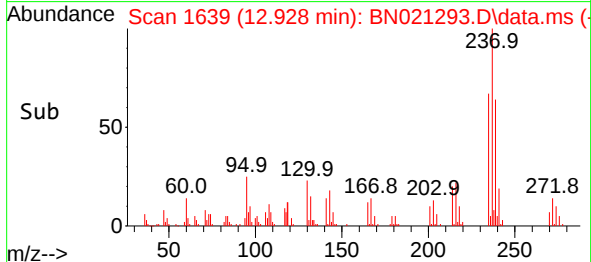

#41
2,4,6-Trichlorophenol
Concen: 8.950 ng/ul
RT: 13.187 min Scan# 1683
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:196	Resp:	37513
Ion Ratio	Lower	Upper
196	100	
198	84.7	79.8 119.8
200	29.0	25.0 37.6




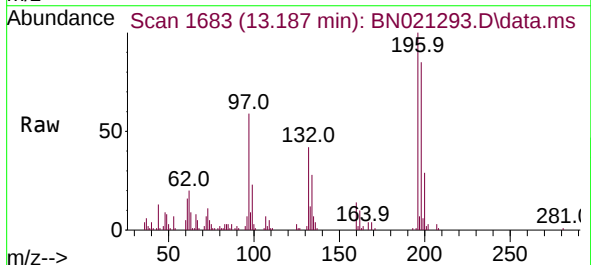




#42
2,4,5-Trichlorophenol
Concen: 8.748 ng/ul
RT: 13.257 min Scan# 1695
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:196 Resp: 39858
Ion Ratio Lower Upper
196 100
198 99.7 77.6 116.4
200 30.8 24.4 36.6

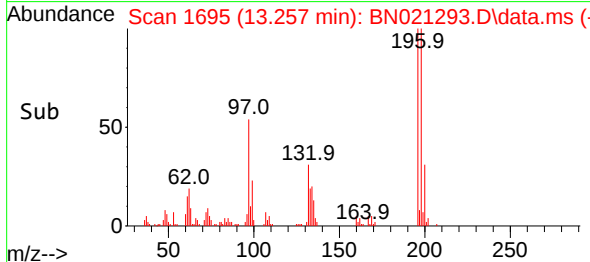

#43
1,1'-Biphenyl
Concen: 9.803 ng/ul
RT: 13.592 min Scan# 1752
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:154 Resp: 189665
Ion Ratio Lower Upper
154 100
153 39.8 31.5 47.3
76 12.6 10.5 15.7

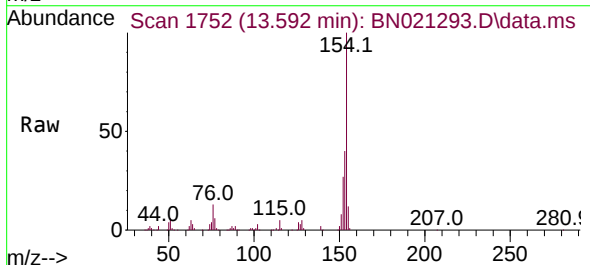



#44

2-Chloronaphthalene

Concen: 9.867 ng/ul

RT: 13.634 min Scan# 1759

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Instrument :

BNA_N

ClientSampleId :

SSTD010232





Tgt Ion:162 Resp: 143947

Ion Ratio Lower Upper

162 100

164 31.4 25.8 38.6

127 38.8 31.4 47.2

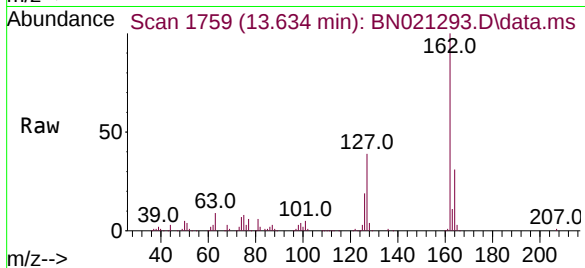

#45

2-Nitroaniline

Concen: 9.777 ng/ul

RT: 13.834 min Scan# 1793

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20




Tgt Ion: 65 Resp: 29520


Ion Ratio Lower Upper

65 100

92 70.8 54.1 81.1

138 107.7 77.0 115.4




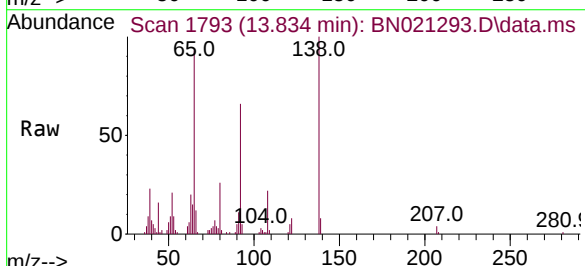




#47
Dimethylphthalate
Concen: 10.224 ng/ul
RT: 14.204 min Scan# 1856
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:163 Resp: 178498
Ion Ratio Lower Upper
163 100
194 3.9 3.4 5.0
164 10.4 7.7 11.5

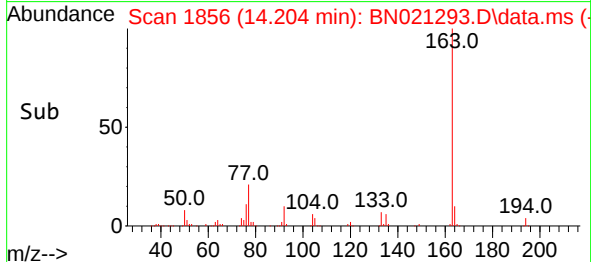

#48
2,6-Dinitrotoluene
Concen: 9.861 ng/ul
RT: 14.322 min Scan# 1876
Delta R.T. -0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:165 Resp: 25257
Ion Ratio Lower Upper
165 100
89 65.7 50.6 75.8
121 24.4 17.9 26.9




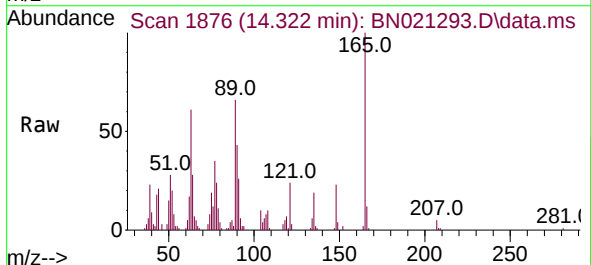




#50
Acenaphthylene
Concen: 10.068 ng/ul
RT: 14.475 min Scan# 1902
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:152 Resp: 239021
Ion Ratio Lower Upper
152 100
151 19.5 16.0 24.0
153 13.4 10.7 16.1

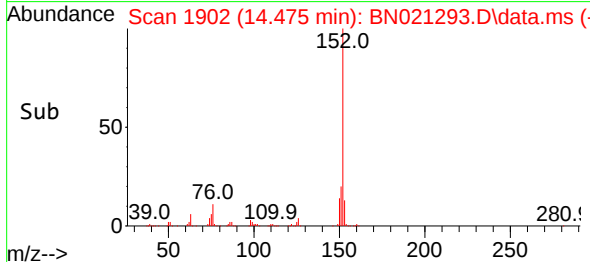

#51
3-Nitroaniline
Concen: 8.336 ng/ul
RT: 14.651 min Scan# 1932
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:138 Resp: 24912
Ion Ratio Lower Upper
138 100
108 16.7 8.6 12.8#
92 122.0 92.9 139.3




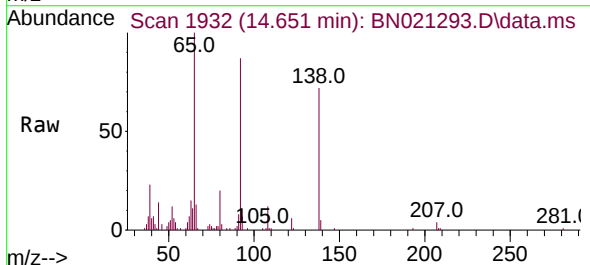




#52
Acenaphthene
Concen: 10.345 ng/ul
RT: 14.816 min Scan# 1960
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:153 Resp: 156947
Ion Ratio Lower Upper
153 100
152 47.0 38.4 57.6
154 87.0 69.7 104.5

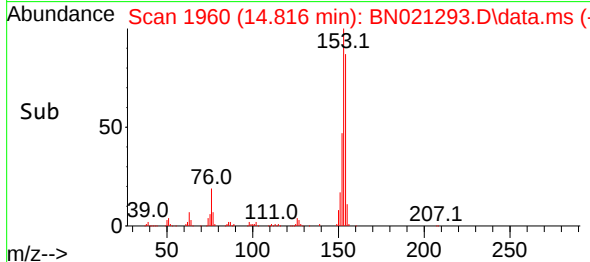

#53
2,4-Dinitrophenol
Concen: 7.434 ng/ul
RT: 14.851 min Scan# 1966
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:184 Resp: 8666
Ion Ratio Lower Upper
184 100
63 75.2 55.9 83.9
154 70.6 53.1 79.7




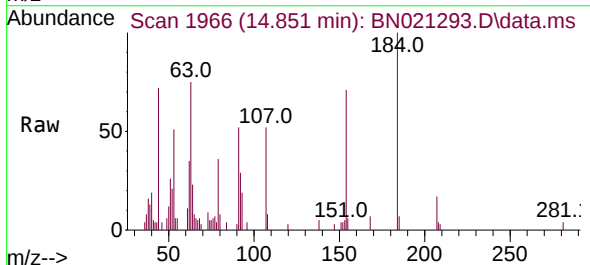




#55
4-Nitrophenol
Concen: 9.576 ng/ul
RT: 14.951 min Scan# 1983
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:109 Resp: 22888
Ion Ratio Lower Upper
109 100
139 138.2 100.1 150.1
65 128.3 104.6 157.0



#56
Dibenzofuran
Concen: 10.405 ng/ul
RT: 15.151 min Scan# 1717
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:168 Resp: 223301
Ion Ratio Lower Upper
168 100
139 37.8 31.1 46.7









#57
2,4-Dinitrotoluene
Concen: 10.360 ng/ul
RT: 15.104 min Scan# 2009
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:165 Resp: 36574
Ion Ratio Lower Upper
165 100
63 48.6 36.3 54.5
182 2.9 2.3 3.5

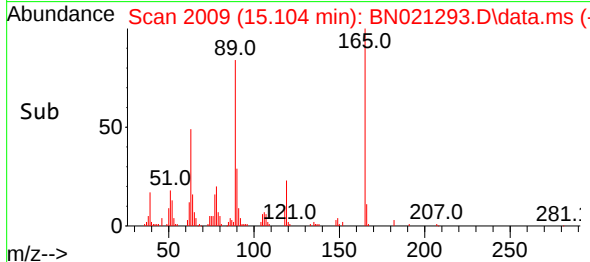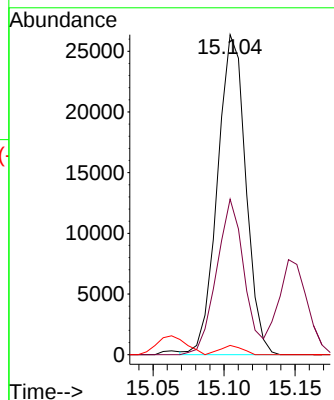

#58
2,3,4,6-Tetrachlorophenol
Concen: 9.415 ng/ul
RT: 15.369 min Scan# 2054
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:232 Resp: 30838
Ion Ratio Lower Upper
232 100
131 51.9 38.5 57.7
130 2.3 2.2 3.2
166 31.4 25.8 38.8



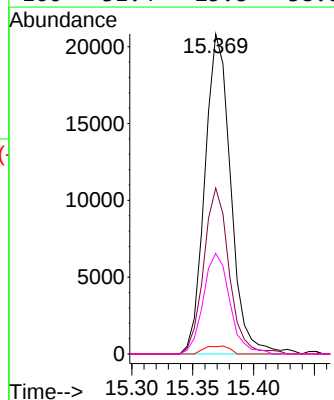
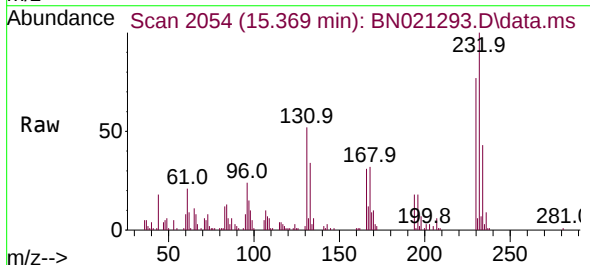




#59
Diethylphthalate
Concen: 10.043 ng/ul
RT: 15.563 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:149 Resp: 175918
Ion Ratio Lower Upper
149 100
177 20.7 17.8 26.8
150 12.2 10.5 15.7

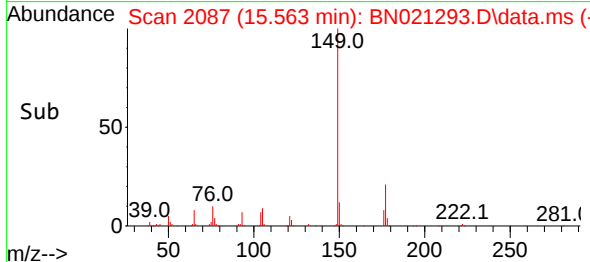

#61
Fluorene
Concen: 10.543 ng/ul
RT: 15.798 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:166 Resp: 178770
Ion Ratio Lower Upper
166 100
165 102.5 77.7 116.5
167 14.3 11.1 16.7




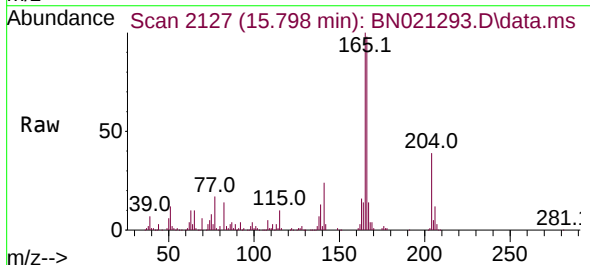




#62
4-Chlorophenyl-phenylether
Concen: 10.741 ng/ul
RT: 15.792 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:204 Resp: 83758
Ion Ratio Lower Upper
204 100
206 30.2 26.7 40.1
141 61.5 50.2 75.2



#63
4-Nitroaniline
Concen: 9.799 ng/ul
RT: 15.810 min Scan# 2129
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:138 Resp: 26706
Ion Ratio Lower Upper
138 100
92 52.1 41.0 61.6
108 75.5 65.3 97.9









#66
 4,6-Dinitro-2-methylphenol
 Concen: 7.677 ng/ul
 RT: 15.863 min Scan# 2138
 Delta R.T. -0.006 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232


Tgt Ion:198 Resp: 14722
 Ion Ratio Lower Upper
 198 100
 182 5.8 3.0 4.4#
 77 35.1 20.1 30.1#

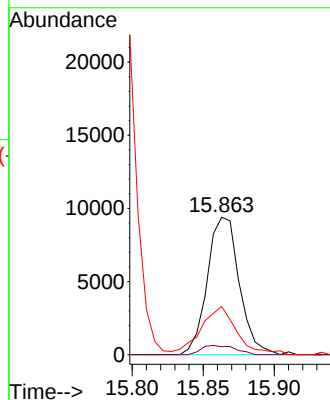

#67
 N-Nitrosodiphenylamine
 Concen: 10.048 ng/ul
 RT: 16.004 min Scan# 2162
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion:169 Resp: 155035
 Ion Ratio Lower Upper
 169 100
 168 65.5 52.4 78.6
 167 35.5 27.5 41.3



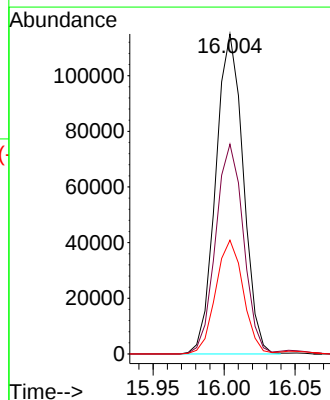





#68
4-Bromophenyl-phenylether
Concen: 9.553 ng/ul
RT: 16.686 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:248 Resp: 47065
Ion Ratio Lower Upper
248 100
250 98.8 77.8 116.8
141 82.0 62.6 93.8



#69
Hexachlorobenzene
Concen: 9.908 ng/ul
RT: 16.792 min Scan# 2296
Delta R.T. -0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:284 Resp: 56797
Ion Ratio Lower Upper
284 100
142 39.8 27.8 41.8
249 29.4 25.7 38.5









#70
 Atrazine
 Concen: 9.480 ng/ul
 RT: 16.951 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232


Tgt Ion:200 Resp: 49857
 Ion Ratio Lower Upper
 200 100
 173 25.7 20.5 30.7
 215 43.4 38.9 58.3

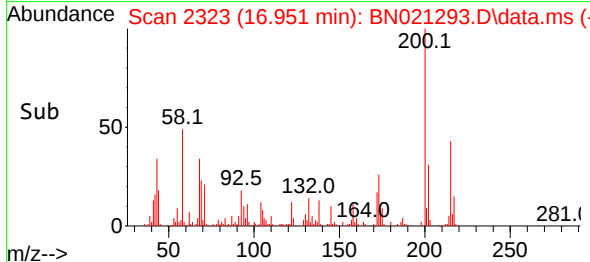

#71
 Pentachlorophenol
 Concen: 7.700 ng/ul
 RT: 17.145 min Scan# 2356
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion:266 Resp: 22994
 Ion Ratio Lower Upper
 266 100
 264 65.9 50.2 75.2
 268 67.2 49.3 73.9




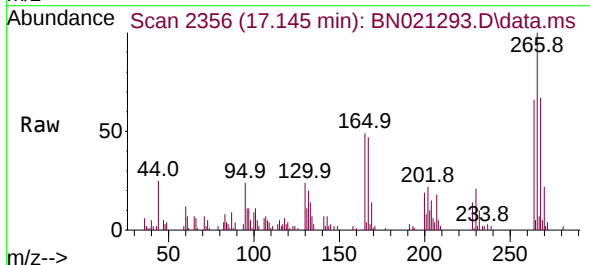


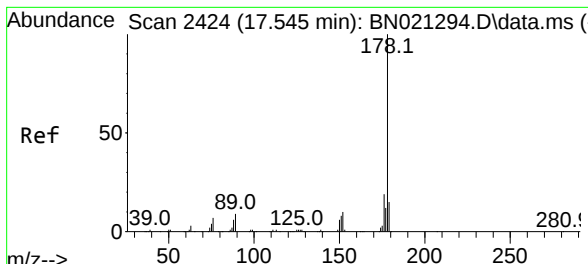

#72
 Phenanthrene
 Concen: 10.515 ng/ul
 RT: 17.545 min Scan# 2424
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232


Tgt Ion:178	Resp:	292112
Ion	Ratio	Lower Upper
178	100	
179	14.2	12.2 18.4
176	17.2	15.2 22.8

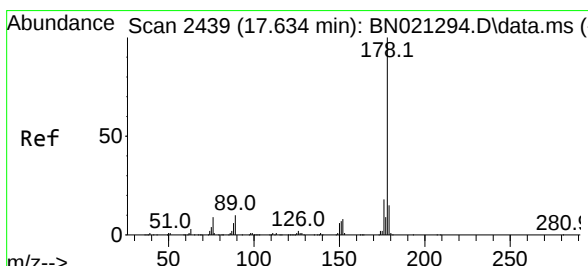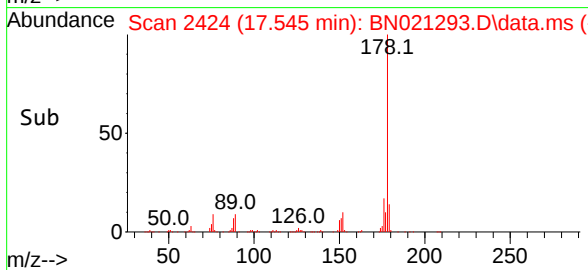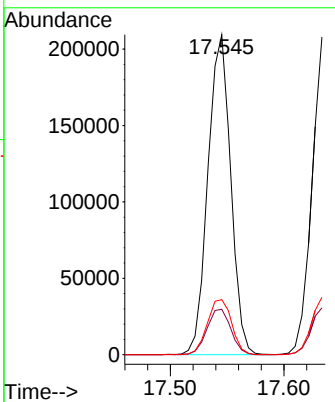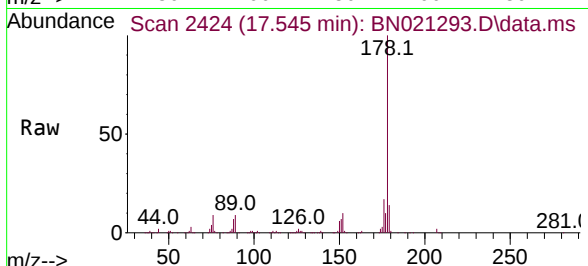

#74
 Anthracene
 Concen: 10.263 ng/ul
 RT: 17.633 min Scan# 2439
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion:178	Resp:	289281
Ion	Ratio	Lower Upper
178	100	
179	14.7	13.0 19.4
176	18.1	15.5 23.3


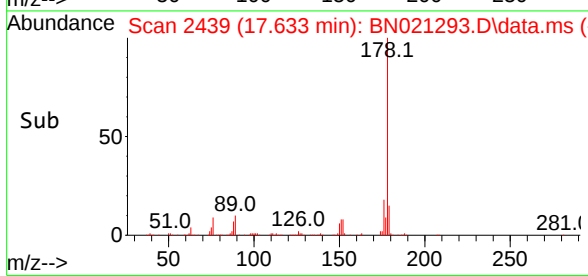
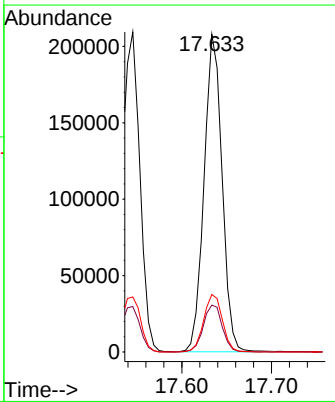
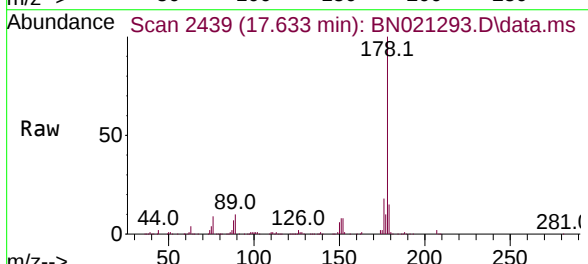


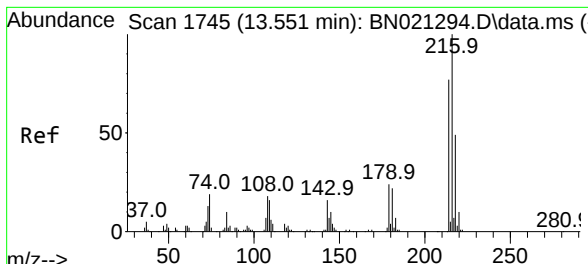

#75
 1,2,3,4-Tetrachlorobenzene
 Concen: 9.190 ng/uL
 RT: 13.551 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SST010232


Tgt Ion:	216	Resp:	69471
Ion Ratio	Lower	Upper	
216	100		
214	79.2	63.2	94.8
218	48.6	37.9	56.9

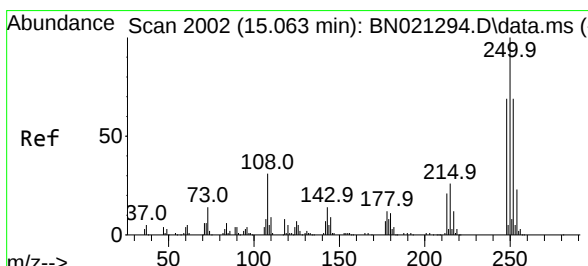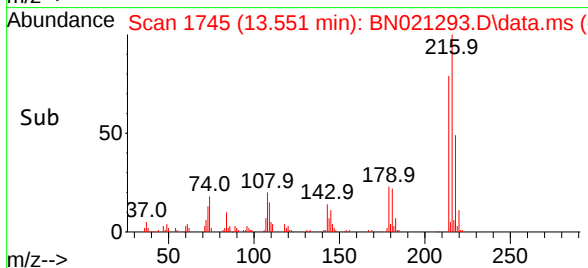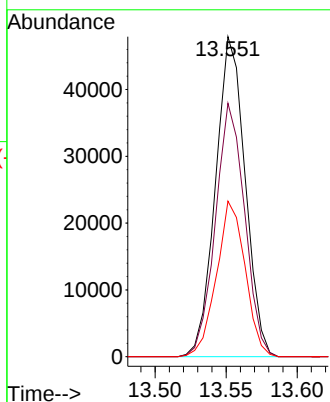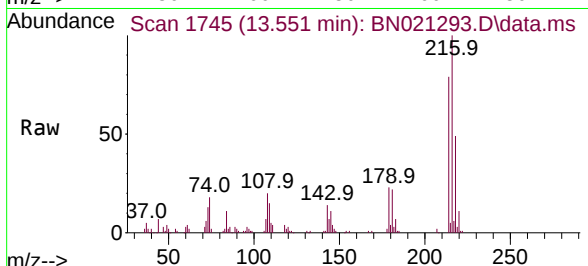

#76
 Pentachlorobenzene
 Concen: 9.773 ng/uL
 RT: 15.063 min Scan# 2002
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion:	250	Resp:	66961
Ion Ratio	Lower	Upper	
250	100		
248	61.4	53.0	79.4
252	65.0	53.4	80.2


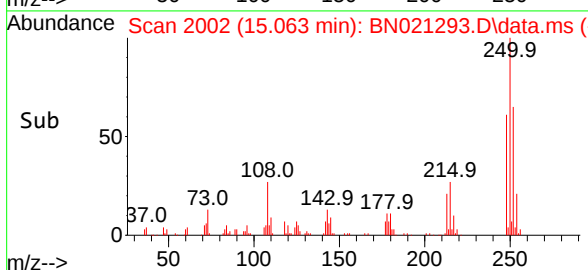
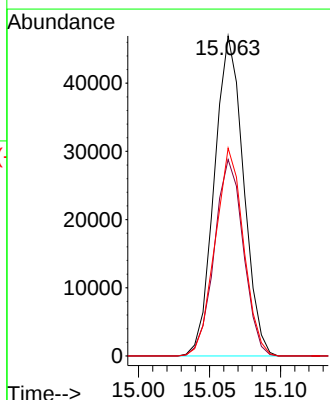
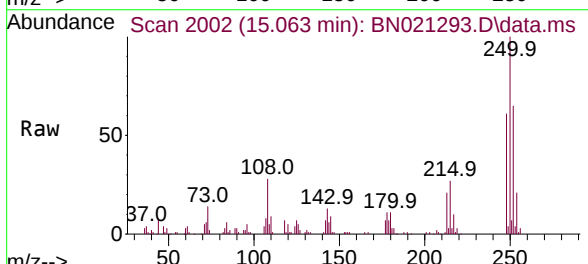




#77
 Carbazole
 Concen: 10.536 ng/ul
 RT: 17.904 min Scan# 2485
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232


Tgt Ion:167 Resp: 270949
 Ion Ratio Lower Upper
 167 100
 166 21.8 16.1 24.1
 139 13.1 10.2 15.2



#78
 Di-n-butylphthalate
 Concen: 8.889 ng/ul
 RT: 18.475 min Scan# 2582
 Delta R.T. -0.000 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion:149 Resp: 277273
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.1 10.7
 104 5.4 4.1 6.1









#80
Fluoranthene
Concen: 8.889 ng/u1
RT: 19.557 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:202 Resp: 327613
Ion Ratio Lower Upper
202 100
101 14.3 8.9 13.3#
100 11.2 6.7 10.1#

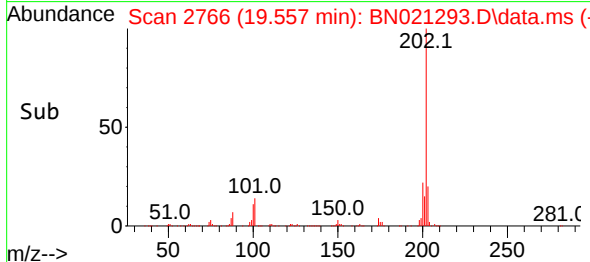

#82
Pyrene
Concen: 9.249 ng/u1
RT: 19.922 min Scan# 2828
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:202 Resp: 352650
Ion Ratio Lower Upper
202 100
101 14.6 9.7 14.5#
100 11.6 8.0 12.0









#83
Butylbenzylphthalate
Concen: 7.257 ng/ul
RT: 20.822 min Scan# 2981
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:149 Resp: 107739
Ion Ratio Lower Upper
149 100
91 79.0 58.8 88.2
206 19.5 18.1 27.1

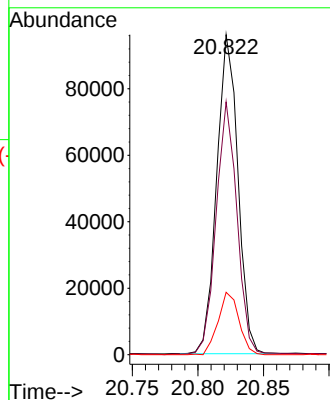

#84
3,3'-Dichlorobenzidine
Concen: 9.484 ng/ul
RT: 21.610 min Scan# 3115
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:252 Resp: 108267
Ion Ratio Lower Upper
252 100
254 66.7 50.8 76.2
126 14.0 8.2 12.4#



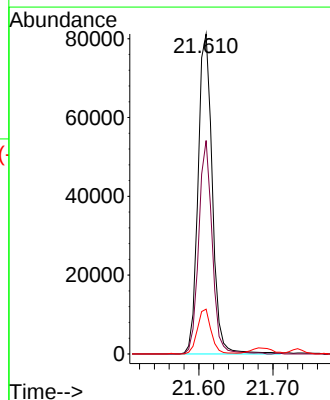





#85
Benzo(a)anthracene
Concen: 9.862 ng/ul
RT: 21.680 min Scan# 3127
Delta R.T. -0.000 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20




Instrument :
BNA_N
ClientSampleId :
SSTD010232


Tgt Ion:228 Resp: 352756
Ion Ratio Lower Upper
228 100
229 20.4 16.3 24.5
226 26.3 23.2 34.8

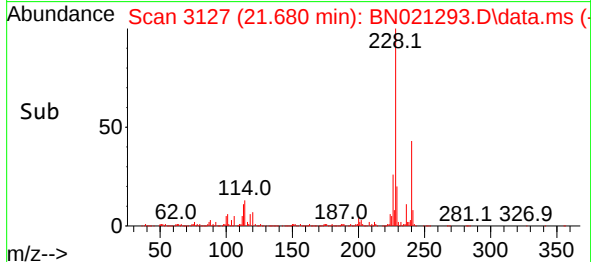

#86
Bis(2-ethylhexyl)phthalate
Concen: 8.000 ng/ul
RT: 21.610 min Scan# 3115
Delta R.T. 0.006 min
Lab File: BN021293.D
Acq: 19 Aug 2022 12:20

Tgt Ion:149 Resp: 188492
Ion Ratio Lower Upper
149 100
167 26.2 22.5 33.7
279 4.0 3.5 5.3

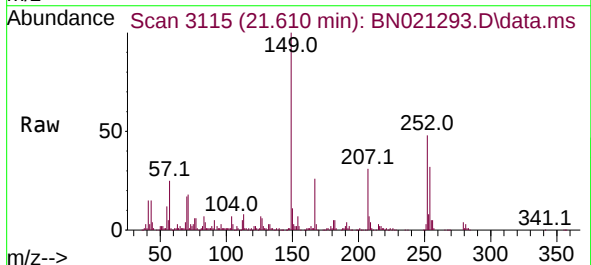



#87

Chrysene

Concen: 10.077 ng/ul

RT: 21.733 min Scan# 31

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Instrument :

BNA_N

ClientSampleId :

SSTD010232





Tgt Ion:228 Resp: 348997

Ion Ratio Lower Upper

228 100

226 28.9 24.2 36.2

229 19.6 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 7.437 ng/ul




RT: 22.586 min Scan# 3281


Delta R.T. 0.006 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Tgt Ion:149 Resp: 316800





#90

Benzo(b)fluoranthene

Concen: 9.754 ng/ul

RT: 23.451 min Scan# 3428

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Instrument :

BNA_N

ClientSampleId :

SSTD010232





Tgt Ion:252 Resp: 381286

Ion Ratio Lower Upper

252 100

253 20.2 16.5 24.7

125 12.6 7.8 11.8#

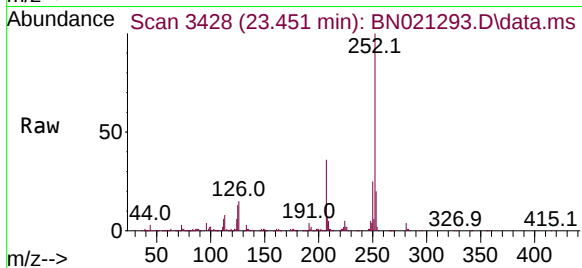

#91

Benzo(k)fluoranthene

Concen: 9.482 ng/ul

RT: 23.504 min Scan# 3437

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20




Tgt Ion:252 Resp: 341667


Ion Ratio Lower Upper

252 100

253 24.3 18.2 27.4

125 13.5 8.2 12.4#

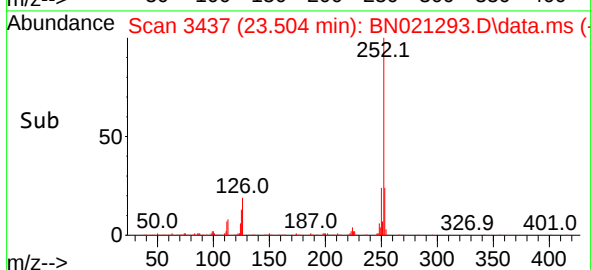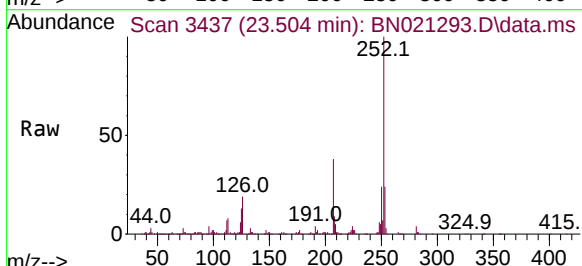



#93

Benzo(a)pyrene

Concen: 9.961 ng/ul

RT: 24.121 min Scan# 3

Delta R.T. -0.000 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20

Instrument :

BNA_N

ClientSampleId :

SSTD010232





Tgt Ion:252 Resp: 374541

Ion Ratio Lower Upper

252 100

253 22.7 18.7 28.1

125 13.0 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 9.962 ng/ul

RT: 26.915 min Scan# 4017

Delta R.T. 0.006 min

Lab File: BN021293.D

Acq: 19 Aug 2022 12:20




Tgt Ion:276 Resp: 443103


Ion Ratio Lower Upper

276 100

138 27.4 19.5 29.3

277 26.5 21.4 32.0


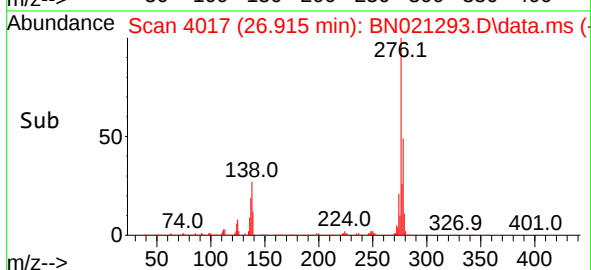






#95
 Dibenzo(a,h)anthracene
 Concen: 10.065 ng/ul
 RT: 26.939 min Scan# 4021
 Delta R.T. -0.006 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010232

Tgt Ion:278 Resp: 381780
 Ion Ratio Lower Upper
 278 100
 139 19.6 13.8 20.8
 279 25.0 18.3 27.5

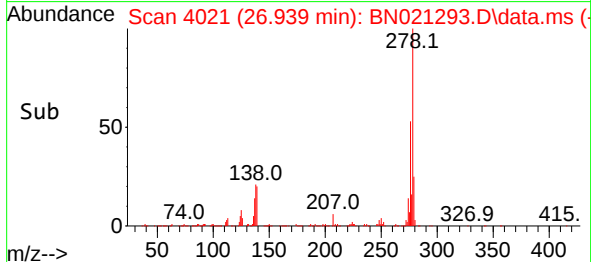

#96
 Benzo(g,h,i)perylene
 Concen: 4.908 ng/ul
 RT: 27.727 min Scan# 4155
 Delta R.T. -0.012 min
 Lab File: BN021293.D
 Acq: 19 Aug 2022 12:20

Tgt Ion:276 Resp: 189828
 Ion Ratio Lower Upper
 276 100
 138 25.6 17.0 25.6#
 277 23.0 17.8 26.6

