


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081924\
Data File : BN033476.D
Acq On : 19 Aug 2024 09:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 19 23:32:18 2024

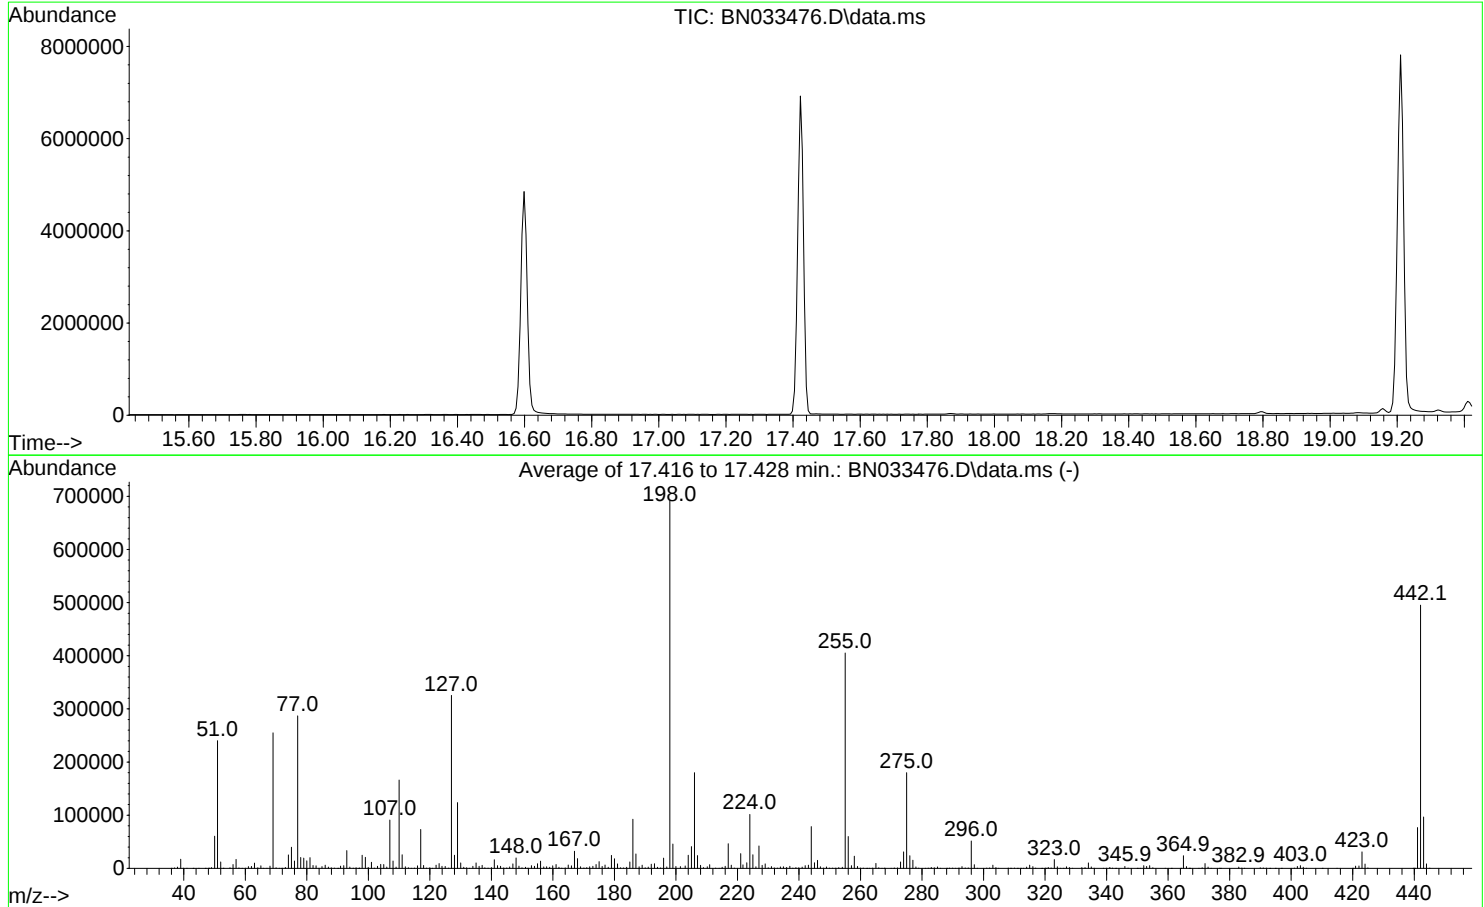




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	34.7	240406	PASS
68	69	0.00	2	1.7	4246	PASS
69	198	0.00	100	36.8	254997	PASS
70	69	0.00	2	0.5	1287	PASS
127	198	10	80	47.0	325376	PASS
197	198	0.00	2	0.4	2681	PASS
198	198	100	100	100.0	692117	PASS
199	198	5	9	6.6	45880	PASS
275	198	10	60	26.0	180075	PASS
365	198	1	100	3.4	23701	PASS
441	198	0.01	100	11.1	76696	PASS
442	442	50	100	100.0	495253	PASS
443	442	15	24	19.5	96547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081924\
Data File : BN033476.D
Acq On : 19 Aug 2024 09:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 04:51:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 04:49:48 2024
Response via : Initial Calibration

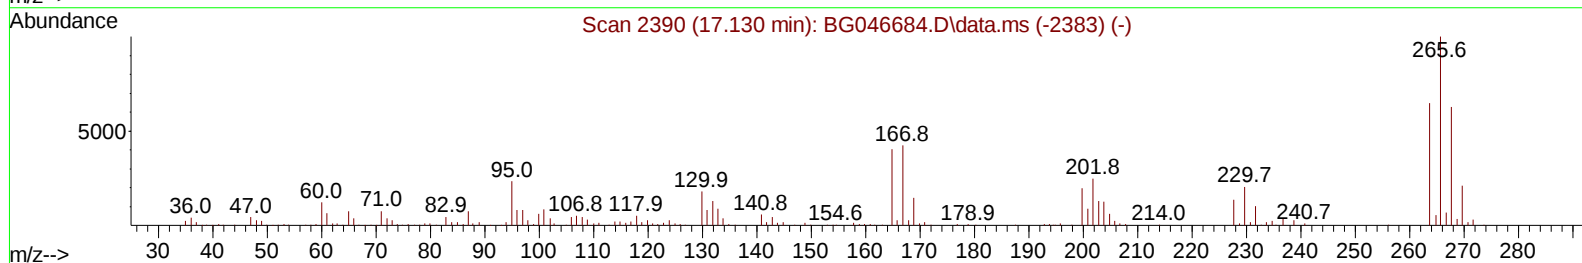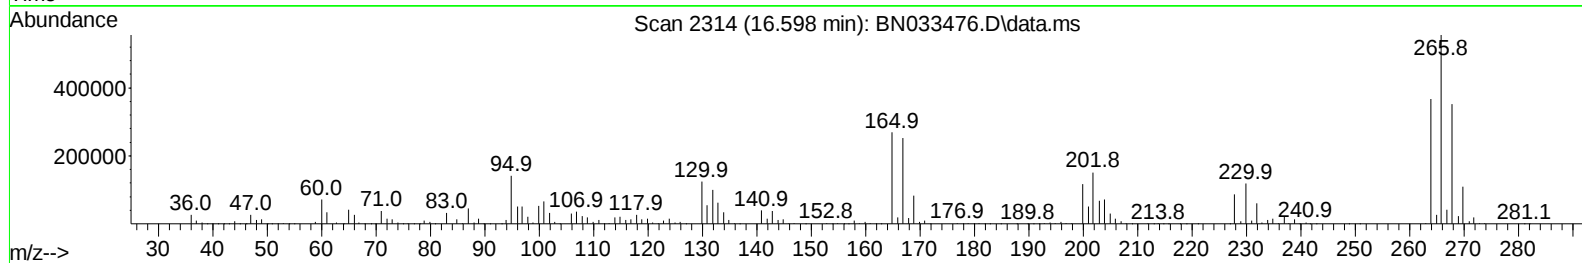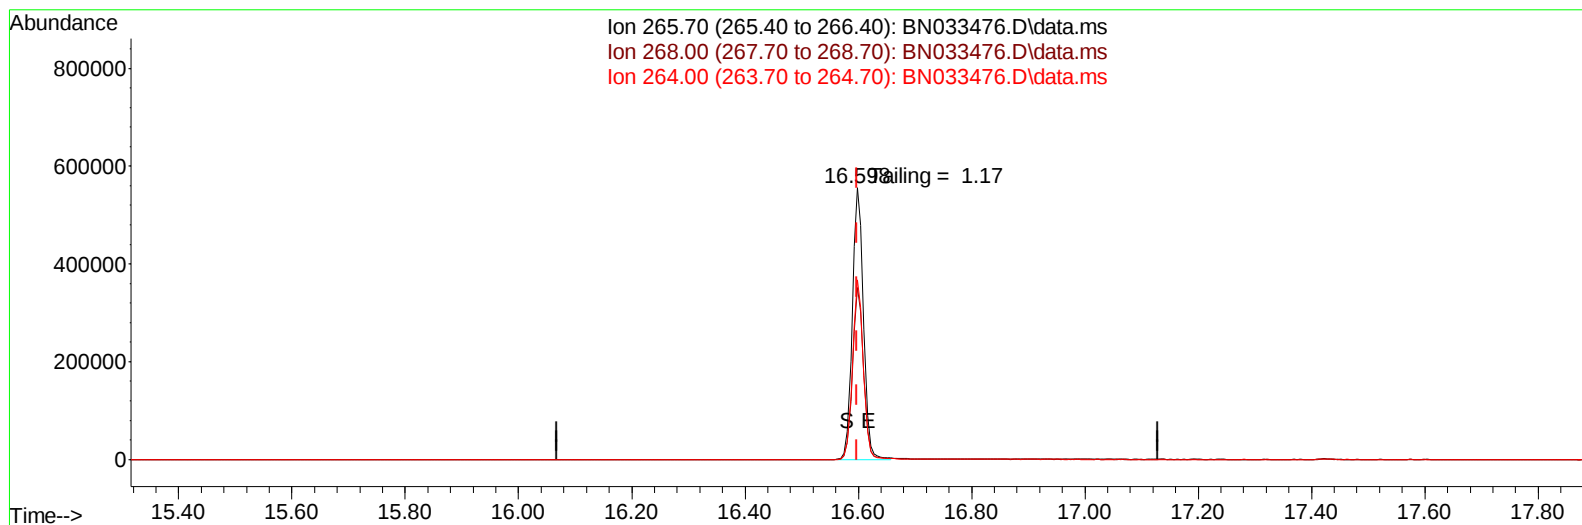

TIC: BN033476.D\data.ms

(70) Pentachlorophenol (C)

16.598min (+ 0.000) 22389.79 ng




response 769256

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.38
264.00	61.60	66.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081924\
Data File : BN033476.D
Acq On : 19 Aug 2024 09:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 04:51:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 04:49:48 2024
Response via : Initial Calibration

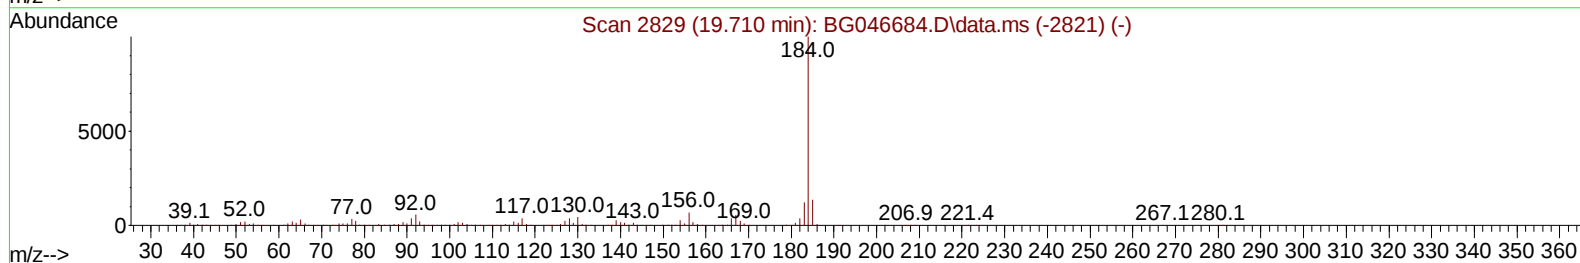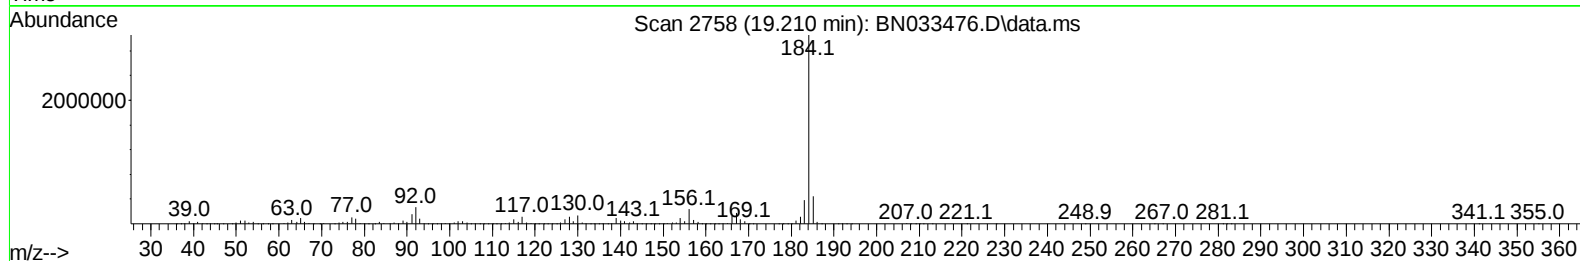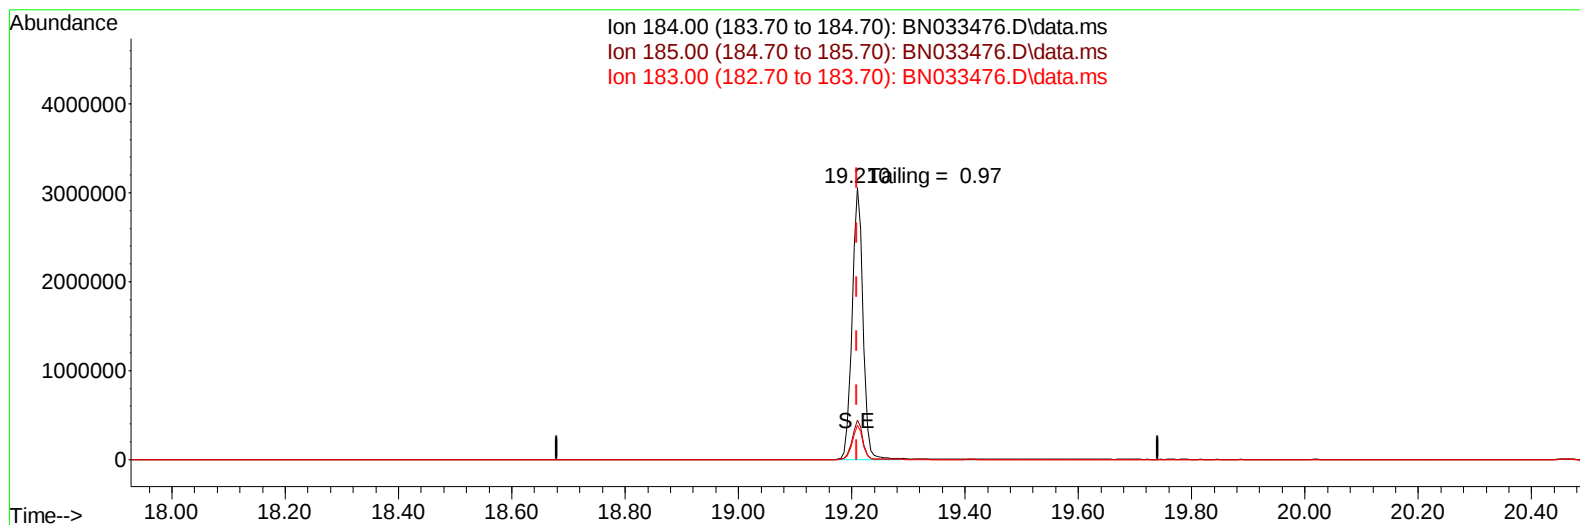

TIC: BN033476.D\data.ms

(77) Benzidine

19.210min (+ 0.000) 0.00 ng

response 4132097

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/19/2024	BNA_N	<u>BN033476.D</u>
Compound Name	Response	Retention Time
DDT	1828194	20.463
DDD	157103	20.016
DDE	3721	19.51
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
160824	1989018	8.09

Instrument :
BNA_N
ClientSampleId :
DFTPP