
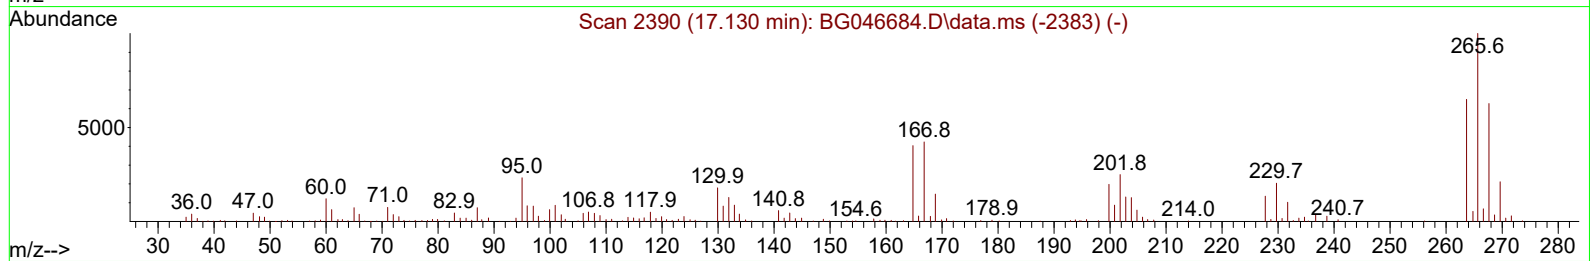
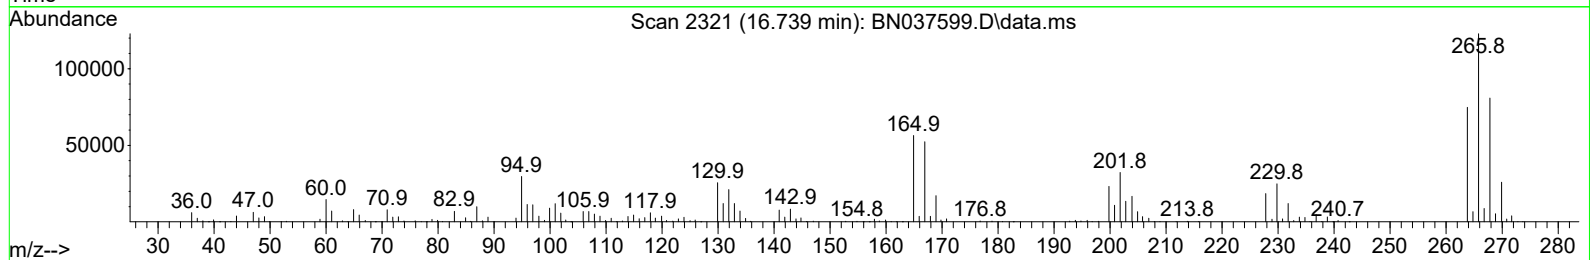


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037599.D
Acq On : 19 Aug 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 06:58:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

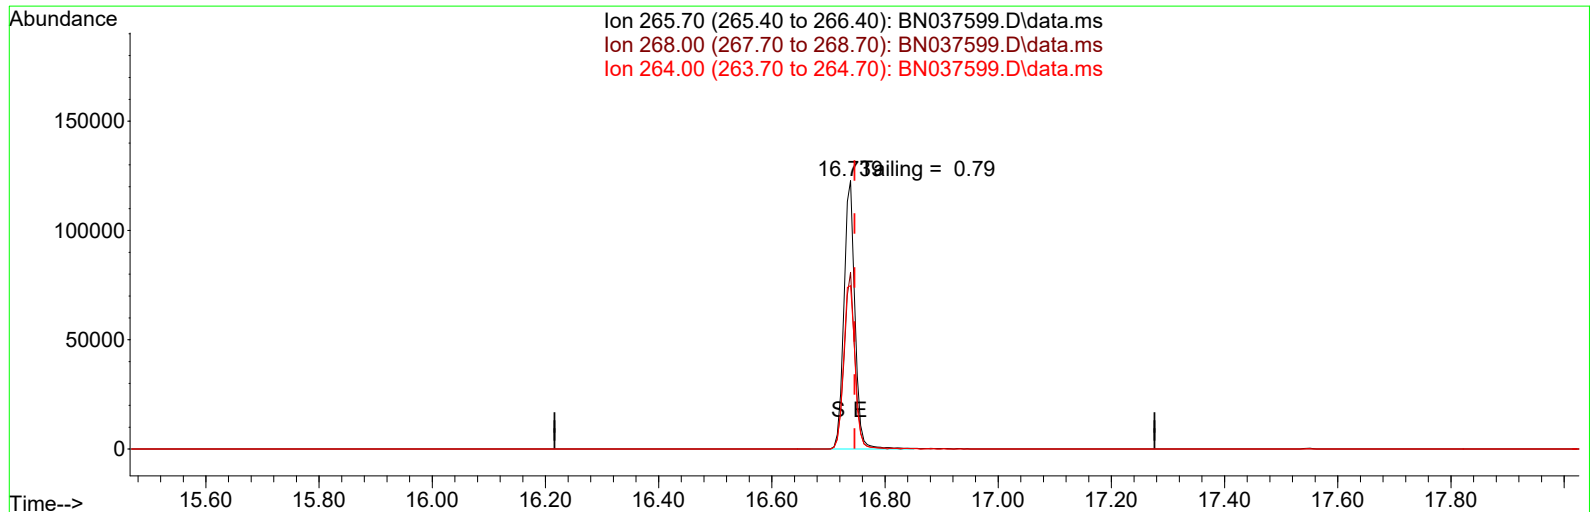

TIC: BN037599.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.007) 26205.47 ng

response 166374

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.84
264.00	61.60	60.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037599.D
Acq On : 19 Aug 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 06:58:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

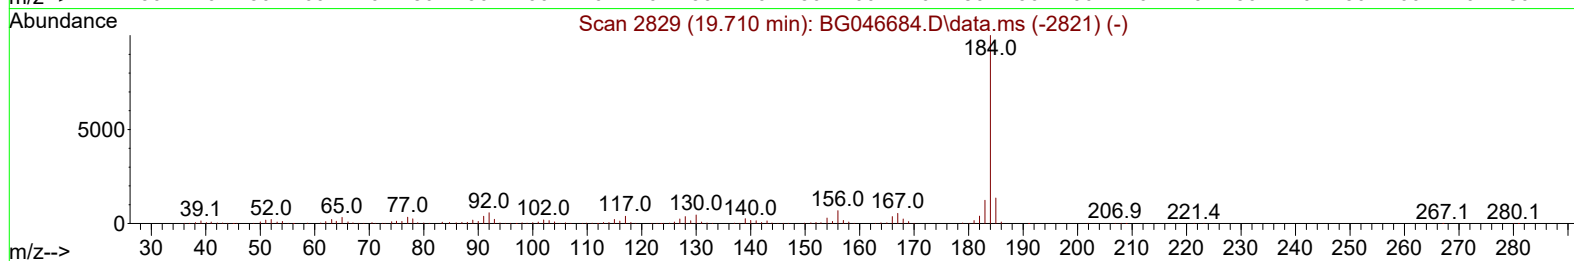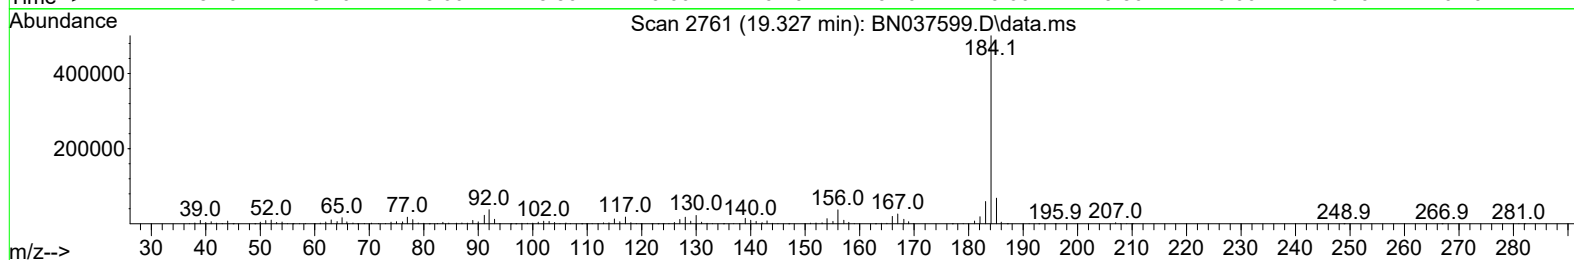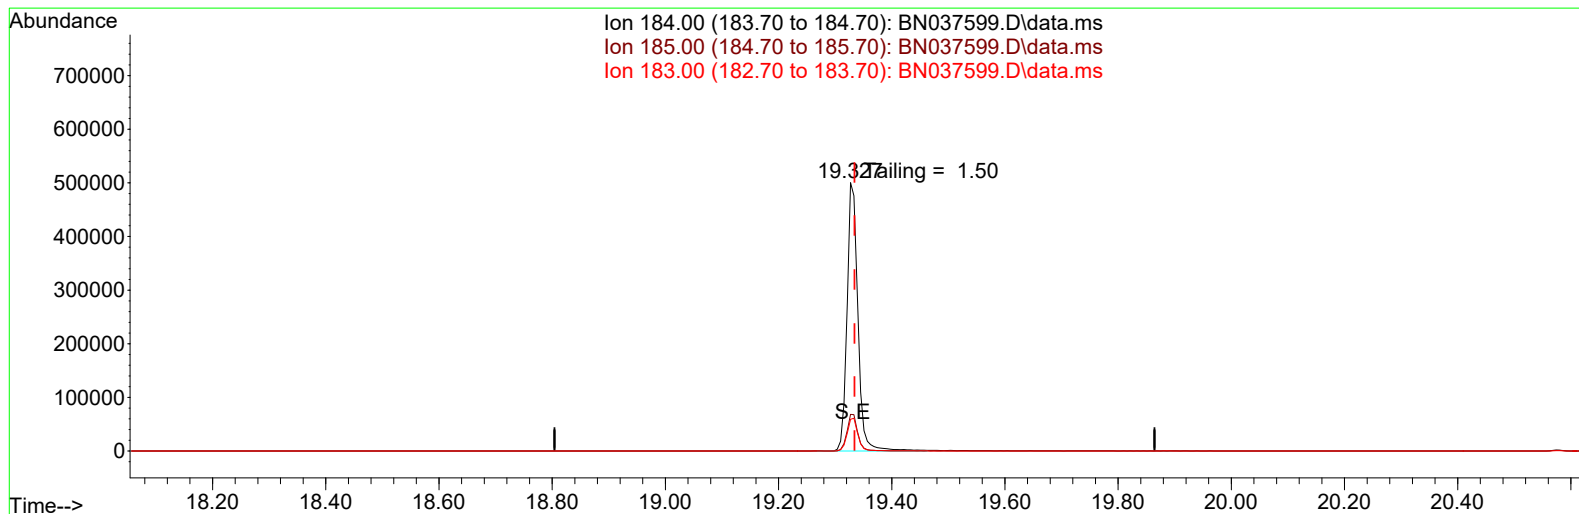

TIC: BN037599.D\data.ms

(77) Benzidine

19.327min (-0.007) 0.00 ng

response 670806

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	11.83
0.00	0.00	0.00